

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021820\
 Data File : PS008880.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Feb 2020 13:43
 Operator : DD\AJ
 Sample : L1547-13
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 19 00:46:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 05 02:36:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.247	6.942	581.9E6	259.4E6	271.108	279.926
Target Compounds							
1) T	Dalapon	0.000	2.594	0	269.6E6	N.D.	224.758
2) T	3,5-DICHL...	0.000	6.116	0	178.9E6	N.D.	130.061
6) T	MCP	7.663	0.000	91116895	0	14.824	N.D. #
7) T	MCPA	7.799	0.000	93416938	0	10.875	N.D. #
12) T	2,4,5-T	9.455	0.000	97530795	0	8.862	N.D. #
13) T	2,4-DB	10.017	0.000	65195517	0	40.081	N.D. #
14) T	DINOSEB	0.000	10.067	0	134.3E6	N.D.	36.577



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021820\
Data File : PS008880.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Feb 2020 13:43
Operator : DD\AJ
Sample : L1547-13
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 19 00:46:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
Quant Title : 8080.M
QLast Update : Wed Feb 05 02:36:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

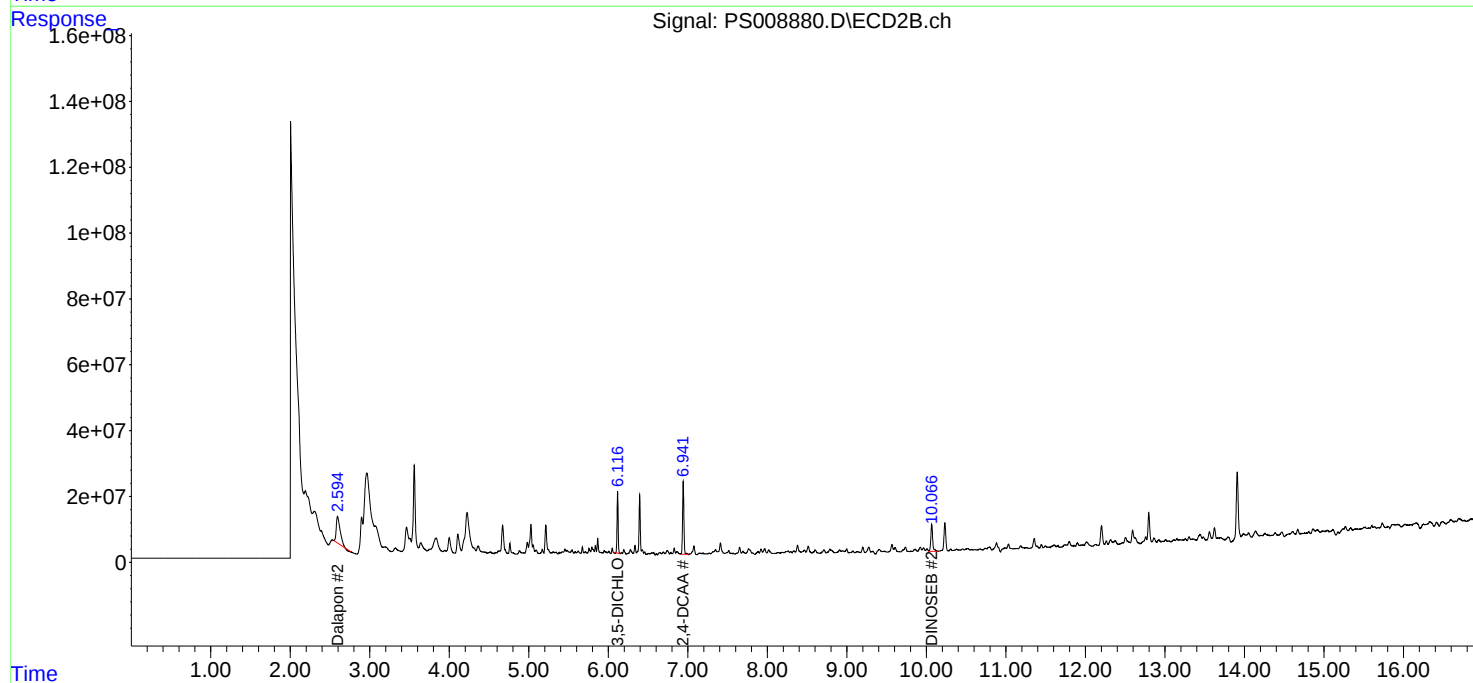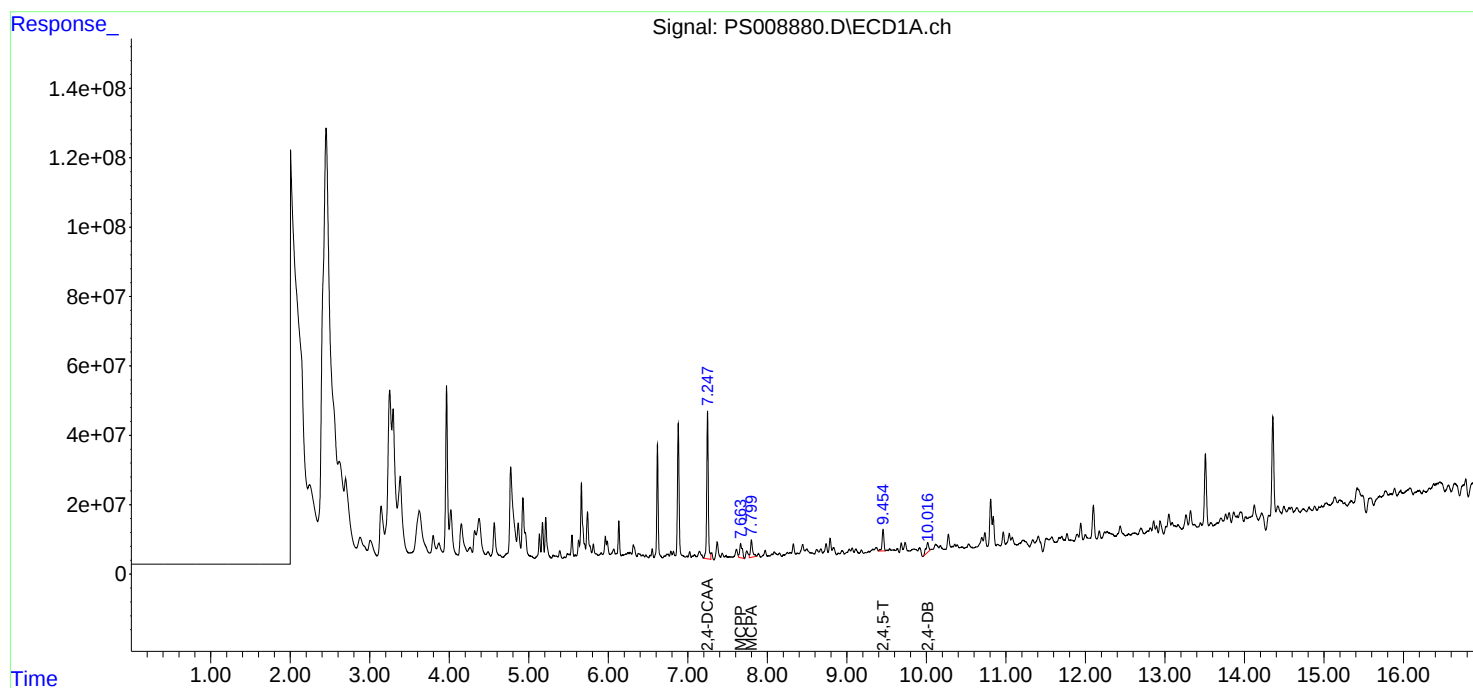


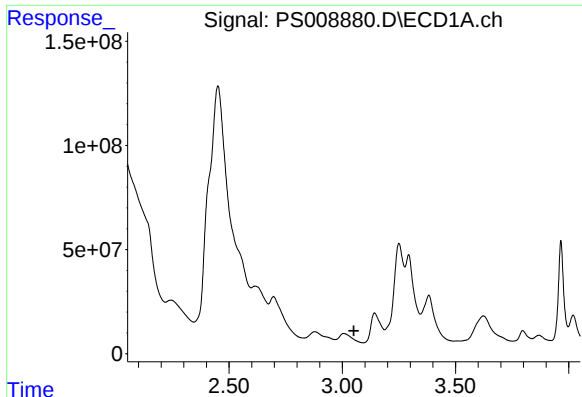

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.051 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

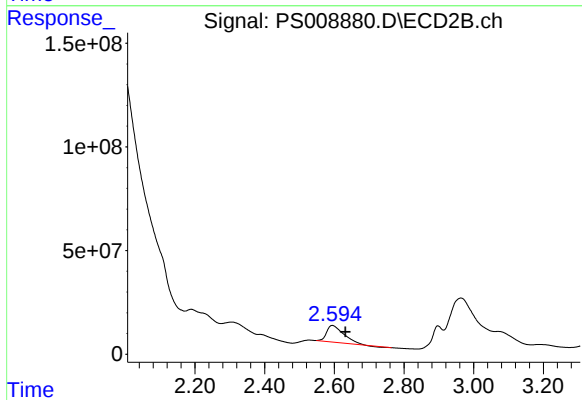


#1 Dalapon

R.T.: 2.594 min
Delta R.T.: -0.037 min
Response: 269556099
Conc: 224.76 ng/ml

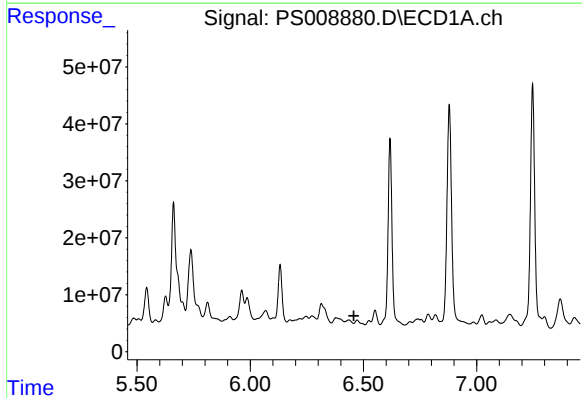


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.458 min
Response: 0
Conc: N.D.

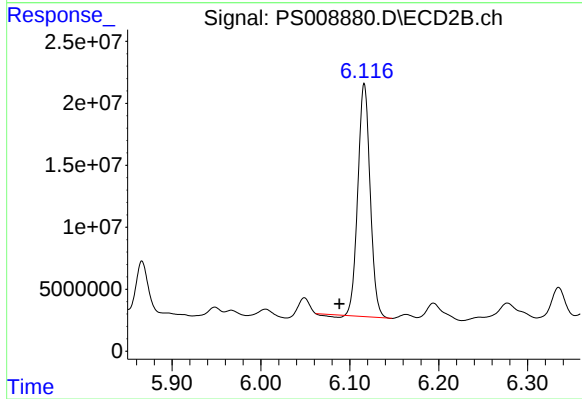

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.116 min
Delta R.T.: 0.028 min
Response: 178949266
Conc: 130.06 ng/ml

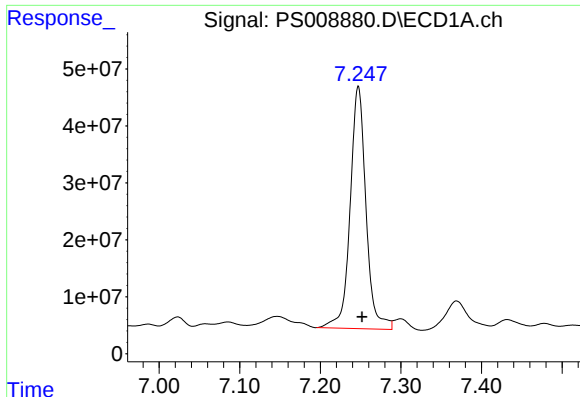

#4 2,4-DCAA


R.T.: 7.247 min
Delta R.T.: -0.005 min
Response: 581881259
Conc: 271.11 ng/ml

Instrument :
ECD_S
ClientSampleId :

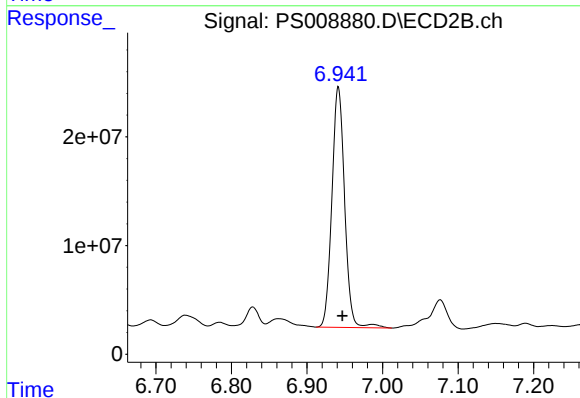


#4 2,4-DCAA

R.T.: 6.942 min
Delta R.T.: -0.005 min
Response: 259442291
Conc: 279.93 ng/ml

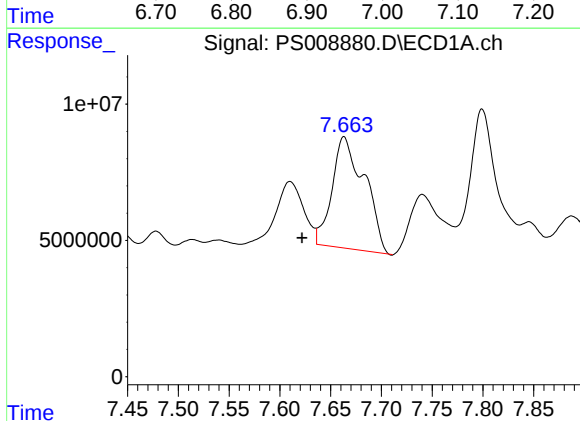


#6 MCP

R.T.: 7.663 min
Delta R.T.: 0.041 min
Response: 91116895
Conc: 14.82 ug/ml

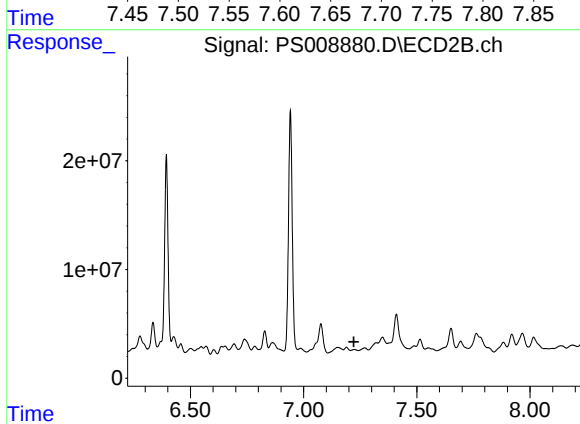

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.222 min
Response: 0
Conc: N.D.

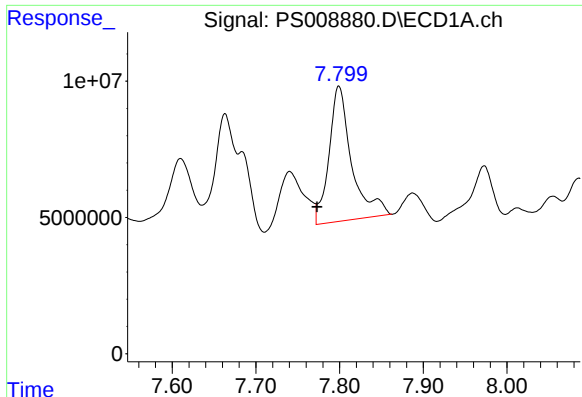

#7 MCPA


R.T.: 7.799 min
Delta R.T.: 0.026 min
Response: 93416938
Conc: 10.87 ug/ml

Instrument :
ECD_S
ClientSampleId :

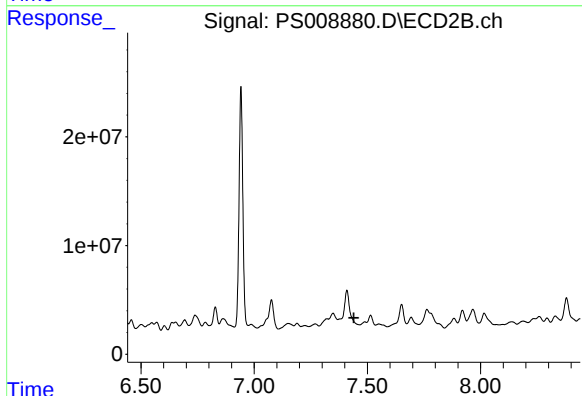


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.441 min
Response: 0
Conc: N.D.

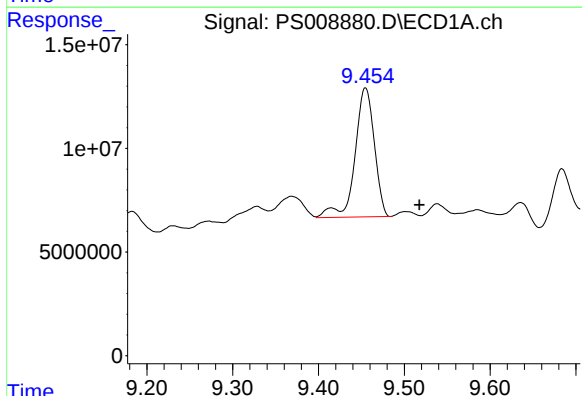


#12 2,4,5-T

R.T.: 9.455 min
Delta R.T.: -0.063 min
Response: 97530795
Conc: 8.86 ng/ml

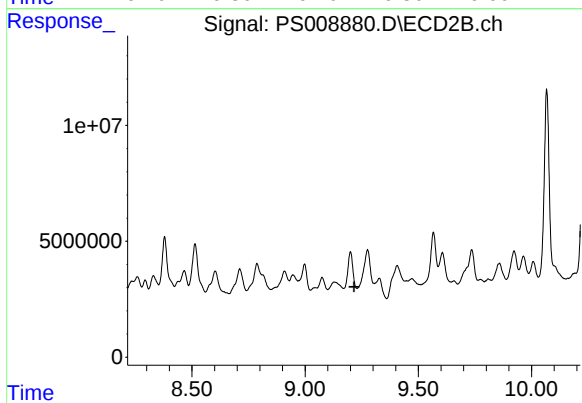

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 9.216 min
Response: 0
Conc: N.D.

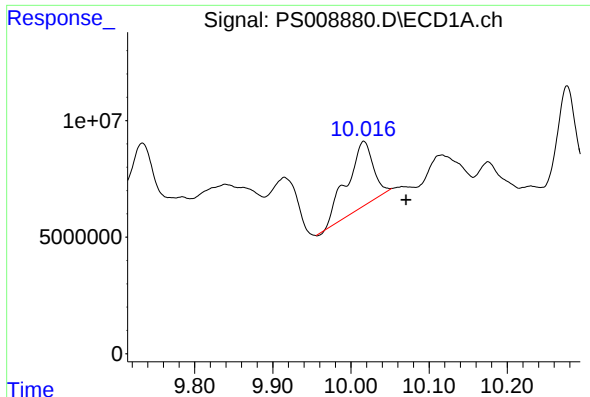

#13 2,4-DB


R.T.: 10.017 min
Delta R.T.: -0.054 min
Response: 65195517
Conc: 40.08 ng/ml

Instrument :
ECD_S
ClientSampleId :

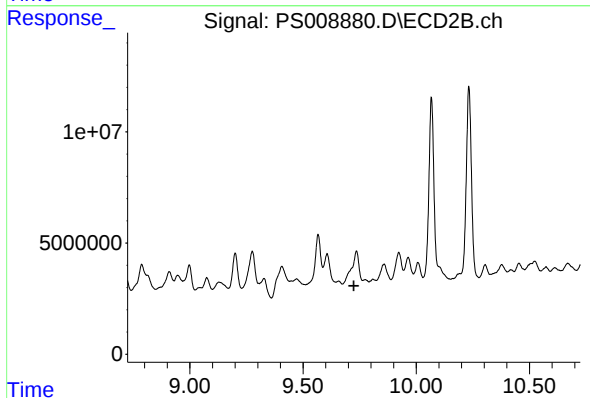


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.724 min
Response: 0
Conc: N.D.

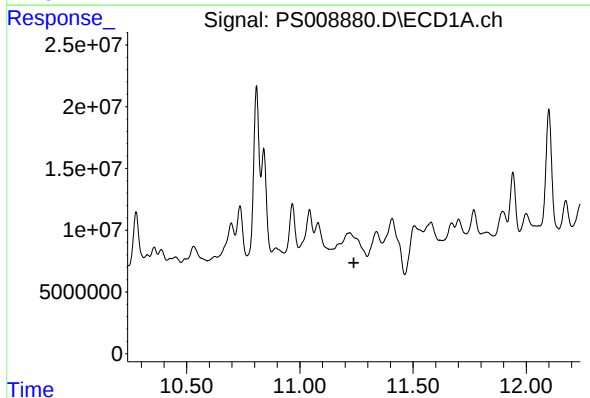

#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.239 min
Response: 0
Conc: N.D.

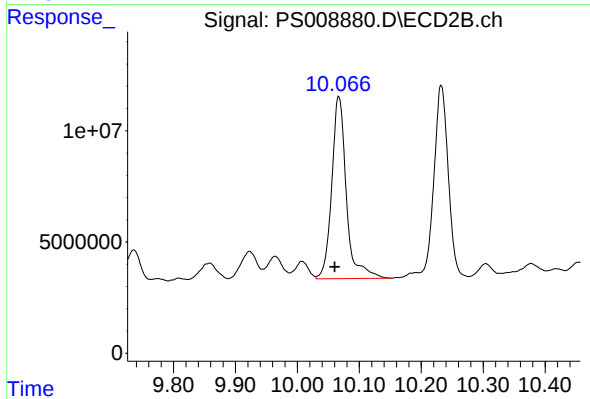

#14 DINOSEB

R.T.: 10.067 min
Delta R.T.: 0.006 min
Response: 134347647
Conc: 36.58 ng/ml