

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021820\
 Data File : PS008885.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Feb 2020 15:38
 Operator : DD\AJ
 Sample : L1551-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 19 00:47:02 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 05 02:36:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.247	6.942	976.4E6	446.7E6	454.900	481.966
Target Compounds							
1) T	Dalapon	0.000	2.598	0	503.4E6	N.D.	419.736
2) T	3,5-DICHL...	0.000	6.117	0	129.1E6	N.D.	93.800
10) T	Pentachlo...	8.677	8.468	199.5E6	102.2E6	7.017	7.749
15) T	Picloram	11.043	11.033	309.4E6	199.5E6	20.430	26.426 #
16) T	DCPA	0.000	11.033	0	199.5E6	N.D.	30.667



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021820\
Data File : PS008885.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Feb 2020 15:38
Operator : DD\AJ
Sample : L1551-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 19 00:47:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
Quant Title : 8080.M
QLast Update : Wed Feb 05 02:36:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

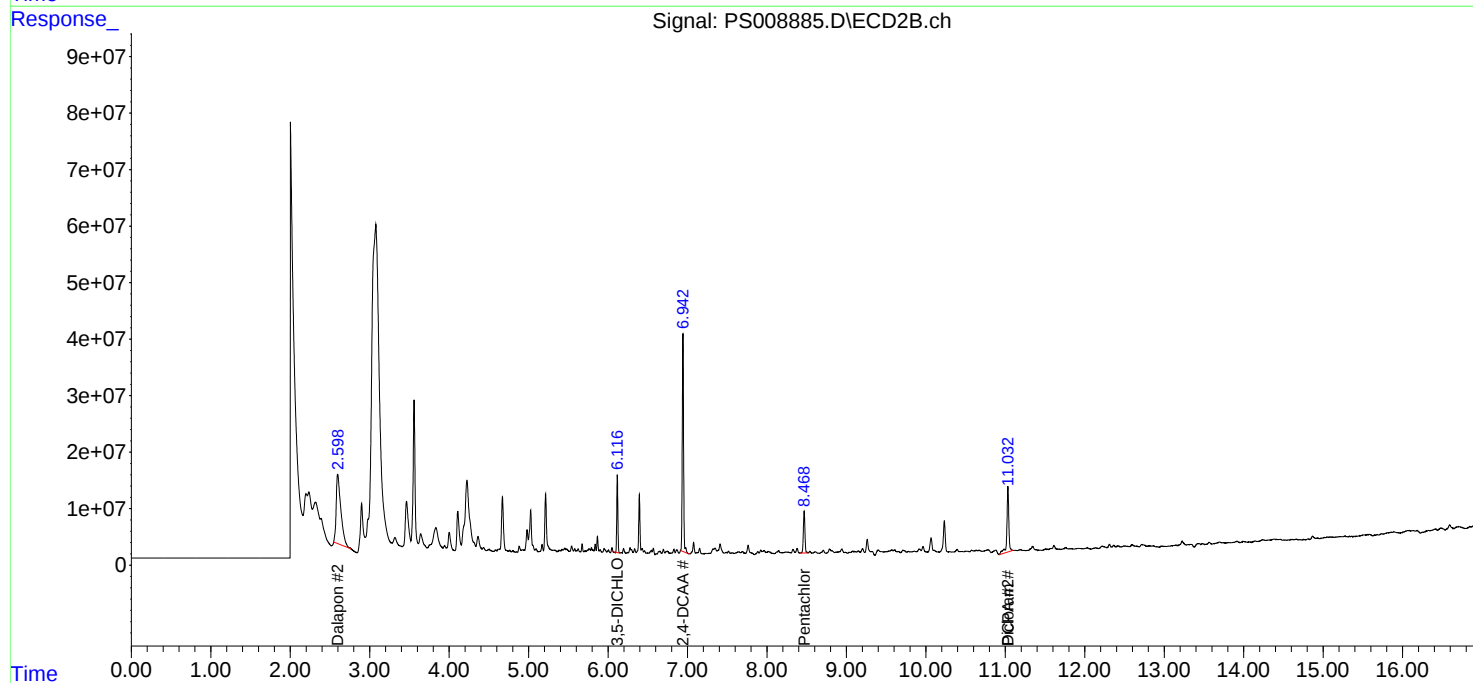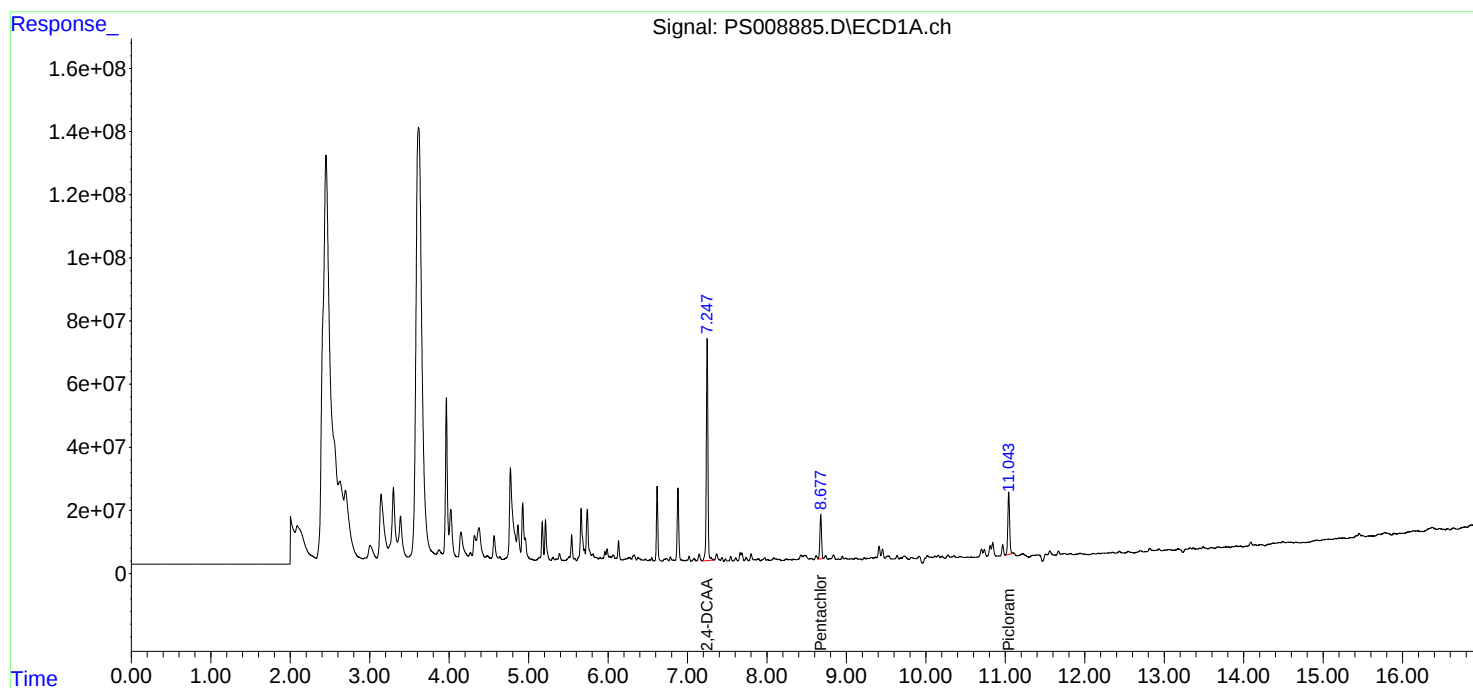


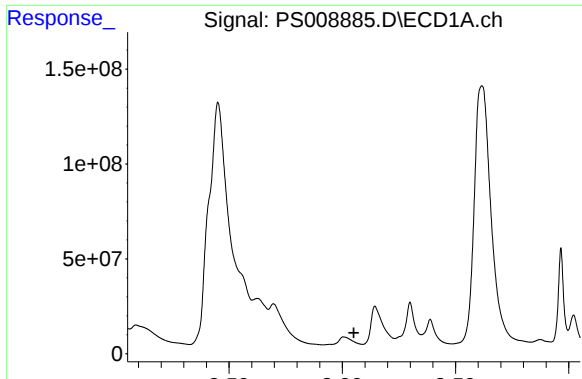

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.051 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

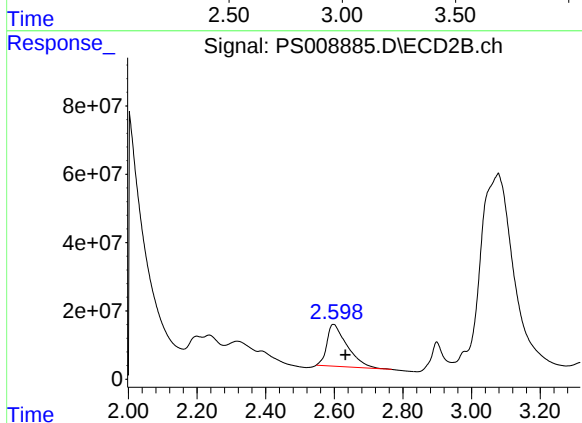


#1 Dalapon

R.T.: 2.598 min
Delta R.T.: -0.034 min
Response: 503397149
Conc: 419.74 ng/ml

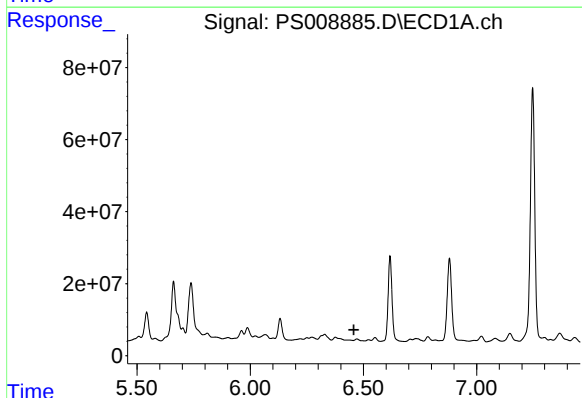


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.458 min
Response: 0
Conc: N.D.

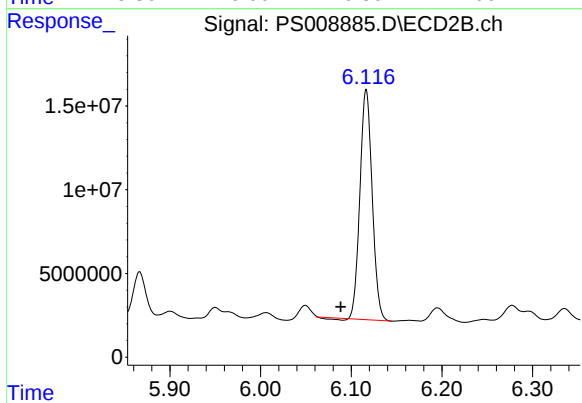

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.117 min
Delta R.T.: 0.028 min
Response: 129057977
Conc: 93.80 ng/ml

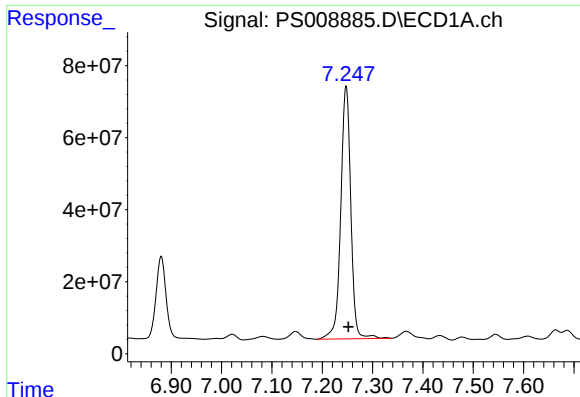

#4 2,4-DCAA


R.T.: 7.247 min
Delta R.T.: -0.004 min
Response: 976354939
Conc: 454.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

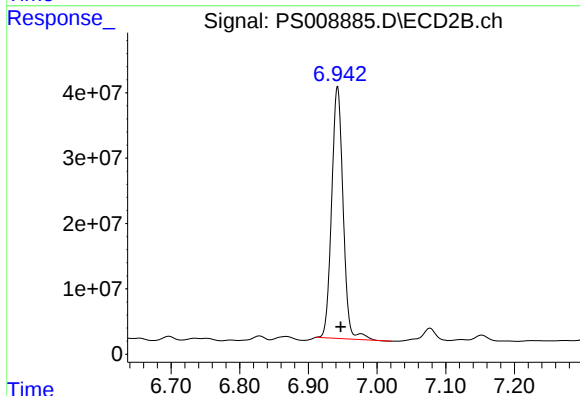


#4 2,4-DCAA

R.T.: 6.942 min
Delta R.T.: -0.004 min
Response: 446698172
Conc: 481.97 ng/ml

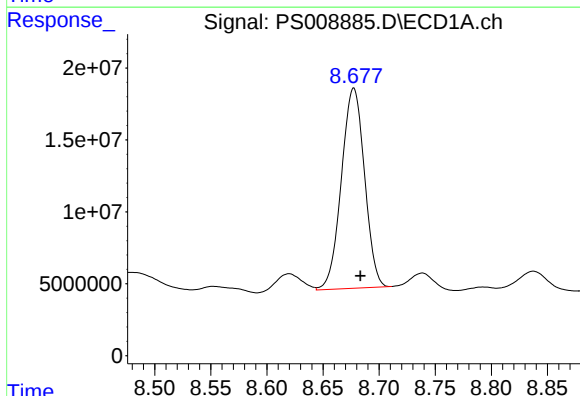


#10 Pentachlorophenol

R.T.: 8.677 min
Delta R.T.: -0.006 min
Response: 199473319
Conc: 7.02 ng/ml

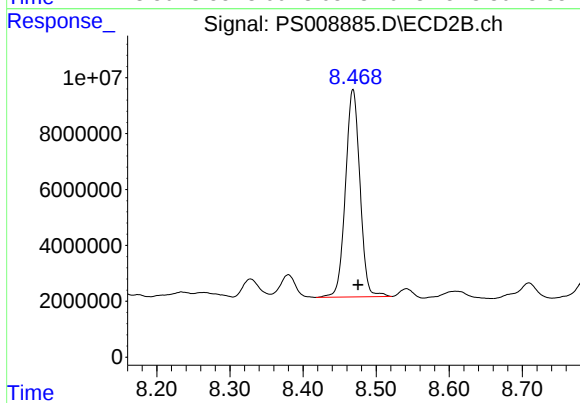

#10 Pentachlorophenol


R.T.: 8.468 min
Delta R.T.: -0.007 min
Response: 102196264
Conc: 7.75 ng/ml

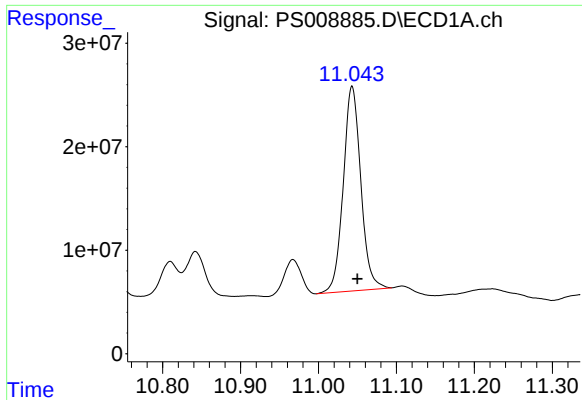

#15 Picloram


R.T.: 11.043 min
Delta R.T.: -0.007 min
Response: 309382057
Conc: 20.43 ng/ml

Instrument :
ECD_S
ClientSampleId :

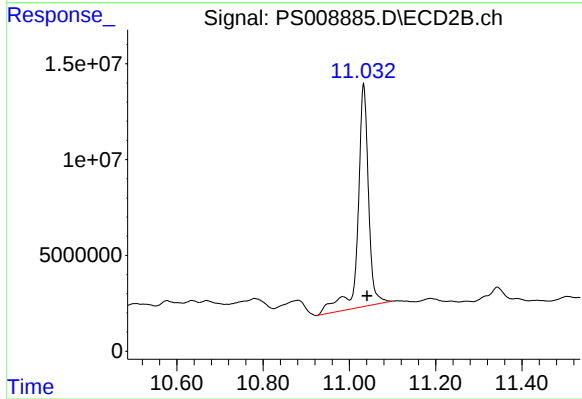


#15 Picloram

R.T.: 11.033 min
Delta R.T.: -0.008 min
Response: 199463810
Conc: 26.43 ng/ml

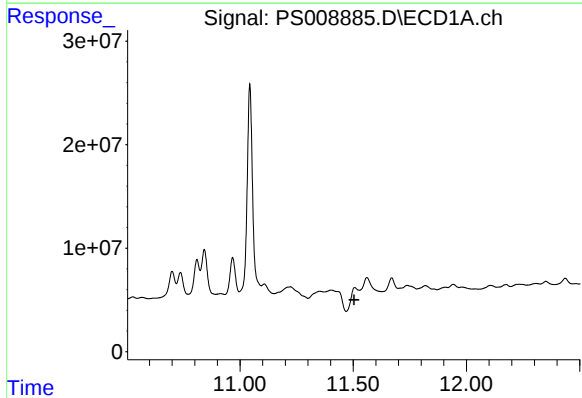

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.503 min
Response: 0
Conc: N.D.

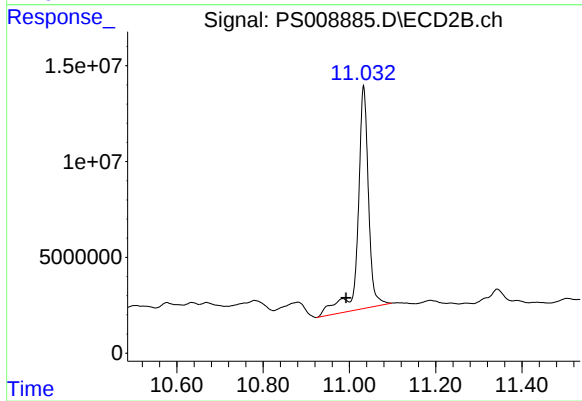

#16 DCPA

R.T.: 11.033 min
Delta R.T.: 0.041 min
Response: 199463810
Conc: 30.67 ng/ml