

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021820\
 Data File : PS008887.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Feb 2020 16:23
 Operator : DD\AJ
 Sample : L1552-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 19 00:47:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 05 02:36:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.246	6.942	471.4E6	137.0E6	219.627	147.864 #
Target Compounds							
1) T	Dalapon	0.000	2.593	0	262.6E6	N.D.	218.937
2) T	3,5-DICHL...	0.000	6.116	0	127.2E6	N.D.	92.446
5) T	DICAMBA	0.000	7.153	0	46050561	N.D.	11.834
6) T	MCPD	0.000	7.153	0	46050561	N.D.	15.693
7) T	MCPA	7.800	0.000	64177086	0	7.471	N.D. #
10) T	Pentachlo...	8.677	8.469	325.9E6	170.5E6	11.463	12.924
12) T	2,4,5-T	9.456	0.000	84108783	0	7.642	N.D. #
14) T	DINOSEB	0.000	10.068	0	49847392	N.D.	13.571
16) T	DCPA	11.561	0.000	64779744	0	4.621	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021820\
Data File : PS008887.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Feb 2020 16:23
Operator : DD\AJ
Sample : L1552-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 19 00:47:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
Quant Title : 8080.M
QLast Update : Wed Feb 05 02:36:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

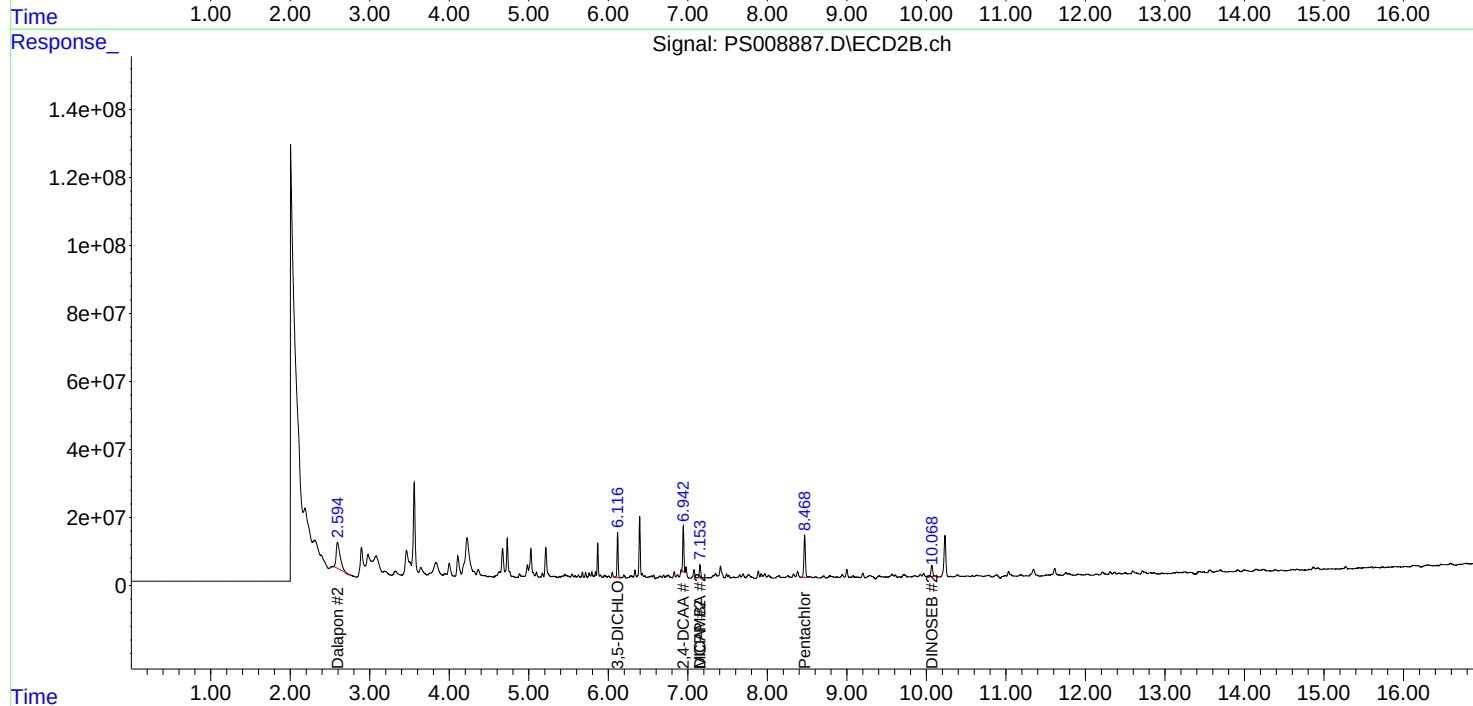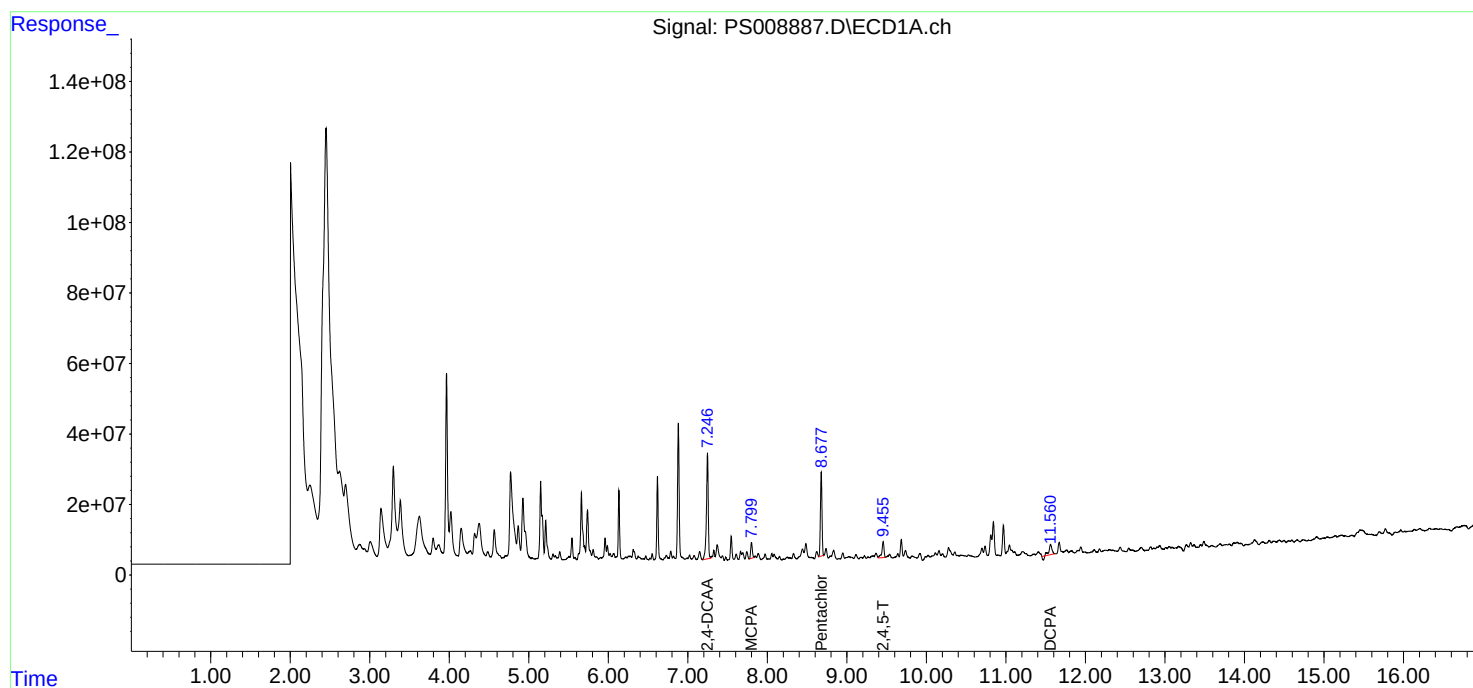


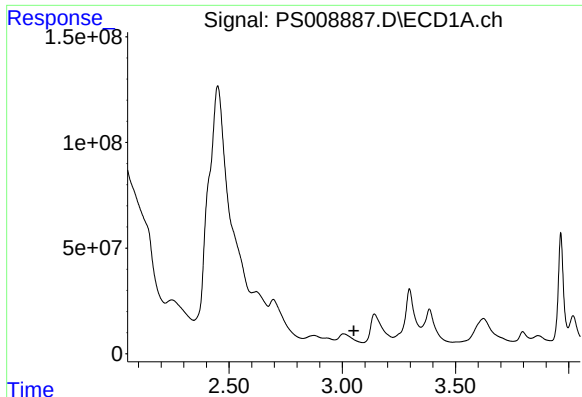

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.051 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

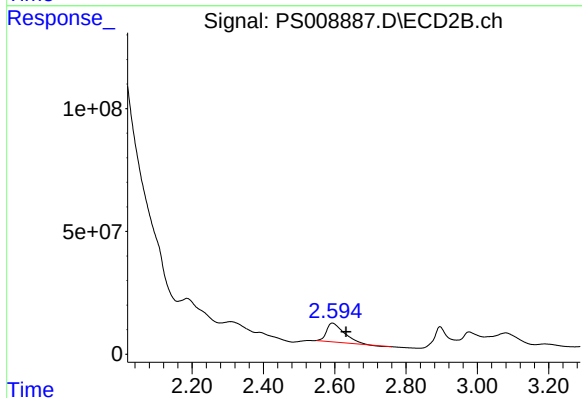


#1 Dalapon

R.T.: 2.593 min
Delta R.T.: -0.038 min
Response: 262574580
Conc: 218.94 ng/ml

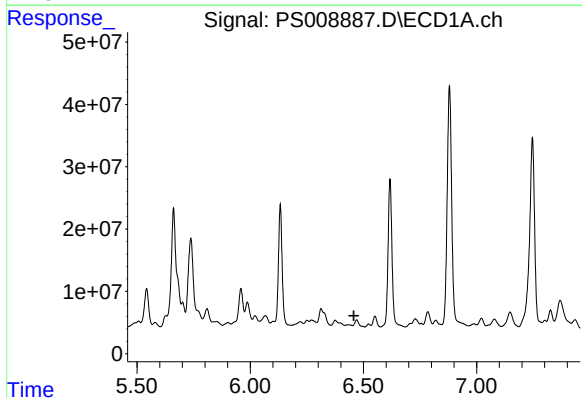


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.458 min
Response: 0
Conc: N.D.

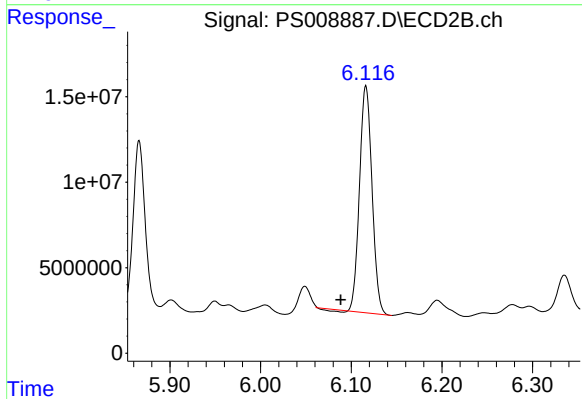

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.116 min
Delta R.T.: 0.028 min
Response: 127194717
Conc: 92.45 ng/ml

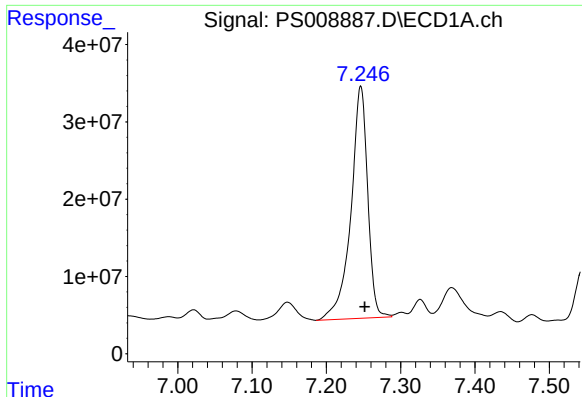

#4 2,4-DCAA


R.T.: 7.246 min
Delta R.T.: -0.005 min
Response: 471388308
Conc: 219.63 ng/ml

Instrument :
ECD_S
ClientSampleId :

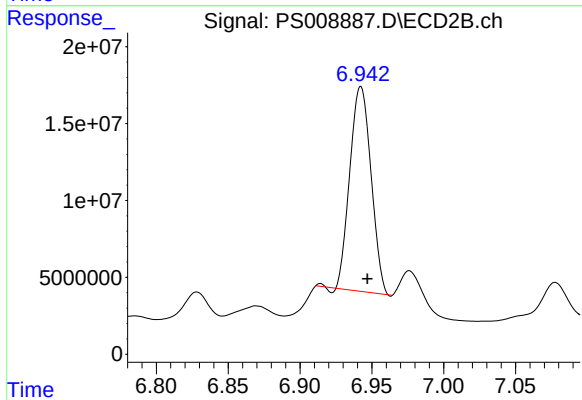


#4 2,4-DCAA

R.T.: 6.942 min
Delta R.T.: -0.004 min
Response: 137043967
Conc: 147.86 ng/ml

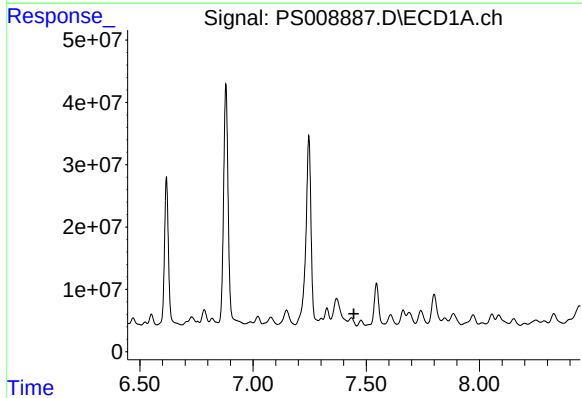


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.445 min
Response: 0
Conc: N.D.

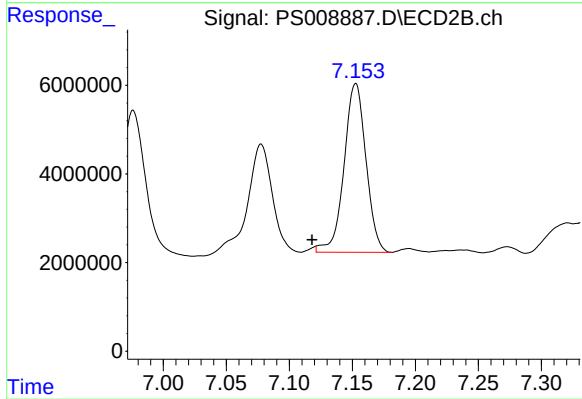

#5 DICAMBA


R.T.: 7.153 min
Delta R.T.: 0.035 min
Response: 46050561
Conc: 11.83 ng/ml

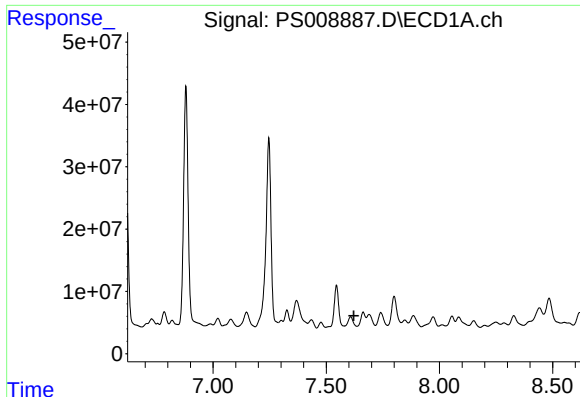

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 7.622 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

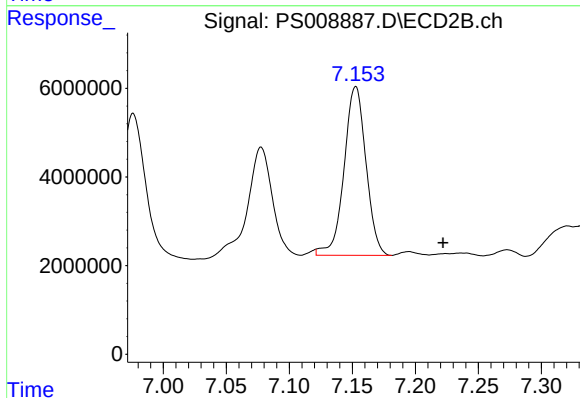


#6 MCPP

R.T.: 7.153 min
Delta R.T.: -0.069 min
Response: 46050561
Conc: 15.69 ug/ml

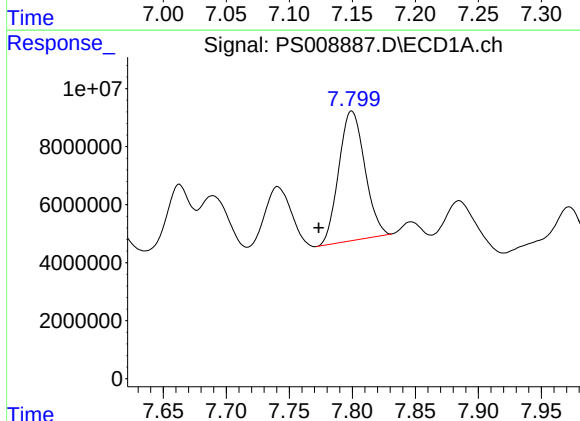


#7 MCPA

R.T.: 7.800 min
Delta R.T.: 0.026 min
Response: 64177086
Conc: 7.47 ug/ml

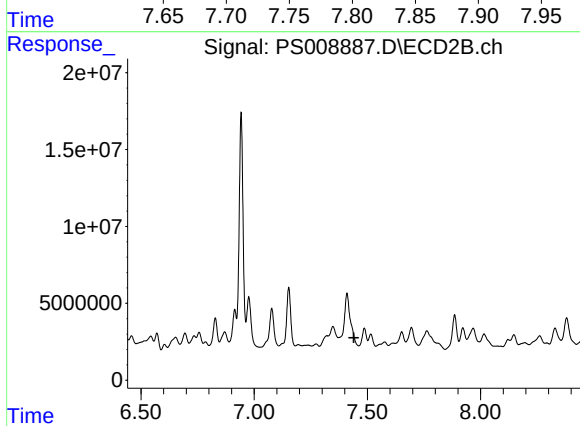

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.441 min
Response: 0
Conc: N.D.

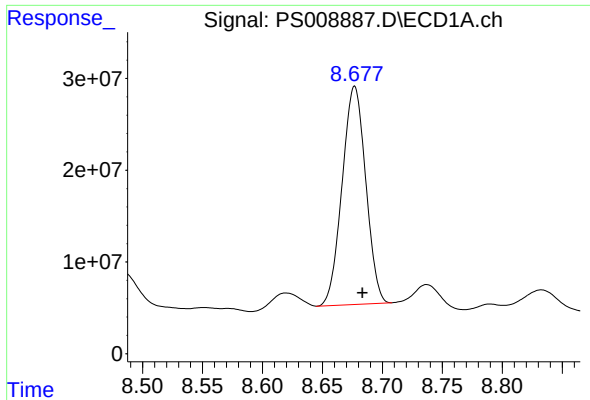

#10 Pentachlorophenol


R.T.: 8.677 min
Delta R.T.: -0.006 min
Response: 325886189
Conc: 11.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

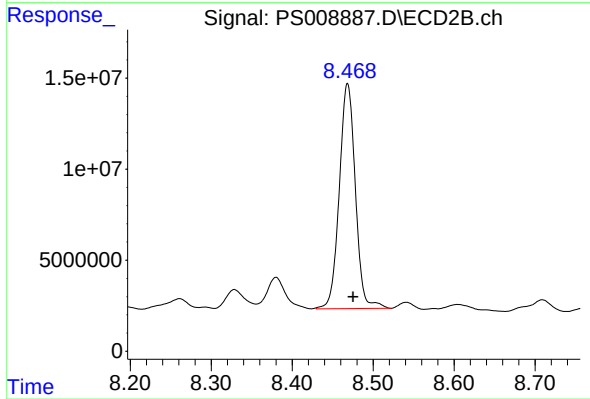


#10 Pentachlorophenol

R.T.: 8.469 min
Delta R.T.: -0.007 min
Response: 170455440
Conc: 12.92 ng/ml

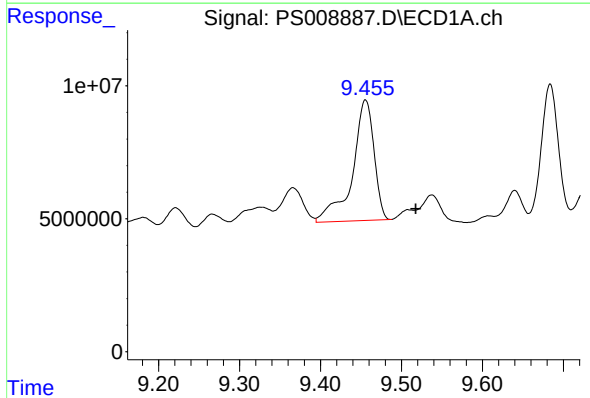


#12 2,4,5-T

R.T.: 9.456 min
Delta R.T.: -0.062 min
Response: 84108783
Conc: 7.64 ng/ml

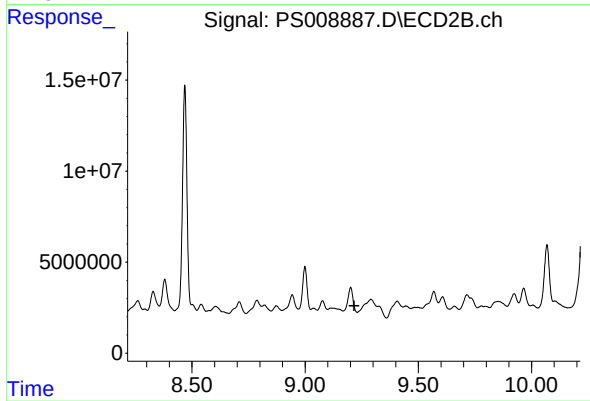

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.216 min
Response: 0
Conc: N.D.

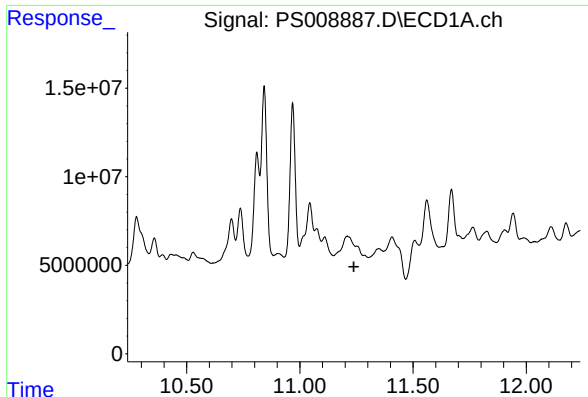

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 11.239 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

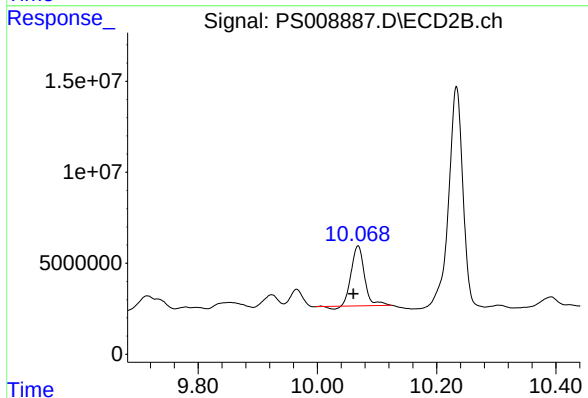


#14 DINOSEB

R.T.: 10.068 min
Delta R.T.: 0.007 min
Response: 49847392
Conc: 13.57 ng/ml

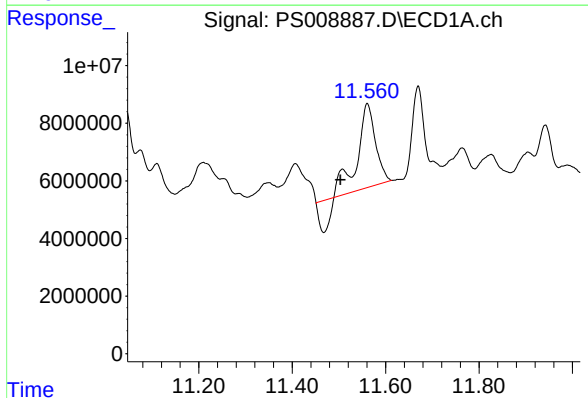

#16 DCPA

R.T.: 11.561 min
Delta R.T.: 0.058 min
Response: 64779744
Conc: 4.62 ng/ml

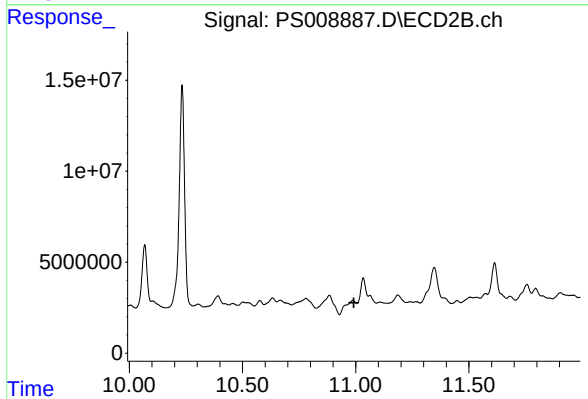

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.992 min
Response: 0
Conc: N.D.