

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021820\
 Data File : PS008892.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Feb 2020 18:17
 Operator : DD\AJ
 Sample : PB126894TB
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 19 00:48:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 05 02:36:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.247	6.942	716.8E6	355.1E6	333.972	383.086
Target Compounds							
2) T	3,5-DICHL...	0.000	6.116	0	130.6E6	N.D.	94.944
6) T	MCP	7.691	0.000	214.9E6	0	34.954	N.D. #
12) T	2,4,5-T	9.452	0.000	102.4E6	0	9.301	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021820\
Data File : PS008892.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Feb 2020 18:17
Operator : DD\AJ
Sample : PB126894TB
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 19 00:48:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
Quant Title : 8080.M
QLast Update : Wed Feb 05 02:36:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

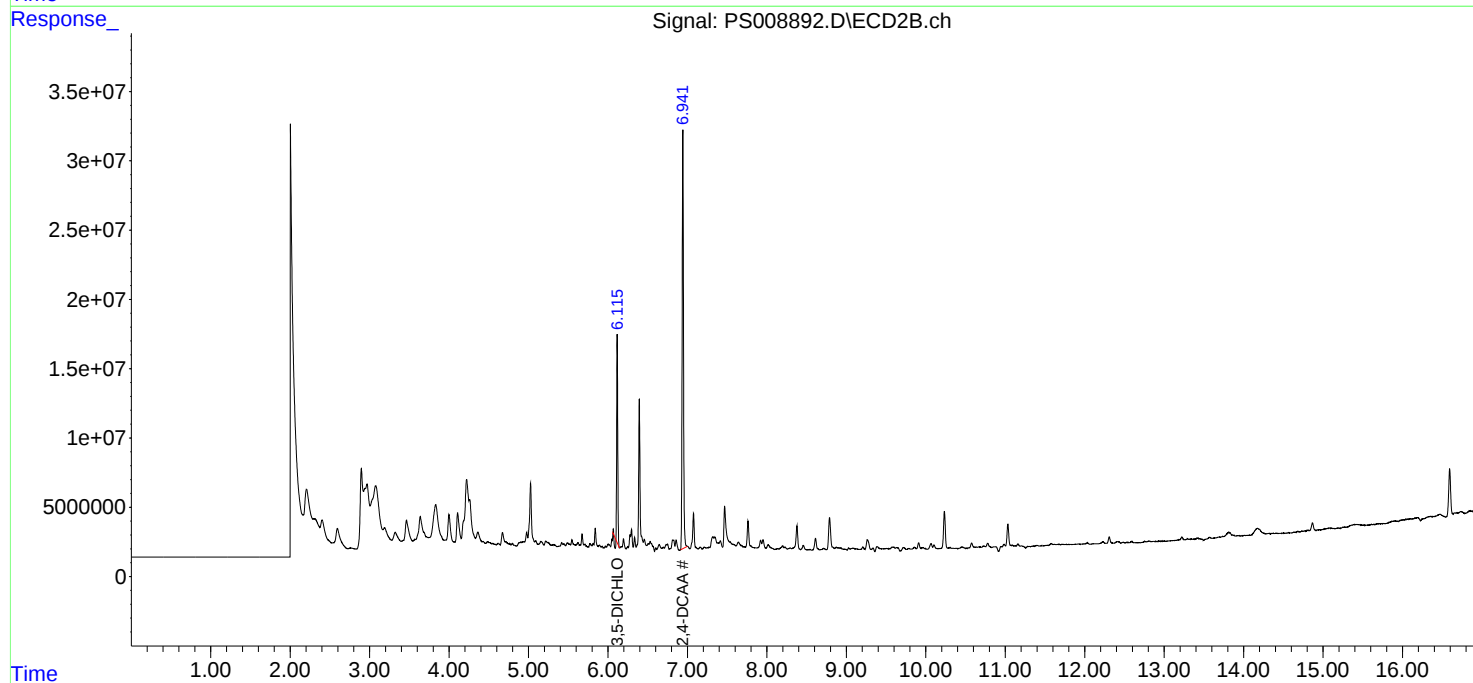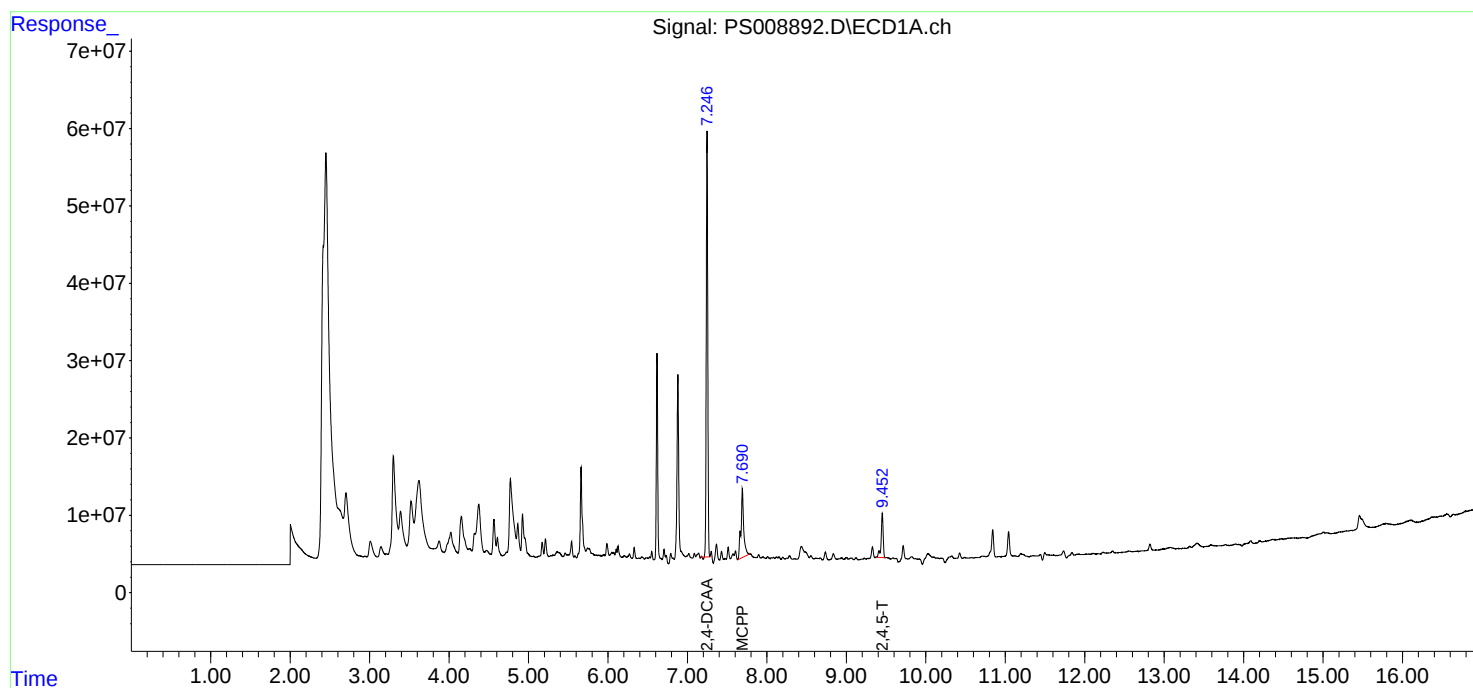


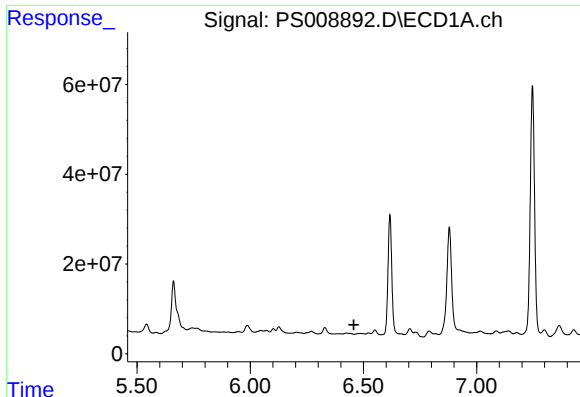

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.458 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

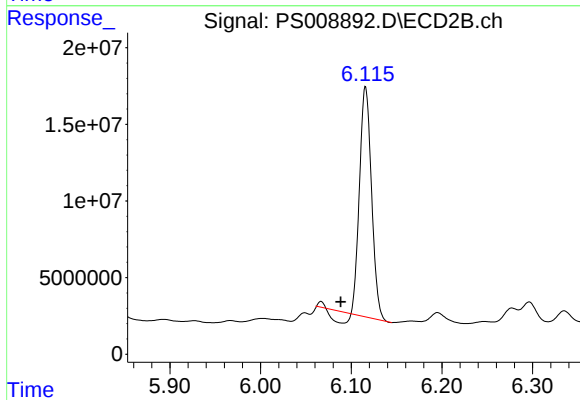


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.116 min
Delta R.T.: 0.028 min
Response: 130631646
Conc: 94.94 ng/ml

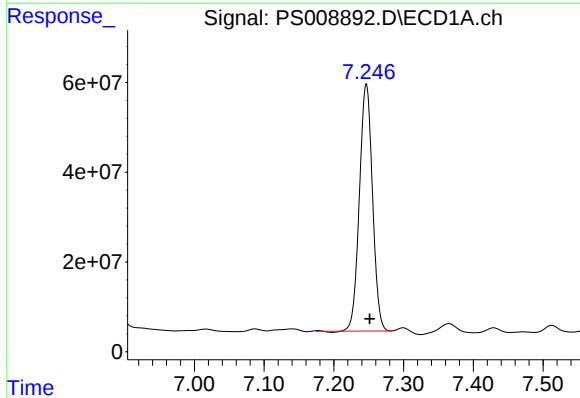


#4 2,4-DCAA

R.T.: 7.247 min
Delta R.T.: -0.005 min
Response: 716807727
Conc: 333.97 ng/ml

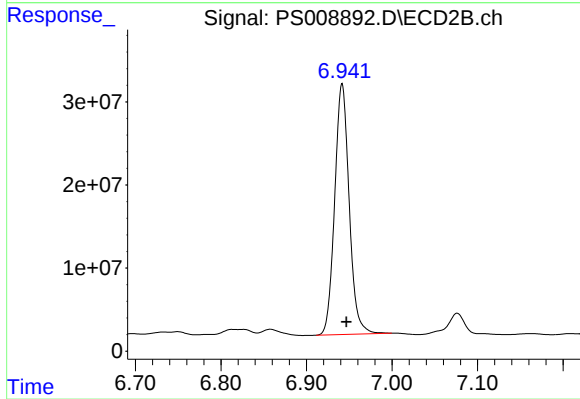

#4 2,4-DCAA


R.T.: 6.942 min
Delta R.T.: -0.005 min
Response: 355053579
Conc: 383.09 ng/ml

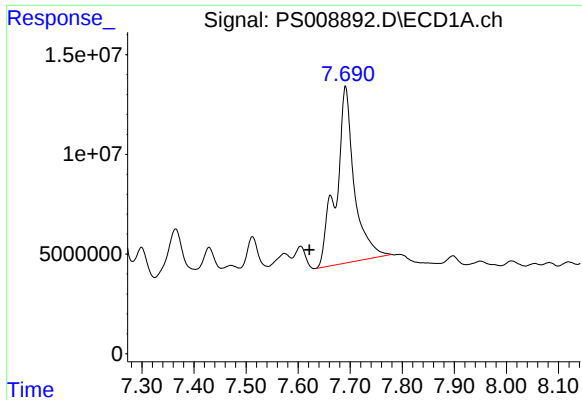

#6 MCP


R.T.: 7.691 min
Delta R.T.: 0.069 min
Response: 214851218
Conc: 34.95 ug/ml

Instrument :
ECD_S
ClientSampleId :

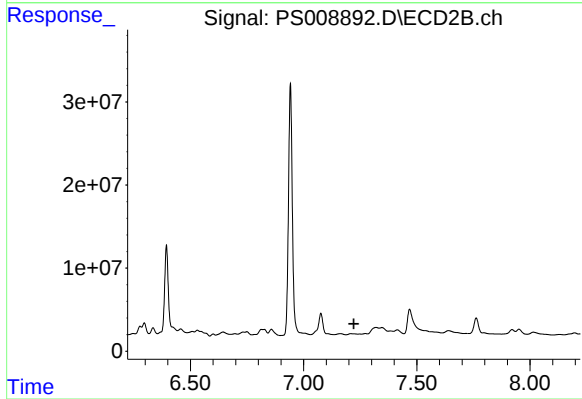


#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.222 min
Response: 0
Conc: N.D.

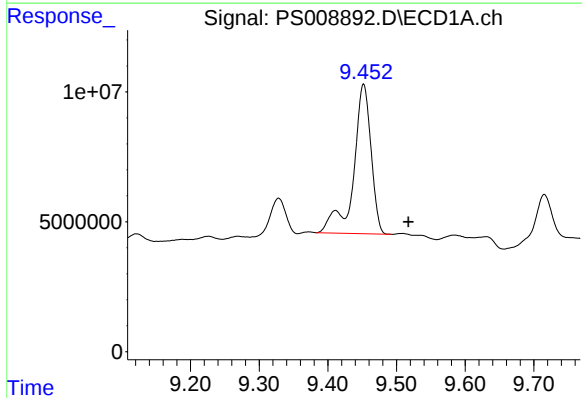

#12 2,4,5-T

R.T.: 9.452 min
Delta R.T.: -0.065 min
Response: 102366164
Conc: 9.30 ng/ml

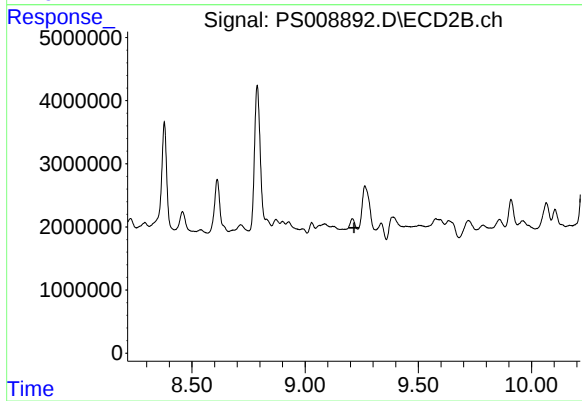

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.216 min
Response: 0
Conc: N.D.