

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021820\
 Data File : PS008897.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Feb 2020 20:12
 Operator : DD\AJ
 Sample : L1365-16
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 19 00:48:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 05 02:36:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.246	6.942	812.5E6	404.7E6	378.568	436.612
Target Compounds							
2) T	3,5-DICHL...	0.000	6.116	0	140.3E6	N.D.	102.004
6) T	MCPP	7.662	0.000	46290972	0	7.531	N.D. #
12) T	2,4,5-T	9.452	0.000	106.2E6	0	9.651	N.D. #
15) T	Picloram	11.043	11.033	232.0E6	109.2E6	15.319	14.468
16) T	DCPA	0.000	11.033	0	109.2E6	N.D.	16.790



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021820\
Data File : PS008897.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Feb 2020 20:12
Operator : DD\AJ
Sample : L1365-16
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 19 00:48:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
Quant Title : 8080.M
QLast Update : Wed Feb 05 02:36:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

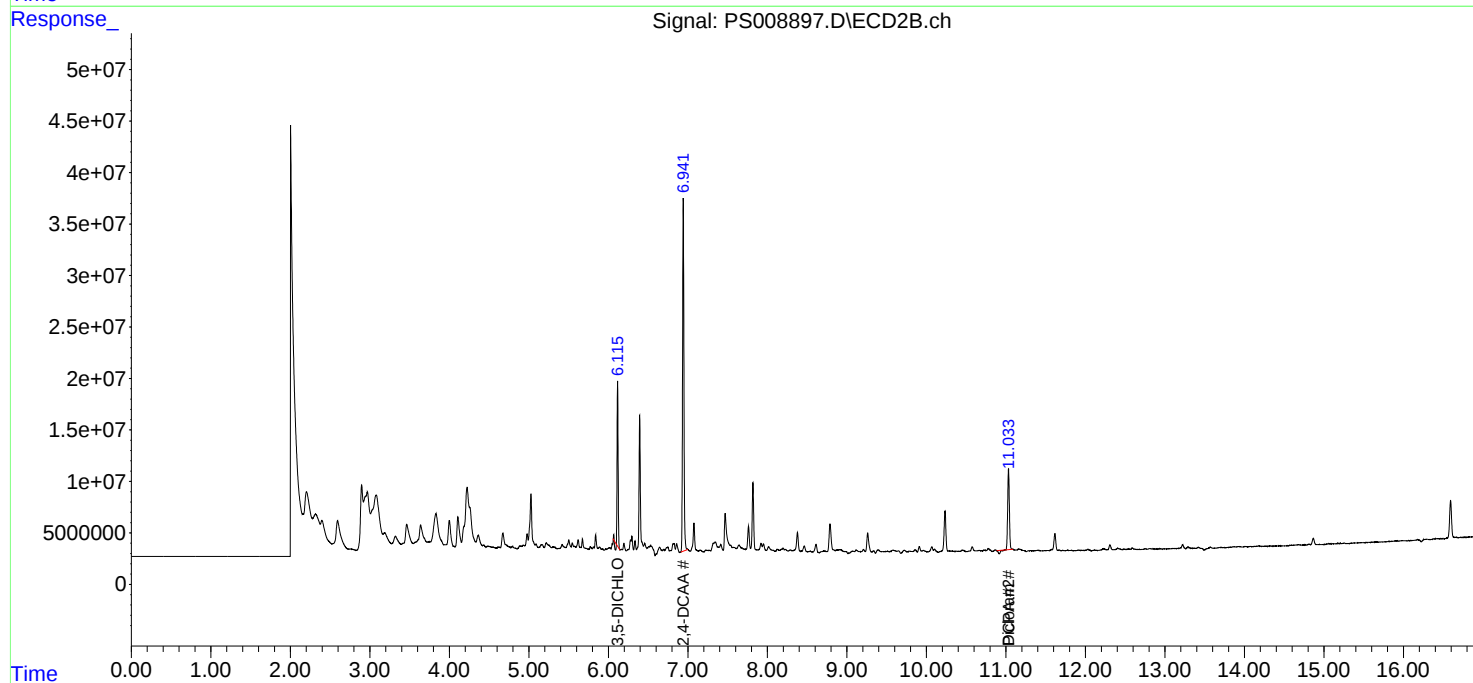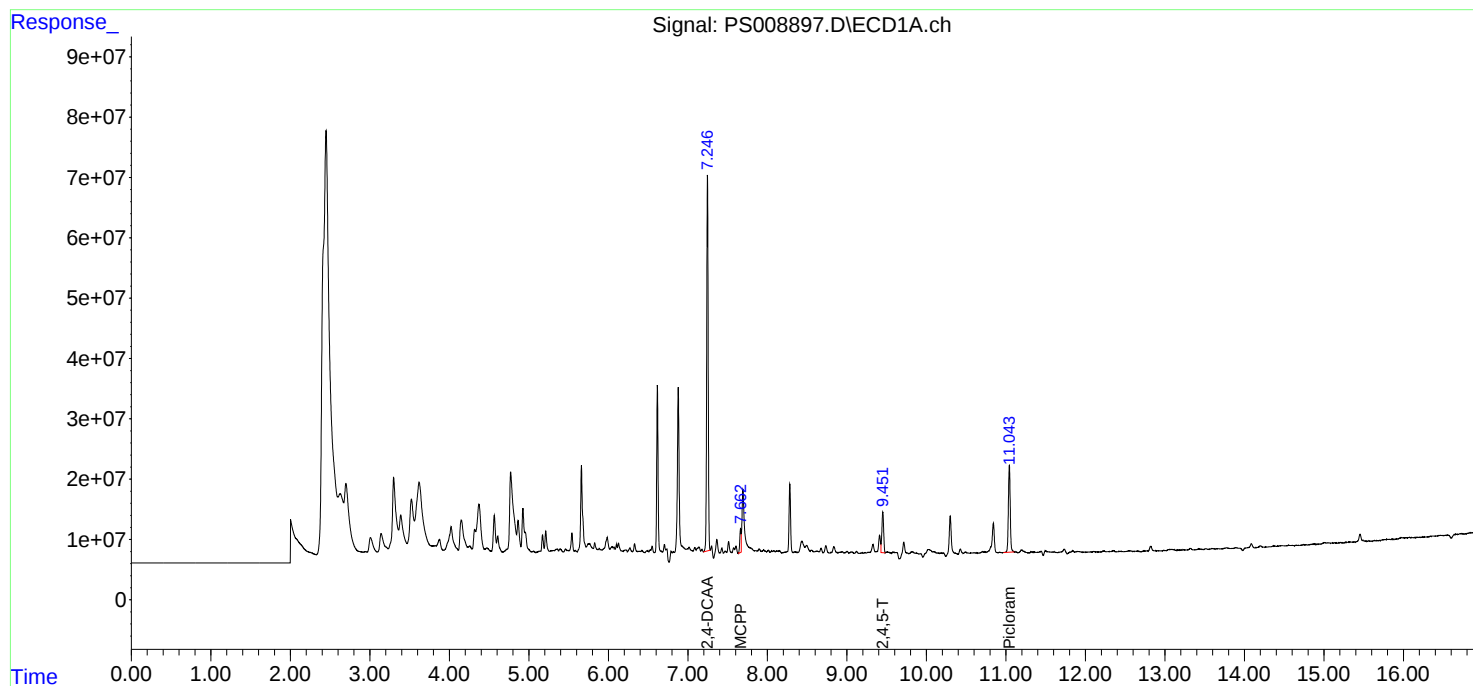


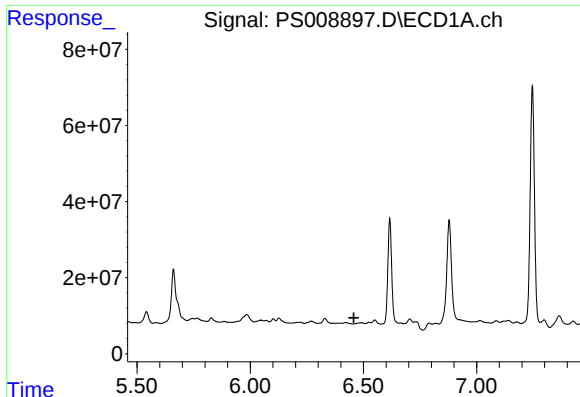

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.458 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

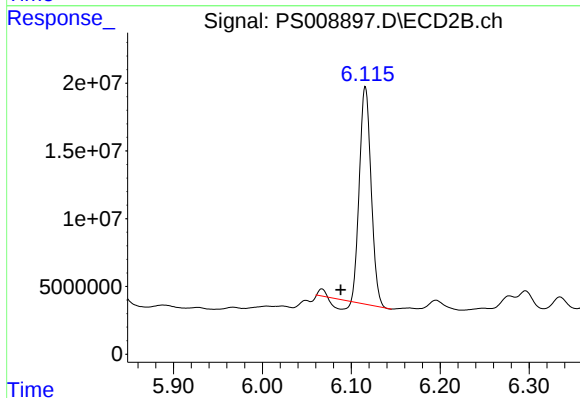


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.116 min
Delta R.T.: 0.028 min
Response: 140345232
Conc: 102.00 ng/ml

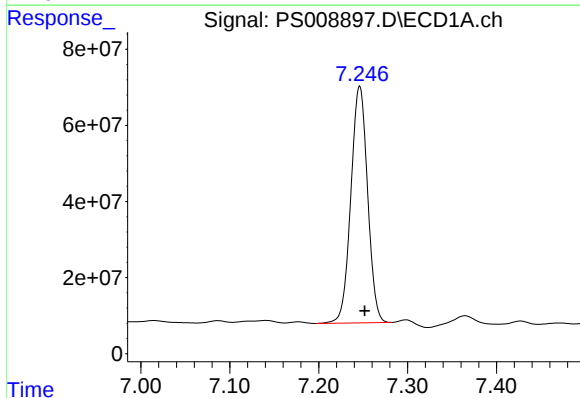


#4 2,4-DCAA

R.T.: 7.246 min
Delta R.T.: -0.006 min
Response: 812523471
Conc: 378.57 ng/ml

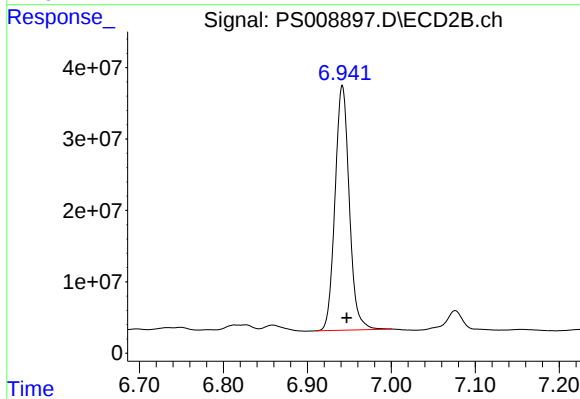

#4 2,4-DCAA


R.T.: 6.942 min
Delta R.T.: -0.005 min
Response: 404662471
Conc: 436.61 ng/ml

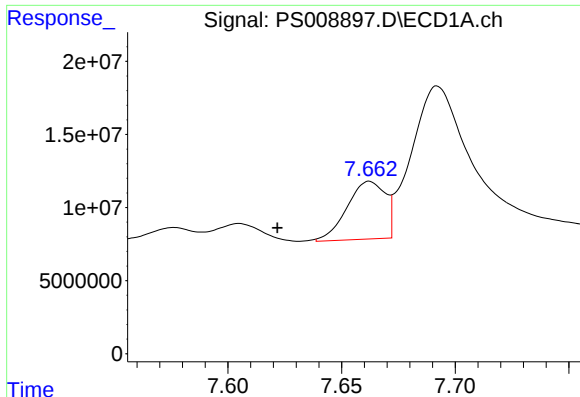

#6 MCP


R.T.: 7.662 min
Delta R.T.: 0.041 min
Response: 46290972
Conc: 7.53 ug/ml

Instrument :
ECD_S
ClientSampleId :

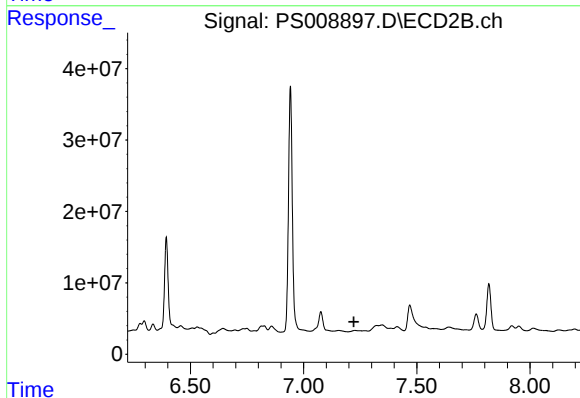


#6 MCP

R.T.: 0.000 min
Exp R.T.: 7.222 min
Response: 0
Conc: N.D.

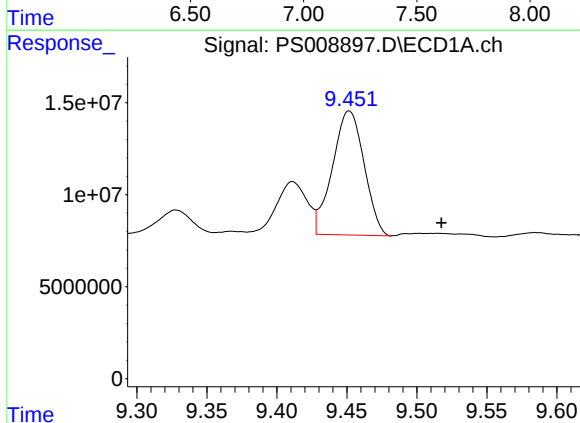


#12 2,4,5-T

R.T.: 9.452 min
Delta R.T.: -0.066 min
Response: 106214773
Conc: 9.65 ng/ml

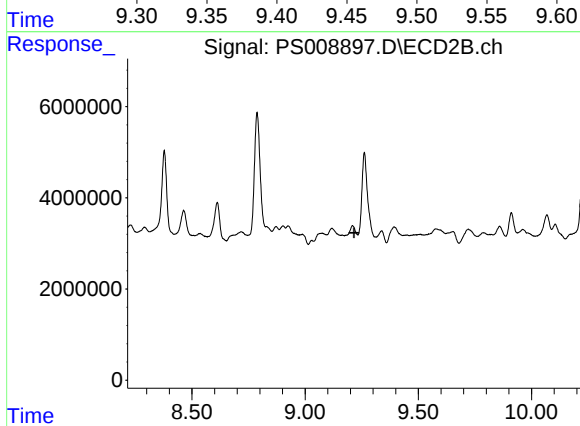

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.216 min
Response: 0
Conc: N.D.

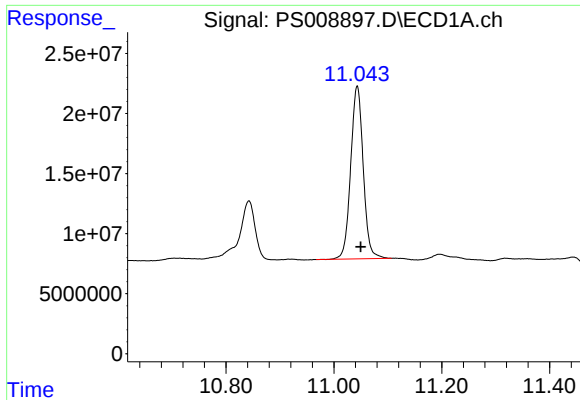

#15 Picloram


R.T.: 11.043 min
Delta R.T.: -0.007 min
Response: 231983973
Conc: 15.32 ng/ml

Instrument :
ECD_S
ClientSampleId :

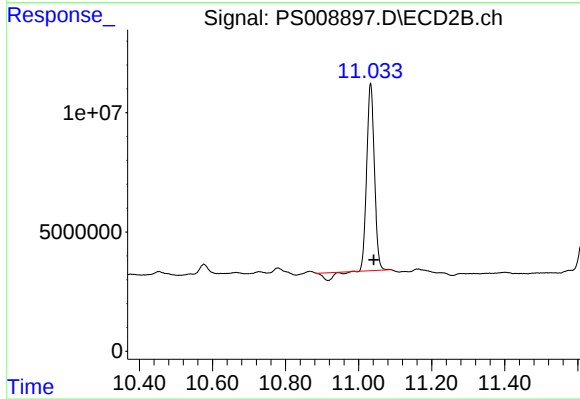


#15 Picloram

R.T.: 11.033 min
Delta R.T.: -0.008 min
Response: 109203571
Conc: 14.47 ng/ml

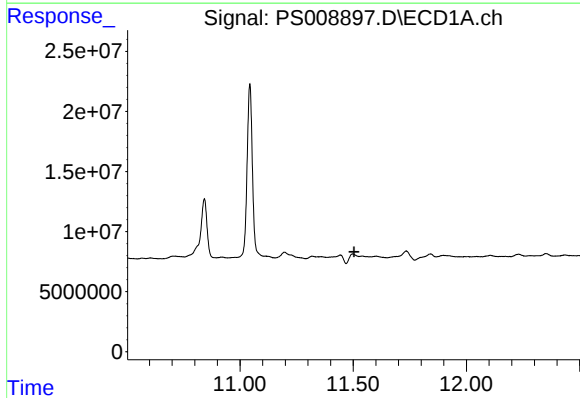

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.503 min
Response: 0
Conc: N.D.

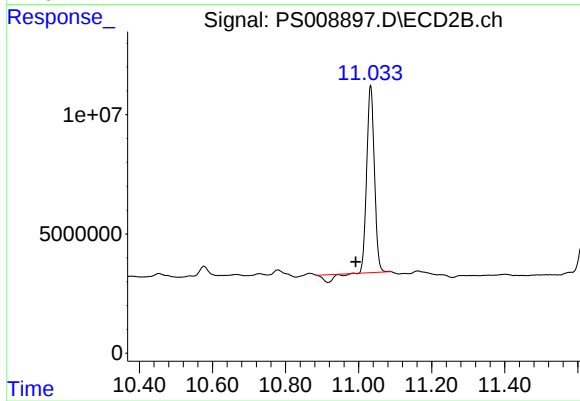

#16 DCPA

R.T.: 11.033 min
Delta R.T.: 0.041 min
Response: 109203571
Conc: 16.79 ng/ml