

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021822\
 Data File : PS018369.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Feb 2022 08:42
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 18 21:39:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020822.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 09 15:57:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
5)	T	DICAMBA	7.216	0.000	9874838	0	1.563 N.D. #
8)	T	DICHLORPROP	7.905	0.000	3558086	0	2.255 N.D. #
9)	T	2,4-D	8.153	0.000	15948481	0	8.661 N.D. #
10)	T	Pentachlo...	8.424	8.098	20211361	8235127	<MDL <MDL #
11)	T	2,4,5-TP ...	8.976	0.000	16225944	0	1.899 N.D. #
12)	T	2,4,5-T	9.270	8.851	59068534	11692922	6.675 3.302 #
13)	T	2,4-DB	9.833	0.000	20294078	0	11.531 N.D. #
14)	T	DINOSEB	10.944	0.000	25591242	0	3.833 N.D. #
15)	T	Picloram	10.798	10.656	426.0E6	204.3E6	37.289 40.767
16)	T	DCPA	11.213	10.585	19103207	12690471	1.733 2.788 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021822\
Data File : PS018369.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Feb 2022 08:42
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 18 21:39:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020822.M
Quant Title : 8080.M
QLast Update : Wed Feb 09 15:57:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

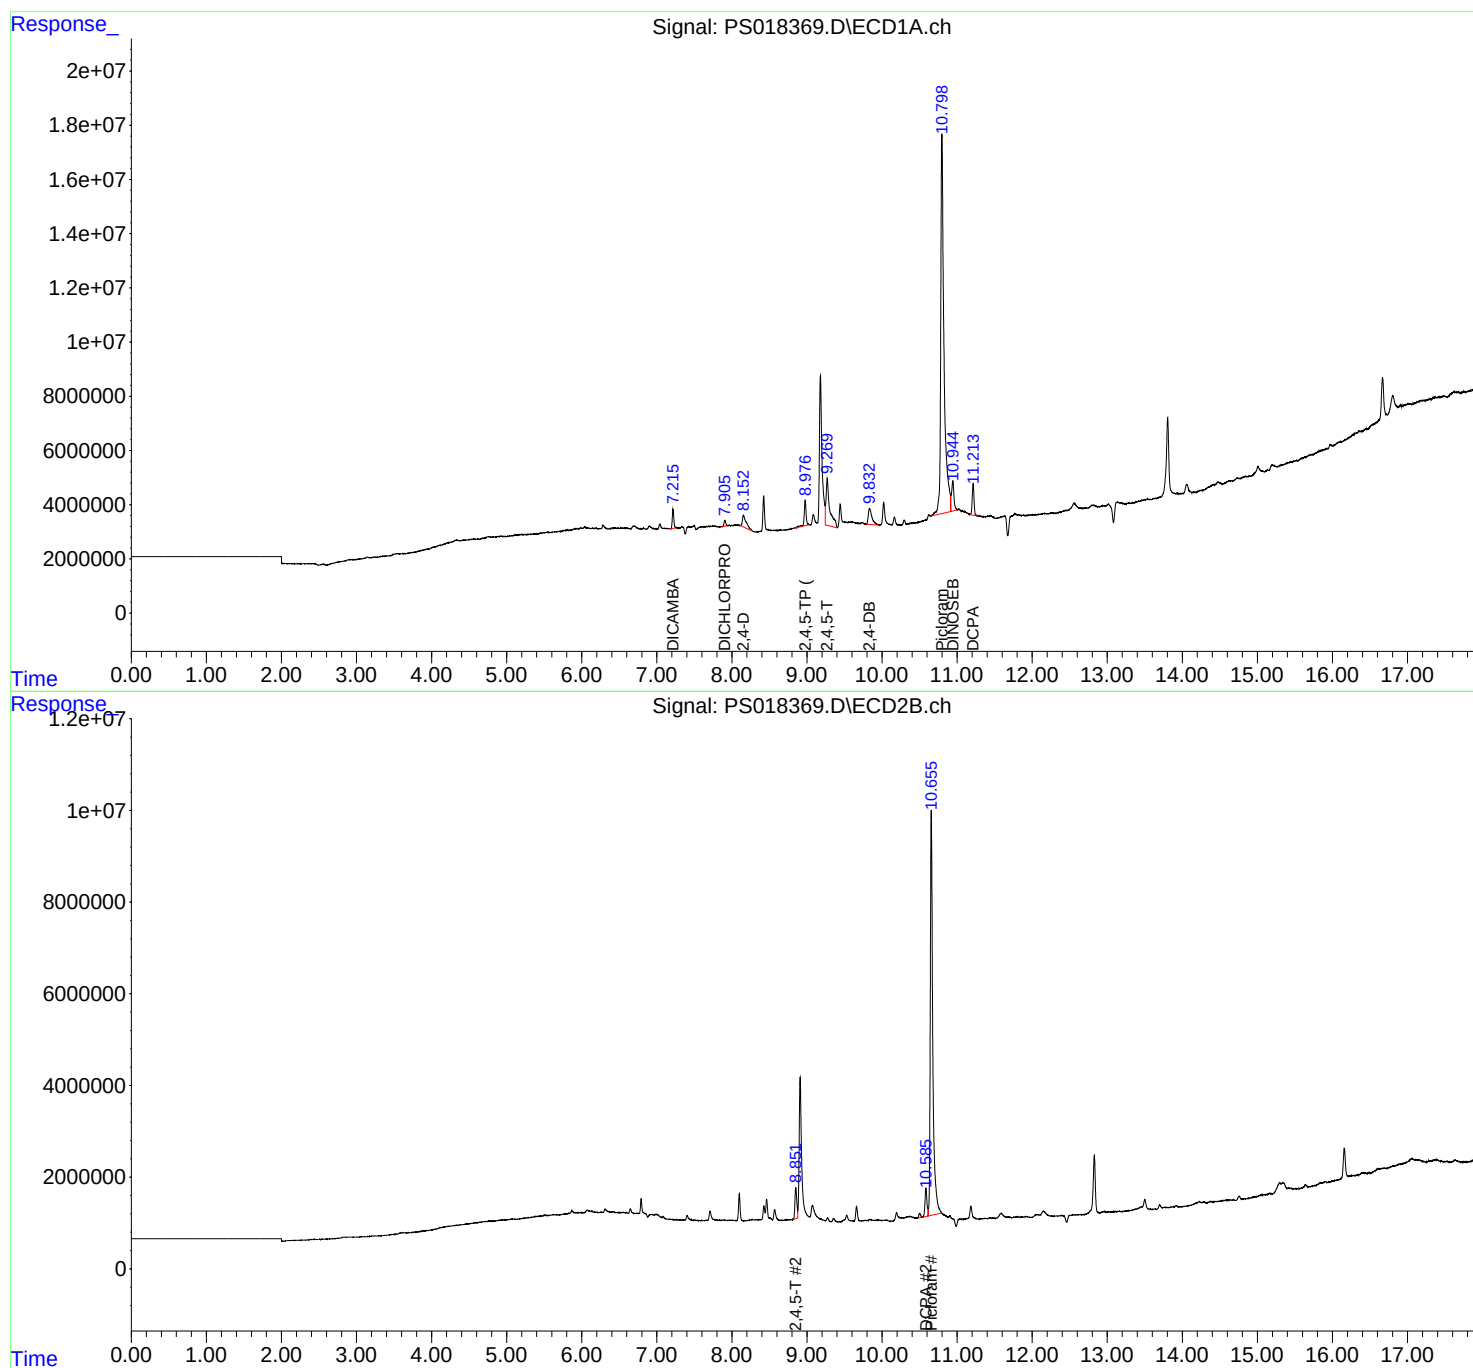


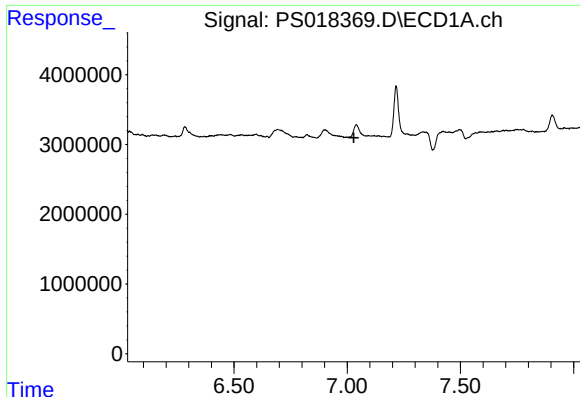

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.029 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

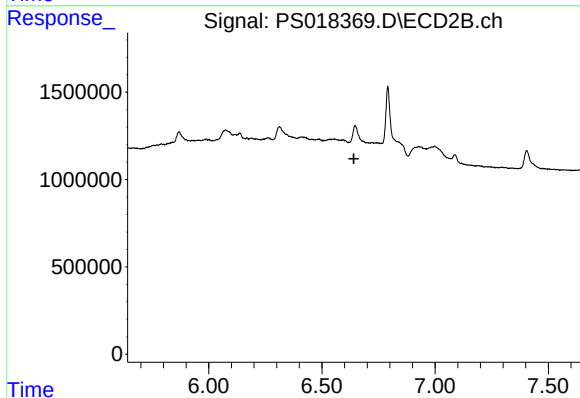


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.641 min
Response: 0
Conc: N.D.

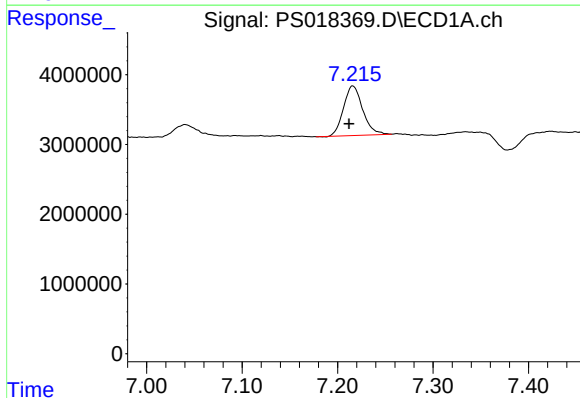


#5 DICAMBA

R.T.: 7.216 min
Delta R.T.: 0.004 min
Response: 9874838
Conc: 1.56 ng/ml

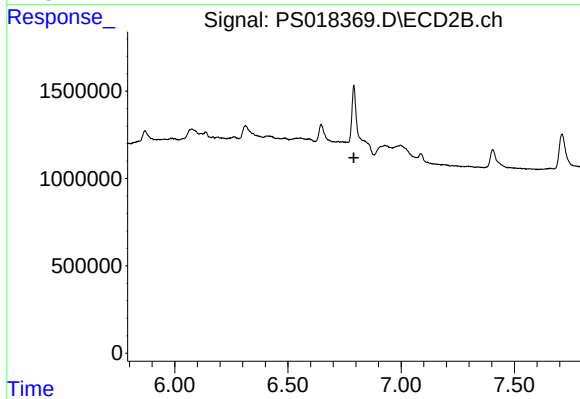

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.791 min
Response: 0
Conc: N.D.

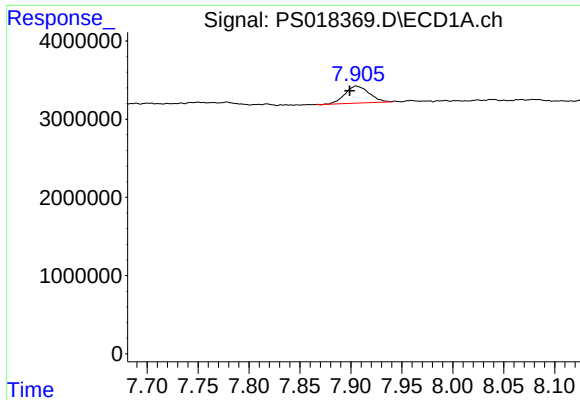

#8 DICHLORPROP


R.T.: 7.905 min
Delta R.T.: 0.006 min
Response: 3558086
Conc: 2.25 ng/ml

Instrument :
ECD_S
ClientSampleId :

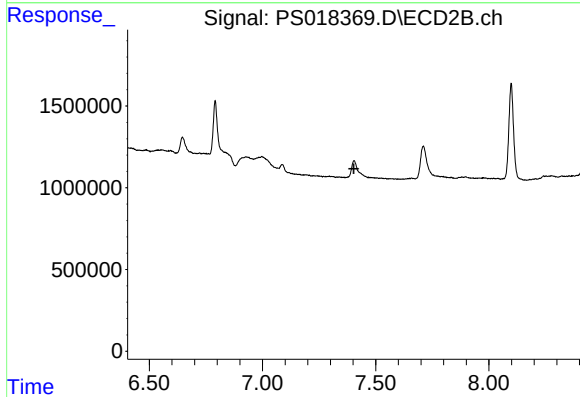


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.404 min
Response: 0
Conc: N.D.

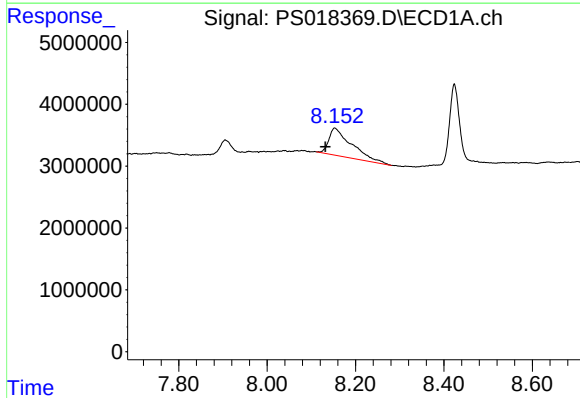


#9 2,4-D

R.T.: 8.153 min
Delta R.T.: 0.020 min
Response: 15948481
Conc: 8.66 ng/ml

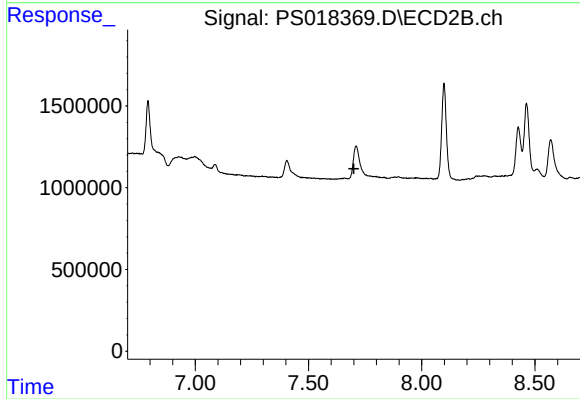

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.701 min
Response: 0
Conc: N.D.

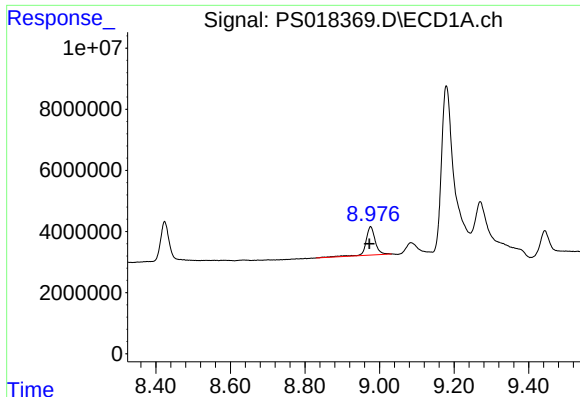

#11 2,4,5-TP (SILVEX)


R.T.: 8.976 min
Delta R.T.: 0.003 min
Response: 16225944
Conc: 1.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

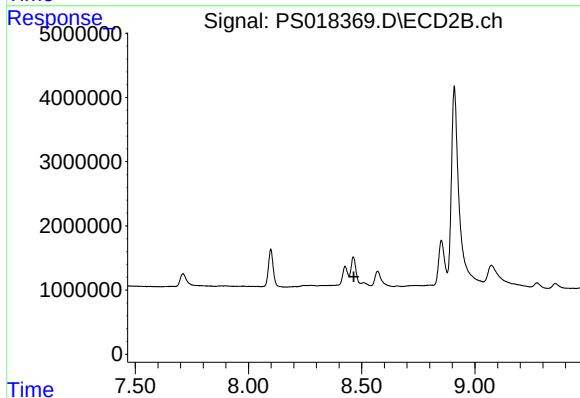


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 8.465 min
Response: 0
Conc: N.D.

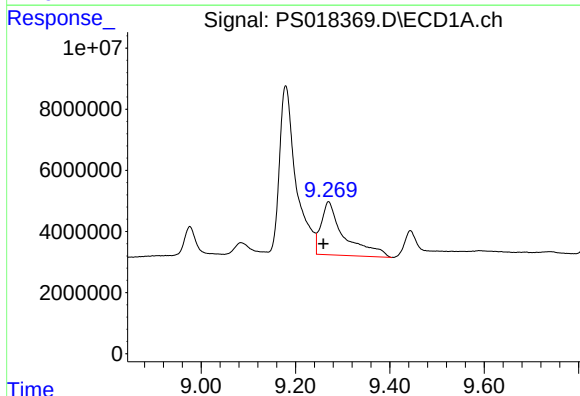


#12 2,4,5-T

R.T.: 9.270 min
Delta R.T.: 0.011 min
Response: 59068534
Conc: 6.67 ng/ml

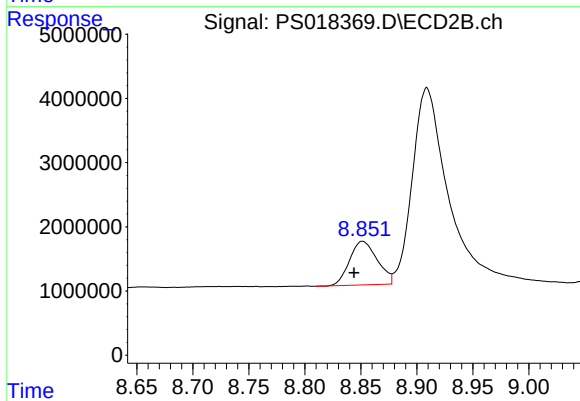

#12 2,4,5-T


R.T.: 8.851 min
Delta R.T.: 0.007 min
Response: 11692922
Conc: 3.30 ng/ml

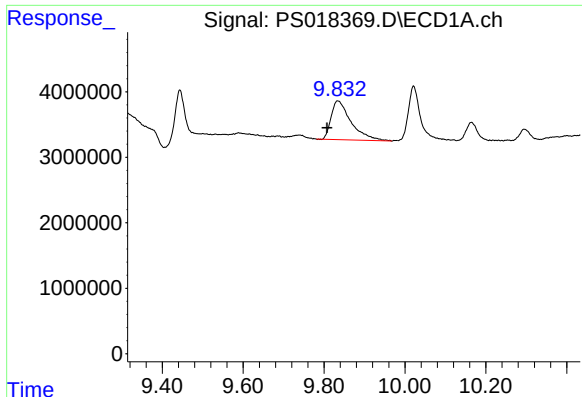

#13 2,4-DB


R.T.: 9.833 min
Delta R.T.: 0.026 min
Response: 20294078
Conc: 11.53 ng/ml

Instrument :
ECD_S
ClientSampleId :

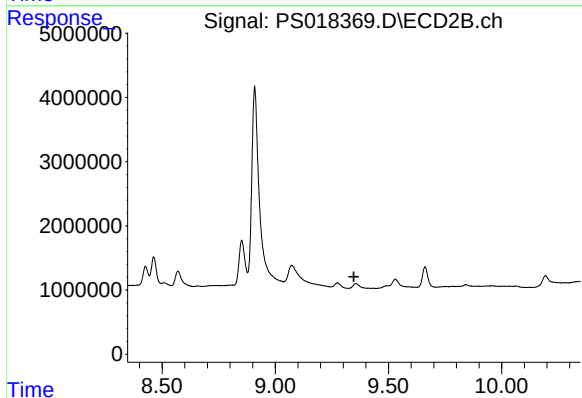


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.347 min
Response: 0
Conc: N.D.

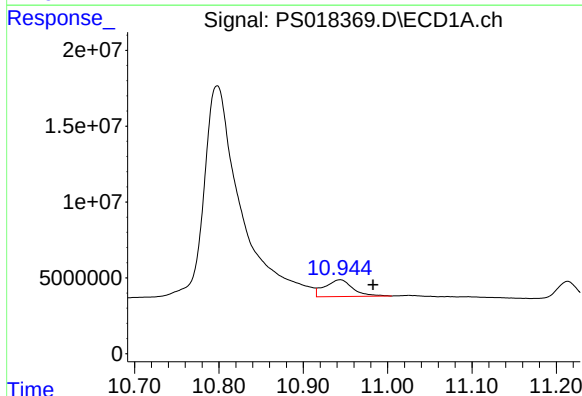


#14 DINOSEB

R.T.: 10.944 min
Delta R.T.: -0.039 min
Response: 25591242
Conc: 3.83 ng/ml

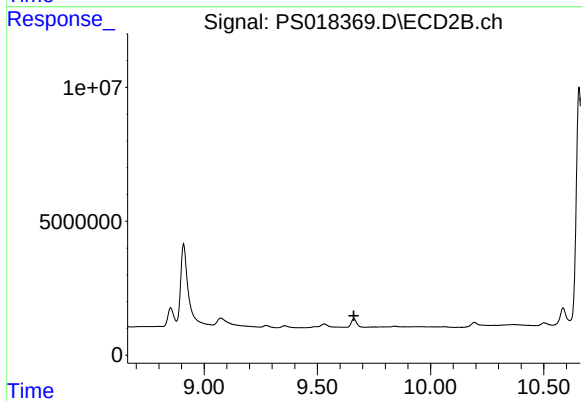

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.661 min
Response: 0
Conc: N.D.

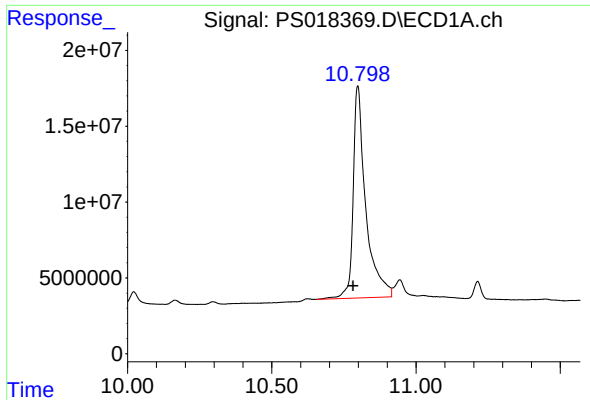

#15 Picloram


R.T.: 10.798 min
Delta R.T.: 0.016 min
Response: 426016653
Conc: 37.29 ng/ml

Instrument :
ECD_S
ClientSampleId :

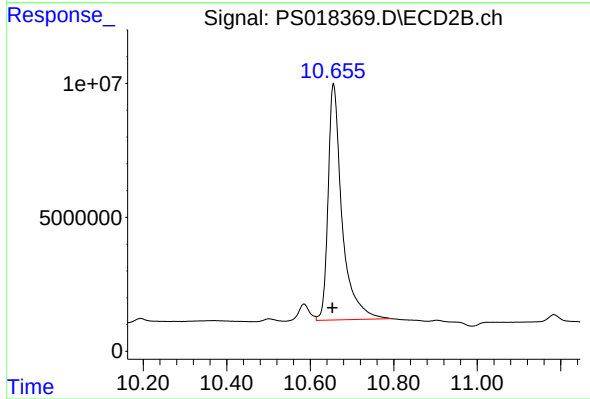


#15 Picloram

R.T.: 10.656 min
Delta R.T.: 0.003 min
Response: 204319264
Conc: 40.77 ng/ml

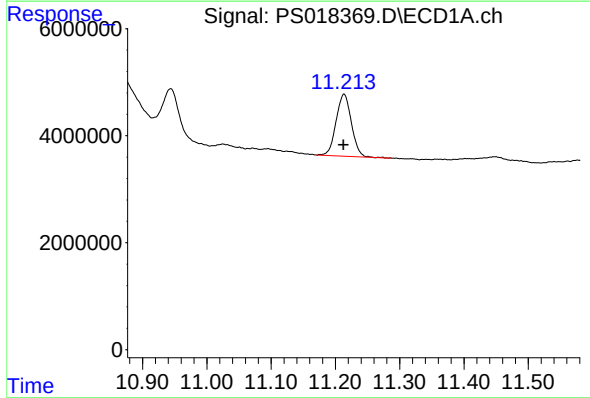

#16 DCPA

R.T.: 11.213 min
Delta R.T.: 0.000 min
Response: 19103207
Conc: 1.73 ng/ml

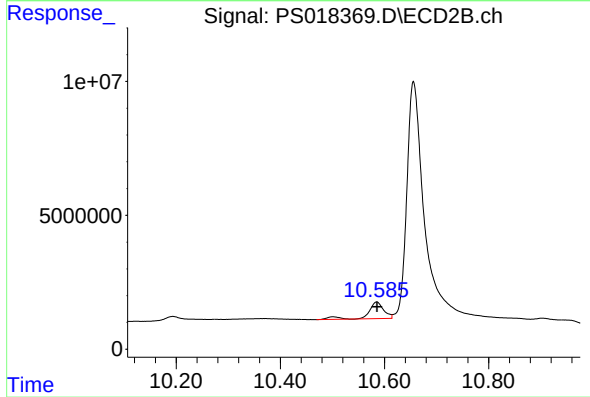

#16 DCPA

R.T.: 10.585 min
Delta R.T.: 0.000 min
Response: 12690471
Conc: 2.79 ng/ml