

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021822\
 Data File : PS018370.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Feb 2022 09:06
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 18 21:39:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020822.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 09 15:57:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.030	6.641	576.9E6	325.8E6	366.715	519.448 #
Target Compounds							
9) T	2,4-D	8.200f	0.000	1853787	0	1.007	N.D. #
12) T	2,4,5-T	9.221	0.000	101.4E6	0	11.460	N.D. #
15) T	Picloram	10.841f	10.686	269.0E6	129.9E6	23.548	25.926



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021822\
Data File : PS018370.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Feb 2022 09:06
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 18 21:39:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020822.M
Quant Title : 8080.M
QLast Update : Wed Feb 09 15:57:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

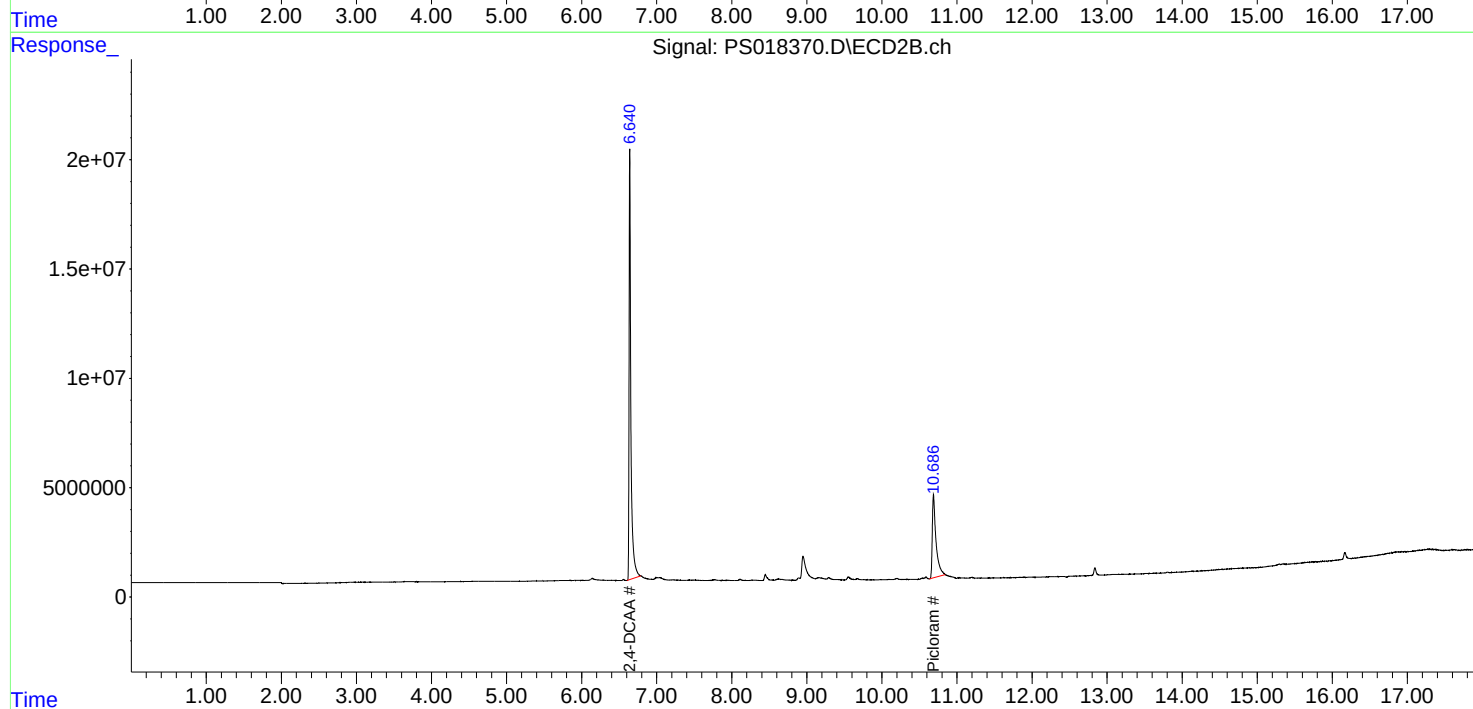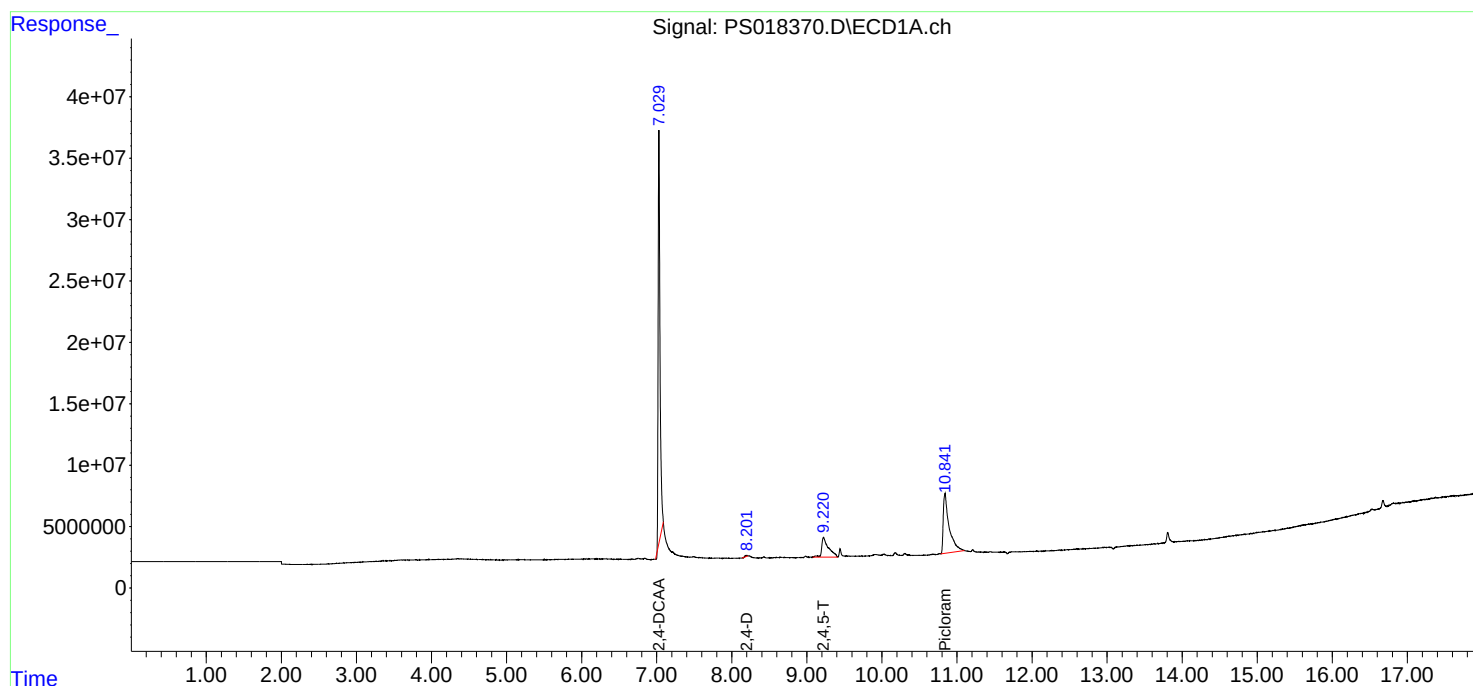


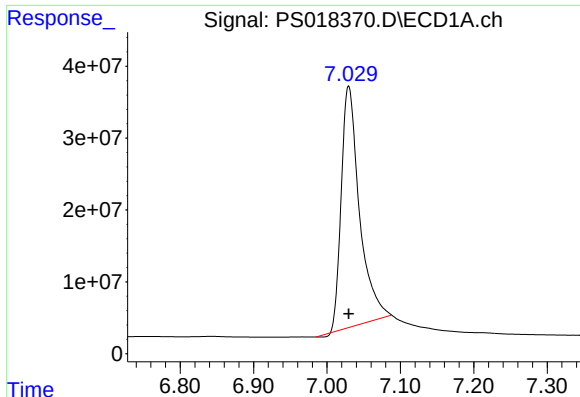

#4 2,4-DCAA


R.T.: 7.030 min
Delta R.T.: 0.000 min
Response: 576870172
Conc: 366.72 ng/ml

Instrument :
ECD_S
ClientSampleId :

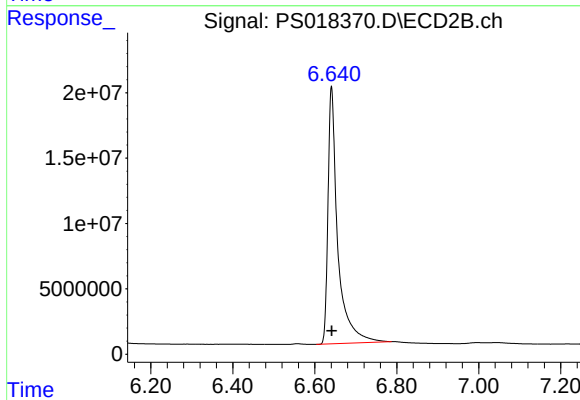


#4 2,4-DCAA

R.T.: 6.641 min
Delta R.T.: 0.000 min
Response: 325813895
Conc: 519.45 ng/ml

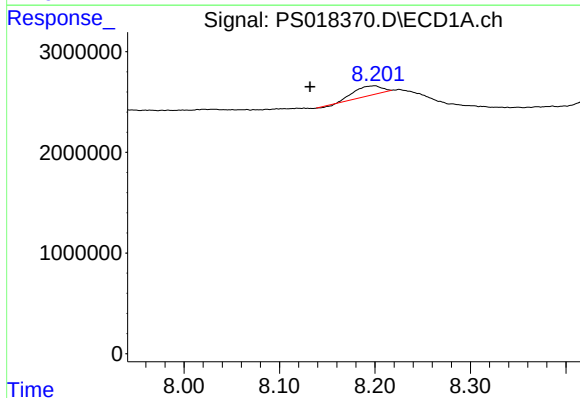


#9 2,4-D

R.T.: 8.200 min
Delta R.T.: 0.068 min
Response: 1853787
Conc: 1.01 ng/ml

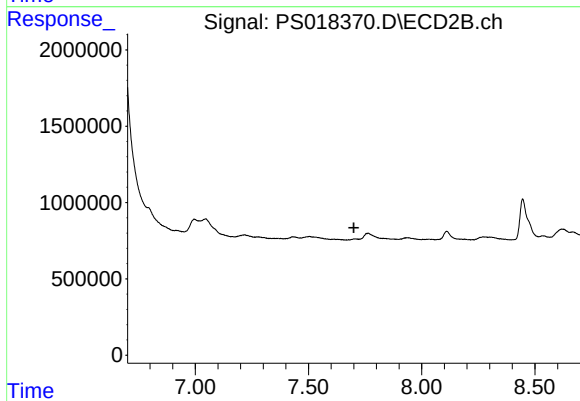

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.701 min
Response: 0
Conc: N.D.

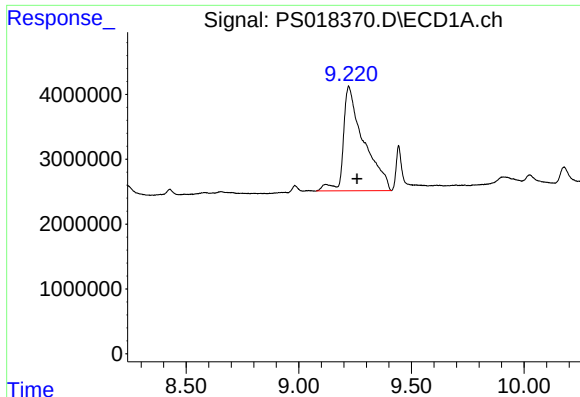

#12 2,4,5-T


R.T.: 9.221 min
Delta R.T.: -0.038 min
Response: 101417523
Conc: 11.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

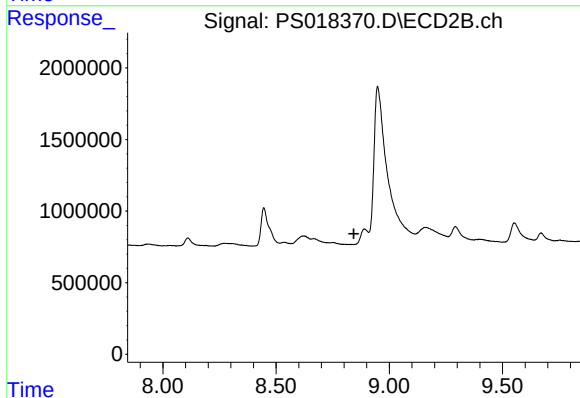


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 8.844 min
Response: 0
Conc: N.D.

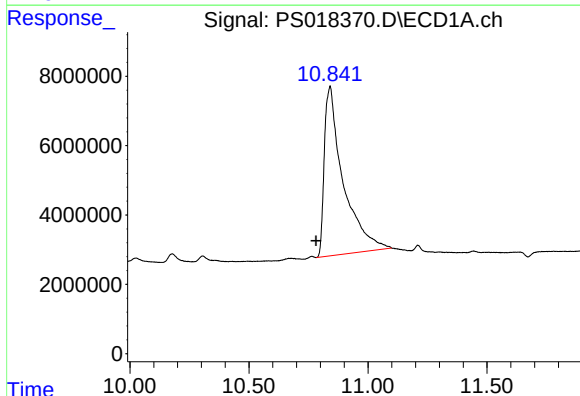

#15 Picloram

R.T.: 10.841 min
Delta R.T.: 0.059 min
Response: 269038432
Conc: 23.55 ng/ml

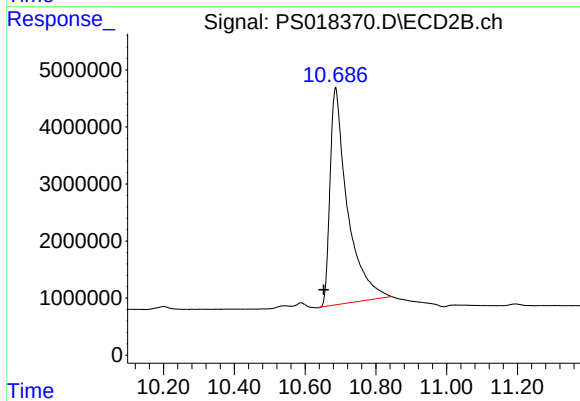

#15 Picloram

R.T.: 10.686 min
Delta R.T.: 0.034 min
Response: 129939487
Conc: 25.93 ng/ml