

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021822\
 Data File : PS018382.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Feb 2022 17:05
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 18 21:43:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020822.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 09 15:57:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.028	6.640	651.9E6	331.8E6	414.402	528.967 #
Target Compounds							
9) T	2,4-D	8.182f	0.000	3999536	0	2.172	N.D. #
12) T	2,4,5-T	9.224	0.000	4086831	0	<MDL	N.D. #
13) T	2,4-DB	0.000	9.283f	0	9468820	N.D.	19.890
15) T	Picloram	10.839f	10.692	29755948	14440285	2.604	2.881



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021822\
Data File : PS018382.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Feb 2022 17:05
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 18 21:43:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020822.M
Quant Title : 8080.M
QLast Update : Wed Feb 09 15:57:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

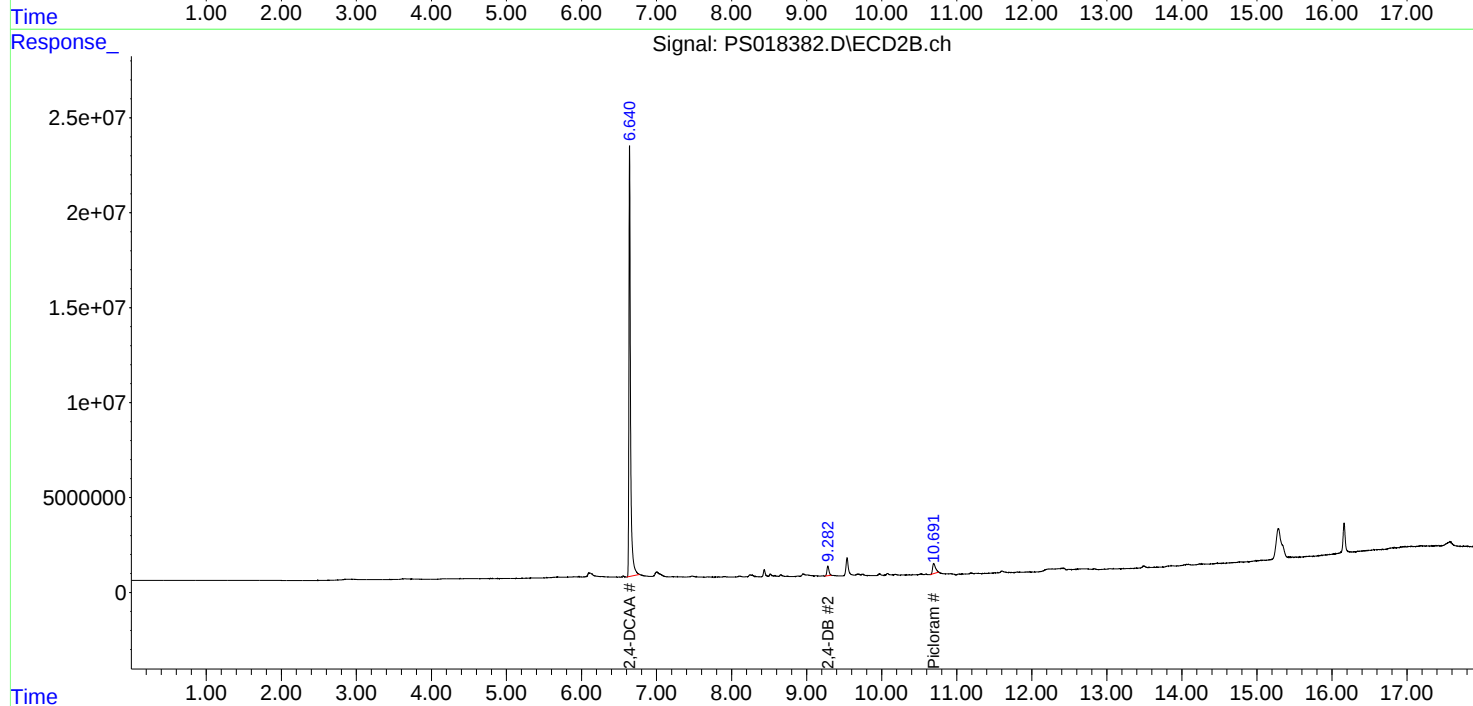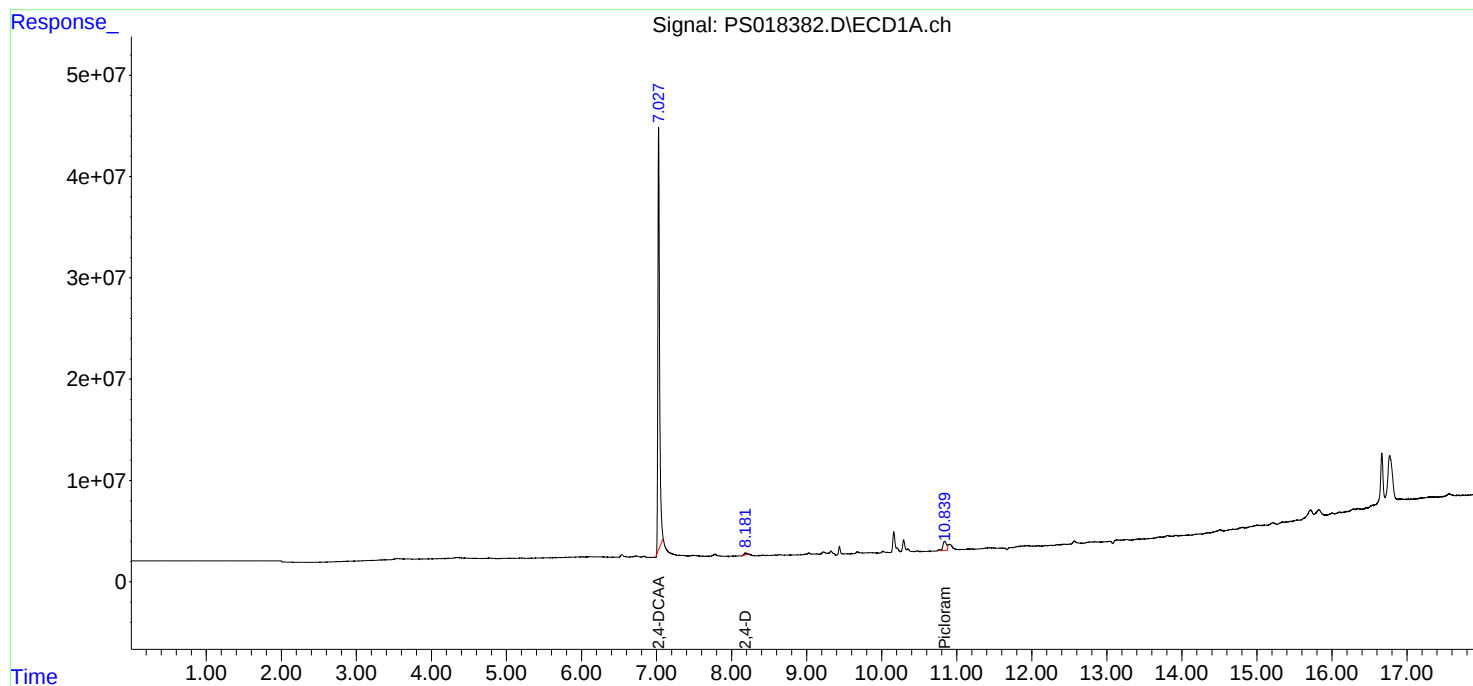


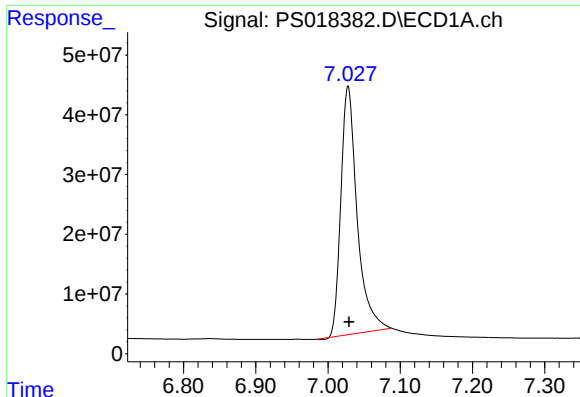

#4 2,4-DCAA


R.T.: 7.028 min
Delta R.T.: -0.002 min
Response: 651885230
Conc: 414.40 ng/ml

Instrument :
ECD_S
ClientSampleId :

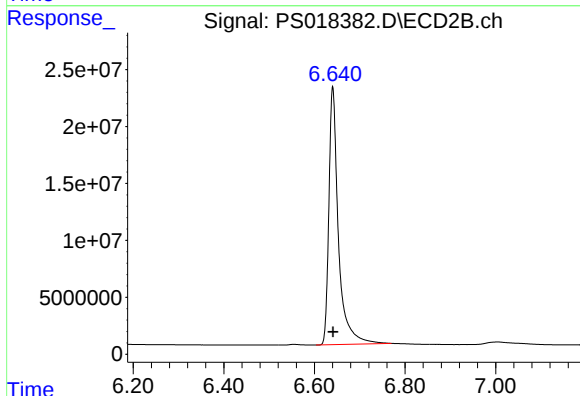


#4 2,4-DCAA

R.T.: 6.640 min
Delta R.T.: 0.000 min
Response: 331784118
Conc: 528.97 ng/ml

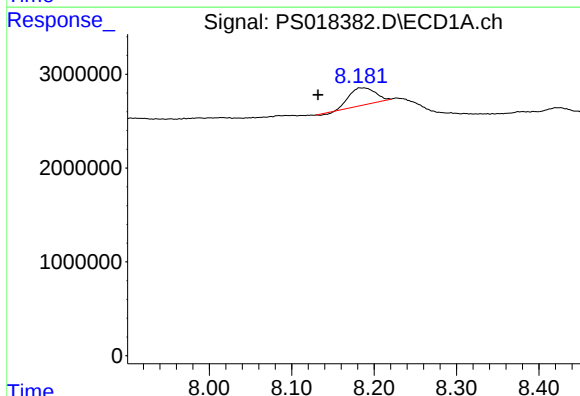


#9 2,4-D

R.T.: 8.182 min
Delta R.T.: 0.050 min
Response: 3999536
Conc: 2.17 ng/ml

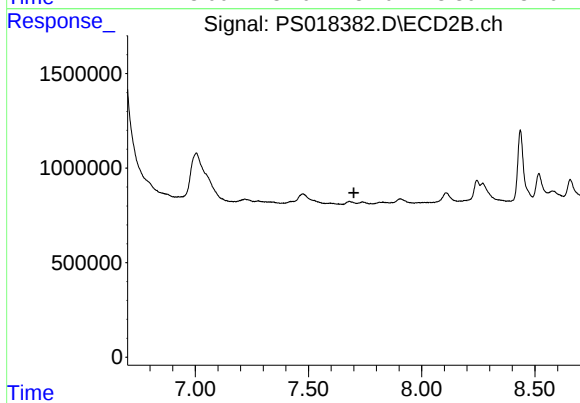

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.701 min
Response: 0
Conc: N.D.

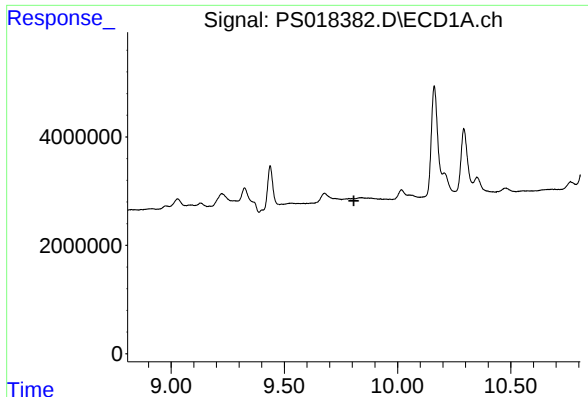

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 9.807 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

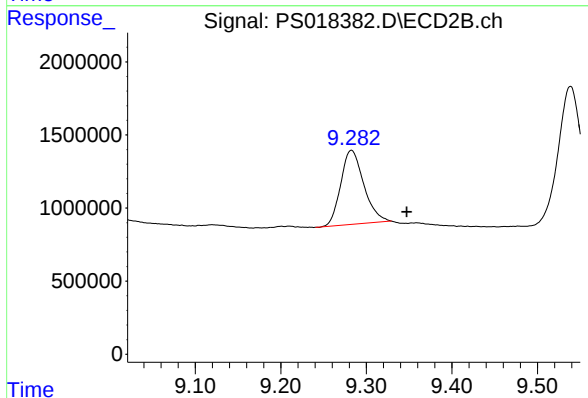


#13 2,4-DB

R.T.: 9.283 min
Delta R.T.: -0.064 min
Response: 9468820
Conc: 19.89 ng/ml

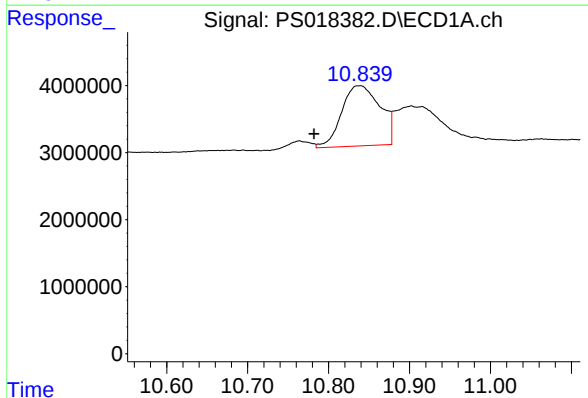

#15 Picloram

R.T.: 10.839 min
Delta R.T.: 0.057 min
Response: 29755948
Conc: 2.60 ng/ml

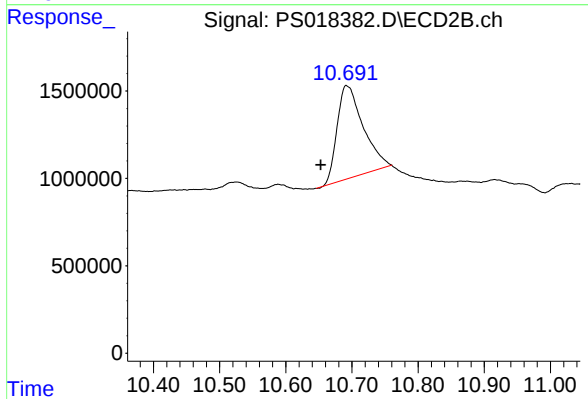

#15 Picloram

R.T.: 10.692 min
Delta R.T.: 0.039 min
Response: 14440285
Conc: 2.88 ng/ml