

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021919\
 Data File : PS003257.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Feb 2019 18:38
 Operator : EI\SJ
 Sample : PB117213TB
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB117213TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 20 00:54:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.275	10.777	71785334	230.1E6	189.088	538.086 #
Target Compounds							
2) T	3,5-DICHL...	0.000	9.027	0	1875928	N.D.	3.329 #
6) T	MCCP	11.960	11.346	13672123	2801049	11.411	2.540 #
11) T	2,4,5-TP ...	14.401	0.000	2425188	0	0.963	N.D. #
12) T	2,4,5-T	0.000	14.399	0	5909621	N.D.	3.088 #
15) T	Picloram	0.000	16.706	0	18298046	N.D.	6.086 #
16) T	DCPA	0.000	16.706	0	18298046	N.D.	5.907 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021919\
Data File : PS003257.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Feb 2019 18:38
Operator : EI\SJ
Sample : PB117213TB
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB117213TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 20 00:54:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

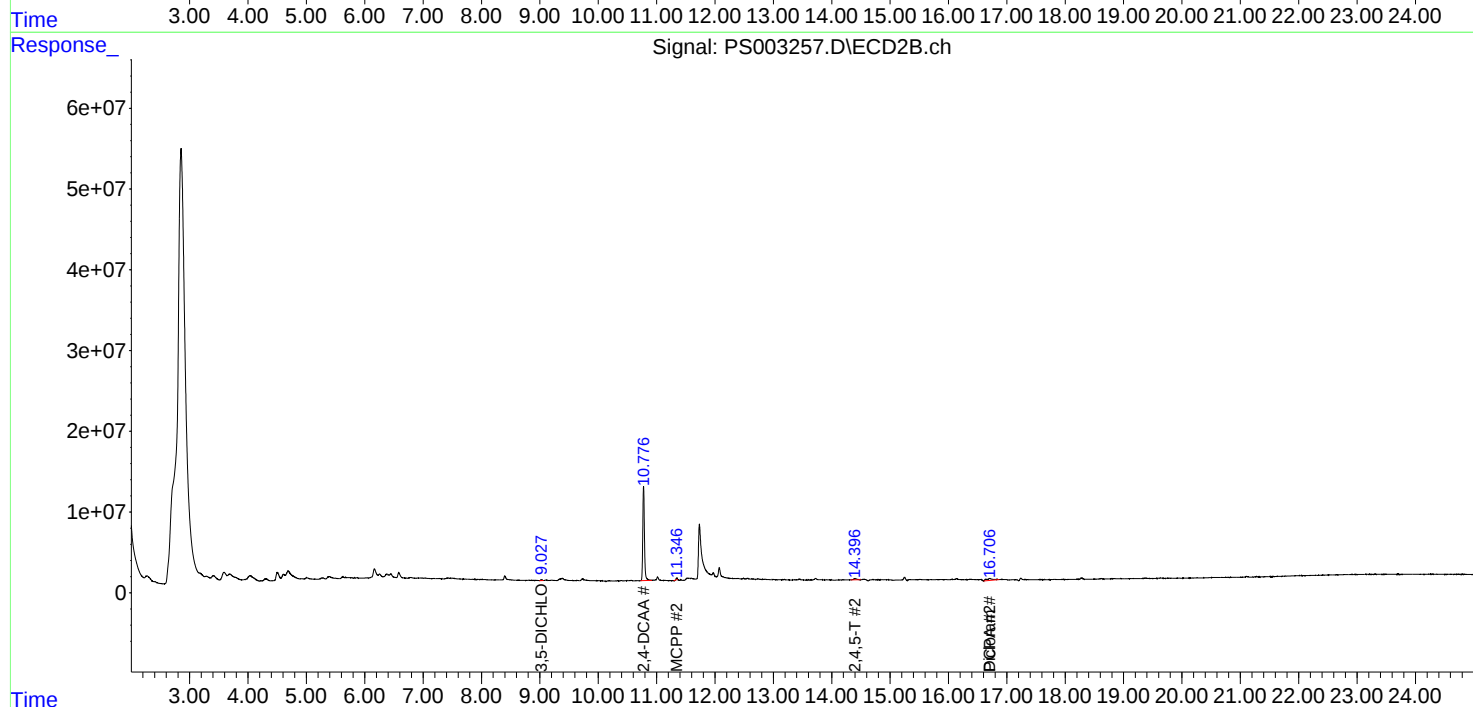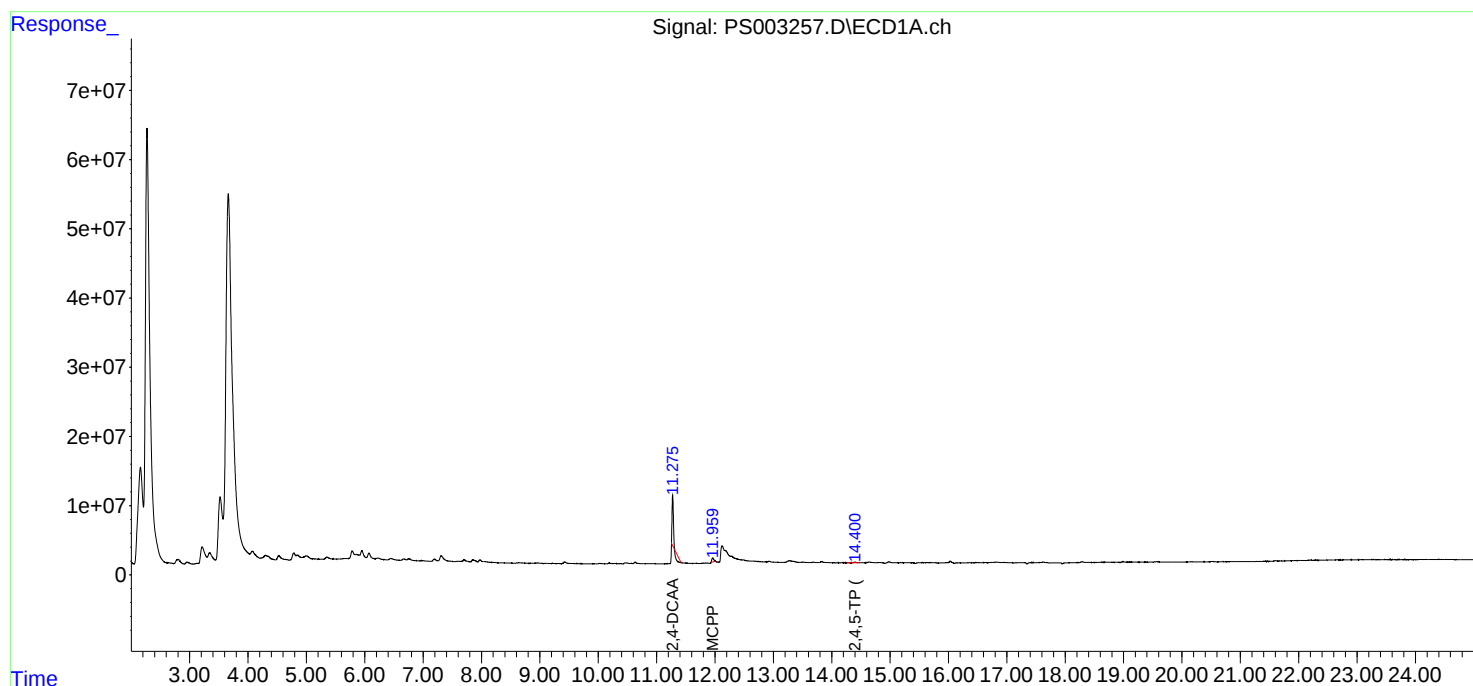


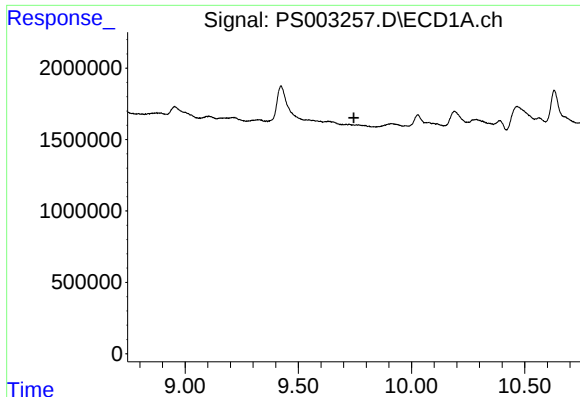

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.745 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB117213TB

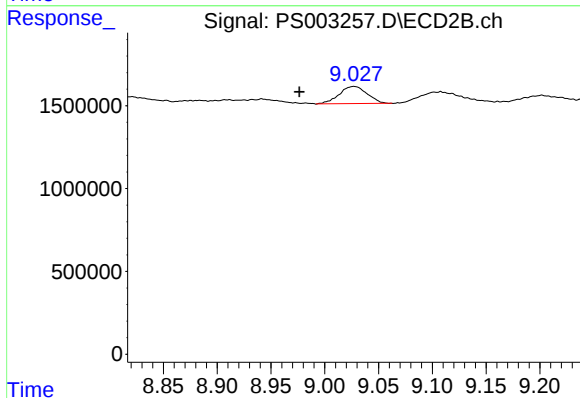


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.027 min
Delta R.T.: 0.051 min
Response: 1875928
Conc: 3.33 ng/ml

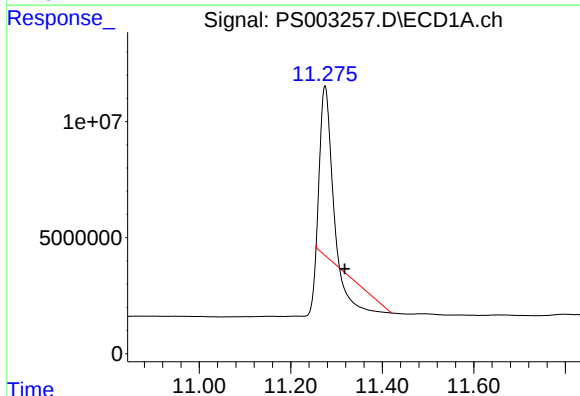


#4 2,4-DCAA

R.T.: 11.275 min
Delta R.T.: -0.043 min
Response: 71785334
Conc: 189.09 ng/ml

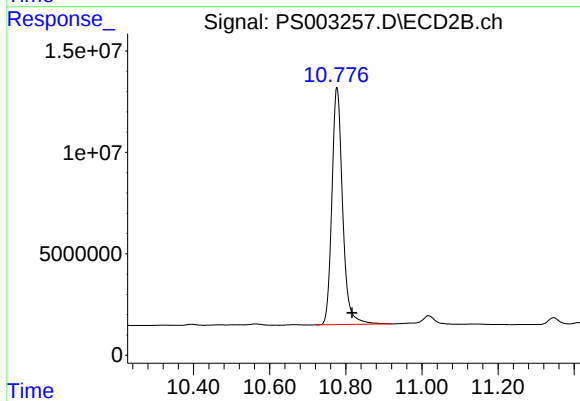

#4 2,4-DCAA


R.T.: 10.777 min
Delta R.T.: -0.040 min
Response: 230056566
Conc: 538.09 ng/ml

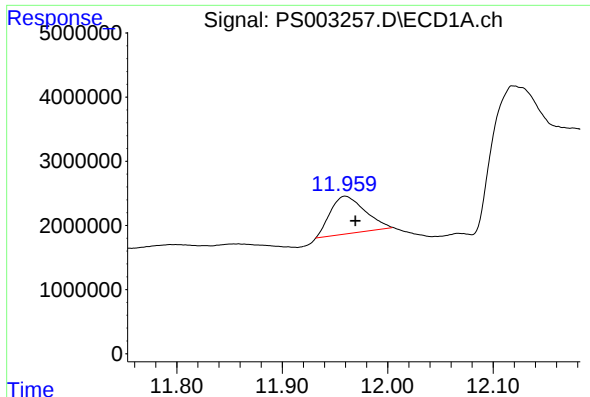

#6 MCP


R.T.: 11.960 min
Delta R.T.: -0.010 min
Response: 13672123
Conc: 11.41 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB117213TB

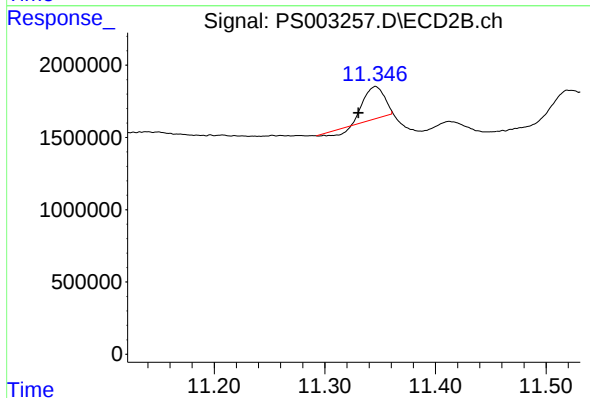


#6 MCP

R.T.: 11.346 min
Delta R.T.: 0.015 min
Response: 2801049
Conc: 2.54 ug/ml

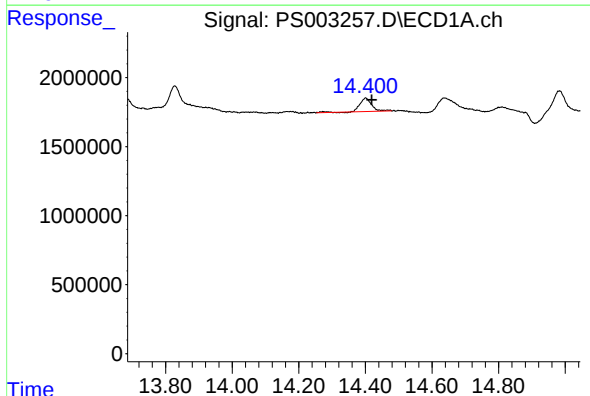


#11 2,4,5-TP (SILVEX)

R.T.: 14.401 min
Delta R.T.: -0.019 min
Response: 2425188
Conc: 0.96 ng/ml

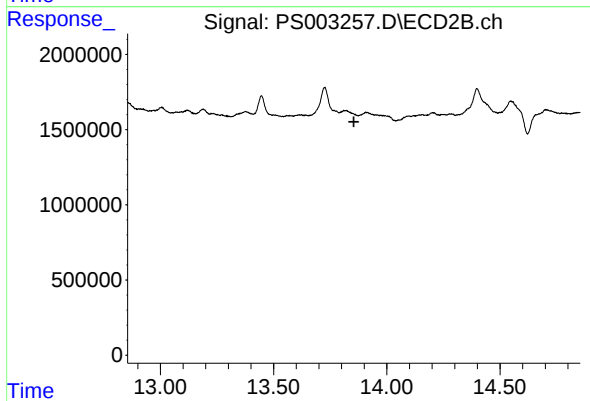

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 13.854 min
Response: 0
Conc: N.D.

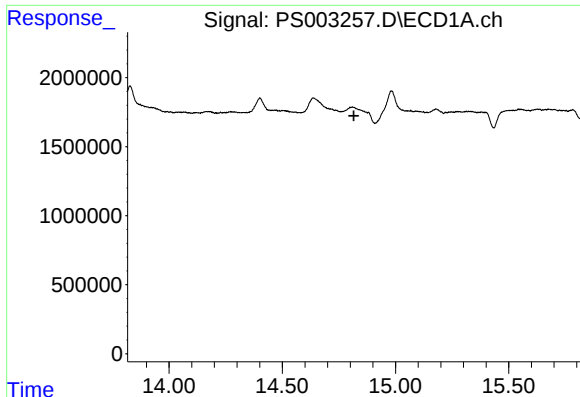

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.817 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB117213TB

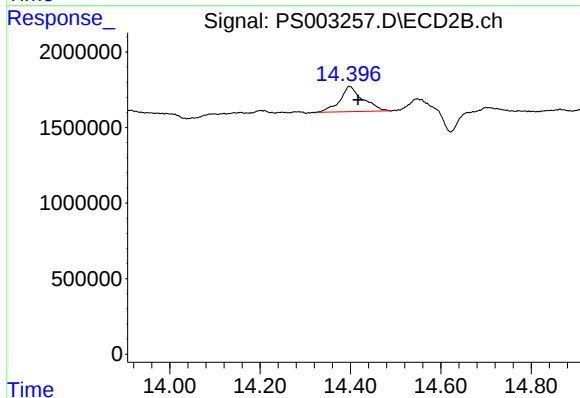


#12 2,4,5-T

R.T.: 14.399 min
Delta R.T.: -0.018 min
Response: 5909621
Conc: 3.09 ng/ml

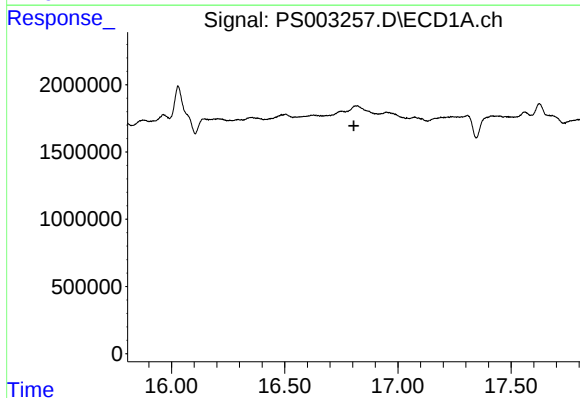


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.806 min
Response: 0
Conc: N.D.

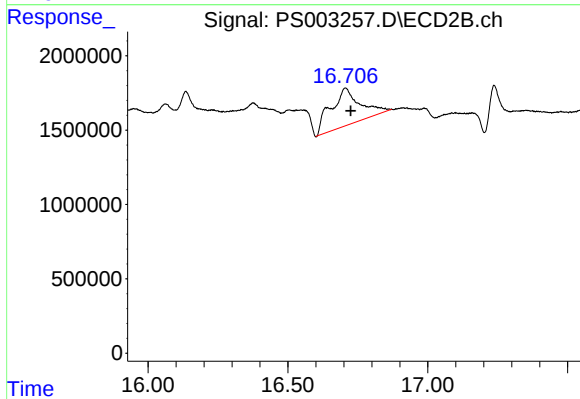

#15 Picloram


R.T.: 16.706 min
Delta R.T.: -0.019 min
Response: 18298046
Conc: 6.09 ng/ml

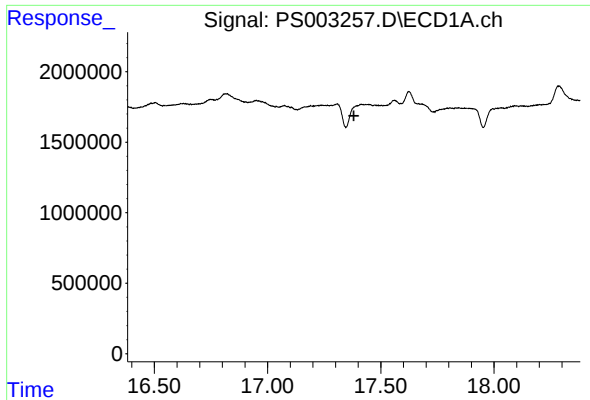

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB117213TB

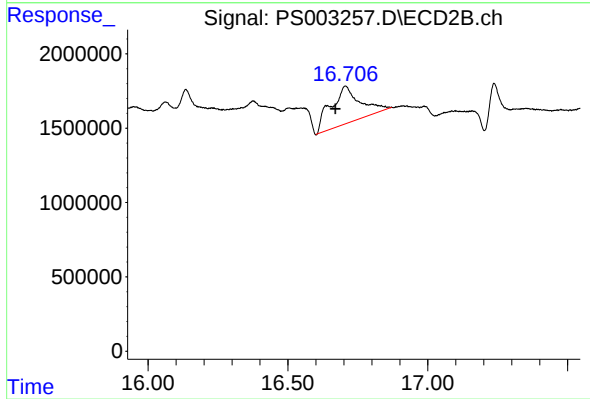

#16 DCPA

R.T.: 16.706 min
Delta R.T.: 0.036 min
Response: 18298046
Conc: 5.91 ng/ml