

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021919\
 Data File : PS003259.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Feb 2019 19:40
 Operator : EI\SJ
 Sample : K1518-02MS
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CABLE-BRIDGE-FOUNDATION-D-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 20 00:54:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.277	10.761	88854719	185.5E6	234.049	433.819 #
Target Compounds							
1) T	Dalapon	2.847	2.303	172.9E6	264.0E6	313.453	492.702 #
6) T	MCPD	0.000	11.318	0	119372	N.D.	0.108 #
7) T	MCPA	0.000	11.711	0	86171120	N.D.	54.779 #
8) T	DICHLORPROP	0.000	12.165	0	260.5E6	N.D.	681.201 #
11) T	2,4,5-TP ...	14.375	13.798	1661.3E6	1472.0E6	659.672	593.468
14) T	DINOSEB	16.987	0.000	642.1E6	0	341.282	N.D. #
15) T	Picloram	16.763	16.763	1645.2E6	52406845	520.025	17.432 #
16) T	DCPA	0.000	16.668	0	1506.8E6	N.D.	486.455 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021919\
Data File : PS003259.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Feb 2019 19:40
Operator : EI\SJ
Sample : K1518-02MS
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
CABLE-BRIDGE-FOUNDATION-D-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 20 00:54:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

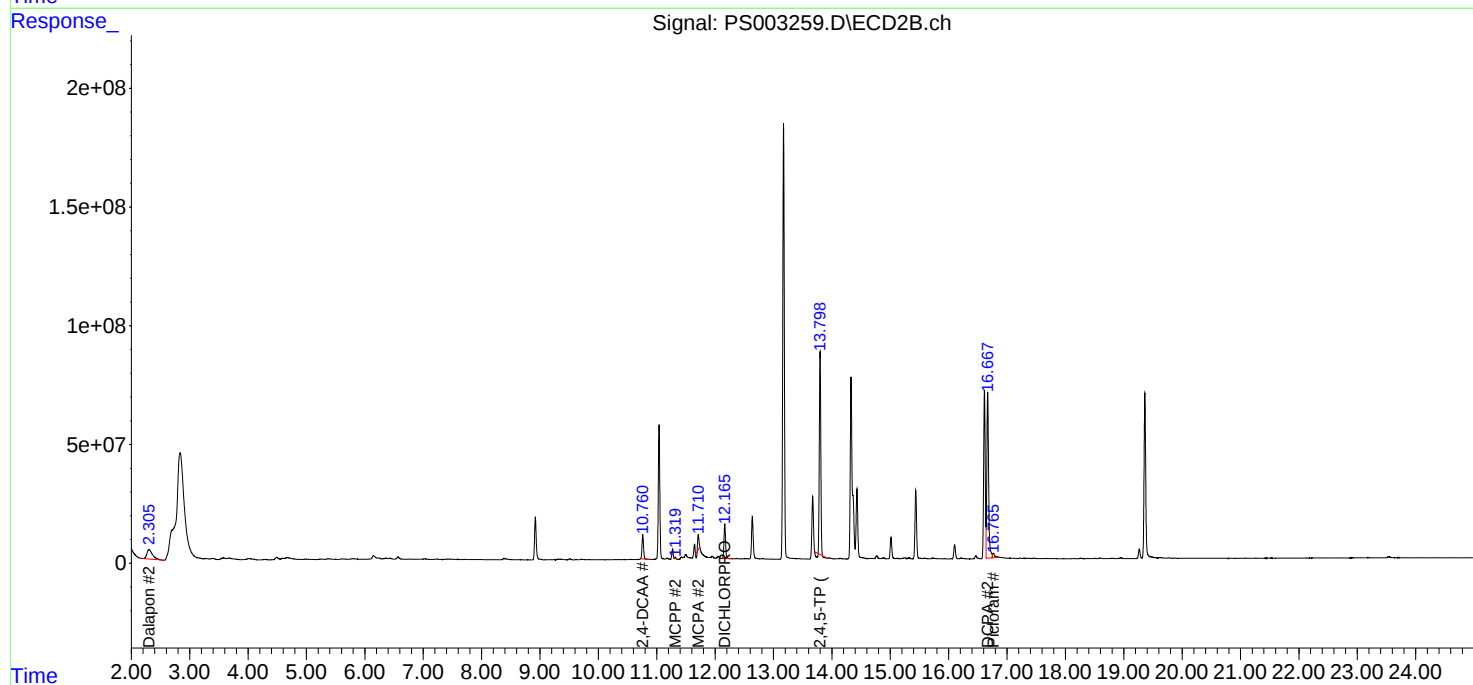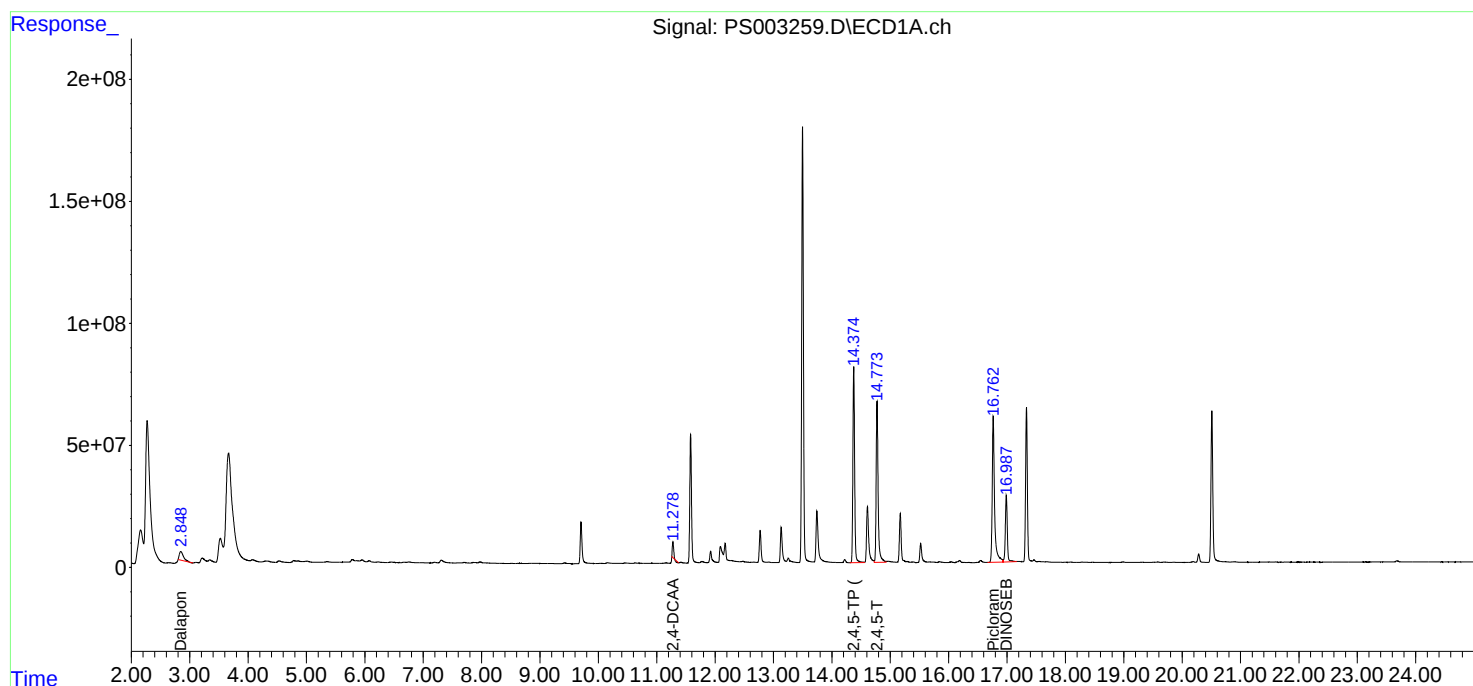


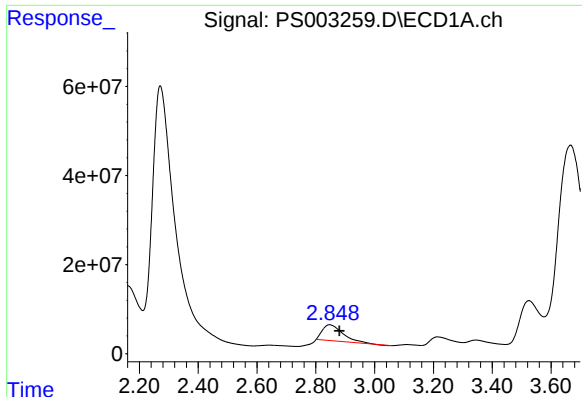

#1 Dalapon


R.T.: 2.847 min
Delta R.T.: -0.033 min
Response: 172915486
Conc: 313.45 ng/ml

Instrument :
ECD_S
ClientSampleId :
CABLE-BRIDGE-FOUNDATION-D-1

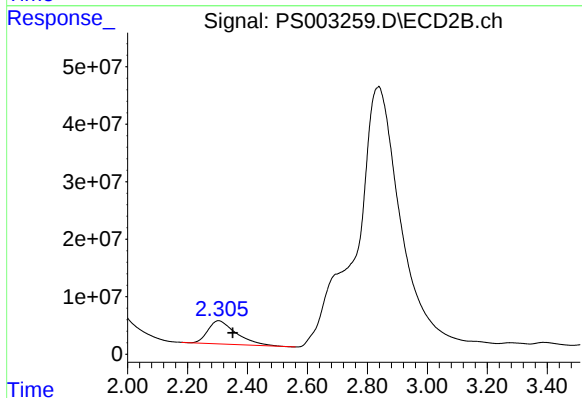


#1 Dalapon

R.T.: 2.303 min
Delta R.T.: -0.047 min
Response: 264049457
Conc: 492.70 ng/ml

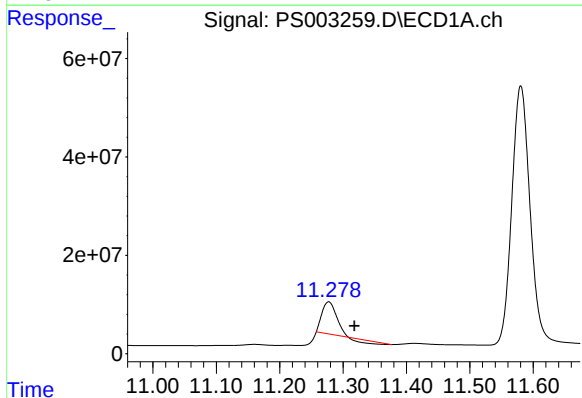


#4 2,4-DCAA

R.T.: 11.277 min
Delta R.T.: -0.040 min
Response: 88854719
Conc: 234.05 ng/ml

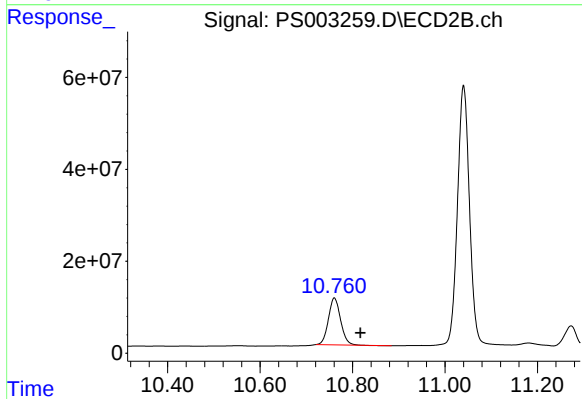

#4 2,4-DCAA


R.T.: 10.761 min
Delta R.T.: -0.056 min
Response: 185477458
Conc: 433.82 ng/ml

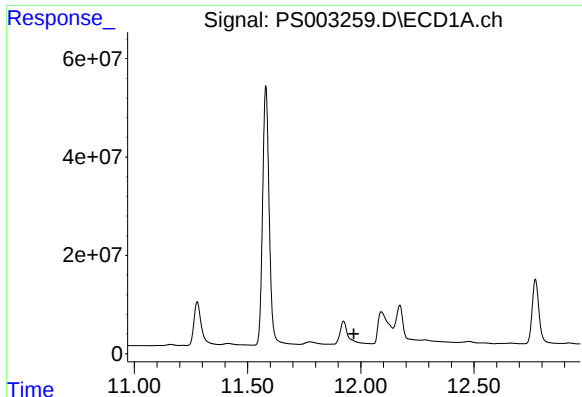

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 11.969 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CABLE-BRIDGE-FOUNDATION-D-1

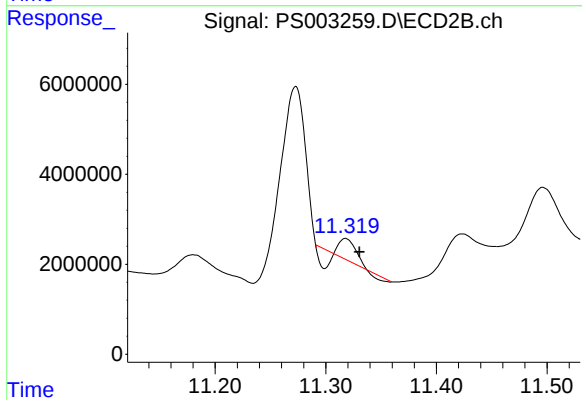


#6 MCPP

R.T.: 11.318 min
Delta R.T.: -0.012 min
Response: 119372
Conc: 0.11 ug/ml

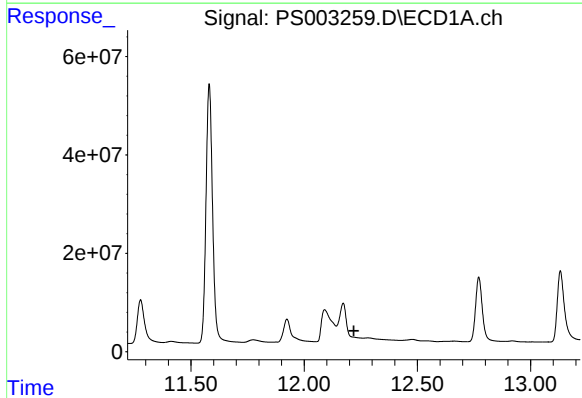


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 12.219 min
Response: 0
Conc: N.D.

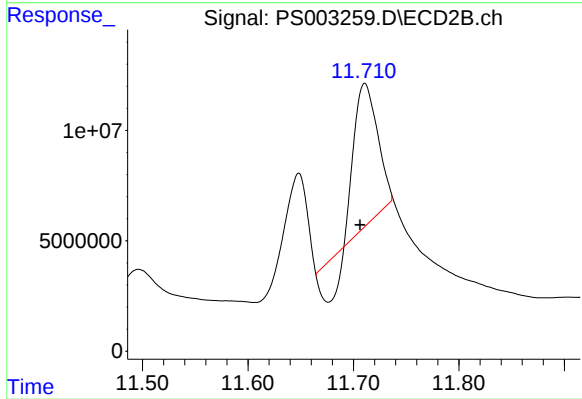

#7 MCPA


R.T.: 11.711 min
Delta R.T.: 0.005 min
Response: 86171120
Conc: 54.78 ug/ml

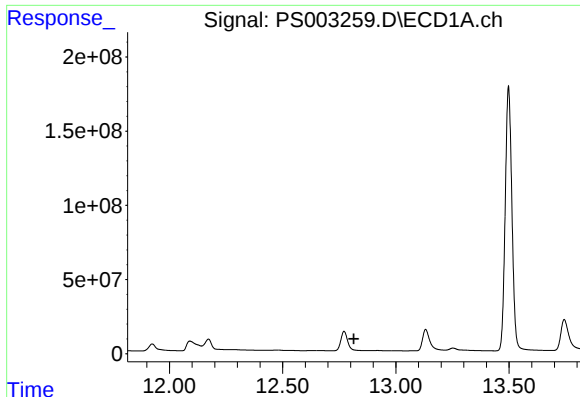

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.815 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CABLE-BRIDGE-FOUNDATION-D-1

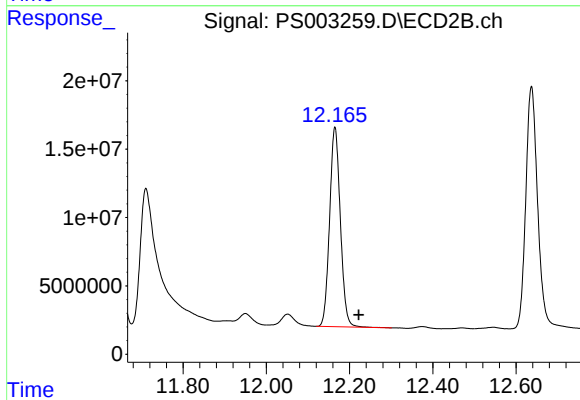


#8 DICHLORPROP

R.T.: 12.165 min
Delta R.T.: -0.057 min
Response: 260451097
Conc: 681.20 ng/ml

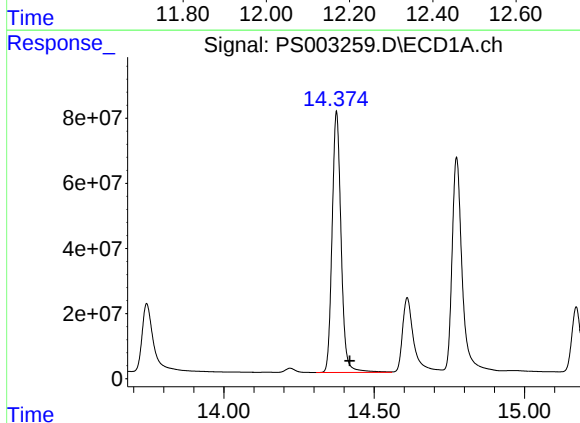


#11 2,4,5-TP (SILVEX)

R.T.: 14.375 min
Delta R.T.: -0.045 min
Response: 1661299305
Conc: 659.67 ng/ml

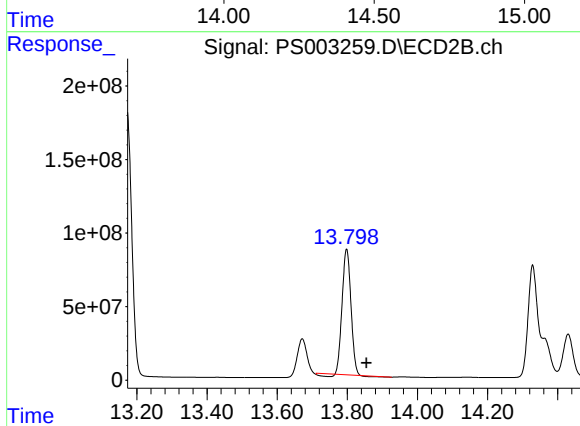

#11 2,4,5-TP (SILVEX)


R.T.: 13.798 min
Delta R.T.: -0.056 min
Response: 1472010446
Conc: 593.47 ng/ml

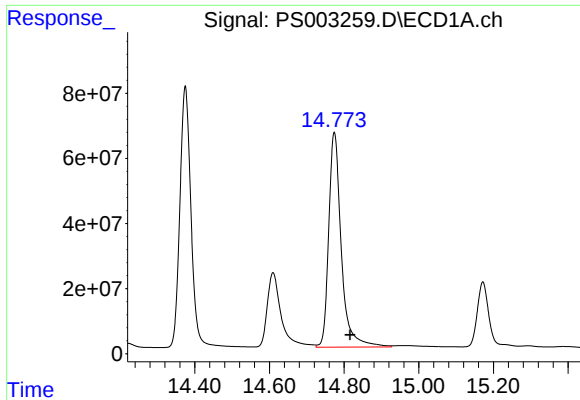

#12 2,4,5-T


R.T.: 14.774 min
Delta R.T.: -0.043 min
Response: 1543222526
Conc: 632.62 ng/ml

Instrument :
ECD_S
ClientSampleId :
CABLE-BRIDGE-FOUNDATION-D-1

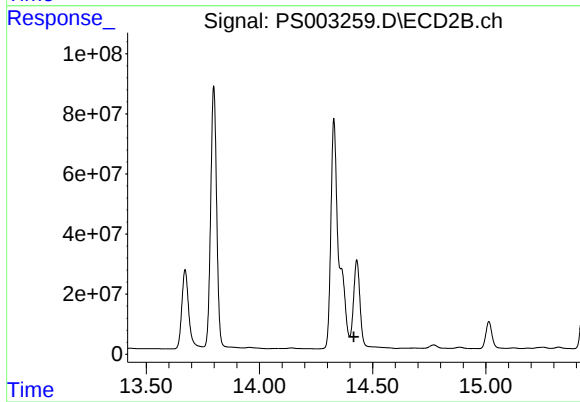


#12 2,4,5-T

R.T.: 14.430 min
Delta R.T.: 0.013 min
Response: -2030196991
Conc: N.D.

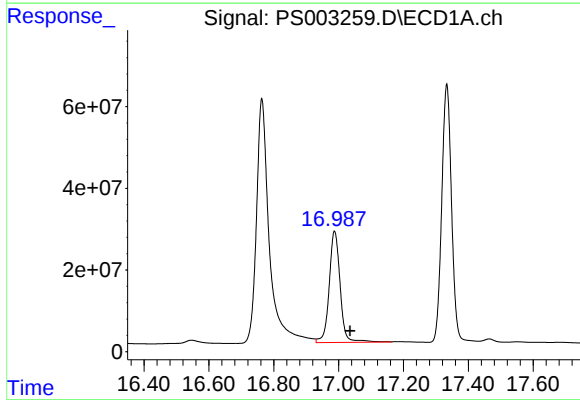


#14 DINOSEB

R.T.: 16.987 min
Delta R.T.: -0.048 min
Response: 642063611
Conc: 341.28 ng/ml

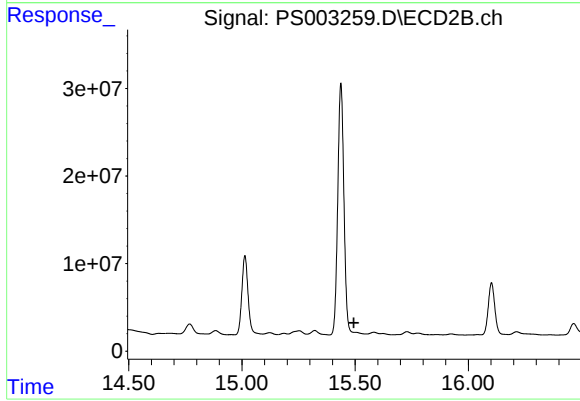

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 15.495 min
Response: 0
Conc: N.D.

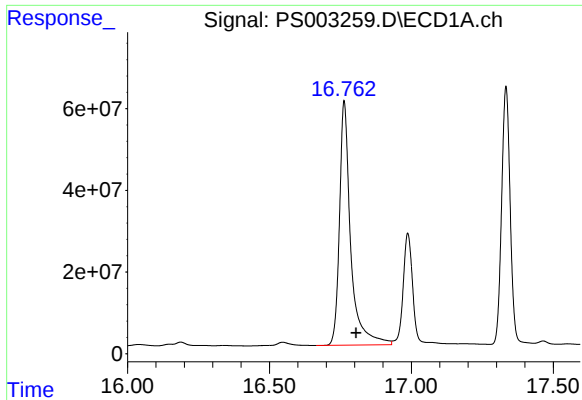

#15 Picloram


R.T.: 16.763 min
Delta R.T.: -0.042 min
Response: 1645169166
Conc: 520.03 ng/ml

Instrument :
ECD_S
ClientSampleId :
CABLE-BRIDGE-FOUNDATION-D-1

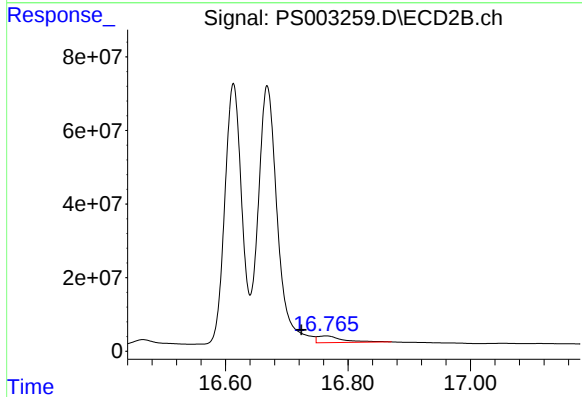


#15 Picloram

R.T.: 16.763 min
Delta R.T.: 0.039 min
Response: 52406845
Conc: 17.43 ng/ml

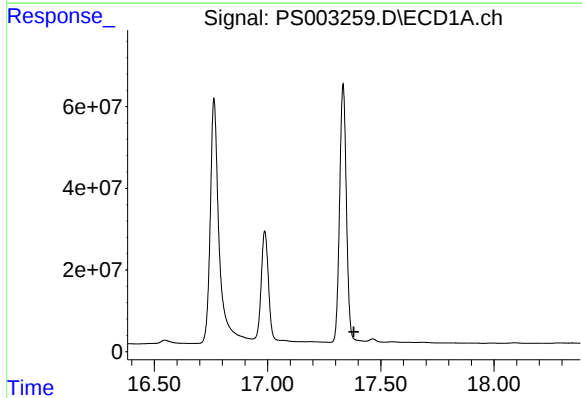

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.382 min
Response: 0
Conc: N.D.

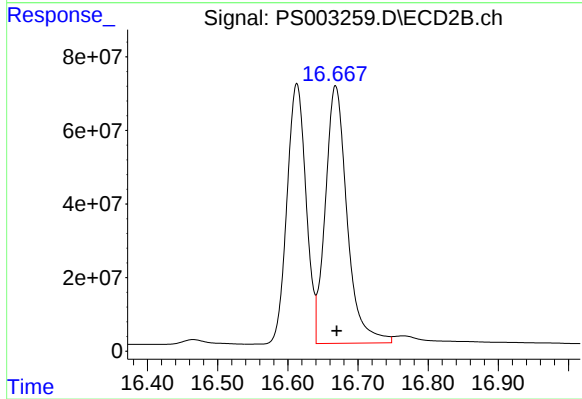

#16 DCPA

R.T.: 16.668 min
Delta R.T.: -0.001 min
Response: 1506837866
Conc: 486.46 ng/ml