

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021919\
 Data File : PS003262.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Feb 2019 21:13
 Operator : EI\SJ
 Sample : K1518-06
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CABLE-BRID3GE-FOUNDATION-D-

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 20 00:55:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.299	10.801	170.4E6	171.2E6	448.763	400.530
Target Compounds							
6) T	MCP	11.984	0.000	2735906	0	2.283	N.D. #
7) T	MCPA	0.000	11.762	0	131.1E6	N.D.	83.367 #
15) T	Picloram	0.000	16.734	0	8381241	N.D.	2.788 #
16) T	DCPA	0.000	16.734	0	8381241	N.D.	2.706 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021919\
Data File : PS003262.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Feb 2019 21:13
Operator : EI\SJ
Sample : K1518-06
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
CABLE-BRID3GE-FOUNDATION-D-

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 20 00:55:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

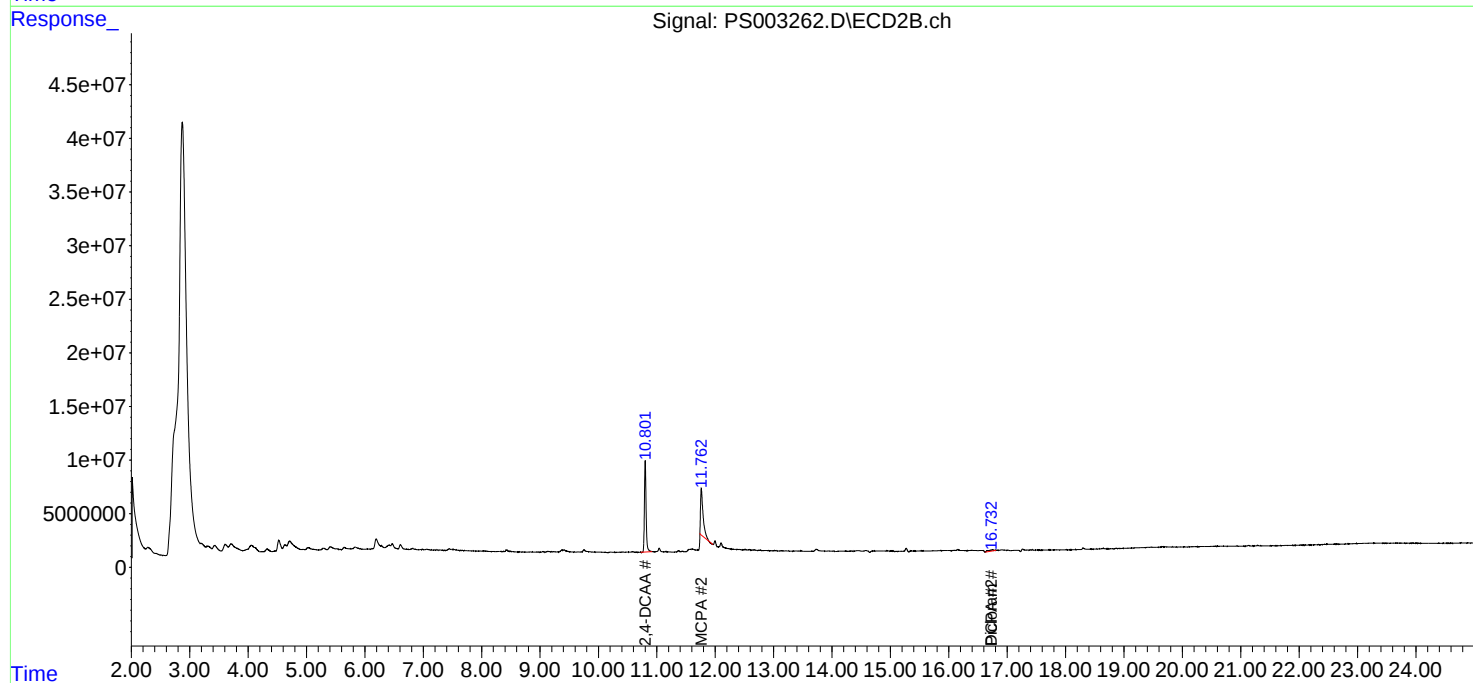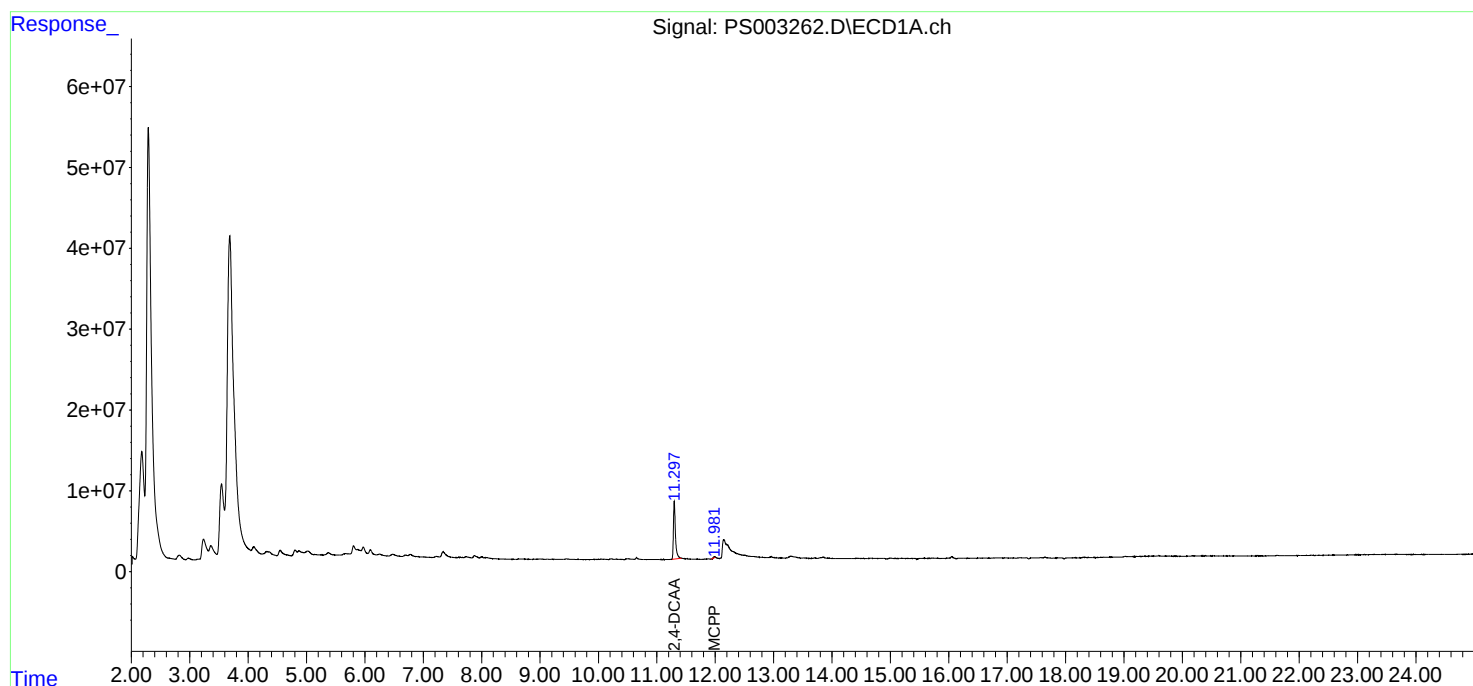


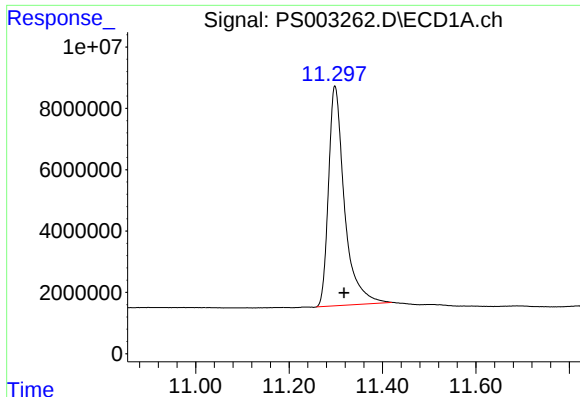

#4 2,4-DCAA


R.T.: 11.299 min
Delta R.T.: -0.019 min
Response: 170368770
Conc: 448.76 ng/ml

Instrument :
ECD_S
ClientSampleId :
CABLE-BRID3GE-FOUNDATION-D-

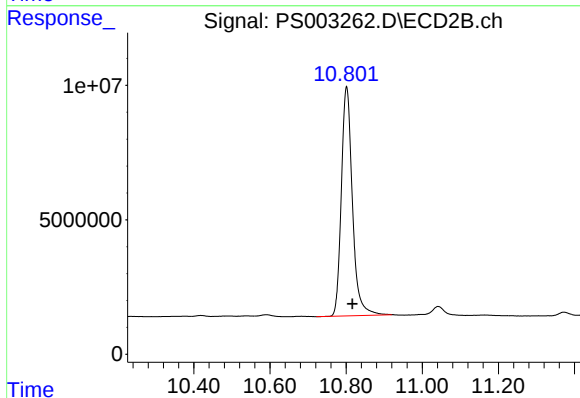


#4 2,4-DCAA

R.T.: 10.801 min
Delta R.T.: -0.015 min
Response: 171244924
Conc: 400.53 ng/ml

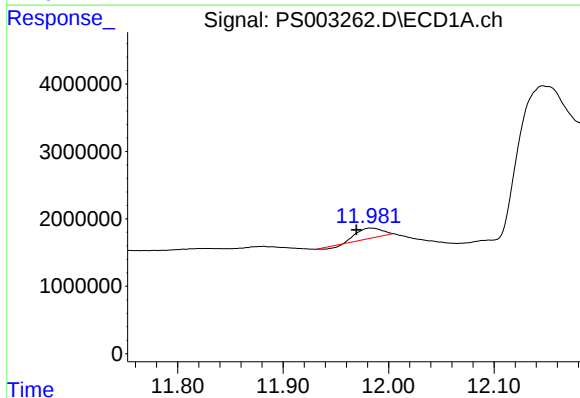


#6 MCP

R.T.: 11.984 min
Delta R.T.: 0.015 min
Response: 2735906
Conc: 2.28 ug/ml

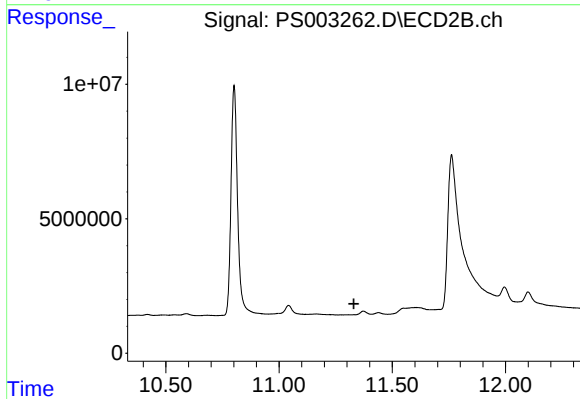

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.330 min
Response: 0
Conc: N.D.

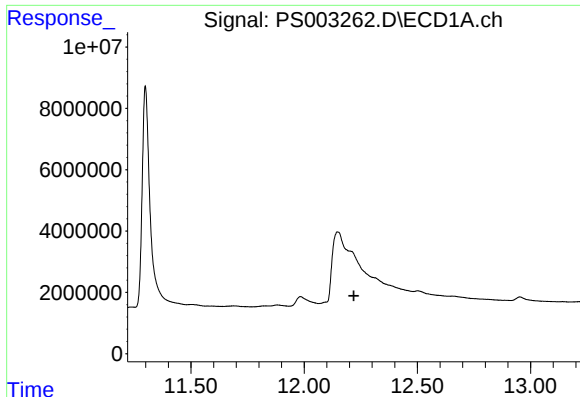

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 12.219 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CABLE-BRID3GE-FOUNDATION-D-

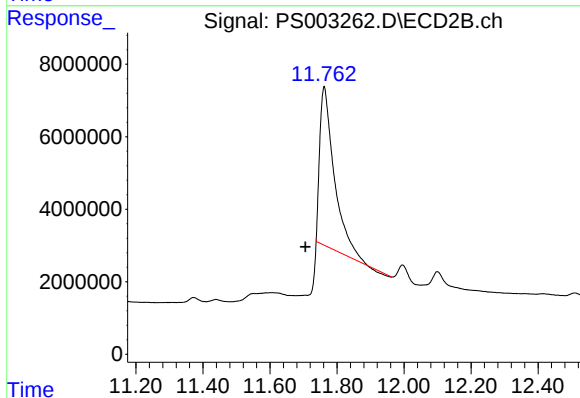


#7 MCPA

R.T.: 11.762 min
Delta R.T.: 0.056 min
Response: 131142062
Conc: 83.37 ug/ml

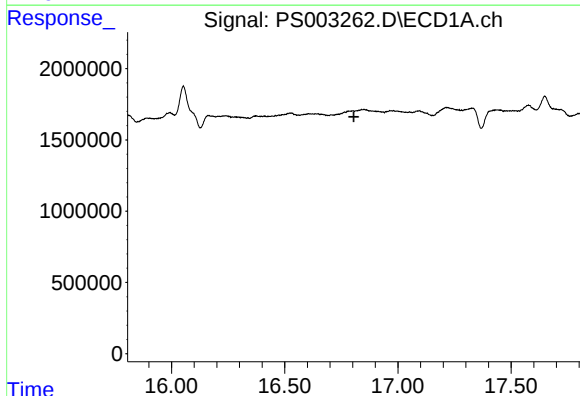


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.806 min
Response: 0
Conc: N.D.

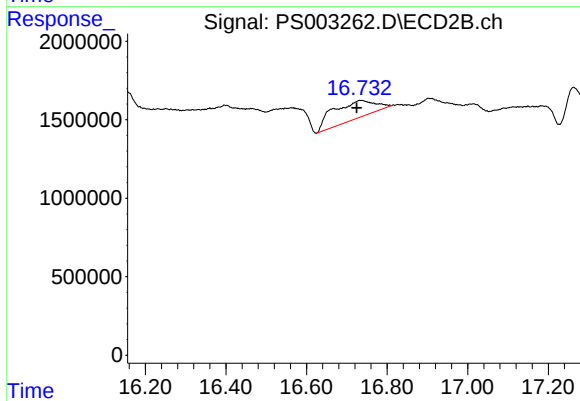

#15 Picloram


R.T.: 16.734 min
Delta R.T.: 0.010 min
Response: 8381241
Conc: 2.79 ng/ml

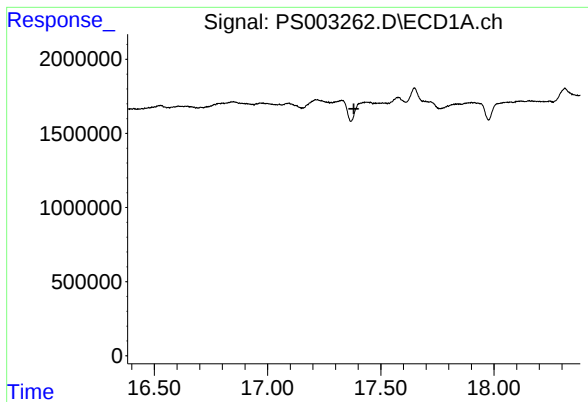

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CABLE-BRID3GE-FOUNDATION-D-

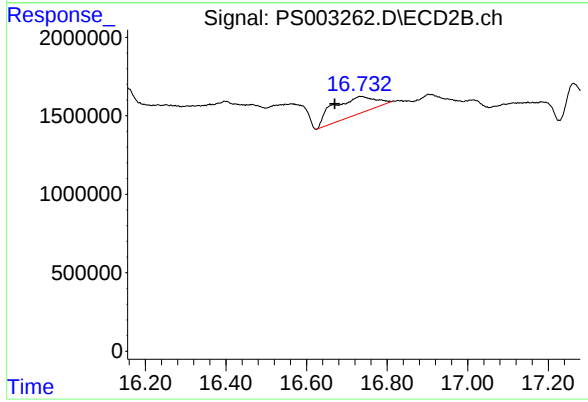

#16 DCPA

R.T.: 16.734 min
Delta R.T.: 0.064 min
Response: 8381241
Conc: 2.71 ng/ml