

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021919\
 Data File : PS003265.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Feb 2019 22:46
 Operator : EI\SJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 20 00:56:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.278	10.779	172.1E6	319.5E6	453.248	747.308 #
Target Compounds							
1) T	Dalapon	2.842	2.313	110.6E6	375.9E6	200.561	701.323 #
3) T	4-Nitroph...	10.872	9.931	90653178	148.8E6	468.397	711.950 #
8) T	DICHLORPROP	0.000	12.185	0	276.6E6	N.D.	723.550 #
9) T	2,4-D	13.135	12.657	93413369	262.8E6	202.606	524.188 #
11) T	2,4,5-TP ...	14.376	13.817	1886.4E6	1761.2E6	749.060	710.055
12) T	2,4,5-T	14.777	14.349	1815.6E6	1821.8E6	744.269	952.067 #
14) T	DINOSEB	16.987	0.000	1431.8E6	0	761.046	N.D. #
15) T	Picloram	16.766	16.688	2051.0E6	1914.1E6	648.294	636.673
16) T	DCPA	0.000	16.688	0	1914.1E6	N.D.	617.931 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021919\
Data File : PS003265.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Feb 2019 22:46
Operator : EI\SJ
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 20 00:56:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

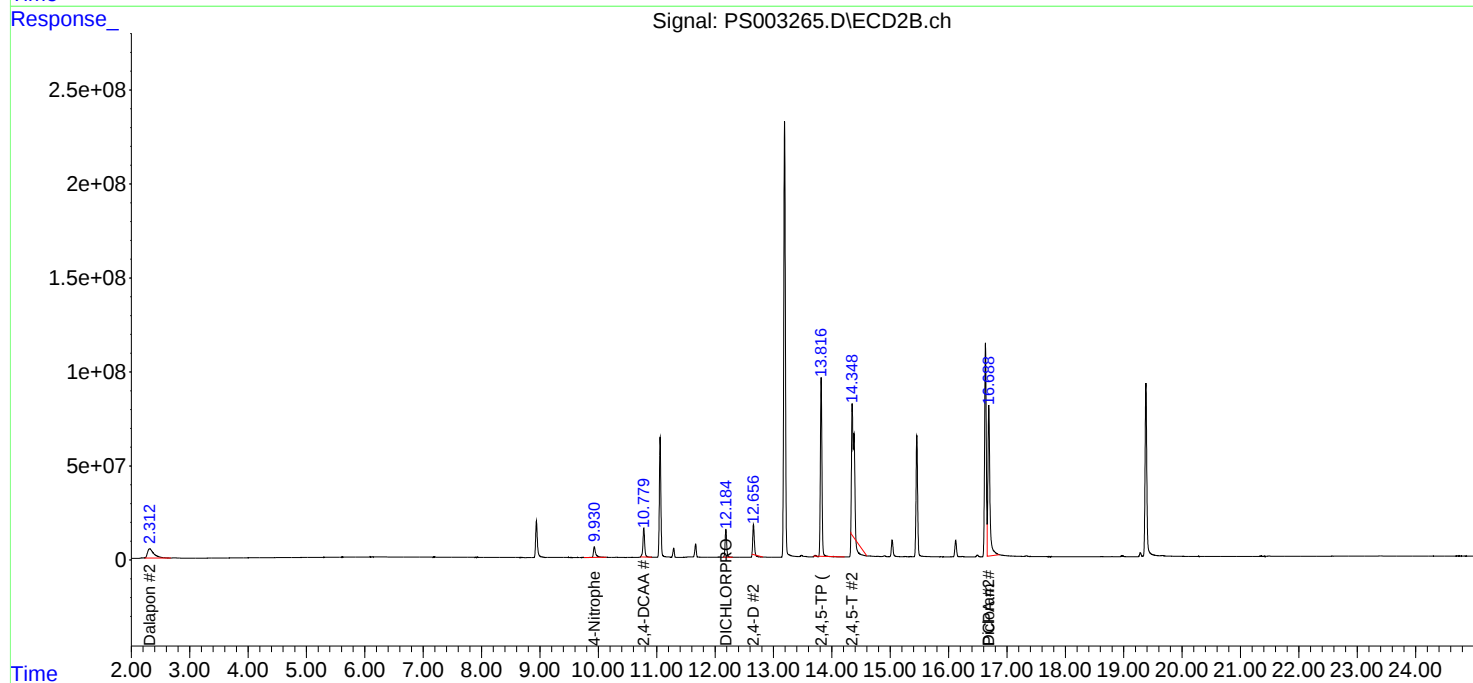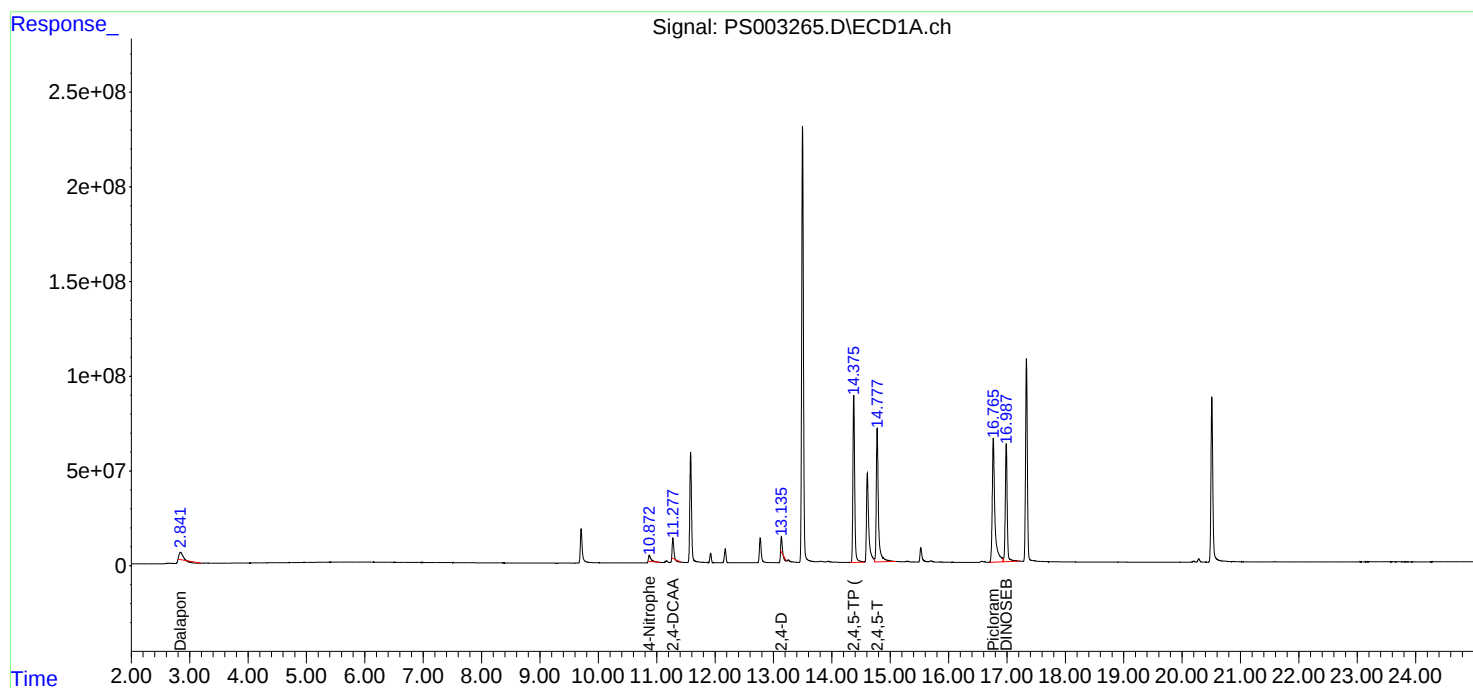


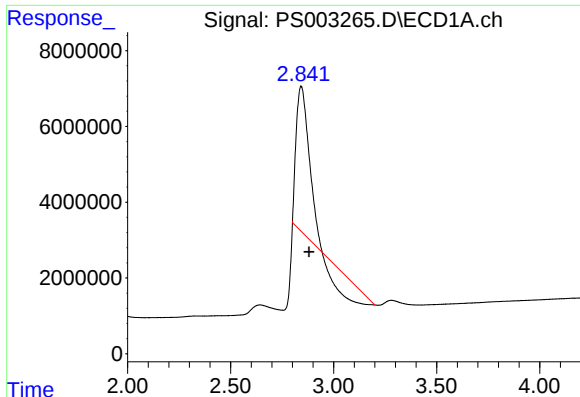

#1 Dalapon


R.T.: 2.842 min
Delta R.T.: -0.038 min
Response: 110638754
Conc: 200.56 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

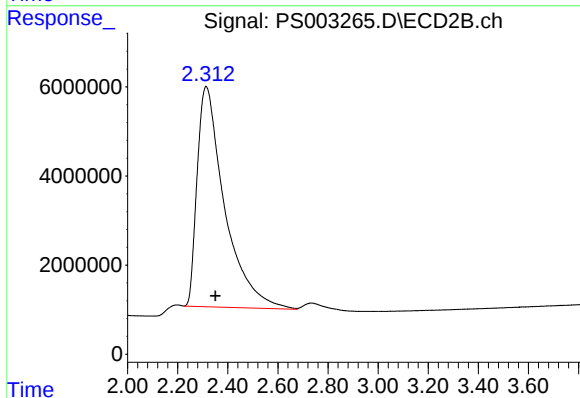


#1 Dalapon

R.T.: 2.313 min
Delta R.T.: -0.037 min
Response: 375853703
Conc: 701.32 ng/ml

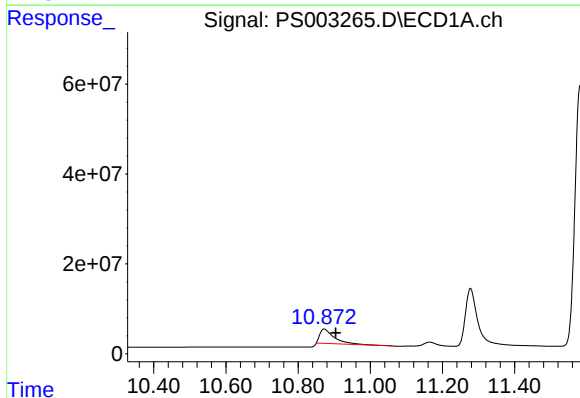


#3 4-Nitrophenol

R.T.: 10.872 min
Delta R.T.: -0.032 min
Response: 90653178
Conc: 468.40 ng/ml

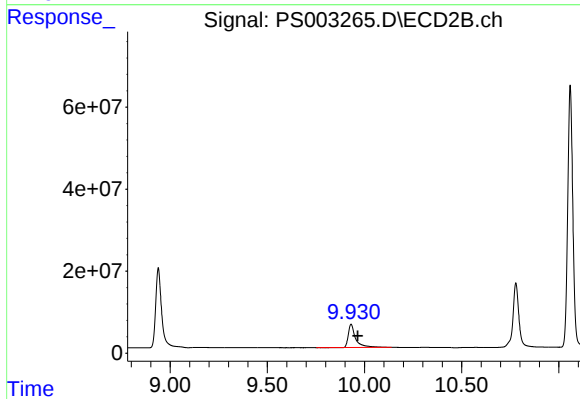

#3 4-Nitrophenol


R.T.: 9.931 min
Delta R.T.: -0.034 min
Response: 148813598
Conc: 711.95 ng/ml

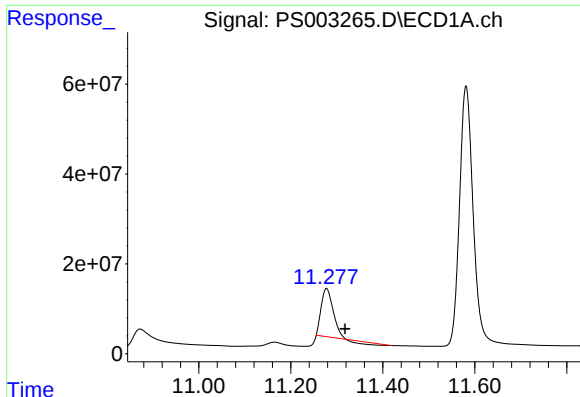

#4 2,4-DCAA


R.T.: 11.278 min
Delta R.T.: -0.040 min
Response: 172071334
Conc: 453.25 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

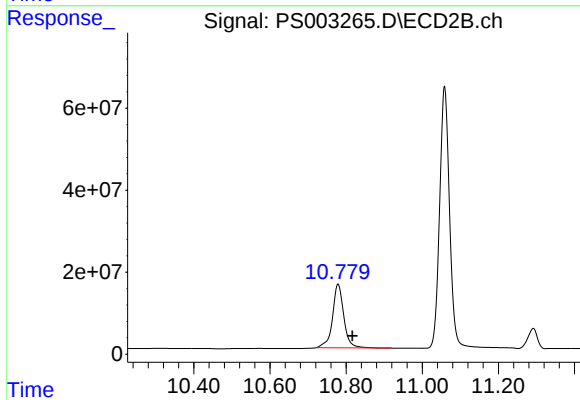


#4 2,4-DCAA

R.T.: 10.779 min
Delta R.T.: -0.038 min
Response: 319508388
Conc: 747.31 ng/ml

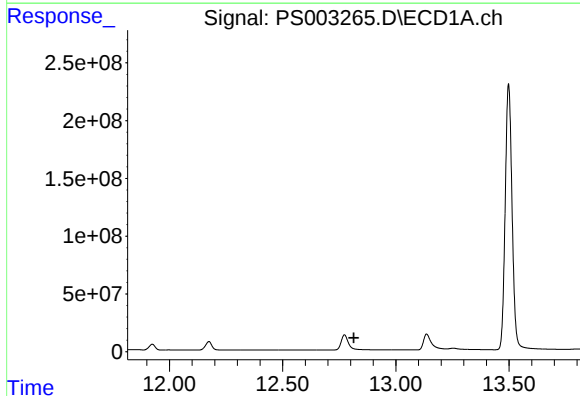


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.815 min
Response: 0
Conc: N.D.

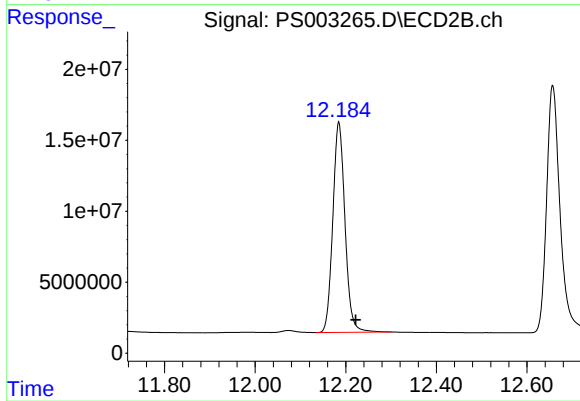

#8 DICHLORPROP


R.T.: 12.185 min
Delta R.T.: -0.037 min
Response: 276642757
Conc: 723.55 ng/ml

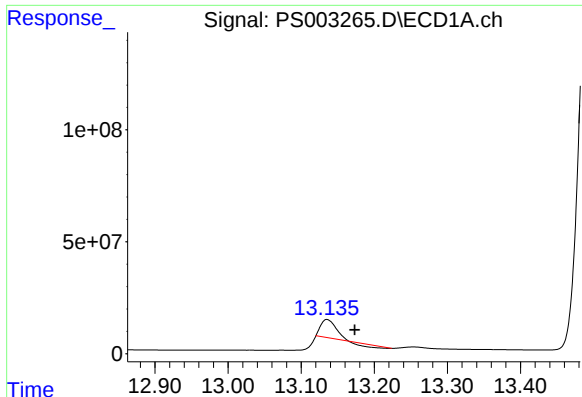

#9 2,4-D


R.T.: 13.135 min
Delta R.T.: -0.038 min
Response: 93413369
Conc: 202.61 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

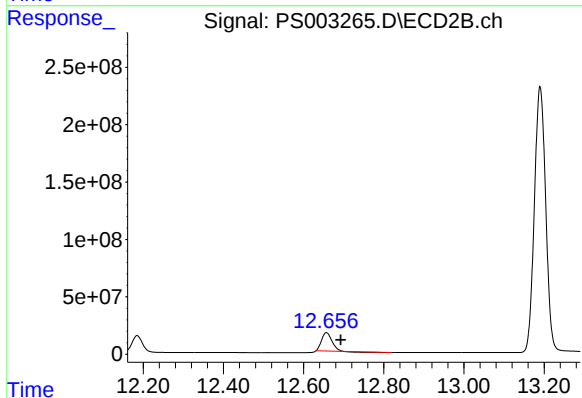


#9 2,4-D

R.T.: 12.657 min
Delta R.T.: -0.036 min
Response: 262820667
Conc: 524.19 ng/ml

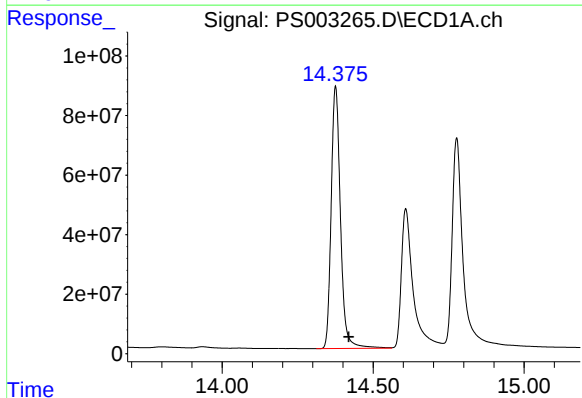


#11 2,4,5-TP (SILVEX)

R.T.: 14.376 min
Delta R.T.: -0.044 min
Response: 1886413642
Conc: 749.06 ng/ml

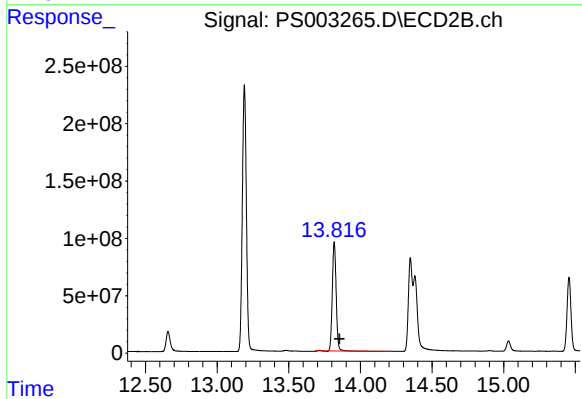

#11 2,4,5-TP (SILVEX)


R.T.: 13.817 min
Delta R.T.: -0.037 min
Response: 1761188656
Conc: 710.05 ng/ml

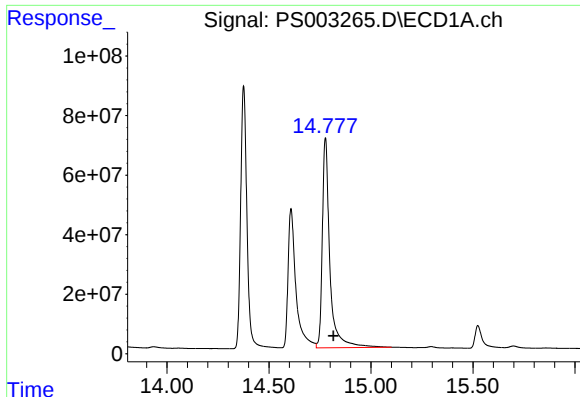

#12 2,4,5-T


R.T.: 14.777 min
Delta R.T.: -0.040 min
Response: 1815573219
Conc: 744.27 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

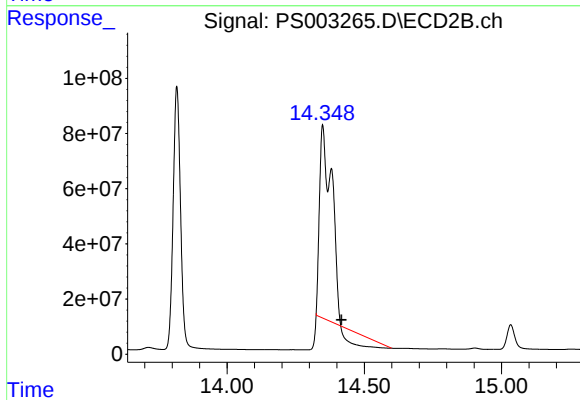


#12 2,4,5-T

R.T.: 14.349 min
Delta R.T.: -0.068 min
Response: 1821768768
Conc: 952.07 ng/ml

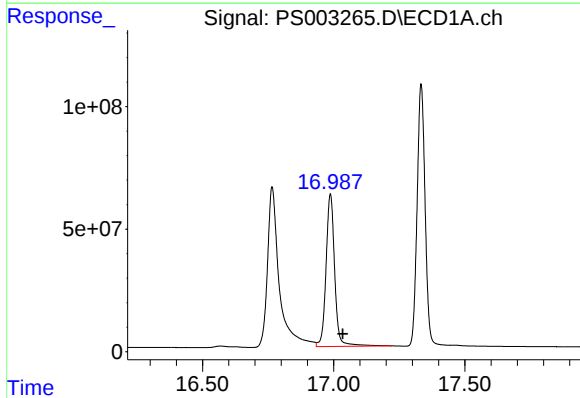


#14 DINOSEB

R.T.: 16.987 min
Delta R.T.: -0.048 min
Response: 1431776232
Conc: 761.05 ng/ml

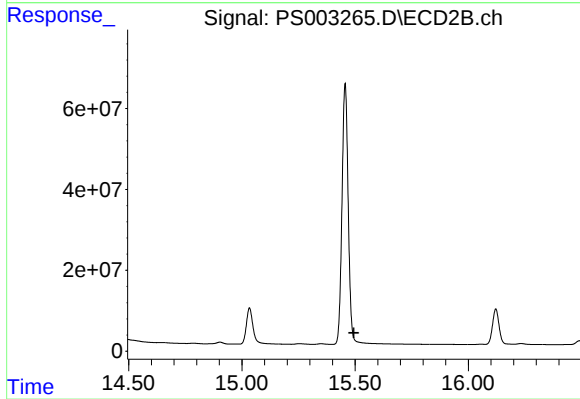

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 15.495 min
Response: 0
Conc: N.D.

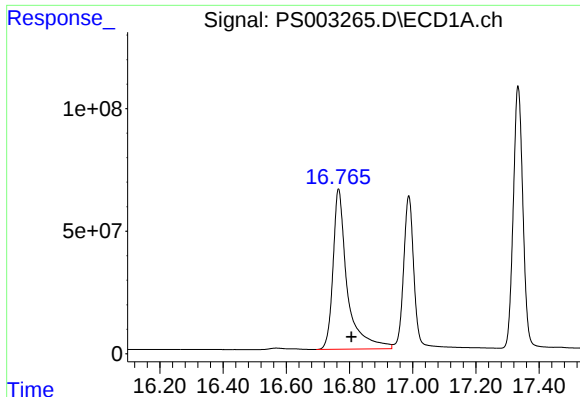

#15 Picloram


R.T.: 16.766 min
Delta R.T.: -0.040 min
Response: 2050962499
Conc: 648.29 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

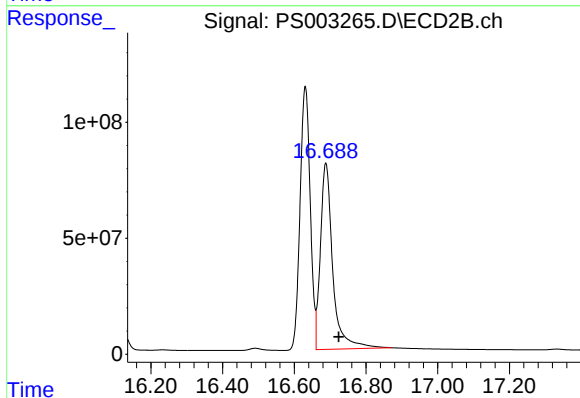


#15 Picloram

R.T.: 16.688 min
Delta R.T.: -0.036 min
Response: 1914096897
Conc: 636.67 ng/ml

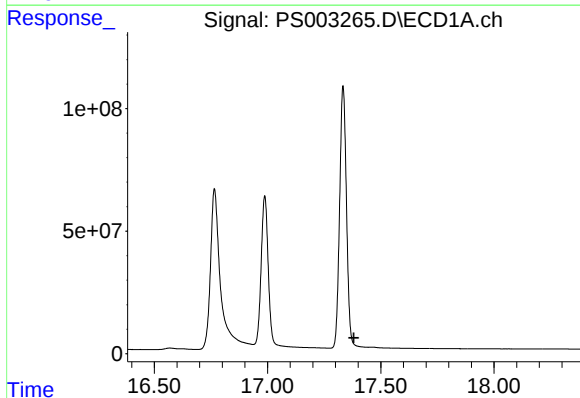

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.382 min
Response: 0
Conc: N.D.

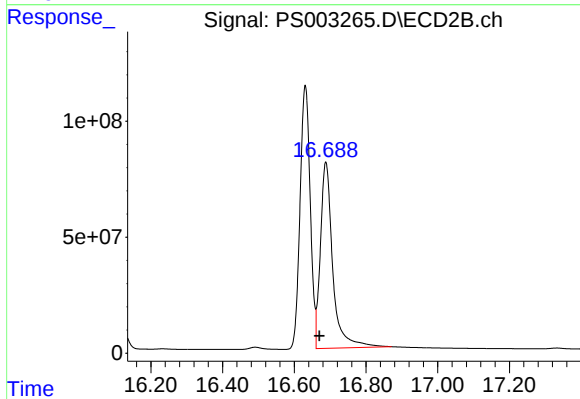

#16 DCPA

R.T.: 16.688 min
Delta R.T.: 0.018 min
Response: 1914096897
Conc: 617.93 ng/ml