

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021919\
 Data File : PS003266.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Feb 2019 23:16
 Operator : EI\SJ
 Sample : K1518-10
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CABLE-BRIDGE-FOUNDATION-D-5

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 20 00:56:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.307	10.803	40920790	43870914	107.788	102.611
Target Compounds							
6) T	MCP	11.986	0.000	3645562	0	3.043	N.D. #
7) T	MCPA	12.219	0.000	7679453	0	4.339	N.D. #
11) T	2,4,5-TP ...	14.422	0.000	1916983	0	0.761	N.D. #
12) T	2,4,5-T	0.000	14.426	0	4976579	N.D.	2.601 #
15) T	Picloram	0.000	16.734	0	14508940	N.D.	4.826 #
16) T	DCPA	0.000	16.661	0	3568432	N.D.	1.152 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021919\
Data File : PS003266.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Feb 2019 23:16
Operator : EI\SJ
Sample : K1518-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
CABLE-BRIDGE-FOUNDATION-D-5

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 20 00:56:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

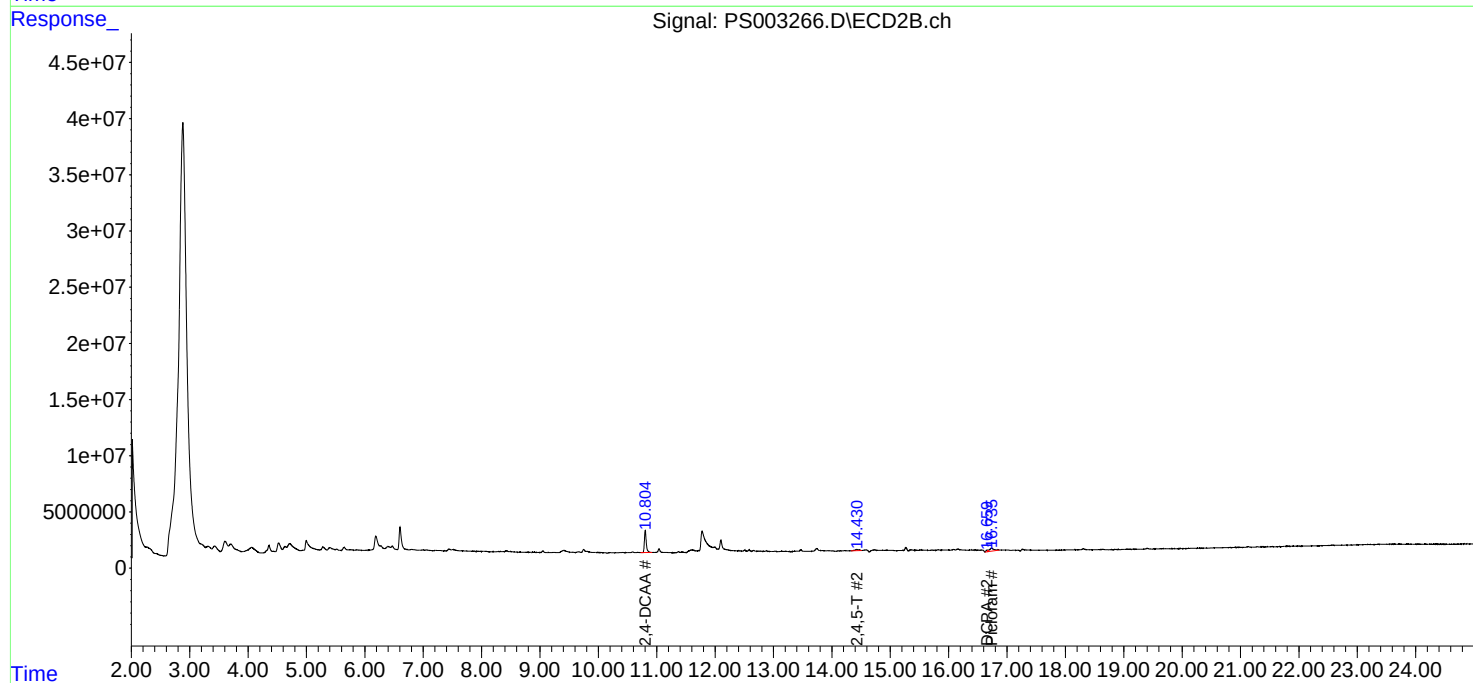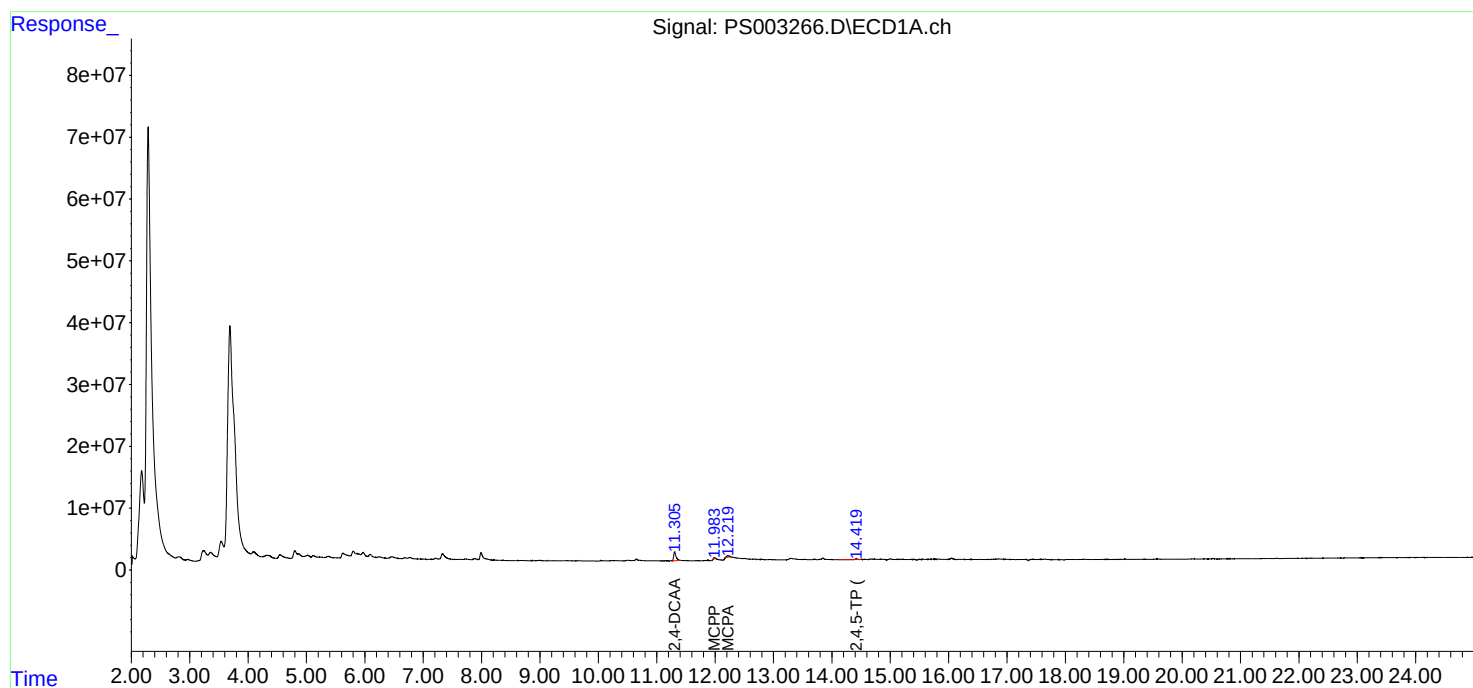


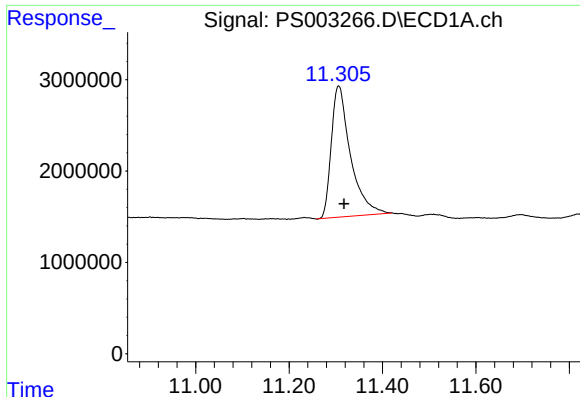

#4 2,4-DCAA


R.T.: 11.307 min
Delta R.T.: -0.011 min
Response: 40920790
Conc: 107.79 ng/ml

Instrument :
ECD_S
ClientSampleId :
CABLE-BRIDGE-FOUNDATION-D-5

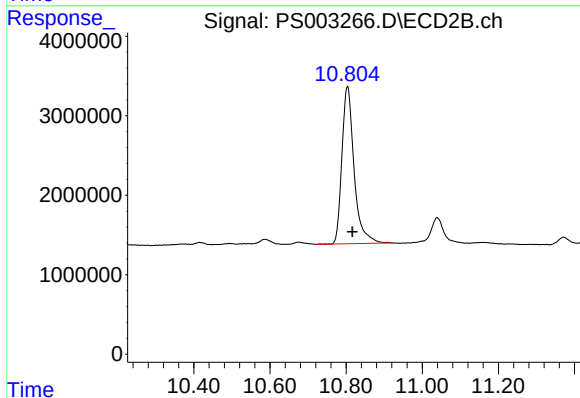


#4 2,4-DCAA

R.T.: 10.803 min
Delta R.T.: -0.013 min
Response: 43870914
Conc: 102.61 ng/ml

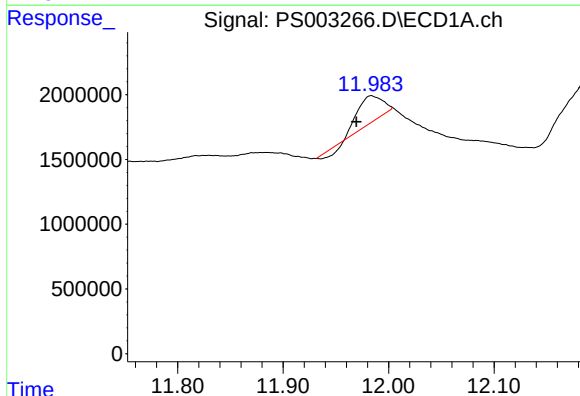


#6 MCP

R.T.: 11.986 min
Delta R.T.: 0.016 min
Response: 3645562
Conc: 3.04 ug/ml

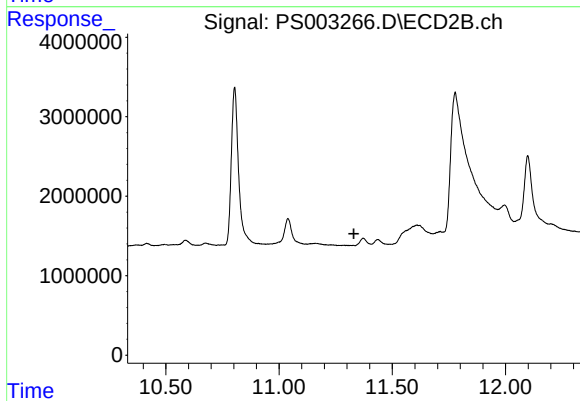

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.330 min
Response: 0
Conc: N.D.

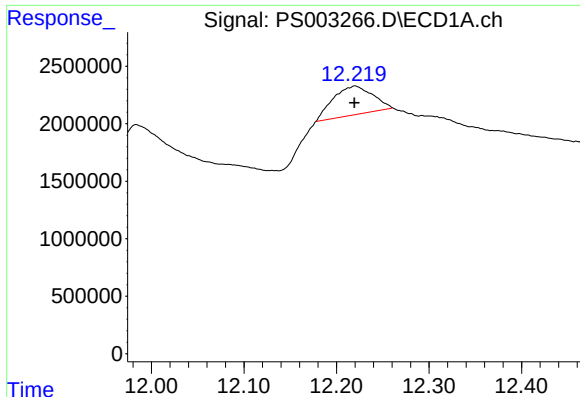

#7 MCPA


R.T.: 12.219 min
Delta R.T.: 0.000 min
Response: 7679453
Conc: 4.34 ug/ml

Instrument :
ECD_S
ClientSampleId :
CABLE-BRIDGE-FOUNDATION-D-5

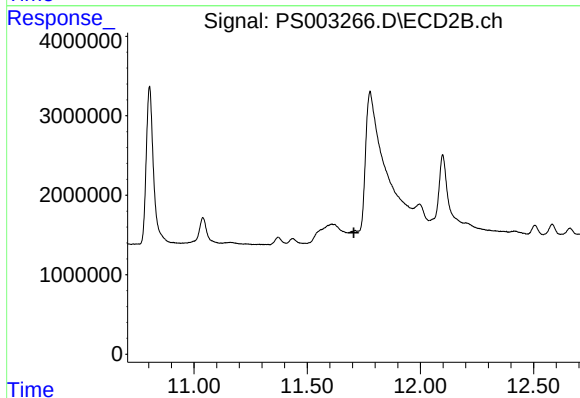


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 11.706 min
Response: 0
Conc: N.D.

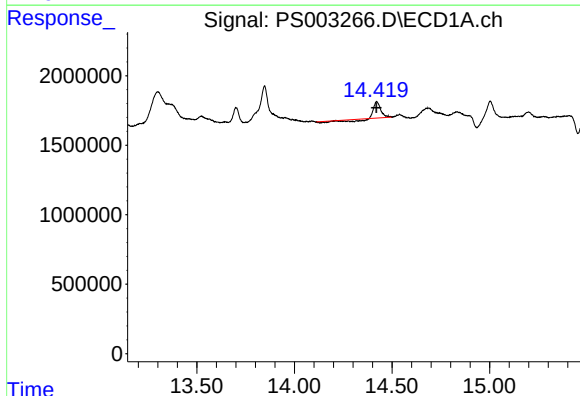


#11 2,4,5-TP (SILVEX)

R.T.: 14.422 min
Delta R.T.: 0.002 min
Response: 1916983
Conc: 0.76 ng/ml

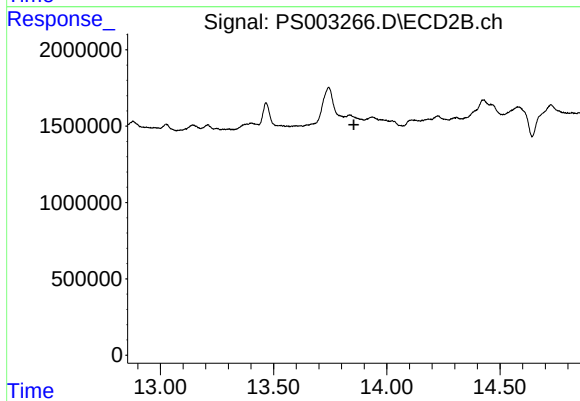

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 13.854 min
Response: 0
Conc: N.D.

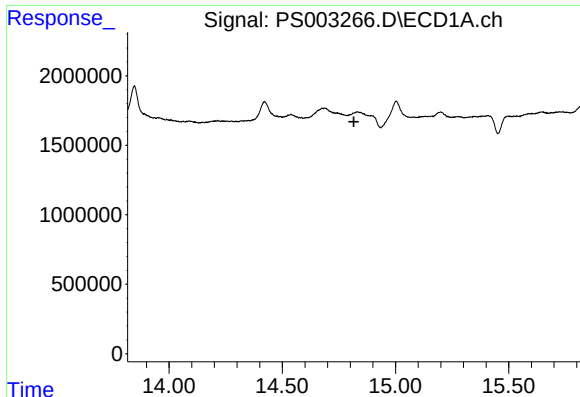

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 14.817 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CABLE-BRIDGE-FOUNDATION-D-5

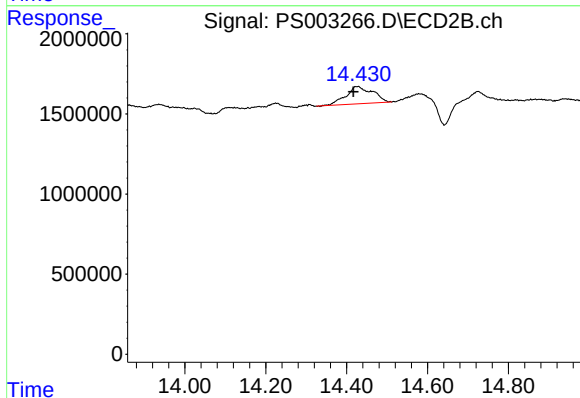


#12 2,4,5-T

R.T.: 14.426 min
Delta R.T.: 0.009 min
Response: 4976579
Conc: 2.60 ng/ml

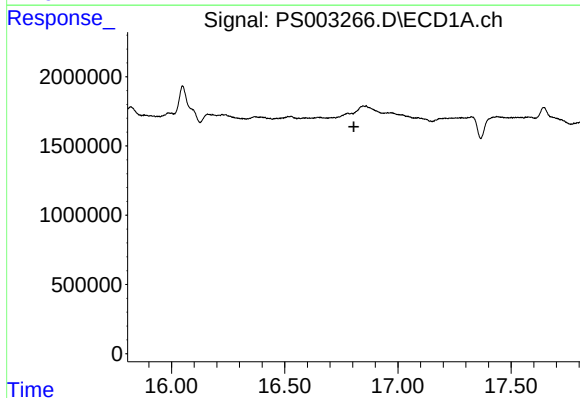


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.806 min
Response: 0
Conc: N.D.

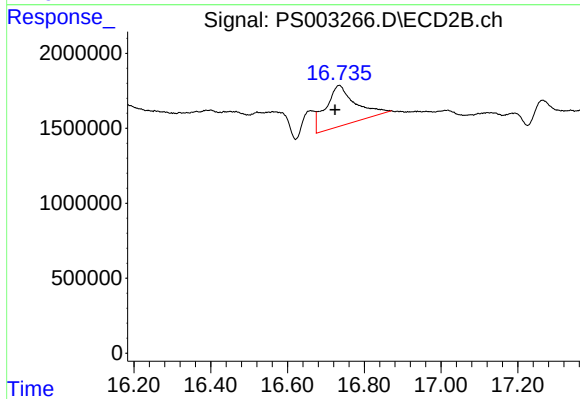

#15 Picloram


R.T.: 16.734 min
Delta R.T.: 0.010 min
Response: 14508940
Conc: 4.83 ng/ml

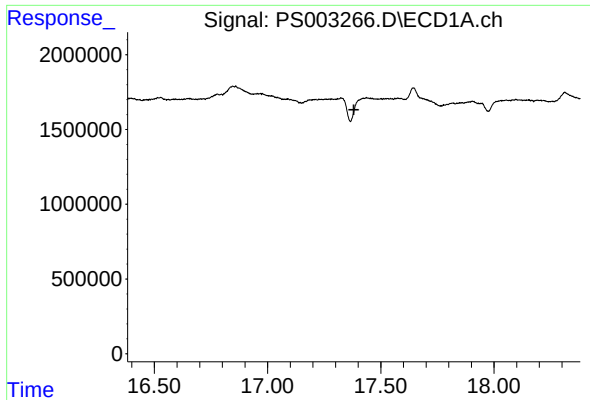

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CABLE-BRIDGE-FOUNDATION-D-5

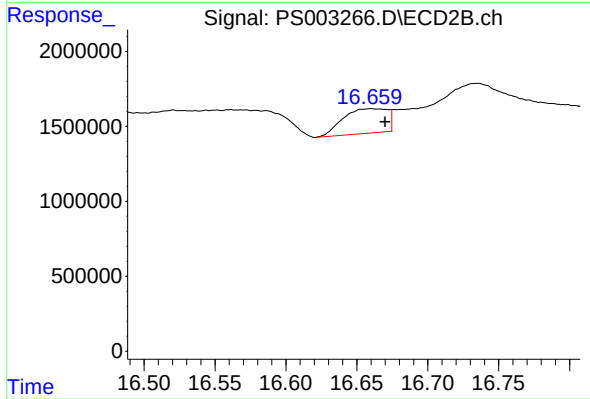

#16 DCPA

R.T.: 16.661 min
Delta R.T.: -0.009 min
Response: 3568432
Conc: 1.15 ng/ml