

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021919\
 Data File : PS003267.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Feb 2019 23:48
 Operator : EI\SJ
 Sample : K1518-12
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CABLE-BRIDGE-FOUNDATION-D-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 20 00:56:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.276	10.778	78354238	189.9E6	206.390	444.207 #
Target Compounds							
6) T	MCP	11.959	11.348	5277102	824324	4.404	0.747 #
14) T	DINOSEB	0.000	15.503	0	3211065	N.D.	1.832 #
15) T	Picloram	0.000	16.711	0	8307471	N.D.	2.763 #
16) T	DCPA	17.417	16.711	-1658103	8307471	N.D.	2.682



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021919\
Data File : PS003267.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Feb 2019 23:48
Operator : EI\SJ
Sample : K1518-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
CABLE-BRIDGE-FOUNDATION-D-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 20 00:56:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

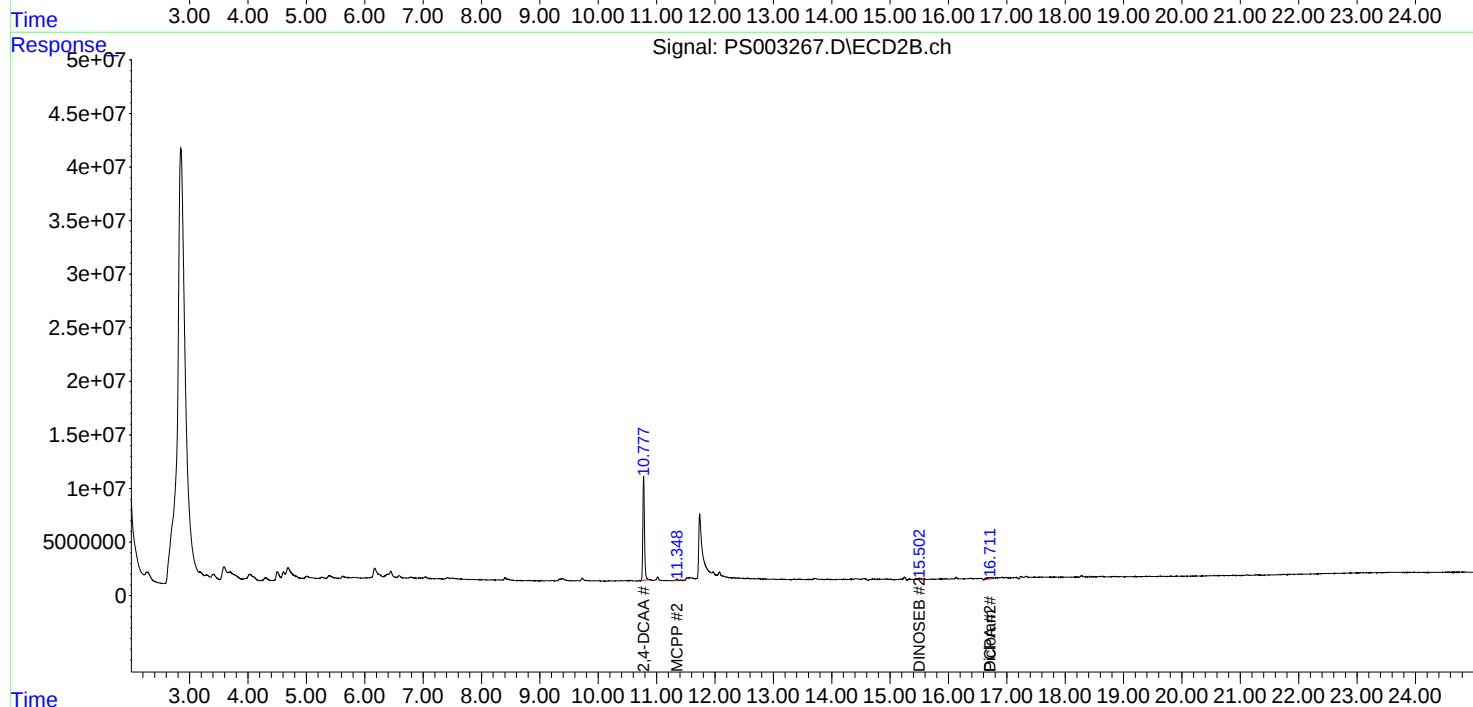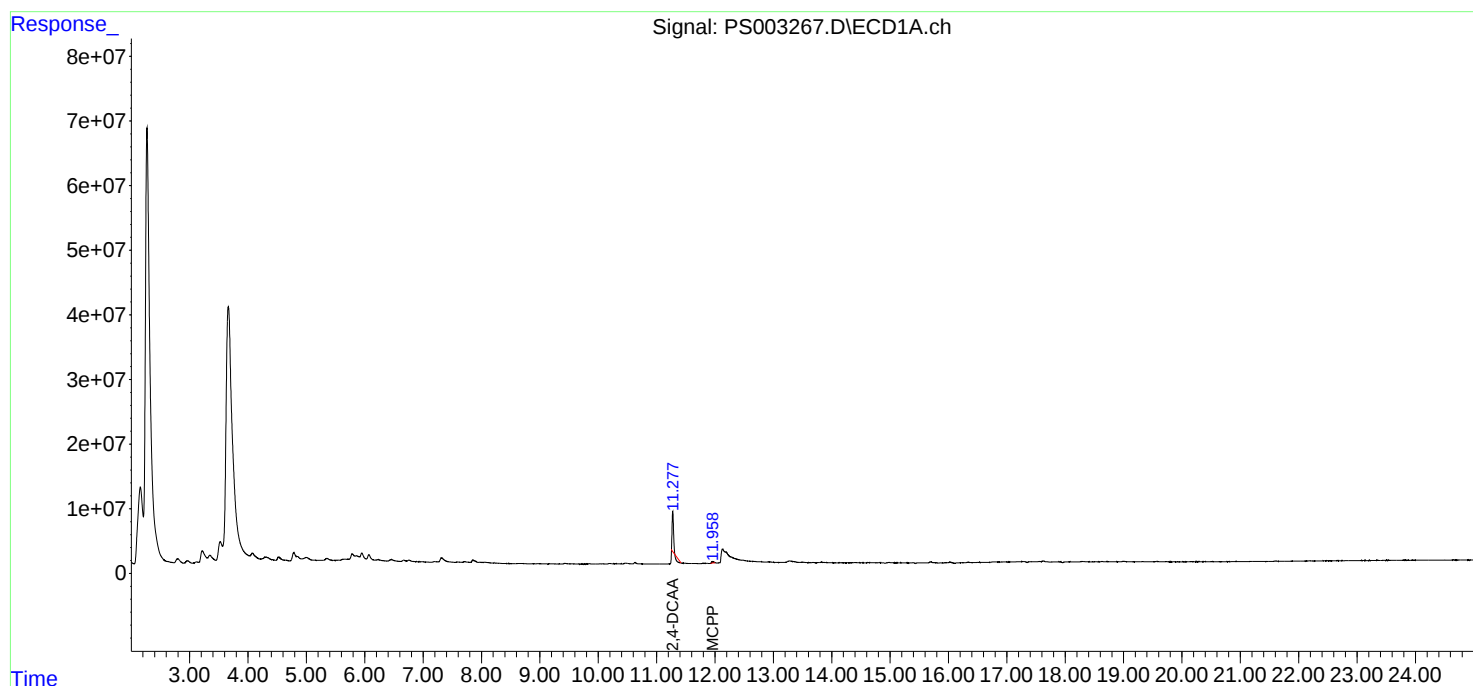


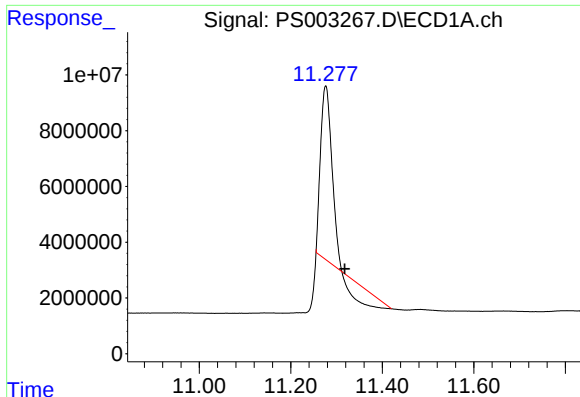

#4 2,4-DCAA


R.T.: 11.276 min
Delta R.T.: -0.041 min
Response: 78354238
Conc: 206.39 ng/ml

Instrument :
ECD_S
ClientSampleId :
CABLE-BRIDGE-FOUNDATION-D-6

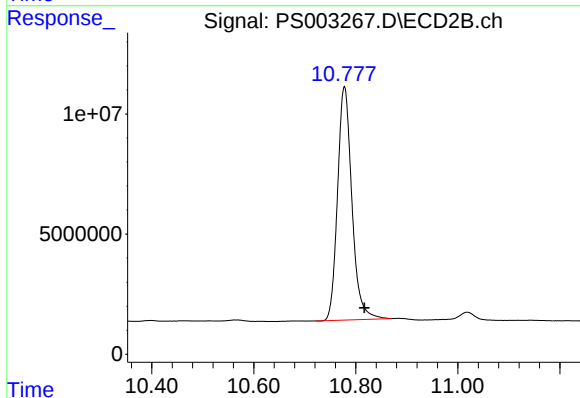


#4 2,4-DCAA

R.T.: 10.778 min
Delta R.T.: -0.039 min
Response: 189918653
Conc: 444.21 ng/ml

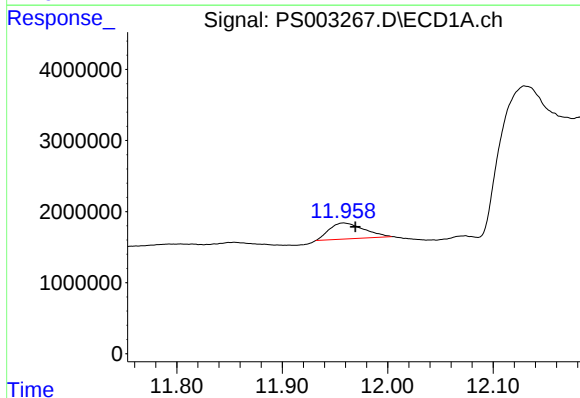


#6 MCP

R.T.: 11.959 min
Delta R.T.: -0.011 min
Response: 5277102
Conc: 4.40 ug/ml

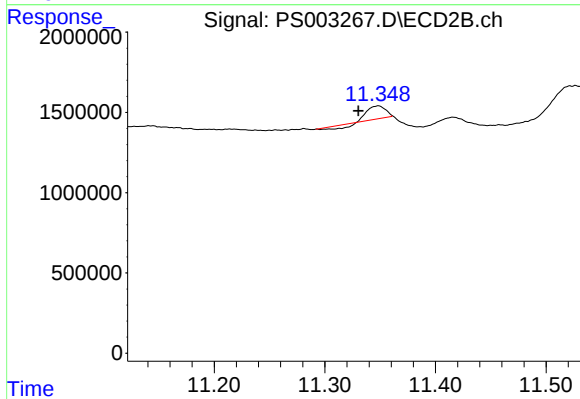

#6 MCP


R.T.: 11.348 min
Delta R.T.: 0.017 min
Response: 824324
Conc: 0.75 ug/ml

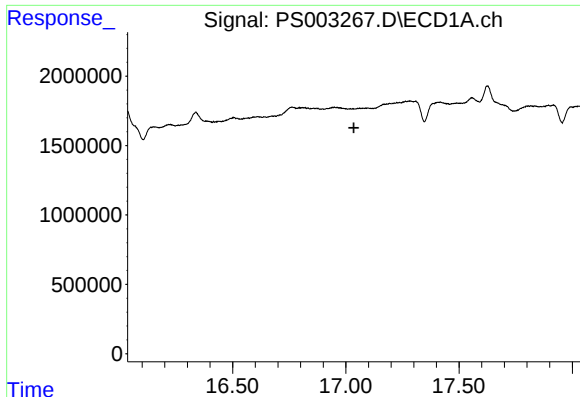

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 17.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CABLE-BRIDGE-FOUNDATION-D-6

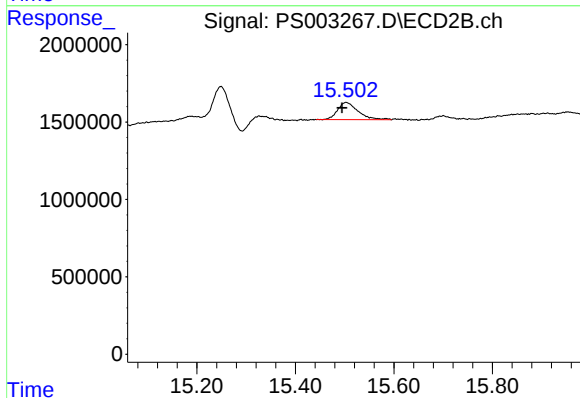


#14 DINOSEB

R.T.: 15.503 min
Delta R.T.: 0.008 min
Response: 3211065
Conc: 1.83 ng/ml

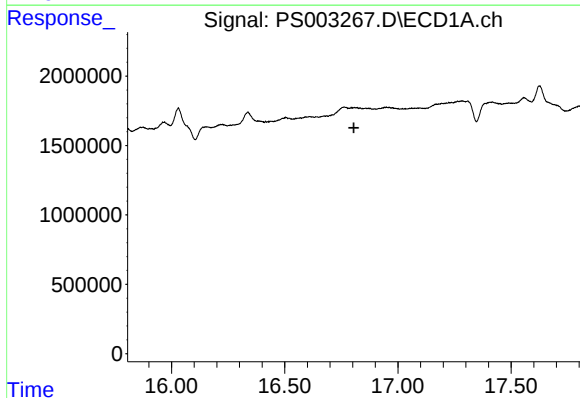


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.806 min
Response: 0
Conc: N.D.

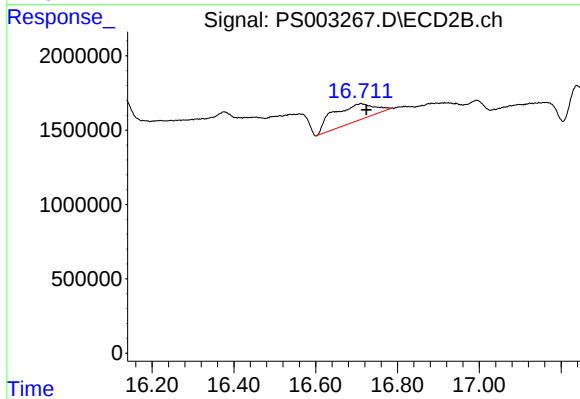

#15 Picloram


R.T.: 16.711 min
Delta R.T.: -0.014 min
Response: 8307471
Conc: 2.76 ng/ml

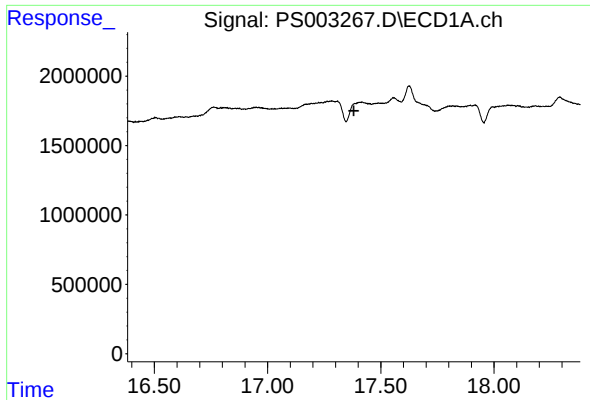

#16 DCPA

R.T.: 17.417 min
Delta R.T.: 0.035 min
Response: -1658103
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CABLE-BRIDGE-FOUNDATION-D-6

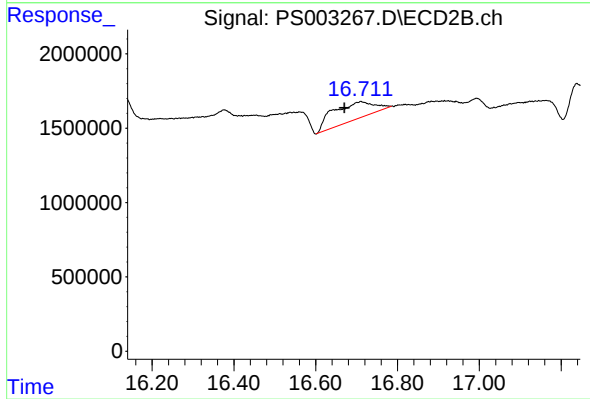

#16 DCPA

R.T.: 16.711 min
Delta R.T.: 0.041 min
Response: 8307471
Conc: 2.68 ng/ml