

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS021919\  
 Data File : PS003268.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 20 Feb 2019 00:19  
 Operator : EI\SJ  
 Sample : K1518-14  
 Misc :  
 ALS Vial : 15 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 CABLE-BRIDGE-FOUNDATION-D-7

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Feb 20 00:56:54 2019  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS012819.M  
 Quant Title : 8080.M  
 QLast Update : Tue Jan 29 06:11:45 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound | RT#1   | RT#2   | Resp#1  | Resp#2  | ng/ml   | ng/ml   |
|-----------------------------|----------|--------|--------|---------|---------|---------|---------|
| -----                       |          |        |        |         |         |         |         |
| System Monitoring Compounds |          |        |        |         |         |         |         |
| 4) S                        | 2,4-DCAA | 11.298 | 10.783 | 175.7E6 | 177.3E6 | 462.852 | 414.608 |
| Target Compounds            |          |        |        |         |         |         |         |
| 6) T                        | MCP      | 11.981 | 0.000  | 2868071 | 0       | 2.394   | N.D. #  |
| 15) T                       | Picloram | 0.000  | 16.749 | 0       | 7202372 | N.D.    | 2.396 # |
| -----                       |          |        |        |         |         |         |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS021919\  
Data File : PS003268.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 20 Feb 2019 00:19  
Operator : EI\SJ  
Sample : K1518-14  
Misc :  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :  
CABLE-BRIDGE-FOUNDATION-D-7

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Feb 20 00:56:54 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS012819.M  
Quant Title : 8080.M  
QLast Update : Tue Jan 29 06:11:45 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

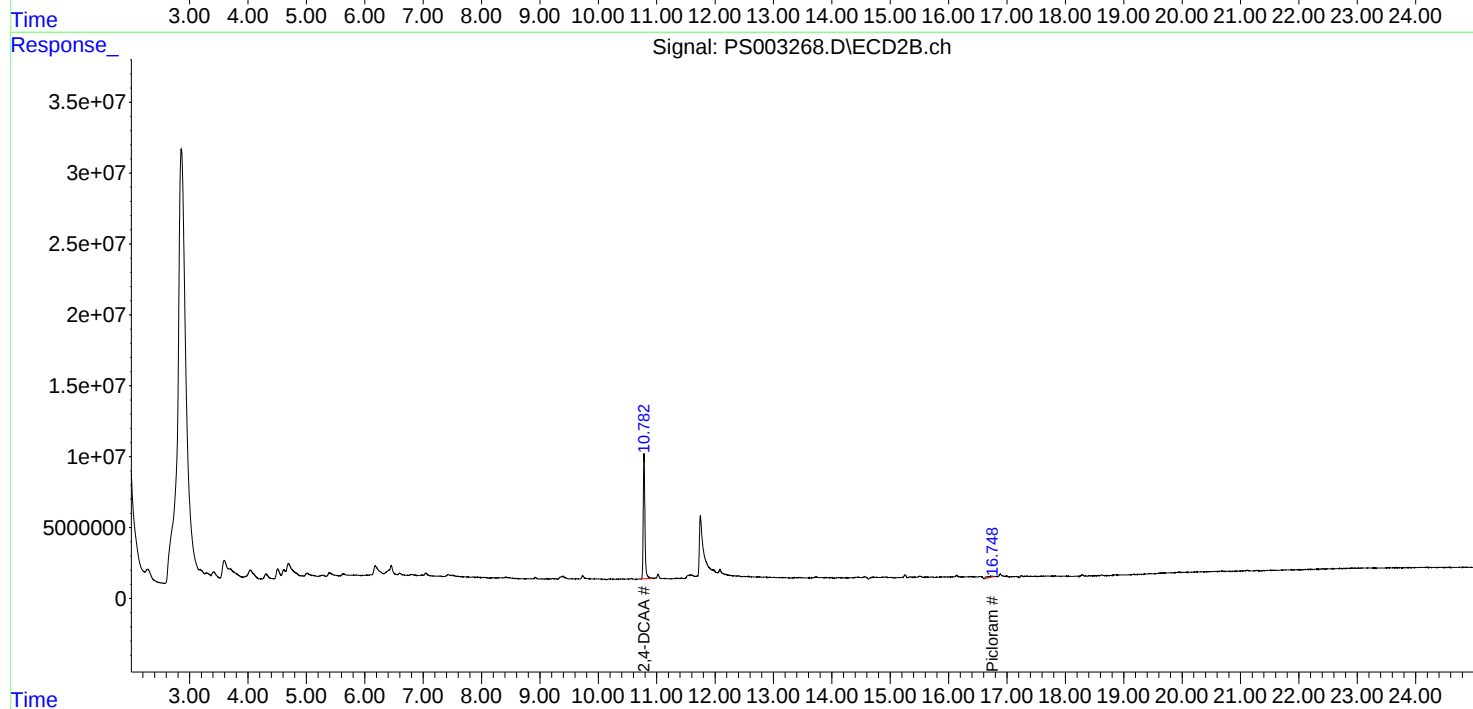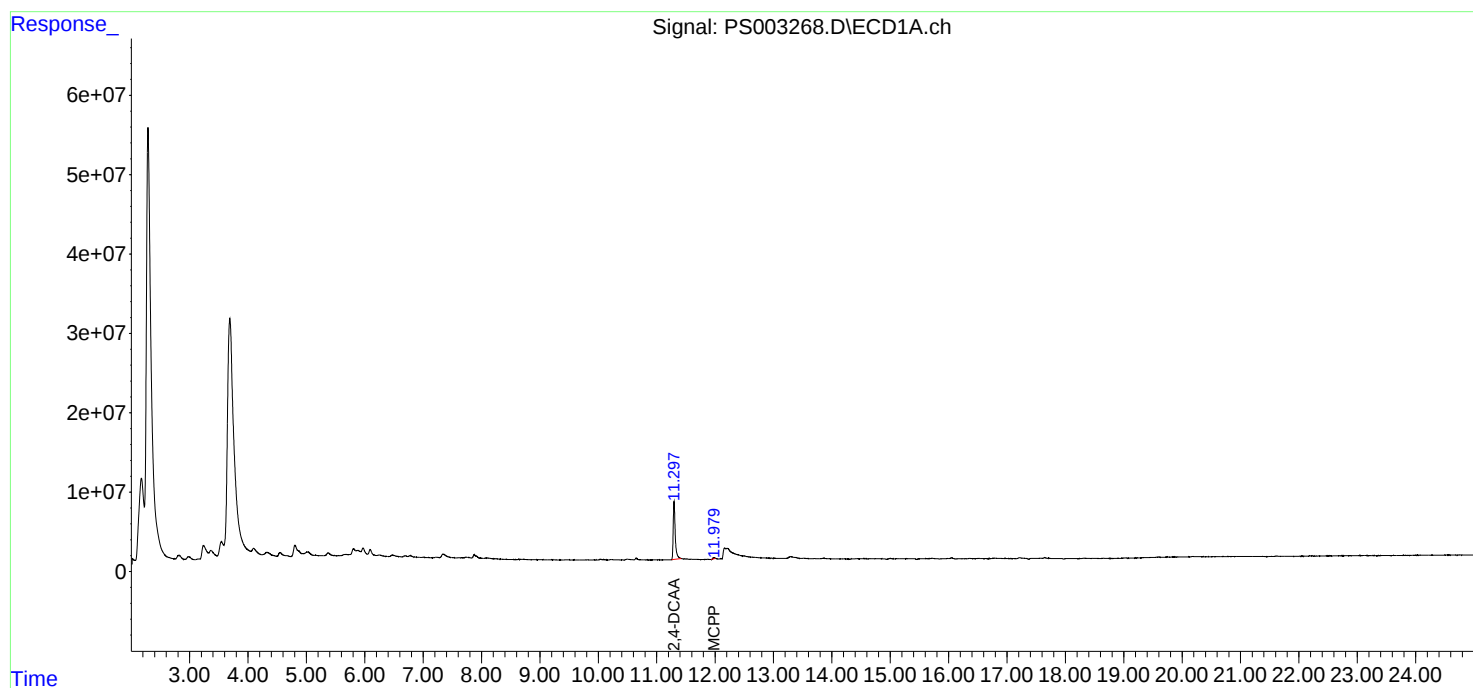


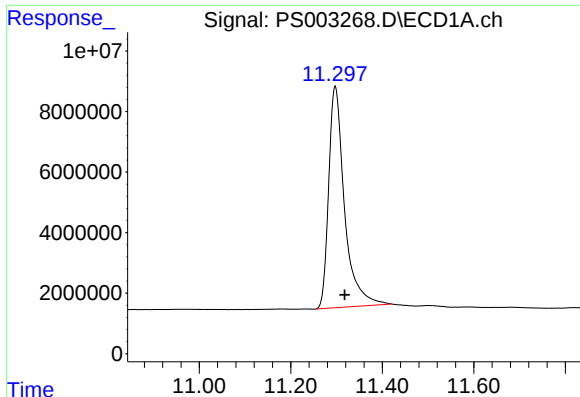

#4 2,4-DCAA


R.T.: 11.298 min  
Delta R.T.: -0.020 min  
Response: 175717483  
Conc: 462.85 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :  
CABLE-BRIDGE-FOUNDATION-D-7

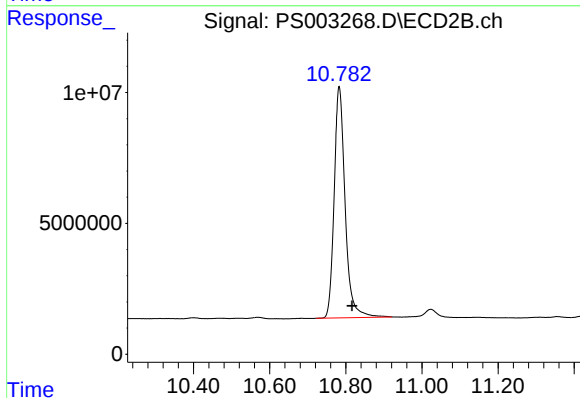


#4 2,4-DCAA

R.T.: 10.783 min  
Delta R.T.: -0.034 min  
Response: 177263944  
Conc: 414.61 ng/ml

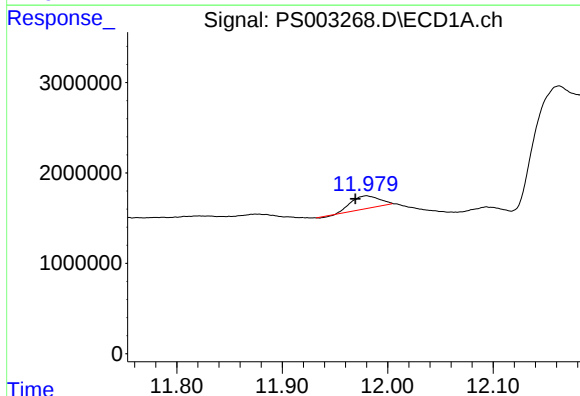


#6 MCP

R.T.: 11.981 min  
Delta R.T.: 0.011 min  
Response: 2868071  
Conc: 2.39 ug/ml

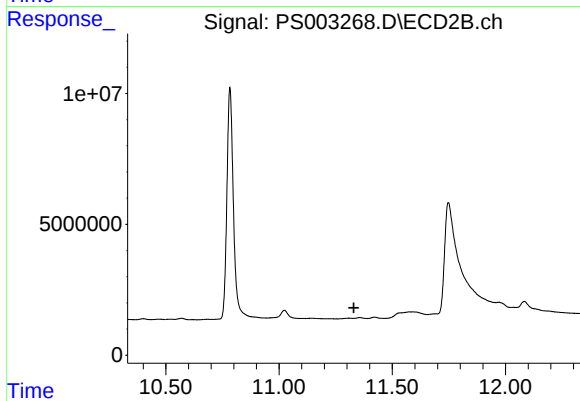

#6 MCP


R.T.: 0.000 min  
Exp R.T.: 11.330 min  
Response: 0  
Conc: N.D.

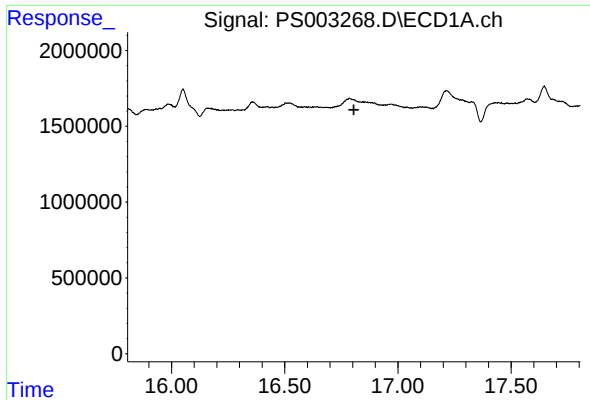

#15 Picloram

R.T.: 0.000 min  
Exp R.T.: 16.806 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :  
CABLE-BRIDGE-FOUNDATION-D-7

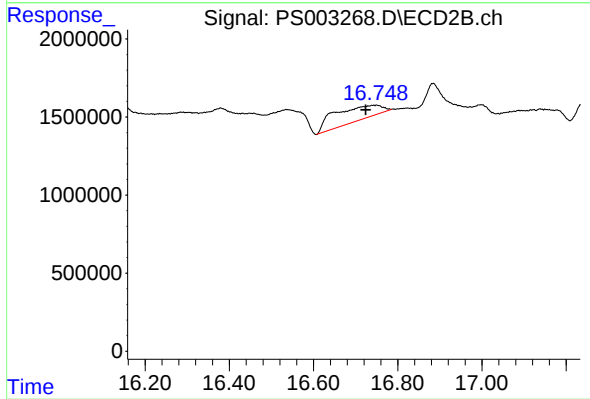

#15 Picloram

R.T.: 16.749 min  
Delta R.T.: 0.025 min  
Response: 7202372  
Conc: 2.40 ng/ml