

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021919\
 Data File : PS003270.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2019 01:21
 Operator : EI\SJ
 Sample : K1518-18
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-MH-C02

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 20 03:06:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	10.778	0	189.1E6	N.D.	442.377 #
Target Compounds							
6) T	MCP	11.960	0.000	6994678	0	5.838	N.D. #
14) T	DINOSEB	0.000	15.503	0	3272734	N.D.	1.867 #
15) T	Picloram	0.000	16.757	0	5864589	N.D.	1.951 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021919\
Data File : PS003270.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2019 01:21
Operator : EI\SJ
Sample : K1518-18
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-MH-C02

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 20 03:06:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

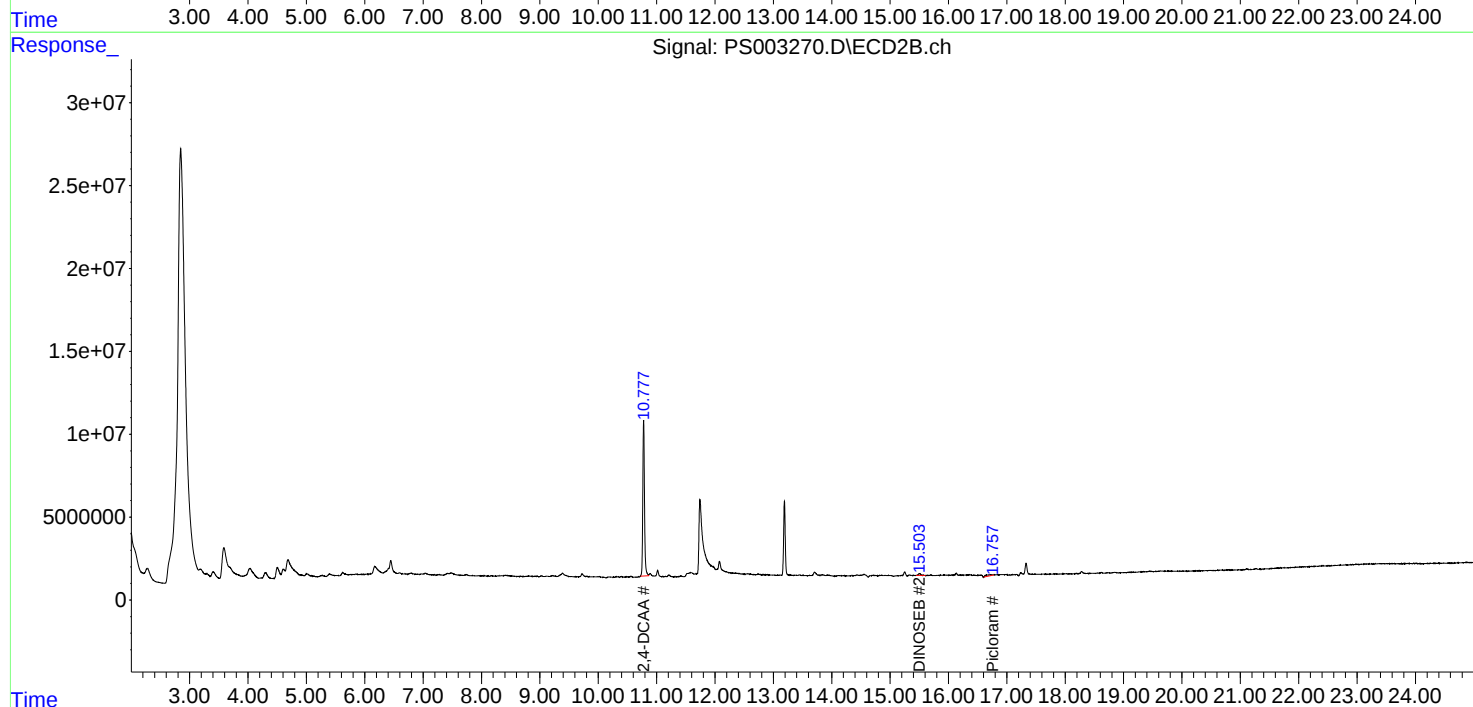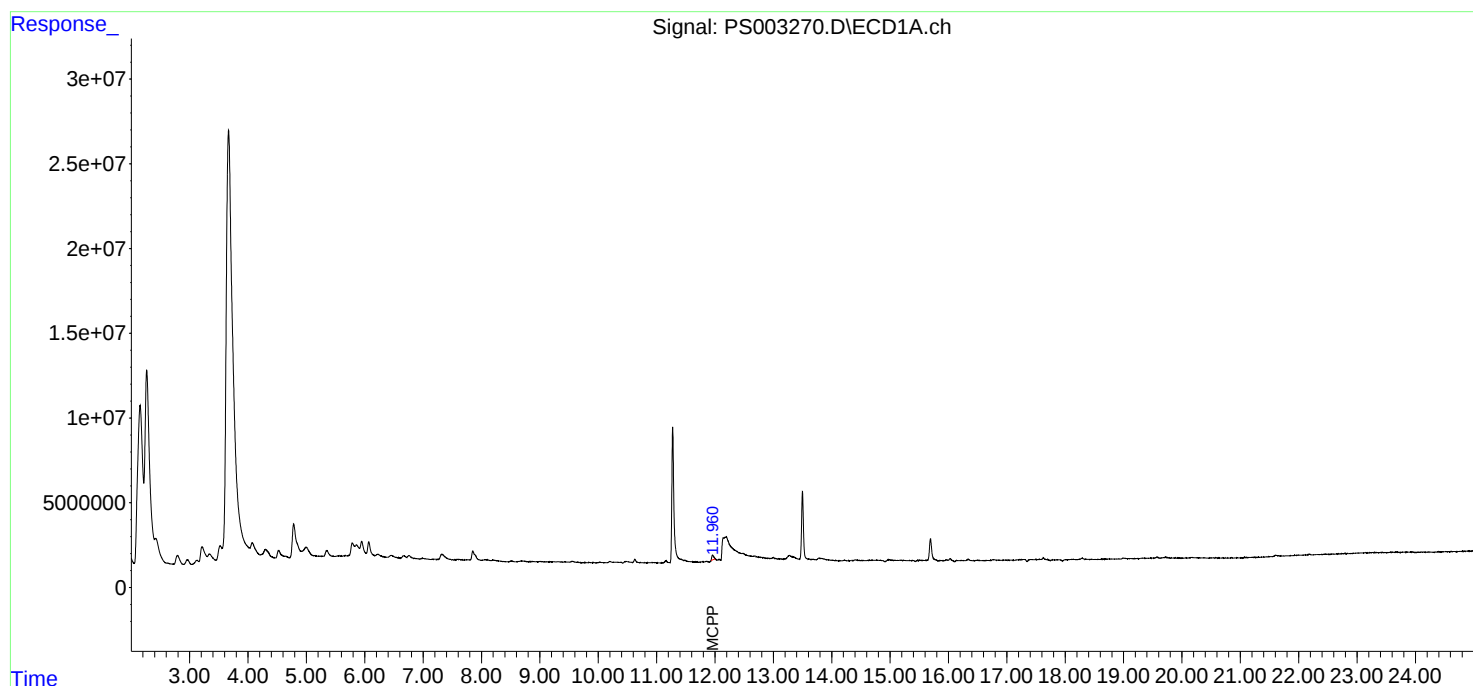


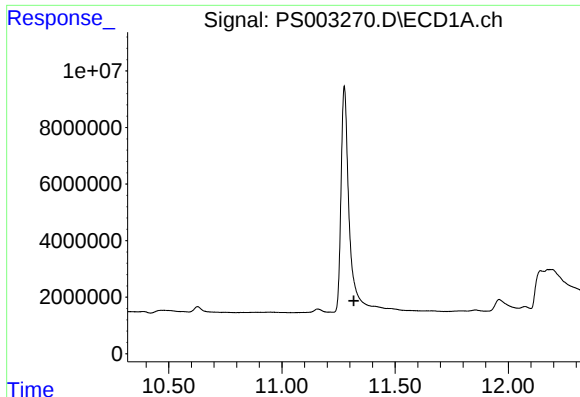

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 11.318 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-MH-C02

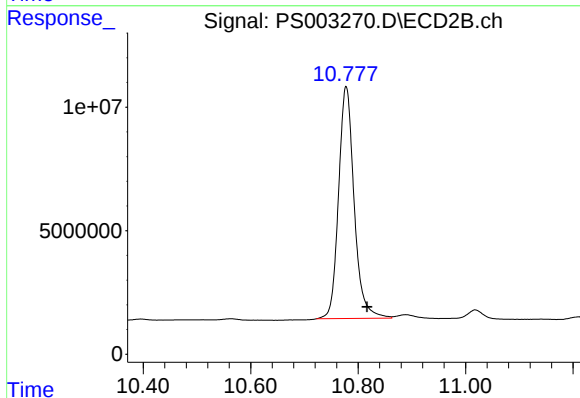


#4 2,4-DCAA

R.T.: 10.778 min
Delta R.T.: -0.039 min
Response: 189136362
Conc: 442.38 ng/ml

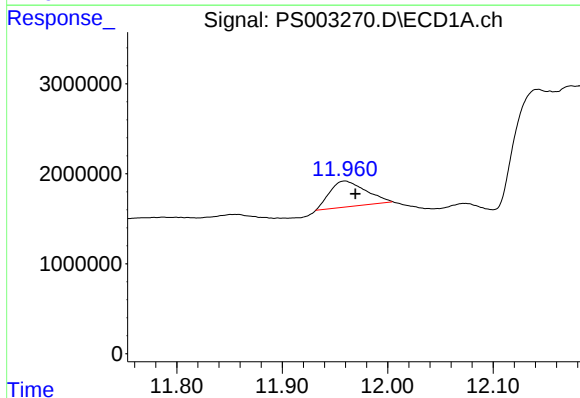


#6 MCP

R.T.: 11.960 min
Delta R.T.: -0.009 min
Response: 6994678
Conc: 5.84 ug/ml

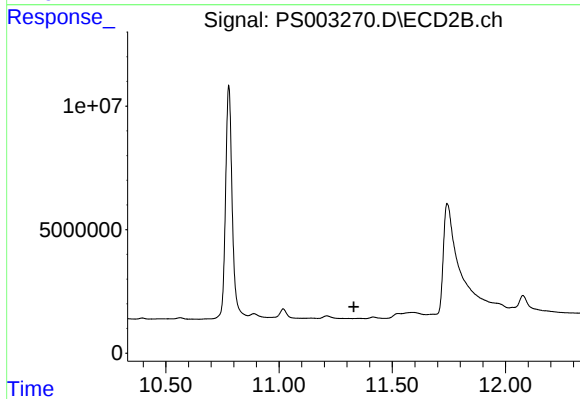

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.330 min
Response: 0
Conc: N.D.

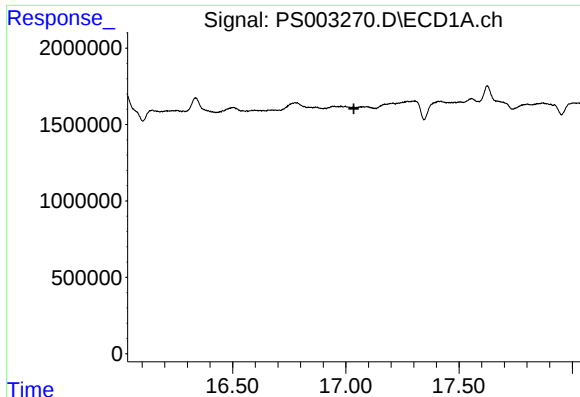

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-MH-C02

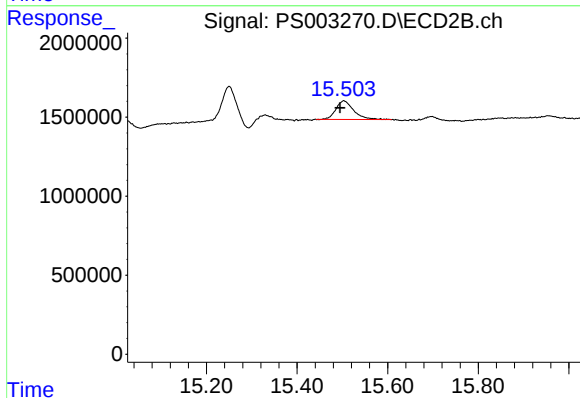


#14 DINOSEB

R.T.: 15.503 min
Delta R.T.: 0.008 min
Response: 3272734
Conc: 1.87 ng/ml

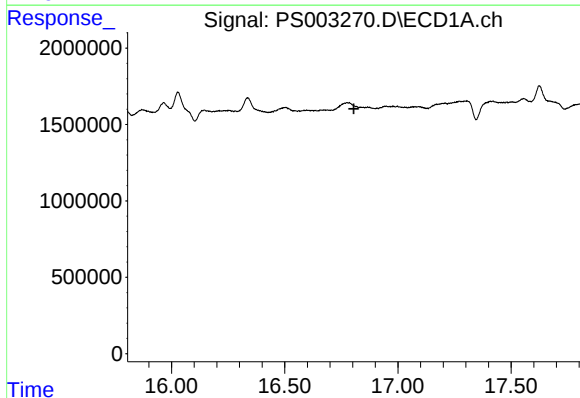

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.806 min
Response: 0
Conc: N.D.

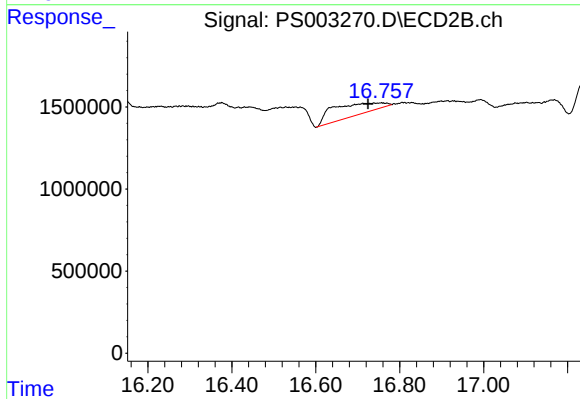

#15 Picloram

R.T.: 16.757 min
Delta R.T.: 0.032 min
Response: 5864589
Conc: 1.95 ng/ml