

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS021919\  
 Data File : PS003271.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 20 Feb 2019 01:52  
 Operator : EI\SJ  
 Sample : K1518-20  
 Misc :  
 ALS Vial : 18 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 TP-MH-C05

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Feb 20 03:07:03 2019  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS012819.M  
 Quant Title : 8080.M  
 QLast Update : Tue Jan 29 06:11:45 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound     | RT#1   | RT#2   | Resp#1   | Resp#2  | ng/ml   | ng/ml   |
|-----------------------------|--------------|--------|--------|----------|---------|---------|---------|
| -----                       |              |        |        |          |         |         |         |
| System Monitoring Compounds |              |        |        |          |         |         |         |
| 4) S                        | 2,4-DCAA     | 11.291 | 10.793 | 186.6E6  | 191.9E6 | 491.561 | 448.734 |
| Target Compounds            |              |        |        |          |         |         |         |
| 1) T                        | Dalapon      | 0.000  | 2.291  | 0        | 2509131 | N.D.    | 4.682 # |
| 5) T                        | DICAMBA      | 0.000  | 11.147 | 0        | 559652  | N.D.    | 0.353 # |
| 6) T                        | MCP          | 11.974 | 0.000  | 6248283  | 0       | 5.215   | N.D. #  |
| 11) T                       | 2,4,5-TP ... | 14.392 | 0.000  | 16432453 | 0       | 6.525   | N.D. #  |
| 15) T                       | Picloram     | 0.000  | 16.729 | 0        | 6622490 | N.D.    | 2.203 # |
| 16) T                       | DCPA         | 0.000  | 16.729 | 0        | 6622490 | N.D.    | 2.138 # |
| -----                       |              |        |        |          |         |         |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS021919\  
Data File : PS003271.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 20 Feb 2019 01:52  
Operator : EI\SJ  
Sample : K1518-20  
Misc :  
ALS Vial : 18 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :  
TP-MH-C05

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Feb 20 03:07:03 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS012819.M  
Quant Title : 8080.M  
QLast Update : Tue Jan 29 06:11:45 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

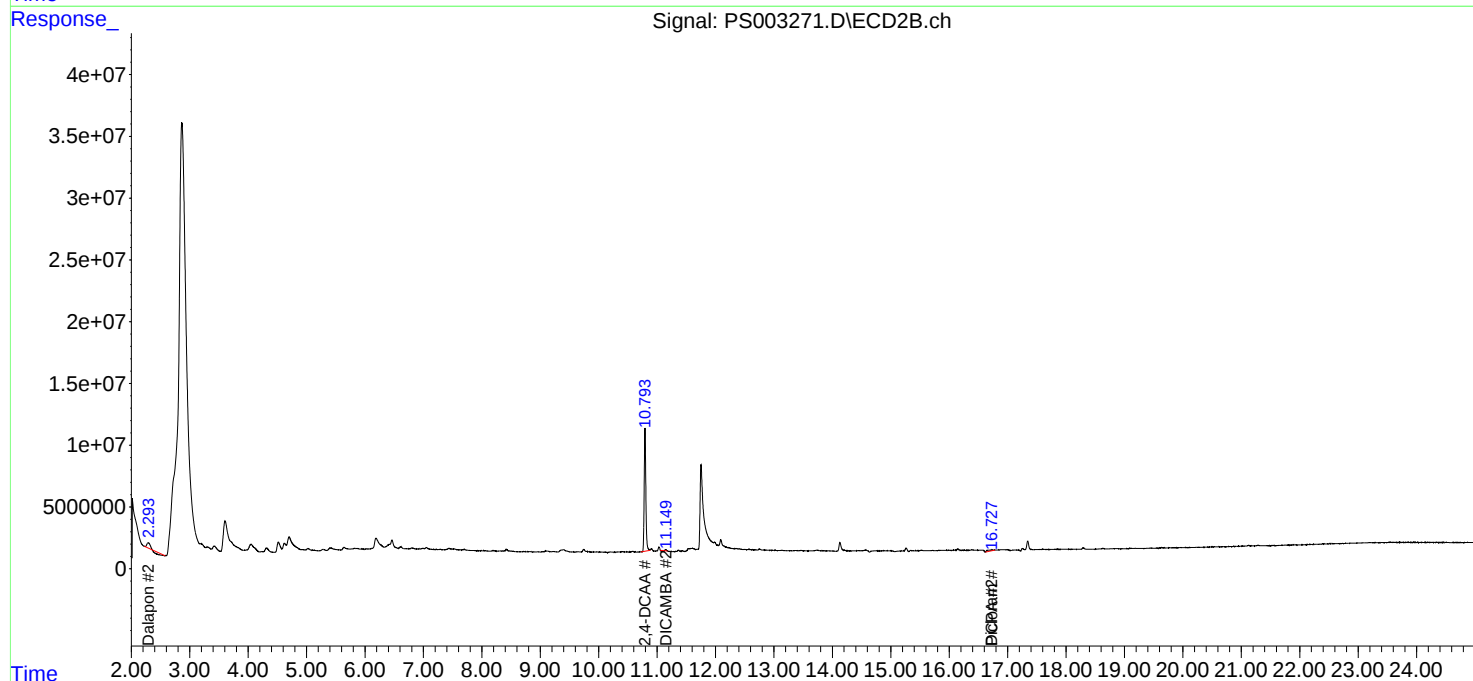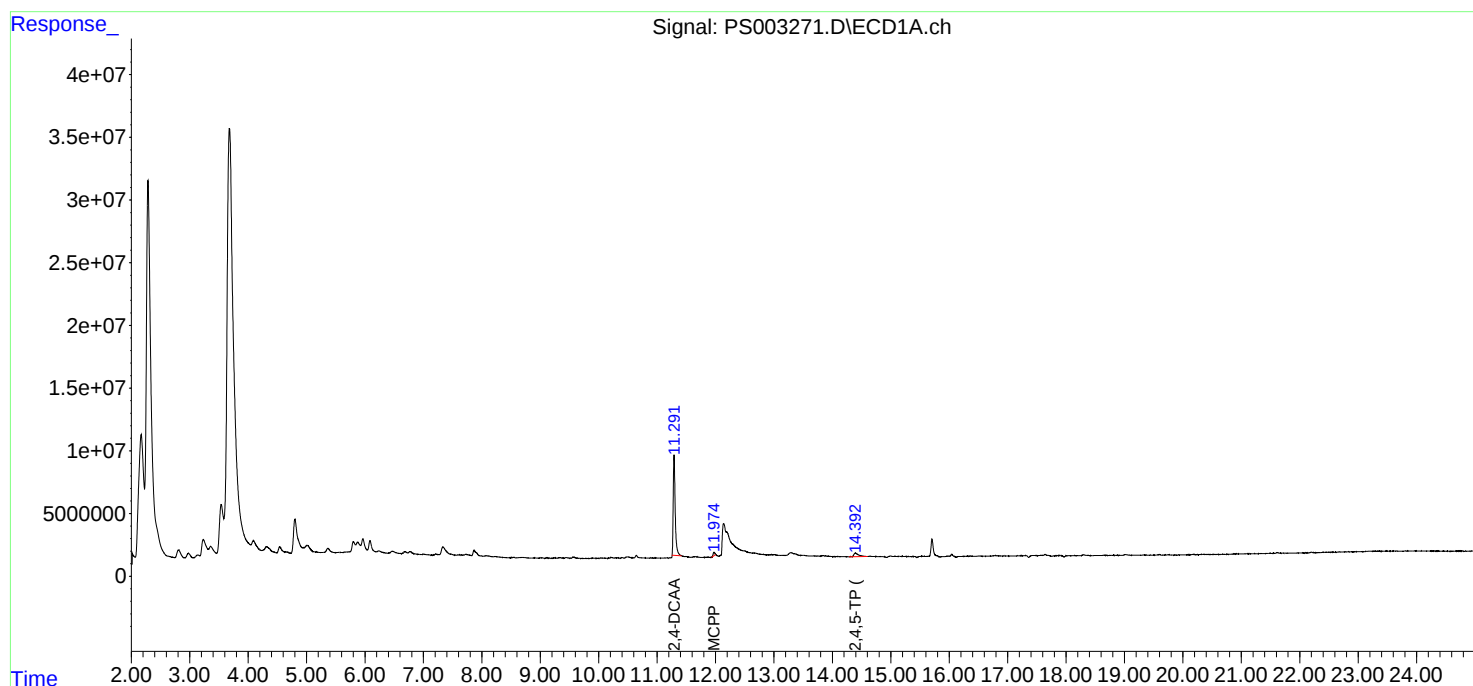


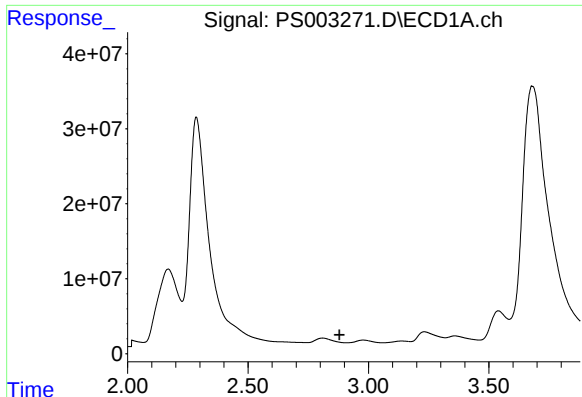

#1 Dalapon


R.T.: 0.000 min  
Exp R.T.: 2.880 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :  
TP-MH-C05

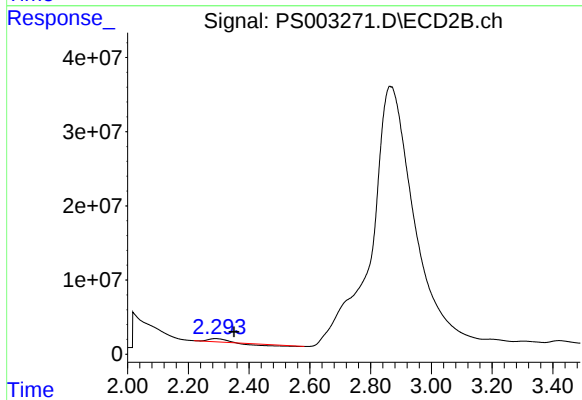


#1 Dalapon

R.T.: 2.291 min  
Delta R.T.: -0.059 min  
Response: 2509131  
Conc: 4.68 ng/ml

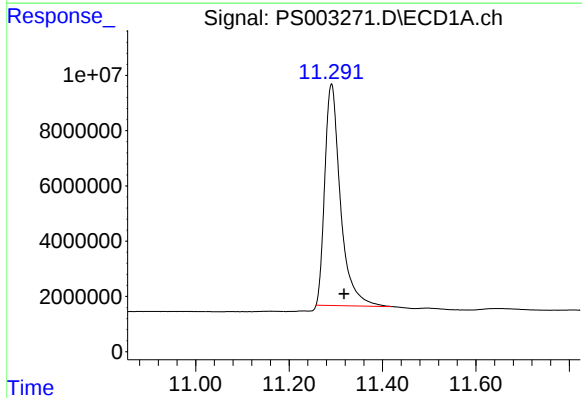


#4 2,4-DCAA

R.T.: 11.291 min  
Delta R.T.: -0.027 min  
Response: 186616647  
Conc: 491.56 ng/ml

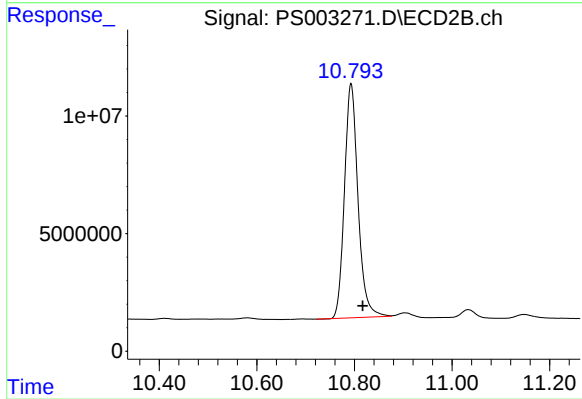

#4 2,4-DCAA


R.T.: 10.793 min  
Delta R.T.: -0.024 min  
Response: 191854347  
Conc: 448.73 ng/ml

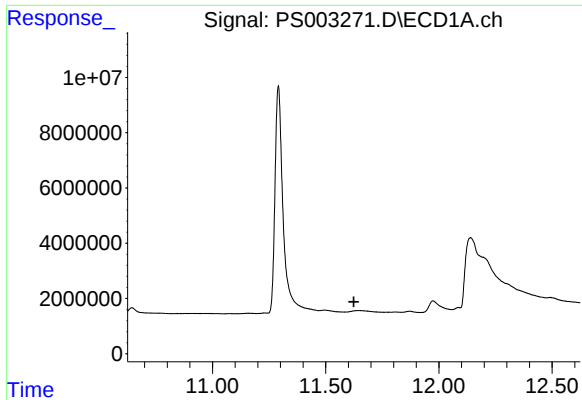

#5 DICAMBA


R.T.: 0.000 min  
Exp R.T.: 11.624 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :  
TP-MH-C05

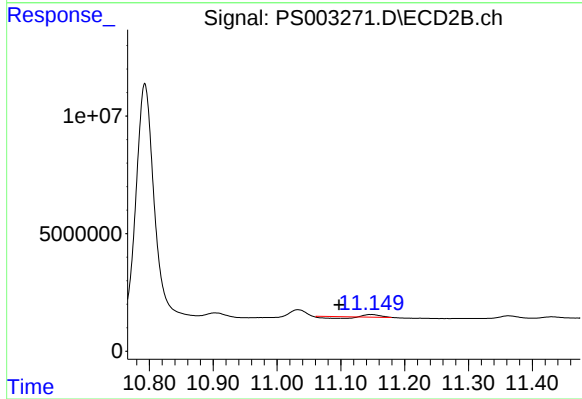


#5 DICAMBA

R.T.: 11.147 min  
Delta R.T.: 0.050 min  
Response: 559652  
Conc: 0.35 ng/ml

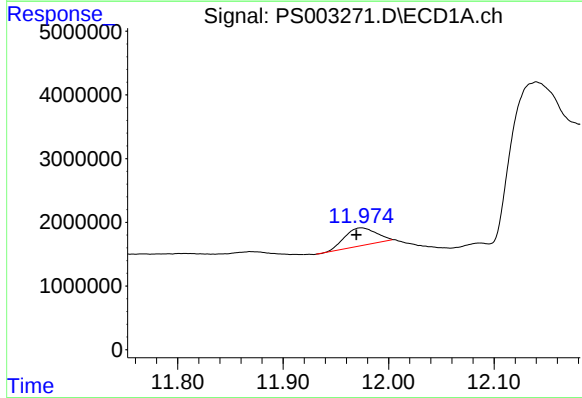


#6 MCP

R.T.: 11.974 min  
Delta R.T.: 0.005 min  
Response: 6248283  
Conc: 5.22 ug/ml

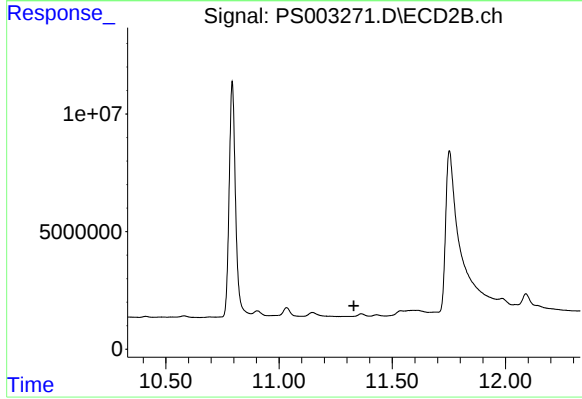

#6 MCP


R.T.: 0.000 min  
Exp R.T.: 11.330 min  
Response: 0  
Conc: N.D.

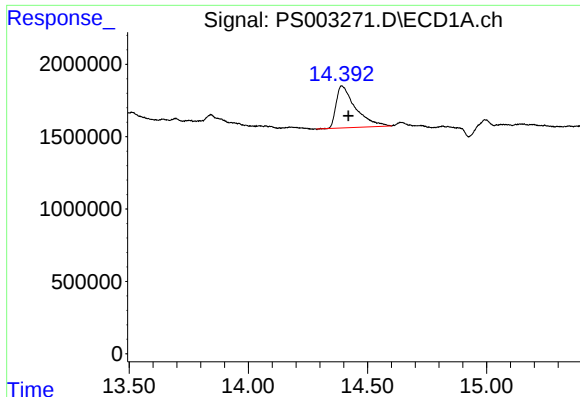

#11 2,4,5-TP (SILVEX)


R.T.: 14.392 min  
Delta R.T.: -0.028 min  
Response: 16432453  
Conc: 6.53 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :  
TP-MH-C05

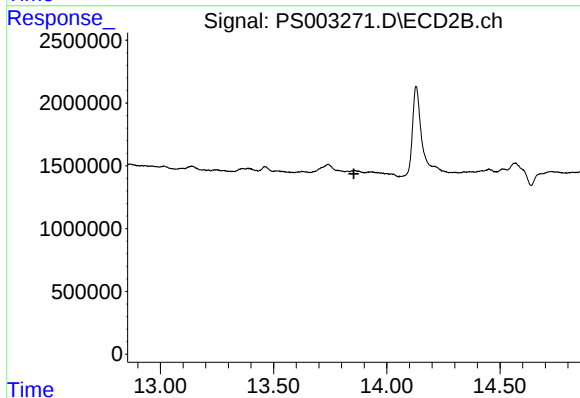


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min  
Exp R.T. : 13.854 min  
Response: 0  
Conc: N.D.

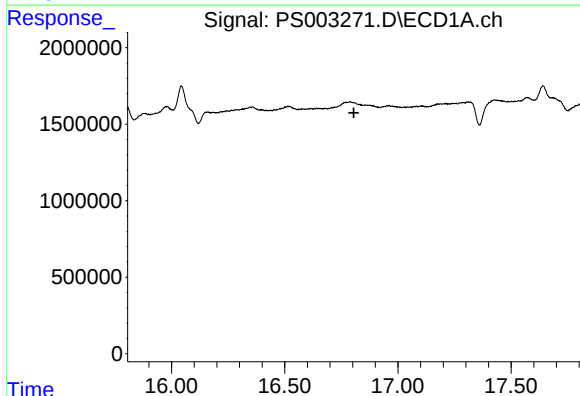


#15 Picloram

R.T.: 0.000 min  
Exp R.T. : 16.806 min  
Response: 0  
Conc: N.D.

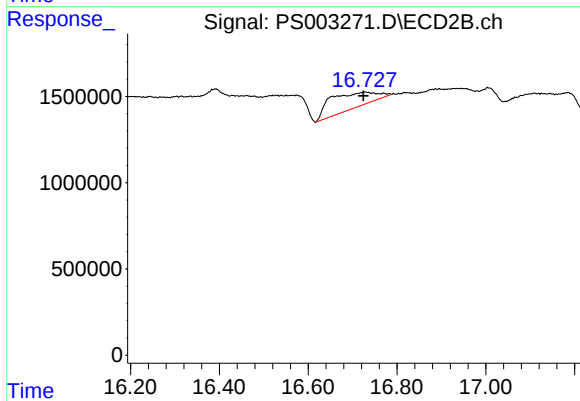

#15 Picloram


R.T.: 16.729 min  
Delta R.T.: 0.005 min  
Response: 6622490  
Conc: 2.20 ng/ml

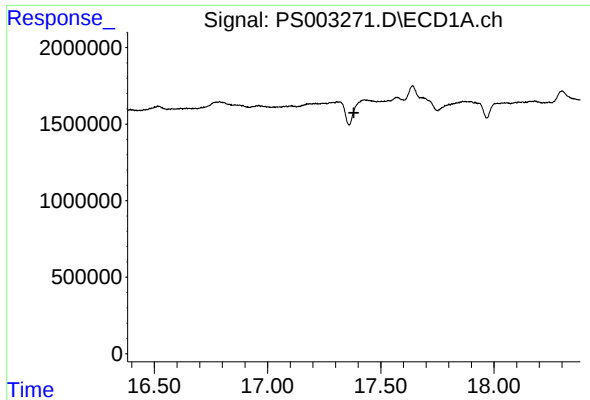

#16 DCPA

R.T.: 0.000 min  
Exp R.T.: 17.382 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :  
TP-MH-C05

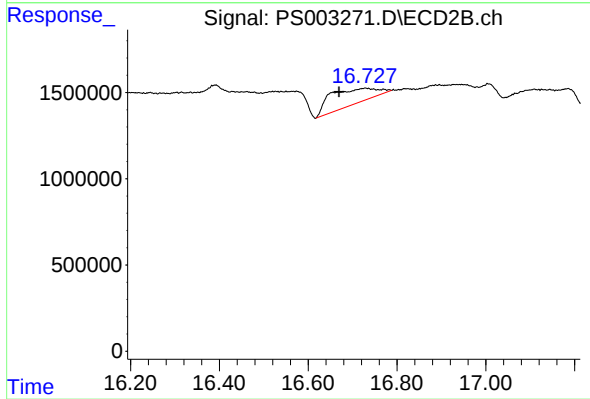

#16 DCPA

R.T.: 16.729 min  
Delta R.T.: 0.059 min  
Response: 6622490  
Conc: 2.14 ng/ml