

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021919\
 Data File : PS003274.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2019 03:25
 Operator : EI\SJ
 Sample : K1525-04
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 M-14-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 20 05:34:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.275	10.777	59646987	201.4E6	157.114	470.967 #
Target Compounds							
6) T	MCCP	11.957	0.000	5398910	0	4.506	N.D. #
14) T	DINOSEB	0.000	15.501	0	4749375	N.D.	2.709 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021919\
Data File : PS003274.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2019 03:25
Operator : EI\SJ
Sample : K1525-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
M-14-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 20 05:34:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

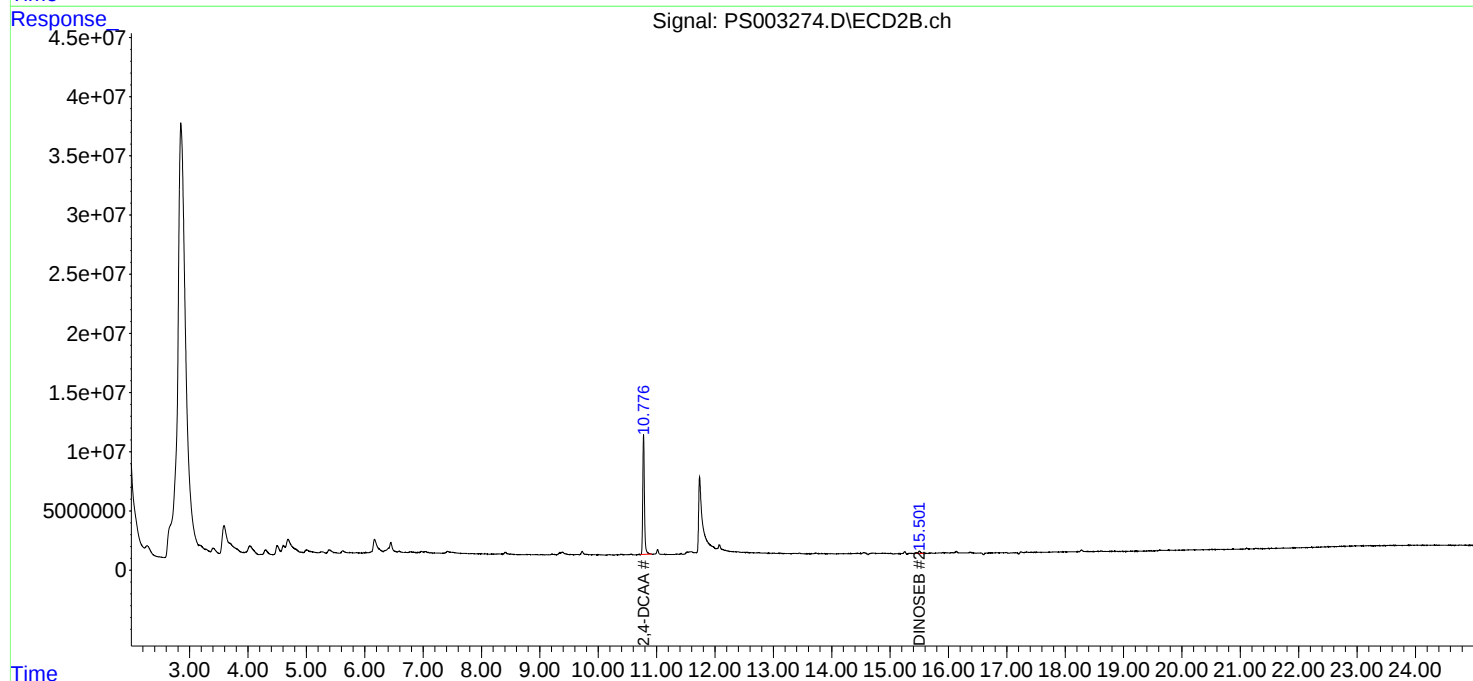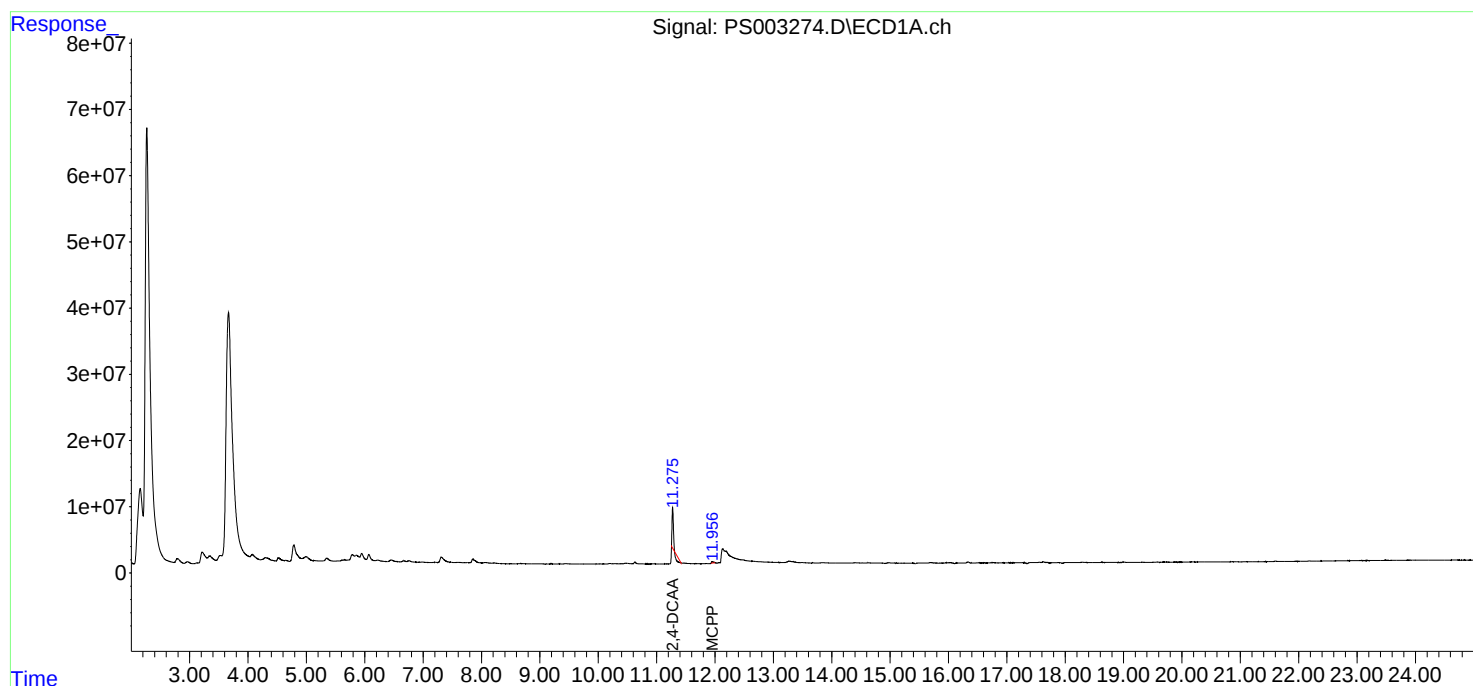


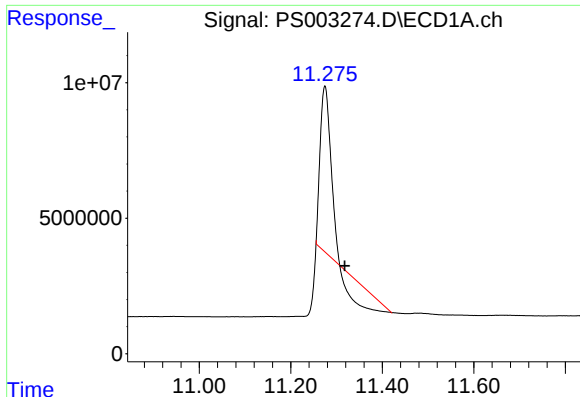

#4 2,4-DCAA


R.T.: 11.275 min
Delta R.T.: -0.043 min
Response: 59646987
Conc: 157.11 ng/ml

Instrument :
ECD_S
ClientSampleId :
M-14-S

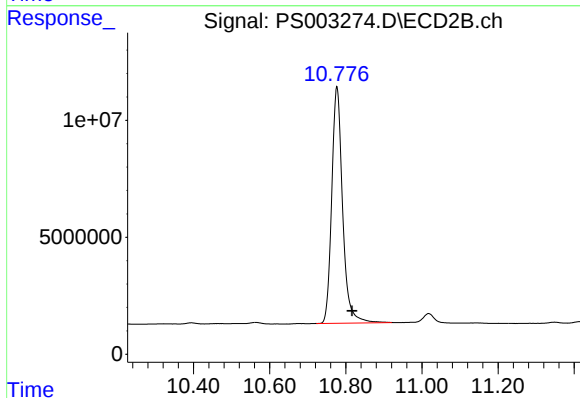


#4 2,4-DCAA

R.T.: 10.777 min
Delta R.T.: -0.040 min
Response: 201359936
Conc: 470.97 ng/ml

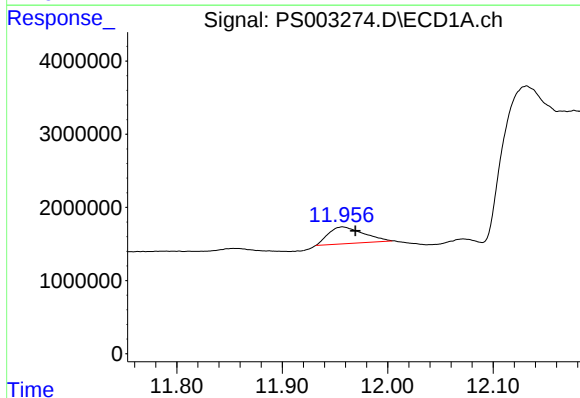


#6 MCP

R.T.: 11.957 min
Delta R.T.: -0.012 min
Response: 5398910
Conc: 4.51 ug/ml

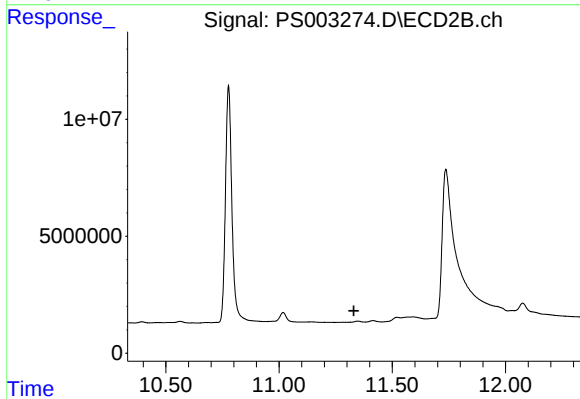

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.330 min
Response: 0
Conc: N.D.

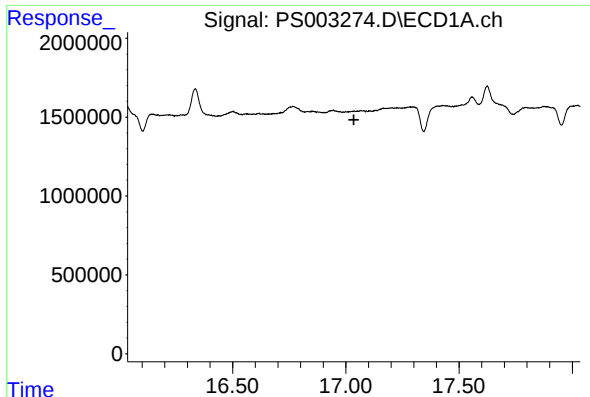

#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 17.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
M-14-S

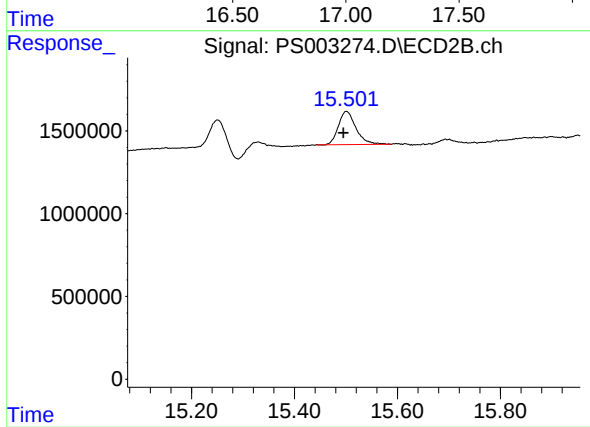

#14 DINOSEB

R.T.: 15.501 min
Delta R.T.: 0.006 min
Response: 4749375
Conc: 2.71 ng/ml