

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021924\
Data File : PS025997.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Feb 2024 20:56
Operator : AR\AJ
Sample : P1514-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
ETGI-343

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/20/2024
Supervised By :Ankita Jodhani 02/20/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 20 00:36:39 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS021424.M
Quant Title : 8080.M
QLast Update : Wed Feb 14 15:17:36 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.268	7.800	882.8E6	263.0E6	333.580m	301.291m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021924\
Data File : PS025997.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Feb 2024 20:56
Operator : AR\AJ
Sample : P1514-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
ETGI-343


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/20/2024
Supervised By : Ankita Jodhani 02/20/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 20 00:36:39 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS021424.M
Quant Title : 8080.M
QLast Update : Wed Feb 14 15:17:36 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

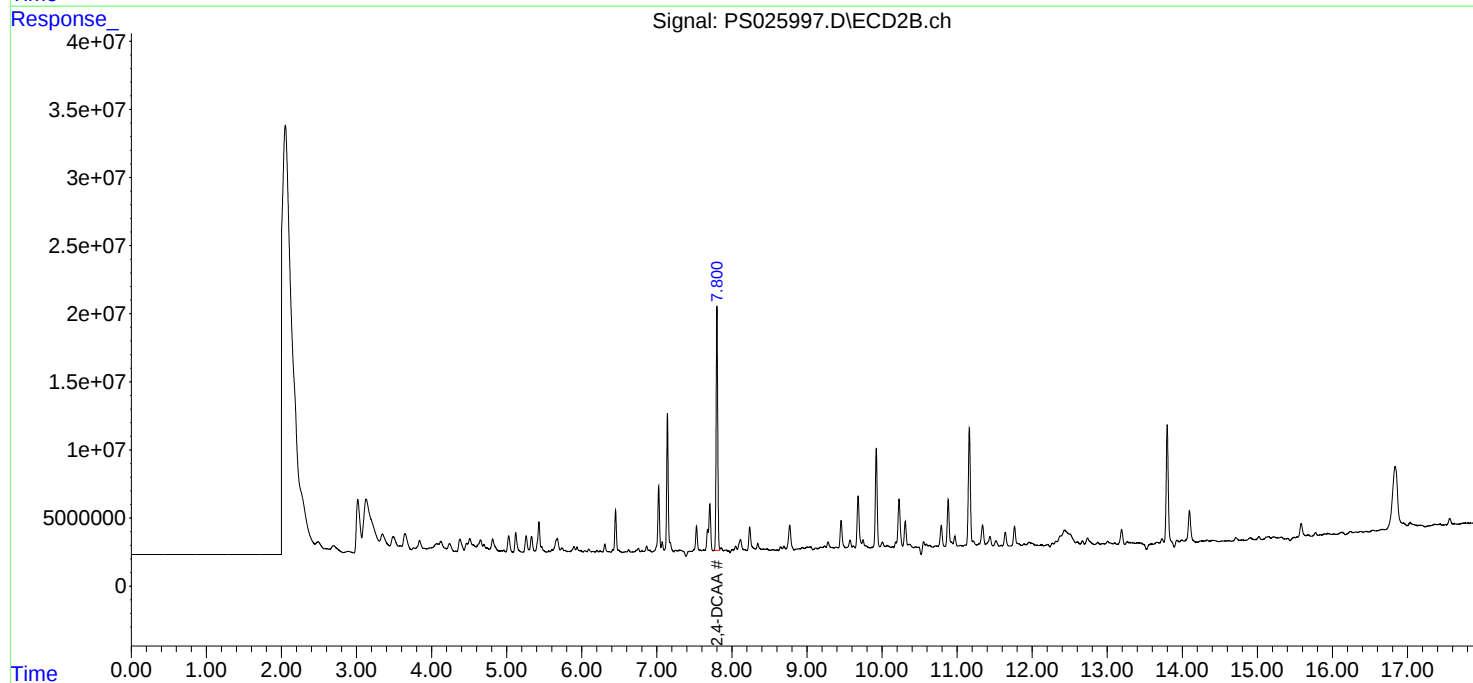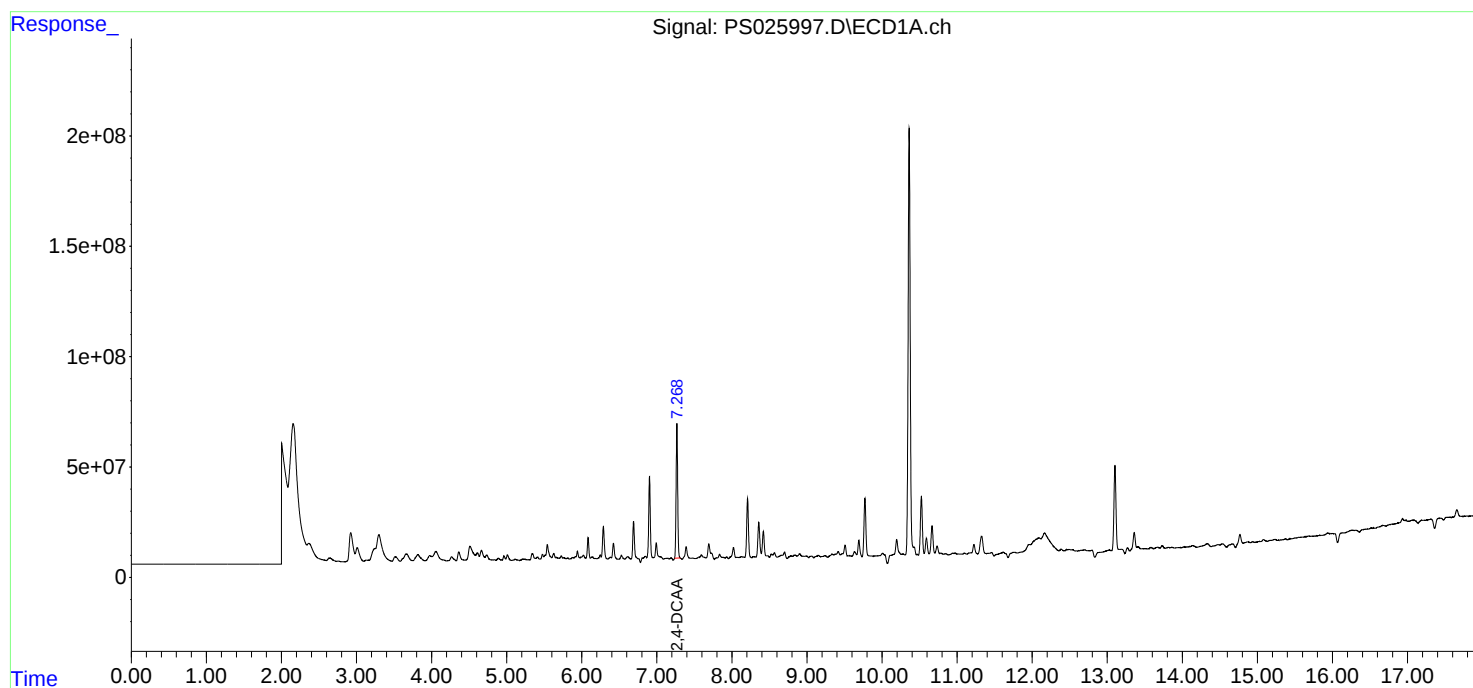

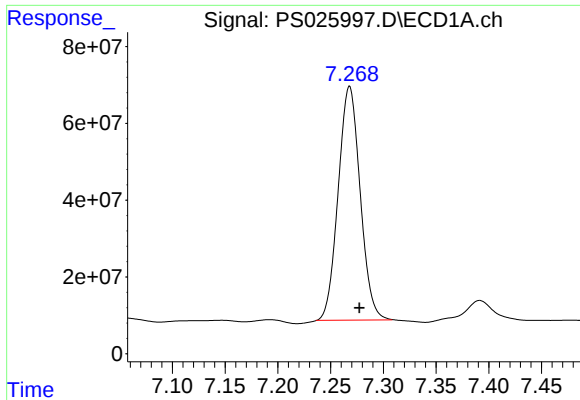


#4 2,4-DCAA

R.T.: 7.268 min
Delta R.T.: -0.010 min
Response: 882843757
Conc: 333.58 ng/ml

Instrument :
ECD_S
ClientSampleId :
ETGI-343

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/20/2024
Supervised By :Ankita Jodhani 02/20/2024

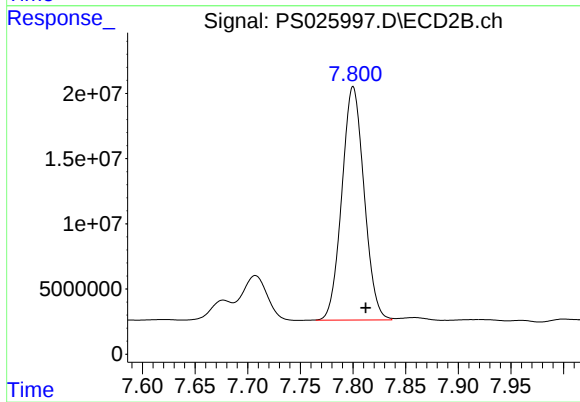

#4 2,4-DCAA

R.T.: 7.800 min
Delta R.T.: -0.012 min
Response: 262982313
Conc: 301.29 ng/ml m