

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022019\
 Data File : PS003279.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2019 12:35
 Operator : EI\SJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 20 21:56:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.282	10.783	237.3E6	319.5E6	625.052	747.325
Target Compounds							
1) T	Dalapon	2.846	2.316	147.3E6	376.2E6	266.971	701.949 #
2) T	3,5-DICHL...	0.000	8.943	0	182.5E6	N.D.	323.770 #
3) T	4-Nitroph...	10.879	9.934	115.0E6	146.4E6	594.351	700.544
5) T	DICAMBA	0.000	11.062	0	420.2E6	N.D.	264.830 #
8) T	DICHLORPROP	0.000	12.188	0	274.4E6	N.D.	717.712 #
9) T	2,4-D	0.000	12.661	0	298.7E6	N.D.	595.807 #
10) T	Pentachlo...	0.000	13.193	0	603.5E6	N.D.	97.649 #
11) T	2,4,5-TP ...	14.379	13.820	1863.5E6	1784.2E6	739.960	719.352
12) T	2,4,5-T	14.781	14.384	1783.2E6	1101.4E6	731.005	575.585
14) T	DINOSEB	16.990	15.459	1422.7E6	-499261936	756.239	N.D. #
15) T	Picloram	16.771	16.692	1950.7E6	1823.2E6	616.589	606.453
16) T	DCPA	0.000	16.692	0	1823.2E6	N.D.	588.600 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022019\
Data File : PS003279.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2019 12:35
Operator : EI\SJ
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 20 21:56:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

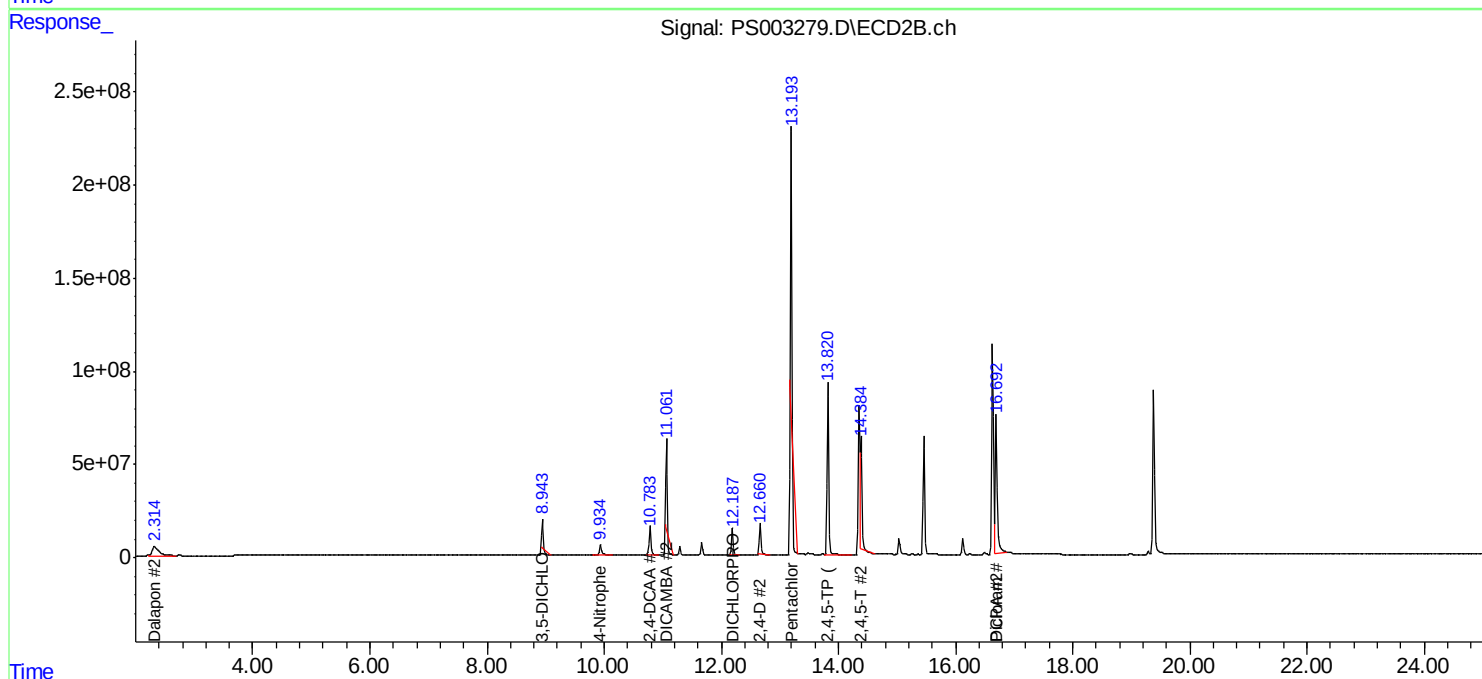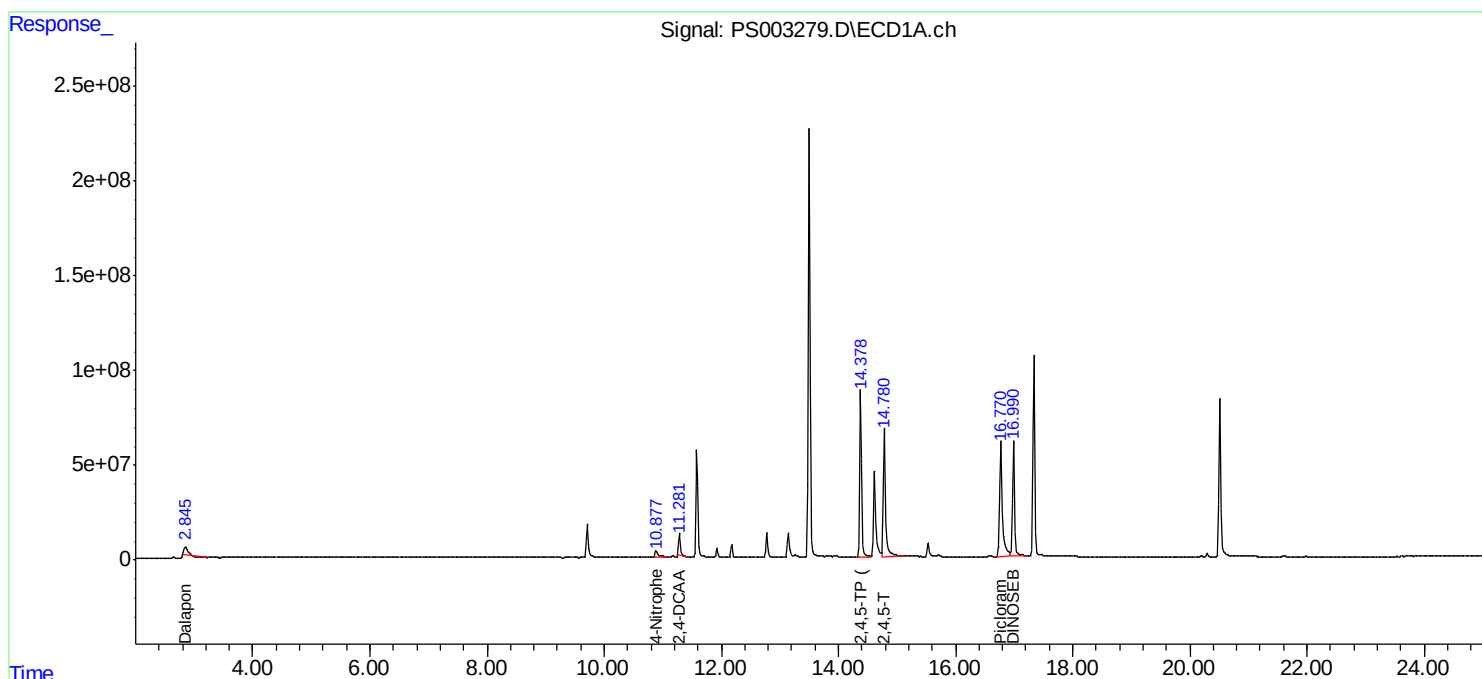


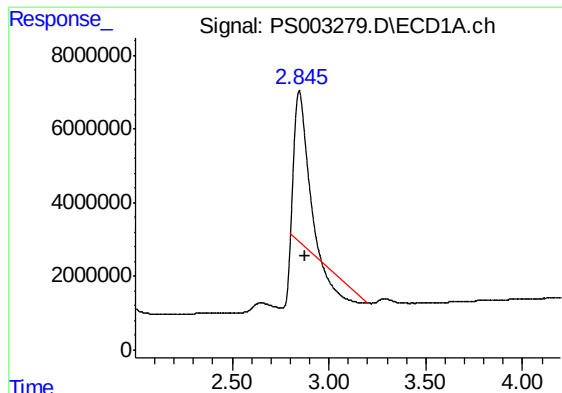

#1 Dalapon


R.T.: 2.846 min
Delta R.T.: -0.034 min
Response: 147274073
Conc: 266.97 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

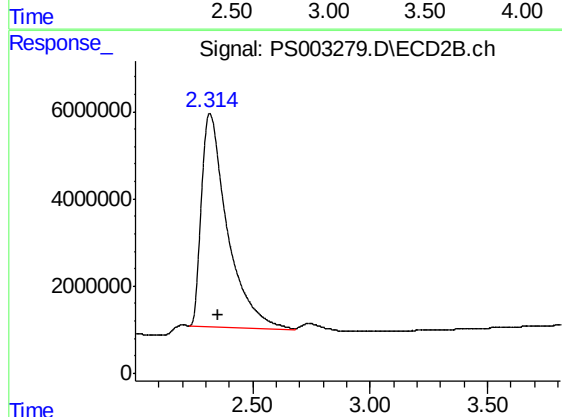


#1 Dalapon

R.T.: 2.316 min
Delta R.T.: -0.035 min
Response: 376189198
Conc: 701.95 ng/ml

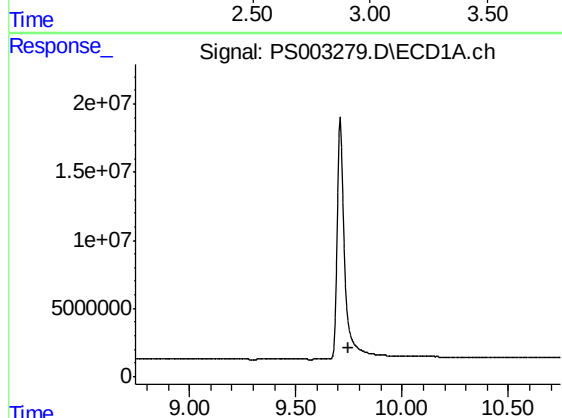


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.745 min
Response: 0
Conc: N.D.

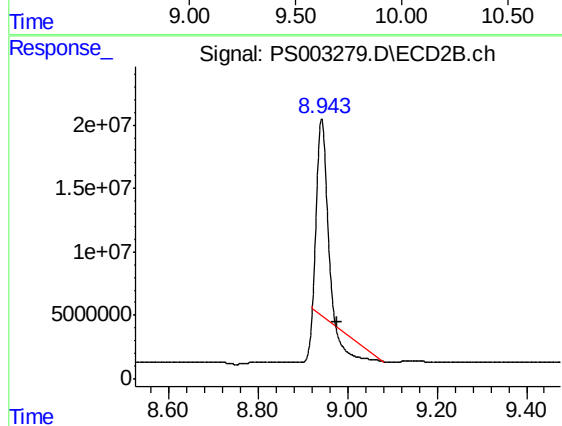

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.943 min
Delta R.T.: -0.034 min
Response: 182466223
Conc: 323.77 ng/ml

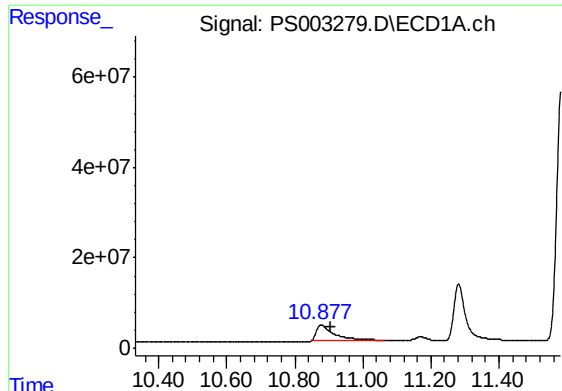

#3 4-Nitrophenol


R.T.: 10.879 min
Delta R.T.: -0.025 min
Response: 115030146
Conc: 594.35 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

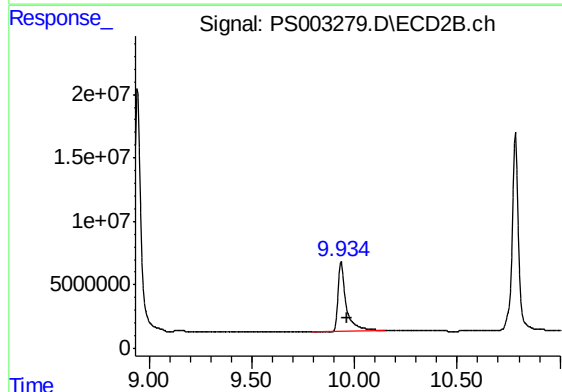


#3 4-Nitrophenol

R.T.: 9.934 min
Delta R.T.: -0.031 min
Response: 146429348
Conc: 700.54 ng/ml

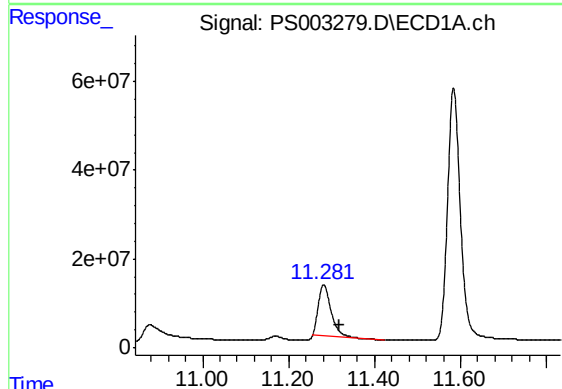


#4 2,4-DCAA

R.T.: 11.282 min
Delta R.T.: -0.036 min
Response: 237295369
Conc: 625.05 ng/ml

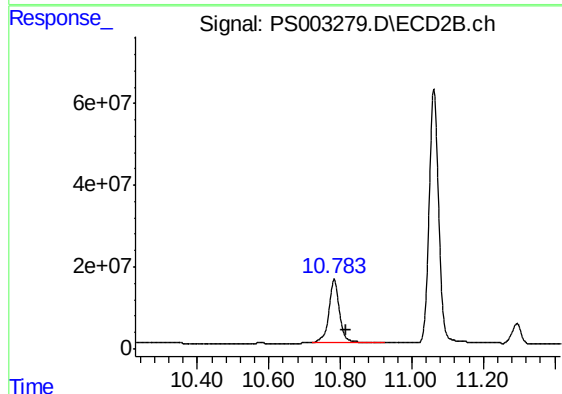

#4 2,4-DCAA


R.T.: 10.783 min
Delta R.T.: -0.034 min
Response: 319515628
Conc: 747.33 ng/ml

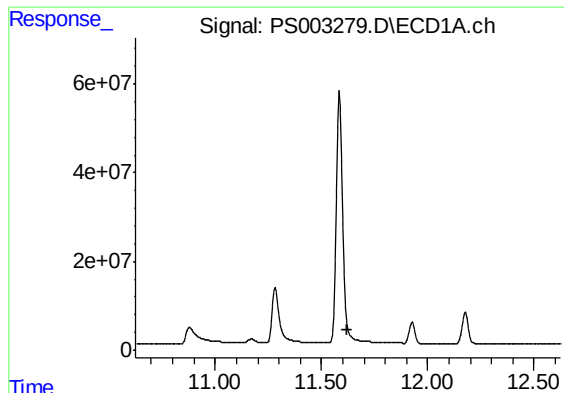

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.624 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

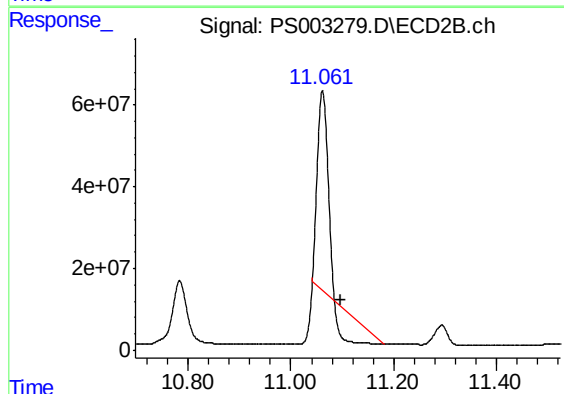


#5 DICAMBA

R.T.: 11.062 min
Delta R.T.: -0.035 min
Response: 420197196
Conc: 264.83 ng/ml

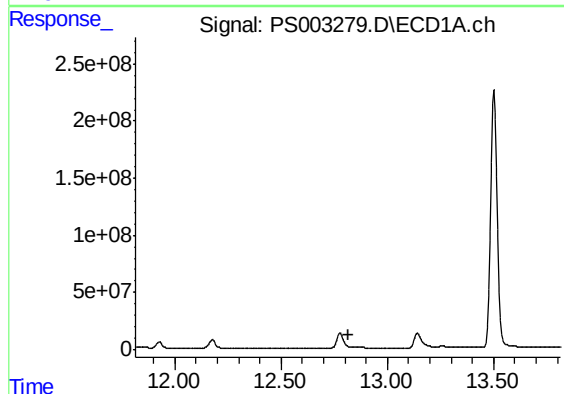


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 12.815 min
Response: 0
Conc: N.D.

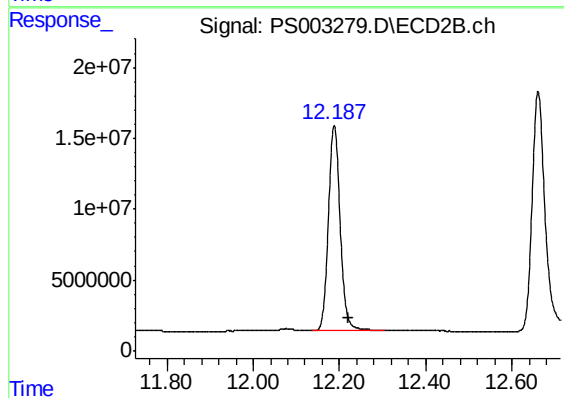

#8 DICHLORPROP


R.T.: 12.188 min
Delta R.T.: -0.034 min
Response: 274410997
Conc: 717.71 ng/ml

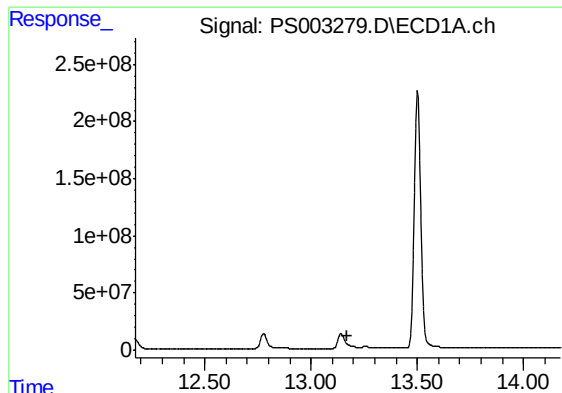

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.173 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

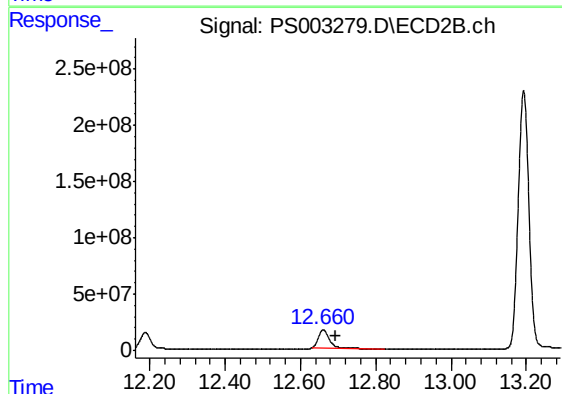


#9 2,4-D

R.T.: 12.661 min
Delta R.T.: -0.032 min
Response: 298729229
Conc: 595.81 ng/ml

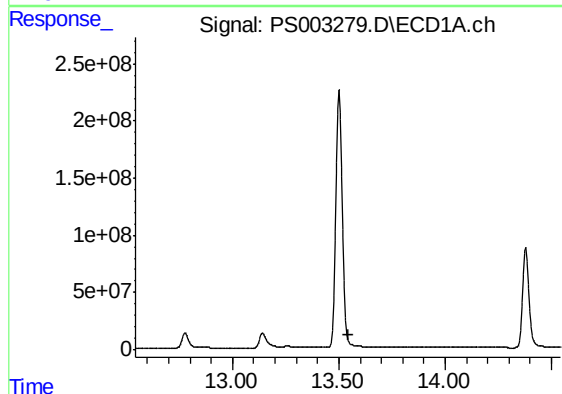


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 13.543 min
Response: 0
Conc: N.D.

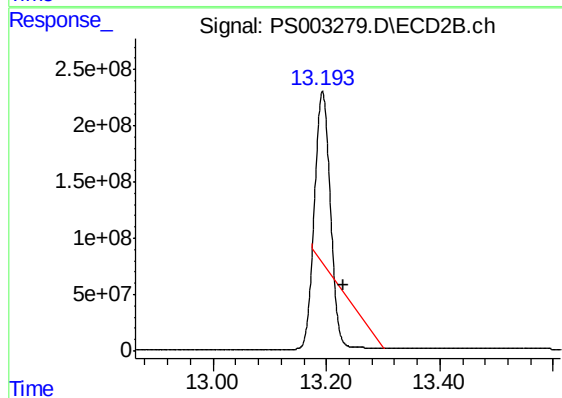

#10 Pentachlorophenol


R.T.: 13.193 min
Delta R.T.: -0.036 min
Response: 603532491
Conc: 97.65 ng/ml

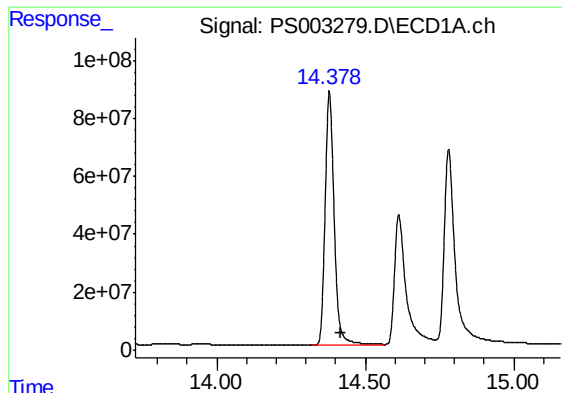

#11 2,4,5-TP (SILVEX)


R.T.: 14.379 min
Delta R.T.: -0.040 min
Response: 1863495157
Conc: 739.96 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

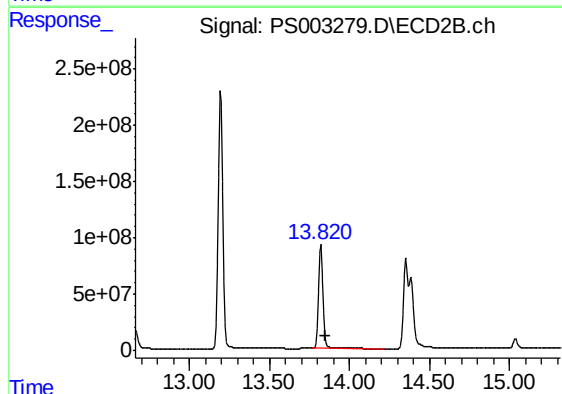


#11 2,4,5-TP (SILVEX)

R.T.: 13.820 min
Delta R.T.: -0.034 min
Response: 1784249790
Conc: 719.35 ng/ml

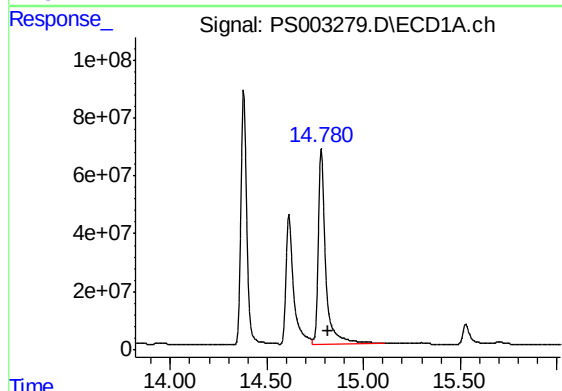


#12 2,4,5-T

R.T.: 14.781 min
Delta R.T.: -0.036 min
Response: 1783217596
Conc: 731.01 ng/ml

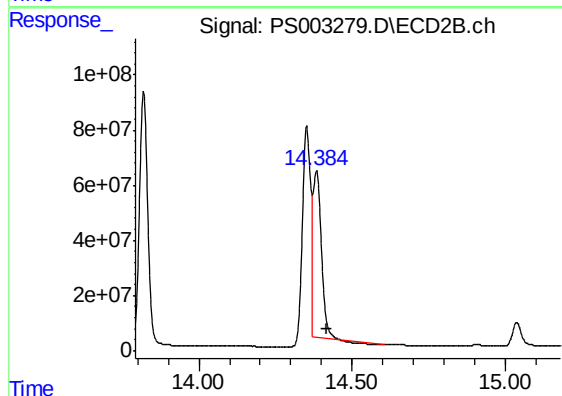

#12 2,4,5-T


R.T.: 14.384 min
Delta R.T.: -0.033 min
Response: 1101376147
Conc: 575.59 ng/ml

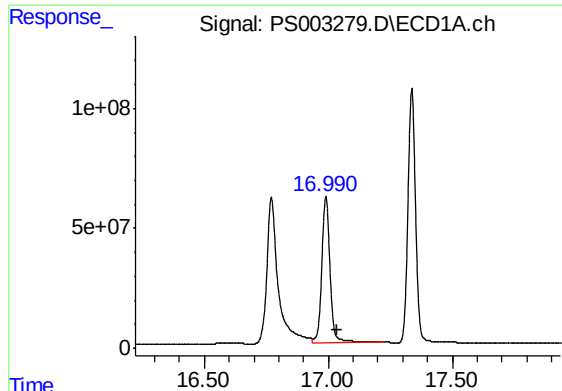

#14 DINOSEB


R.T.: 16.990 min
Delta R.T.: -0.045 min
Response: 1422732955
Conc: 756.24 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

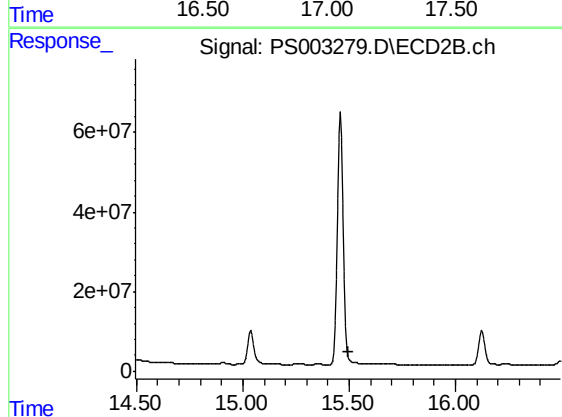


#14 DINOSEB

R.T.: 15.459 min
Delta R.T.: -0.036 min
Response: -499261936
Conc: N.D.

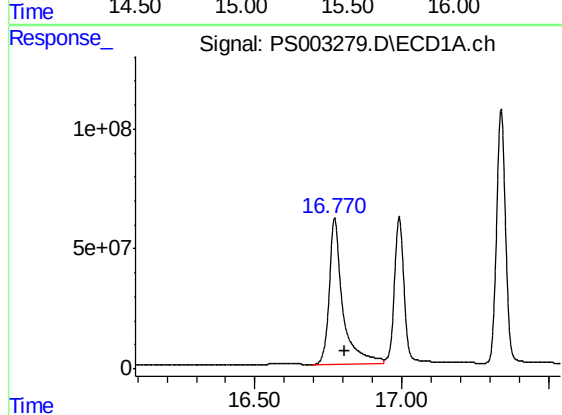


#15 Picloram

R.T.: 16.771 min
Delta R.T.: -0.035 min
Response: 1950660853
Conc: 616.59 ng/ml

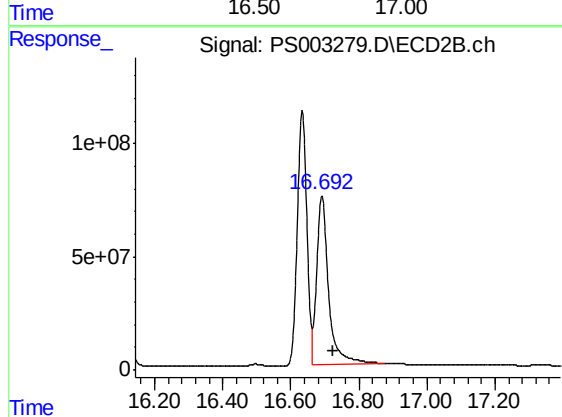

#15 Picloram


R.T.: 16.692 min
Delta R.T.: -0.033 min
Response: 1823242172
Conc: 606.45 ng/ml

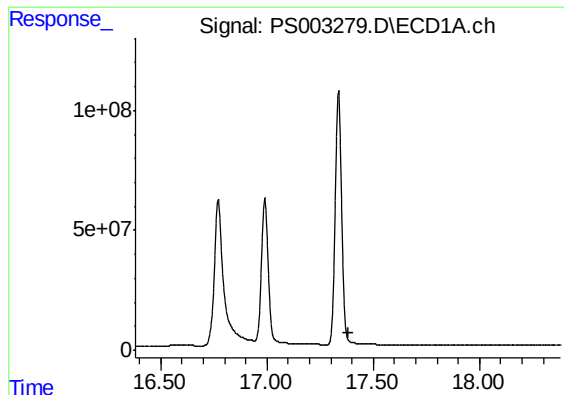

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

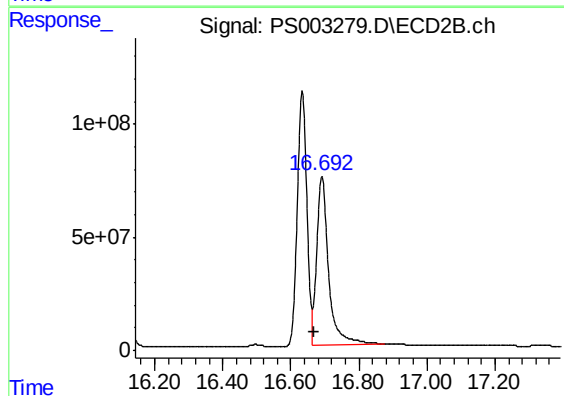

#16 DCPA

R.T.: 16.692 min
Delta R.T.: 0.022 min
Response: 1823242172
Conc: 588.60 ng/ml