

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022019\
 Data File : PS003283.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2019 17:17
 Operator : EI\SJ
 Sample : K1514-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 FK-BPM-004-CLEARBROOK-PILE-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 20 21:57:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	10.775	0	160.0E6	N.D.	374.197 #
Target Compounds							
7) T	MCPA	12.207	0.000	4480741	0	2.532	N.D. #
14) T	DINOSEB	0.000	15.506	0	7809107	N.D.	4.455 #
16) T	DCPA	17.431	0.000	2714896	0	0.903	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022019\
Data File : PS003283.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2019 17:17
Operator : EI\SJ
Sample : K1514-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
FK-BPM-004-CLEARBROOK-PILE-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 20 21:57:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

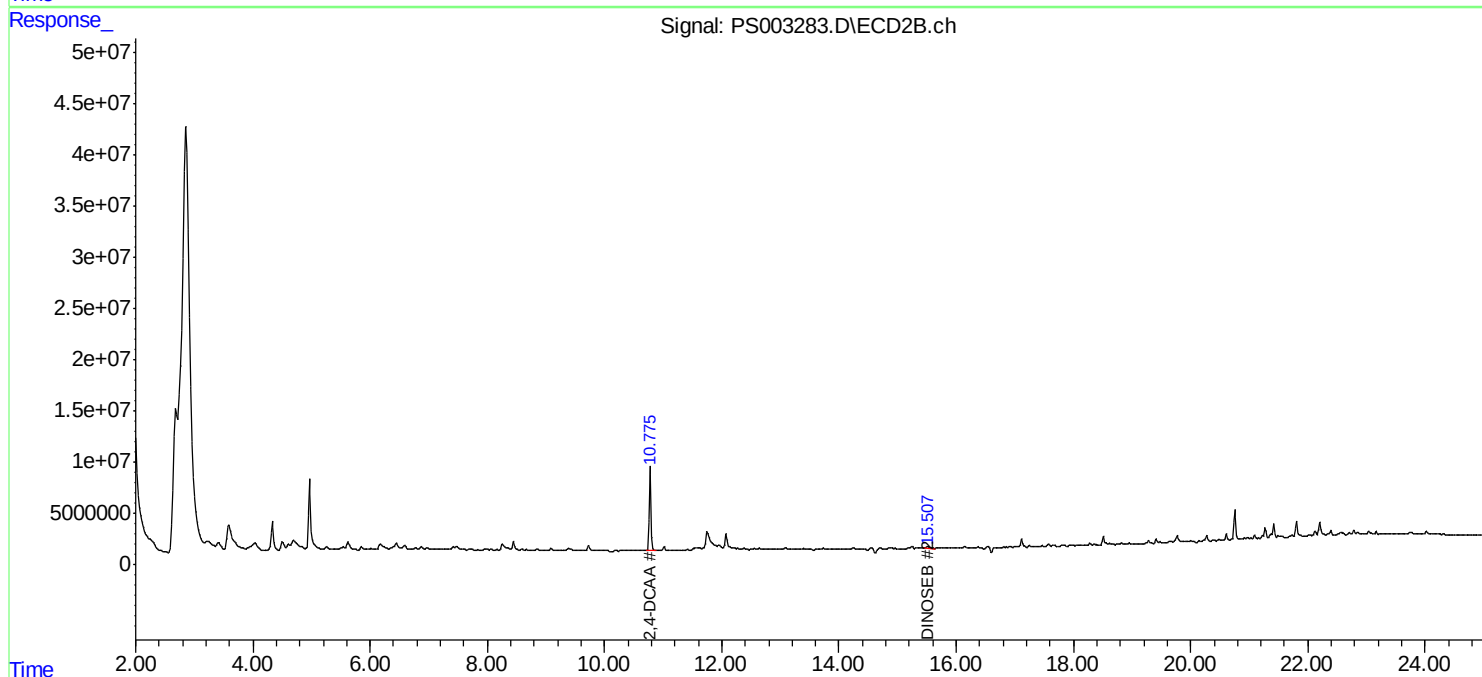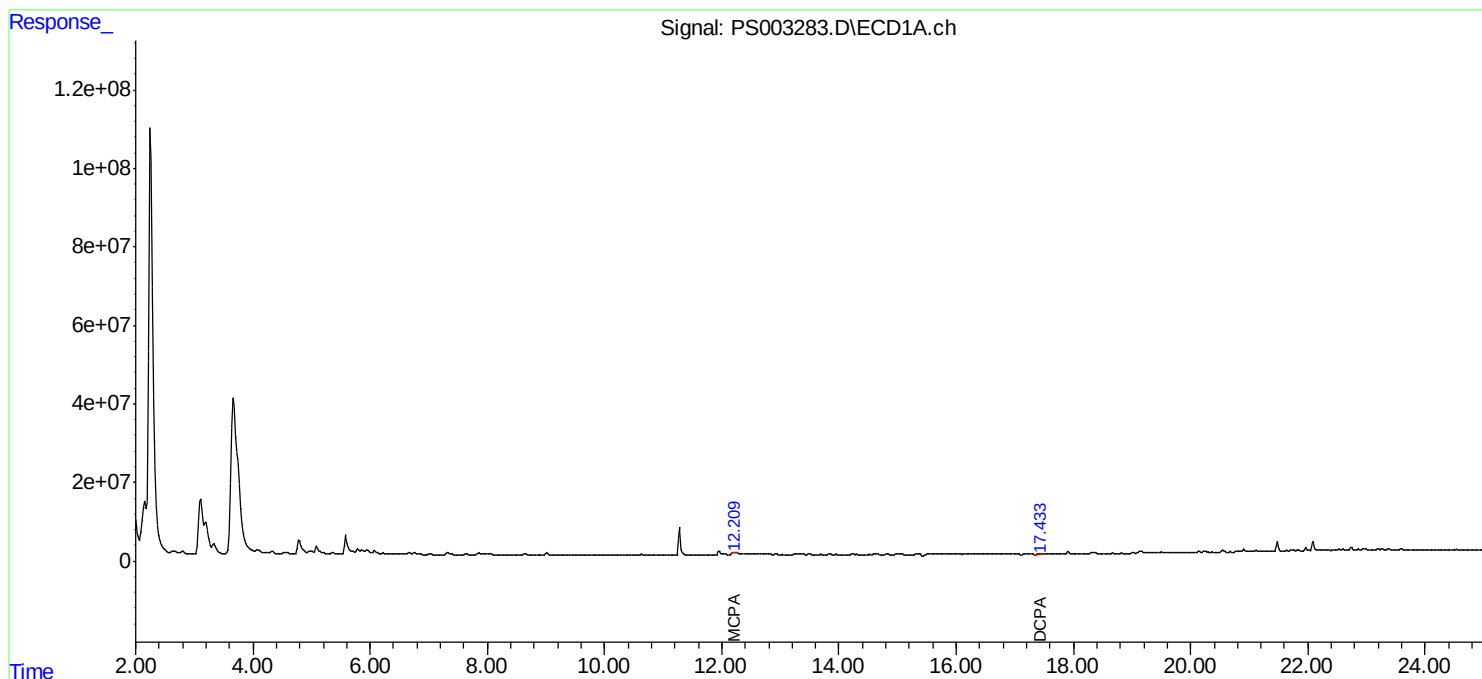


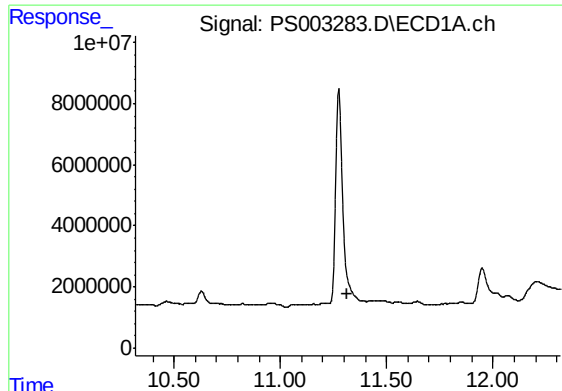

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 11.318 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
FK-BPM-004-CLEARBROOK-PILE-1

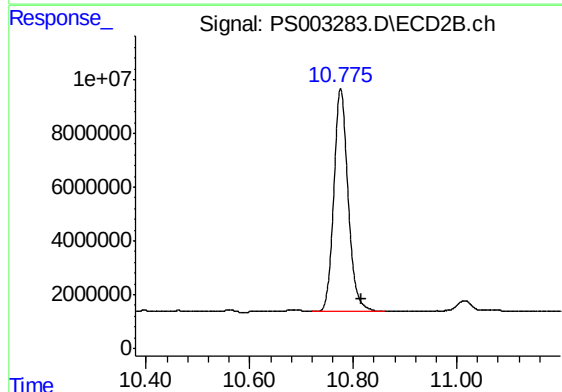


#4 2,4-DCAA

R.T.: 10.775 min
Delta R.T.: -0.041 min
Response: 159986205
Conc: 374.20 ng/ml

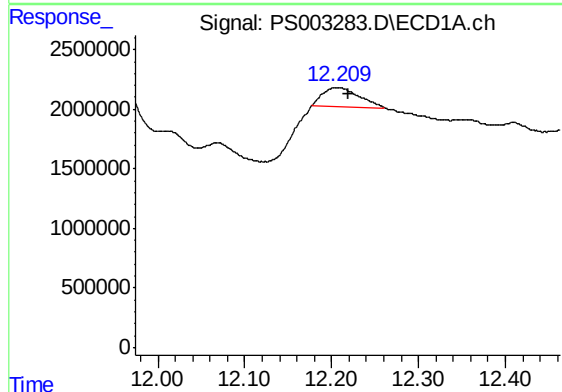


#7 MCPA

R.T.: 12.207 min
Delta R.T.: -0.012 min
Response: 4480741
Conc: 2.53 ug/ml

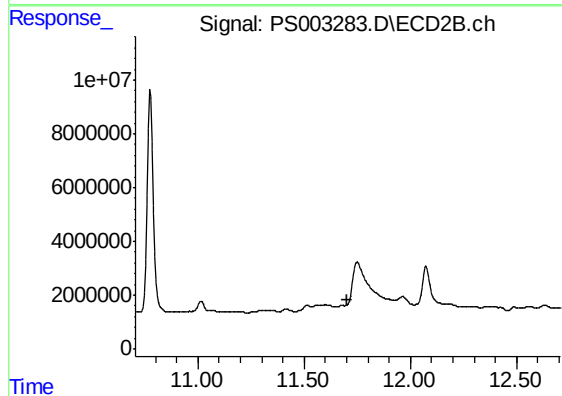

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 11.706 min
Response: 0
Conc: N.D.

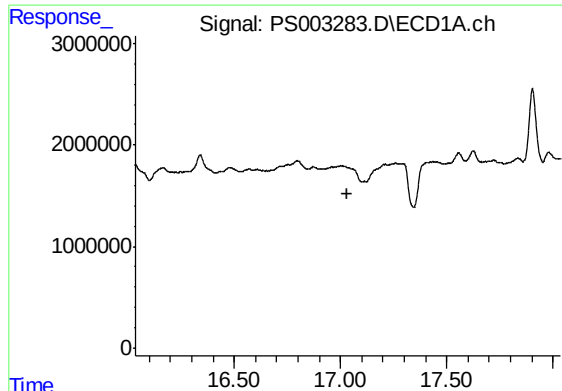

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 17.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
FK-BPM-004-CLEARBROOK-PILE-1

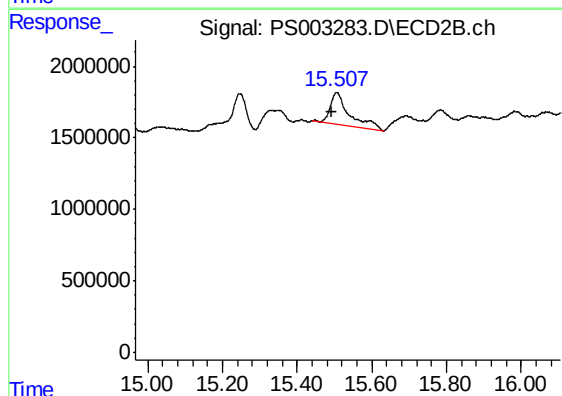


#14 DINOSEB

R.T.: 15.506 min
Delta R.T.: 0.011 min
Response: 7809107
Conc: 4.45 ng/ml

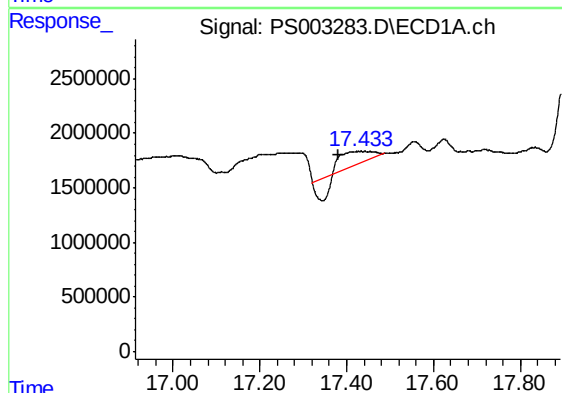

#16 DCPA

R.T.: 17.431 min
Delta R.T.: 0.049 min
Response: 2714896
Conc: 0.90 ng/ml

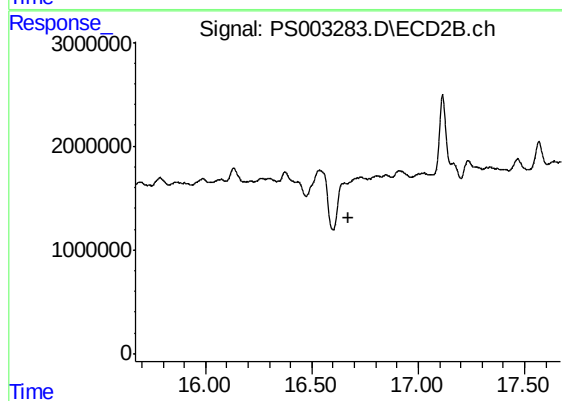

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 16.670 min
Response: 0
Conc: N.D.