

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022019\
 Data File : PS003285.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2019 18:19
 Operator : EI\SJ
 Sample : K1514-01MSD
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 FK-BPM-004-CLEARBROOK-PILE-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 20 21:57:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.278	10.780	72701269	152.2E6	191.500	355.938 #
Target Compounds							
1) T	Dalapon	2.841	2.313	79430633	111.2E6	143.988	207.454 #
2) T	3,5-DICHL...	0.000	8.941	0	119.4E6	N.D.	211.847 #
3) T	4-Nitroph...	10.882	9.935	44232093	60980325	228.543	291.741 #
5) T	DICAMBA	0.000	11.059	0	182.8E6	N.D.	115.206 #
8) T	DICHLORPROP	0.000	12.185	0	137.4E6	N.D.	359.492 #
9) T	2,4-D	0.000	12.658	0	141.8E6	N.D.	282.837 #
11) T	2,4,5-TP ...	14.376	13.816	813.2E6	815.9E6	322.922	328.943
12) T	2,4,5-T	14.778	14.349	764.1E6	853.9E6	313.226	446.278 #
14) T	DINOSEB	16.989	0.000	207.1E6	0	110.073	N.D. #
15) T	Picloram	16.770	16.689	939.1E6	859.7E6	296.846	285.960
16) T	DCPA	0.000	16.689	0	859.7E6	N.D.	277.542 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022019\
Data File : PS003285.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2019 18:19
Operator : EI\SJ
Sample : K1514-01MSD
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
FK-BPM-004-CLEARBROOK-PILE-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 20 21:57:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

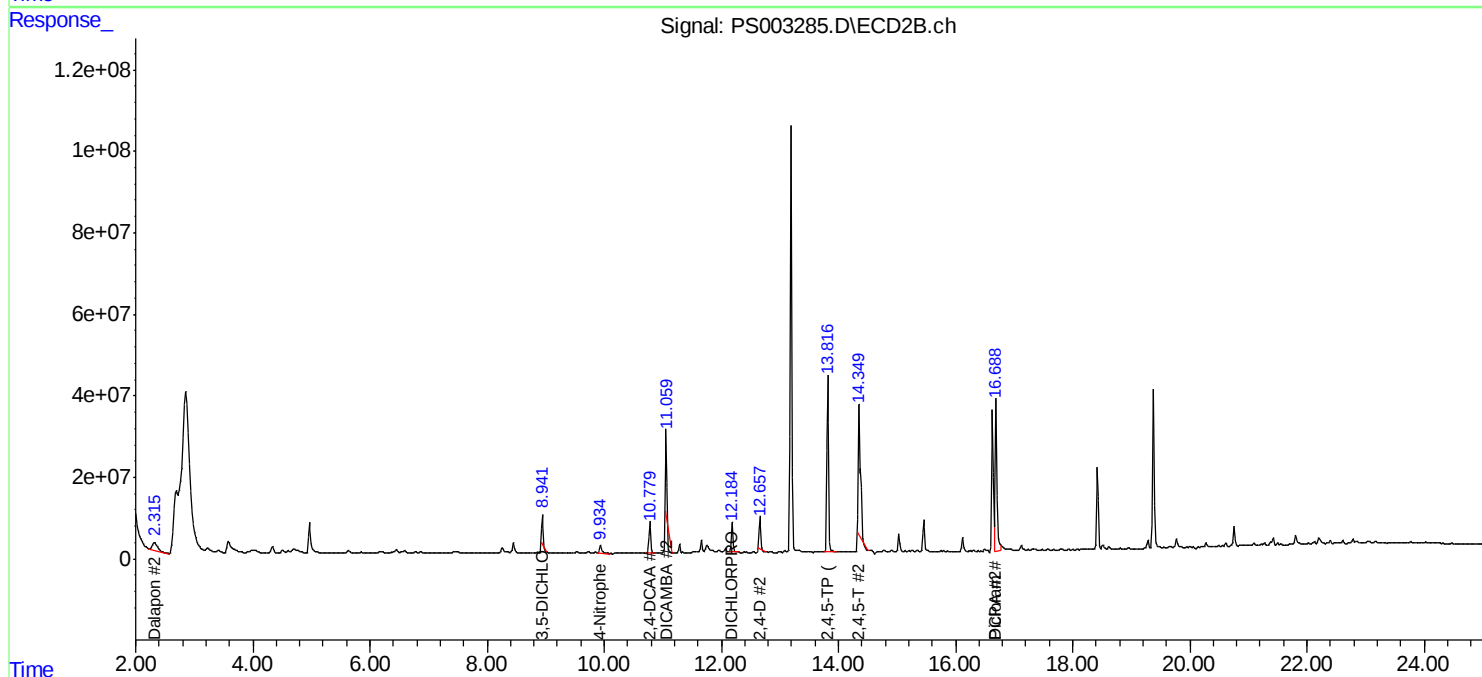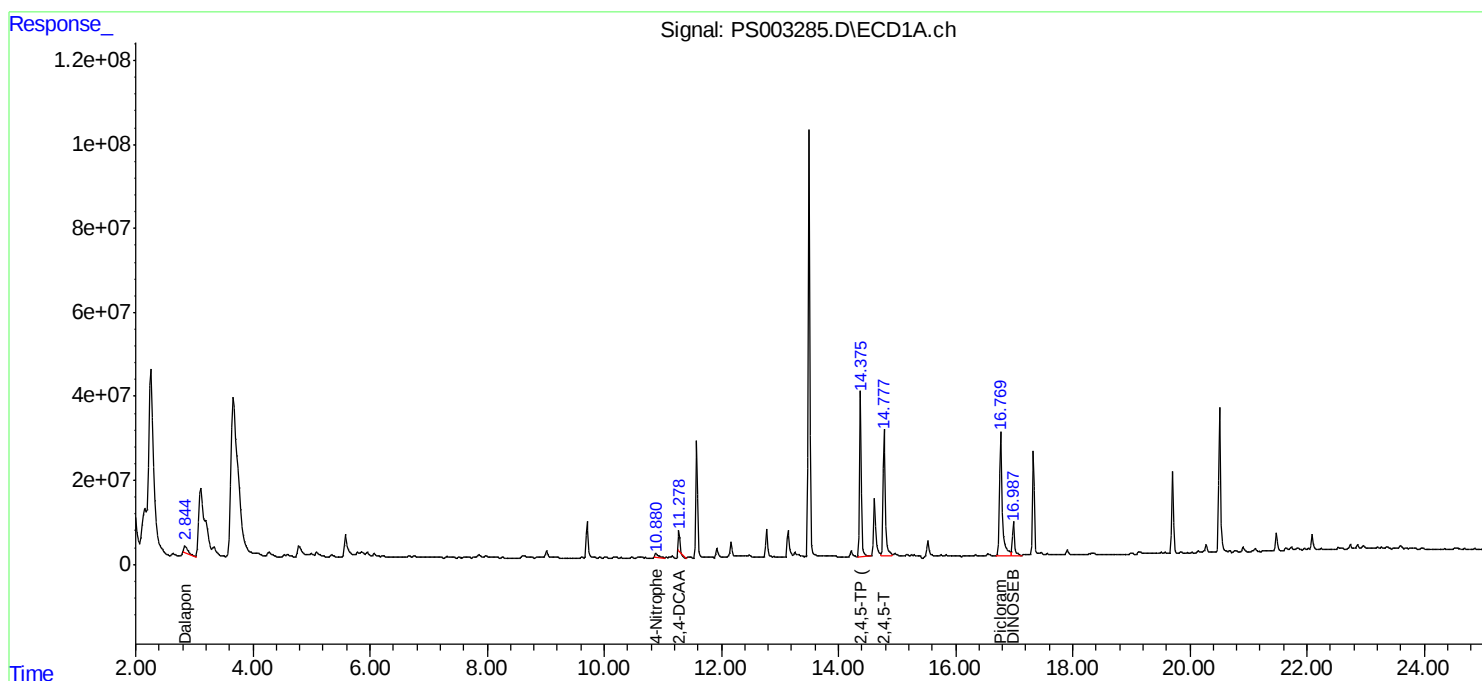


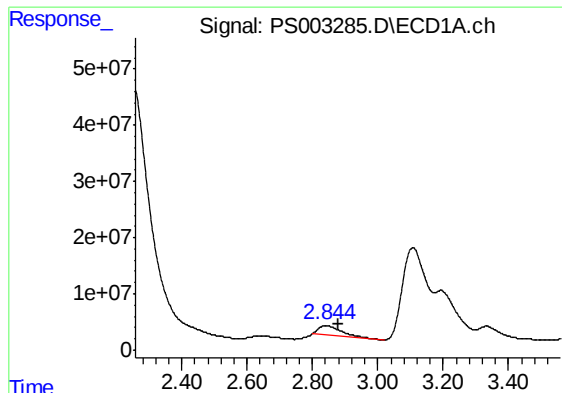

#1 Dalapon


R.T.: 2.841 min
Delta R.T.: -0.039 min
Response: 79430633
Conc: 143.99 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-BPM-004-CLEARBROOK-PILE-1

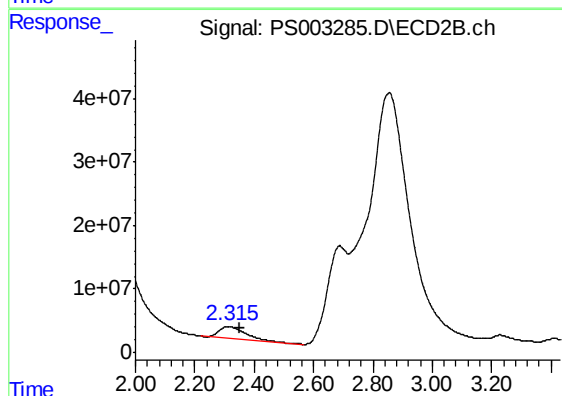


#1 Dalapon

R.T.: 2.313 min
Delta R.T.: -0.038 min
Response: 111179034
Conc: 207.45 ng/ml

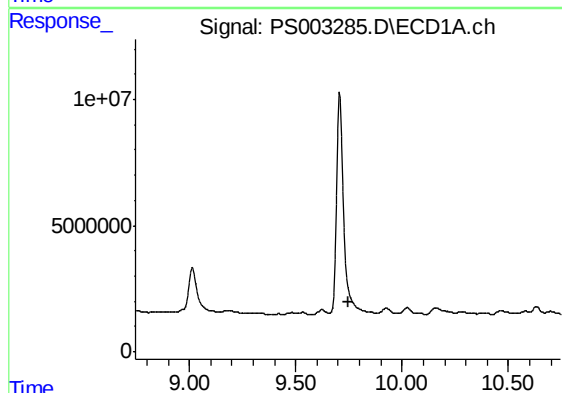


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.745 min
Response: 0
Conc: N.D.

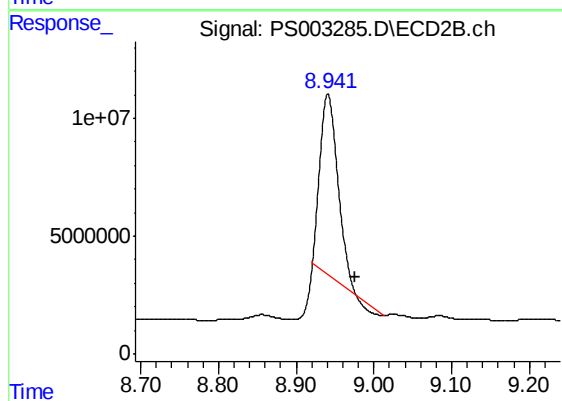

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.941 min
Delta R.T.: -0.035 min
Response: 119390338
Conc: 211.85 ng/ml

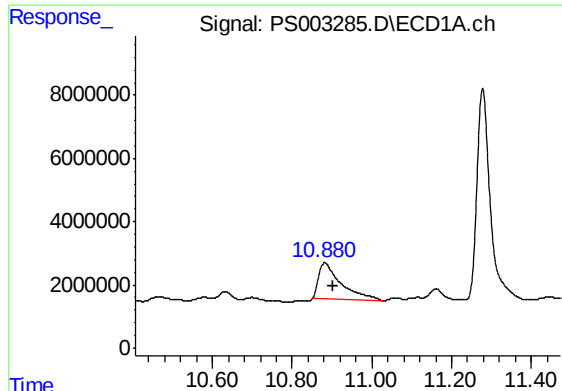

#3 4-Nitrophenol


R.T.: 10.882 min
Delta R.T.: -0.022 min
Response: 44232093
Conc: 228.54 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-BPM-004-CLEARBROOK-PILE-1

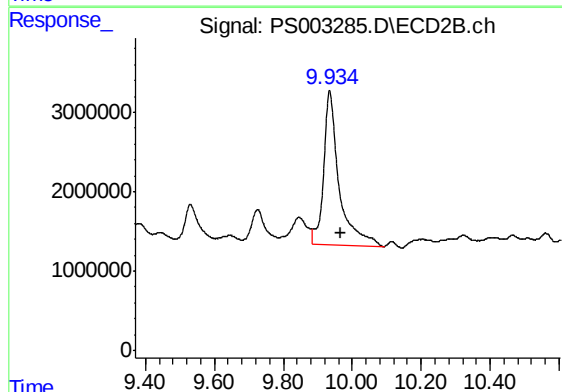


#3 4-Nitrophenol

R.T.: 9.935 min
Delta R.T.: -0.031 min
Response: 60980325
Conc: 291.74 ng/ml

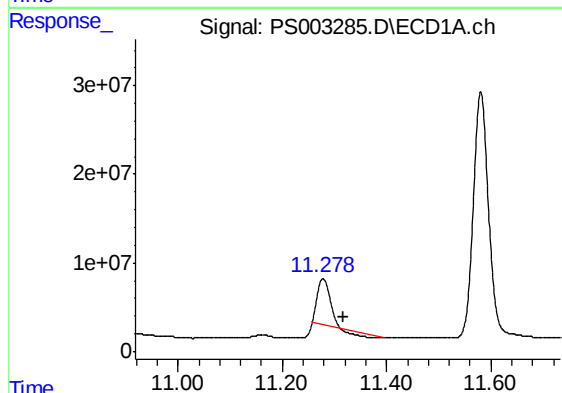


#4 2,4-DCAA

R.T.: 11.278 min
Delta R.T.: -0.040 min
Response: 72701269
Conc: 191.50 ng/ml

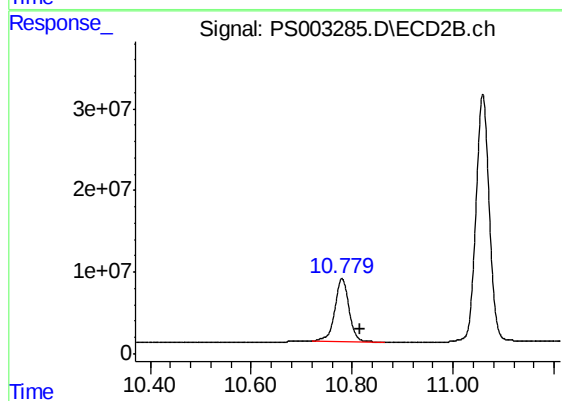

#4 2,4-DCAA


R.T.: 10.780 min
Delta R.T.: -0.037 min
Response: 152179791
Conc: 355.94 ng/ml

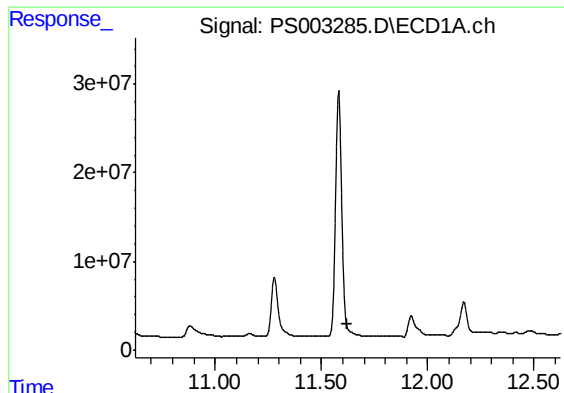

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.624 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
FK-BPM-004-CLEARBROOK-PILE-1

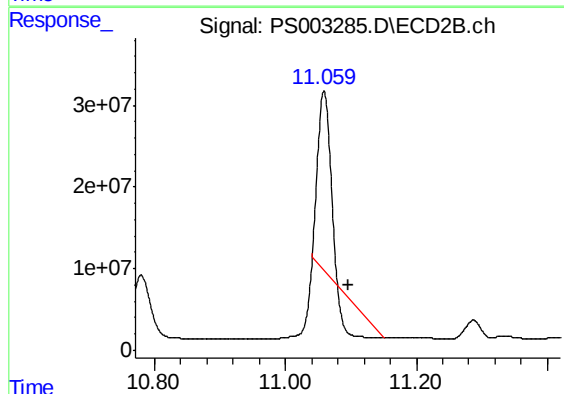


#5 DICAMBA

R.T.: 11.059 min
Delta R.T.: -0.038 min
Response: 182792917
Conc: 115.21 ng/ml

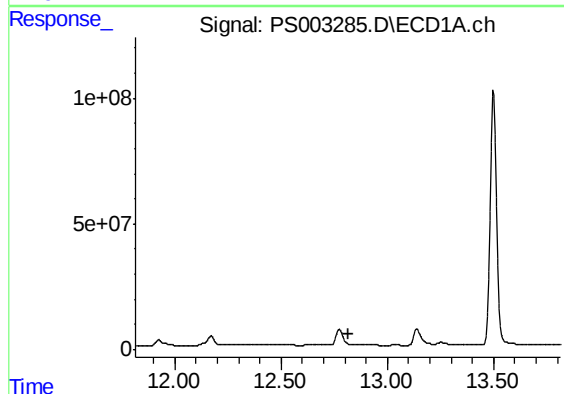


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 12.815 min
Response: 0
Conc: N.D.

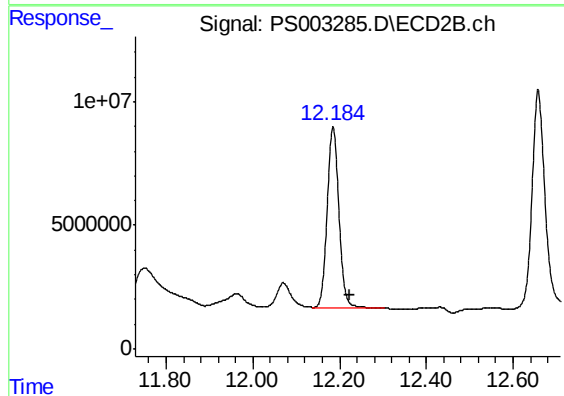

#8 DICHLORPROP


R.T.: 12.185 min
Delta R.T.: -0.037 min
Response: 137448619
Conc: 359.49 ng/ml

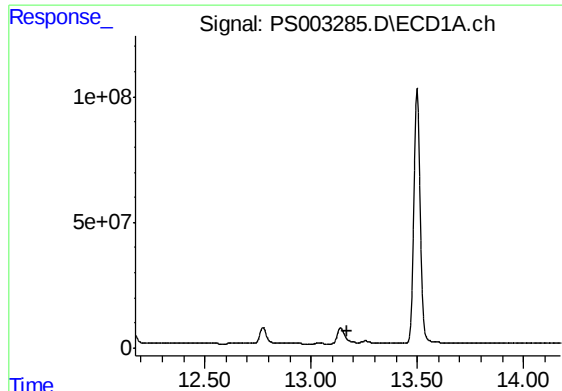

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.173 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
FK-BPM-004-CLEARBROOK-PILE-1

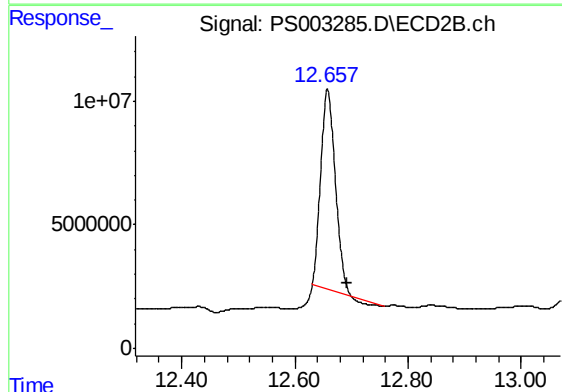


#9 2,4-D

R.T.: 12.658 min
Delta R.T.: -0.035 min
Response: 141810519
Conc: 282.84 ng/ml

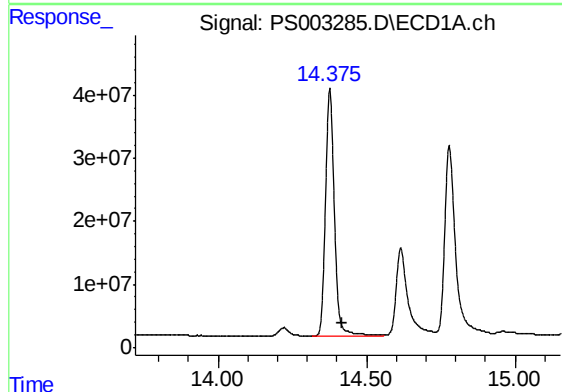


#11 2,4,5-TP (SILVEX)

R.T.: 14.376 min
Delta R.T.: -0.043 min
Response: 813237458
Conc: 322.92 ng/ml

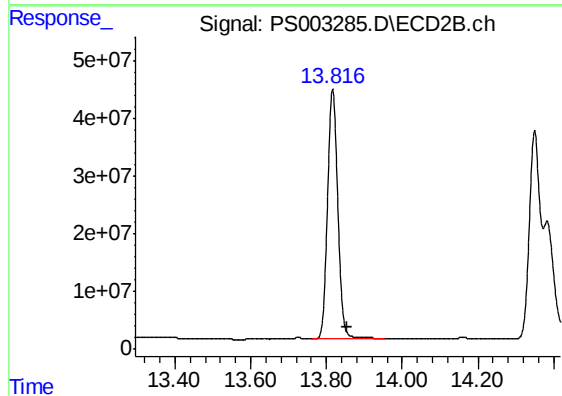

#11 2,4,5-TP (SILVEX)


R.T.: 13.816 min
Delta R.T.: -0.038 min
Response: 815896140
Conc: 328.94 ng/ml

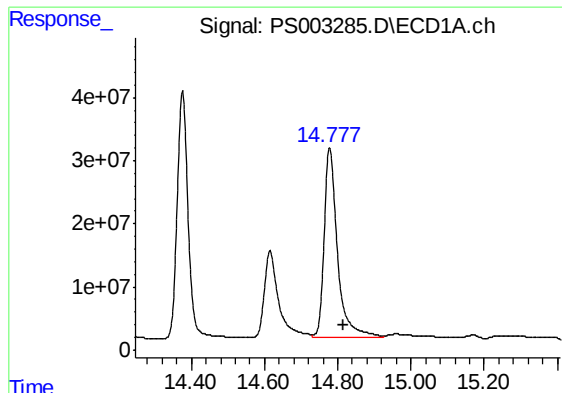

#12 2,4,5-T


R.T.: 14.778 min
Delta R.T.: -0.038 min
Response: 764086041
Conc: 313.23 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-BPM-004-CLEARBROOK-PILE-1

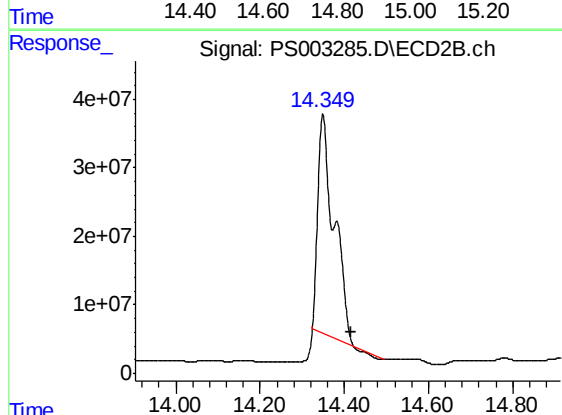


#12 2,4,5-T

R.T.: 14.349 min
Delta R.T.: -0.068 min
Response: 853948529
Conc: 446.28 ng/ml

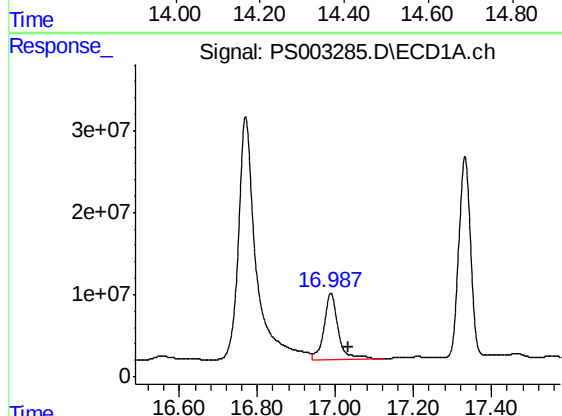


#14 DINOSEB

R.T.: 16.989 min
Delta R.T.: -0.047 min
Response: 207083553
Conc: 110.07 ng/ml

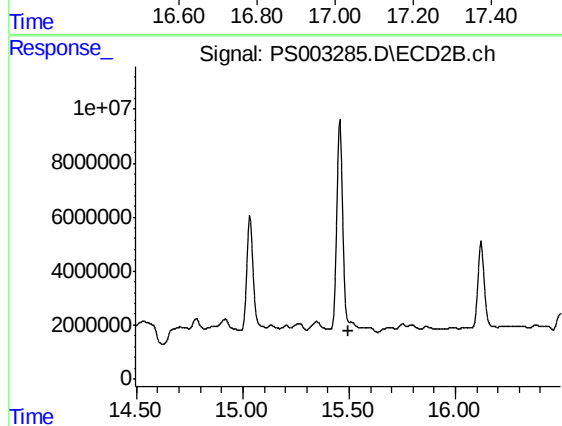

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 15.495 min
Response: 0
Conc: N.D.

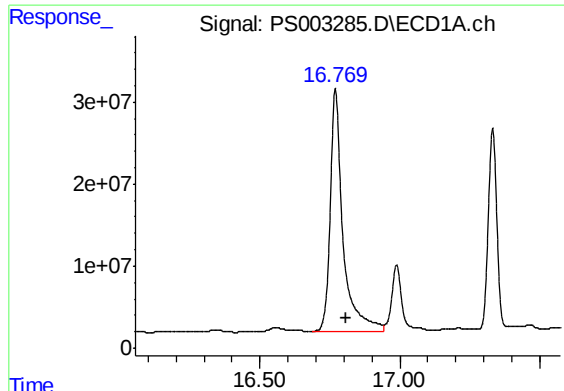

#15 Picloram


R.T.: 16.770 min
Delta R.T.: -0.036 min
Response: 939112608
Conc: 296.85 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-BPM-004-CLEARBROOK-PILE-1

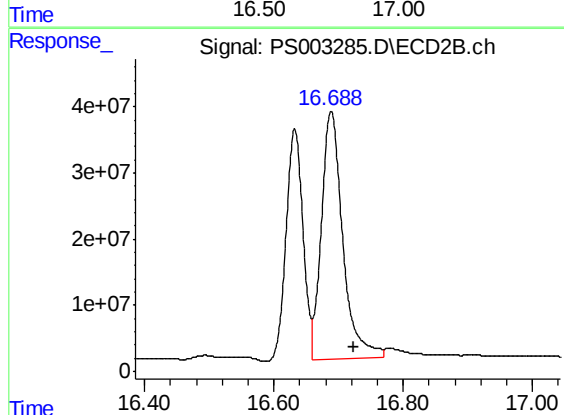


#15 Picloram

R.T.: 16.689 min
Delta R.T.: -0.036 min
Response: 859710673
Conc: 285.96 ng/ml

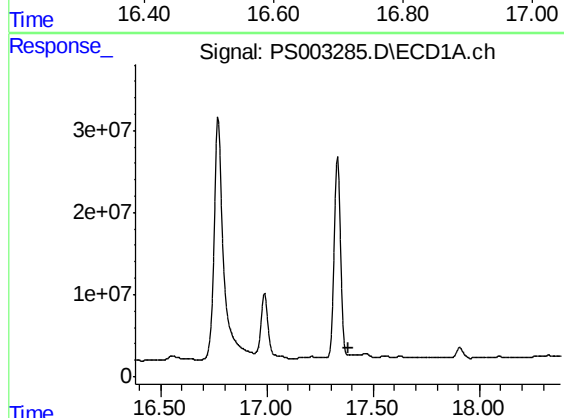

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.382 min
Response: 0
Conc: N.D.

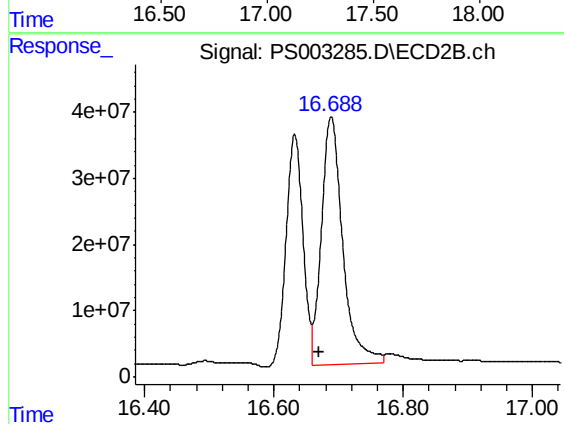

#16 DCPA

R.T.: 16.689 min
Delta R.T.: 0.019 min
Response: 859710673
Conc: 277.54 ng/ml