

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022020\
 Data File : PS008906.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2020 10:25
 Operator : DD\AJ
 Sample : HSTDICC750
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 20 11:18:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:16:54 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.247	6.940	1627.2E6	734.2E6	750.000	750.000
Target Compounds							
1) T	Dalapon	3.048	2.630	2077.7E6	1021.2E6	682.500	682.500
2) T	3,5-DICHL...	6.455	6.083	1991.7E6	1020.2E6	697.500	697.500
3) T	4-Nitroph...	7.075	6.541	734.7E6	396.1E6	682.500	682.500
5) T	DICAMBA	7.440	7.111	5752.2E6	2952.9E6	705.000	705.000
6) T	MCPD	7.611	7.209	438.7E6	220.1E6	70.500	70.500
7) T	MCPA	7.761	7.425	578.7E6	349.0E6	69.750	69.750
8) T	DICHLORPROP	8.135	7.739	1366.1E6	704.9E6	705.000	705.000
9) T	2,4-D	8.363	8.033	1474.6E6	841.9E6	705.000	705.000
10) T	Pentachlo...	8.677	8.467	20631.1E6	10097.9E6	712.500	712.500
11) T	2,4,5-TP ...	9.227	8.828	7839.9E6	3878.1E6	712.500	712.500
12) T	2,4,5-T	9.511	9.208	7712.2E6	3890.1E6	712.500	712.500
13) T	2,4-DB	10.064	9.715	1040.4E6	505.4E6	712.500	712.500
14) T	DINOSEB	11.231	10.052	5983.1E6	2812.8E6	705.000	705.000
15) T	Picloram	11.043	11.031	10027.9E6	5355.3E6	712.500	712.500
16) T	DCPA	11.495	10.982	9835.1E6	5010.4E6	720.000	720.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022020\
Data File : PS008906.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2020 10:25
Operator : DD\AJ
Sample : HSTDICC750
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 20 11:18:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:16:54 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

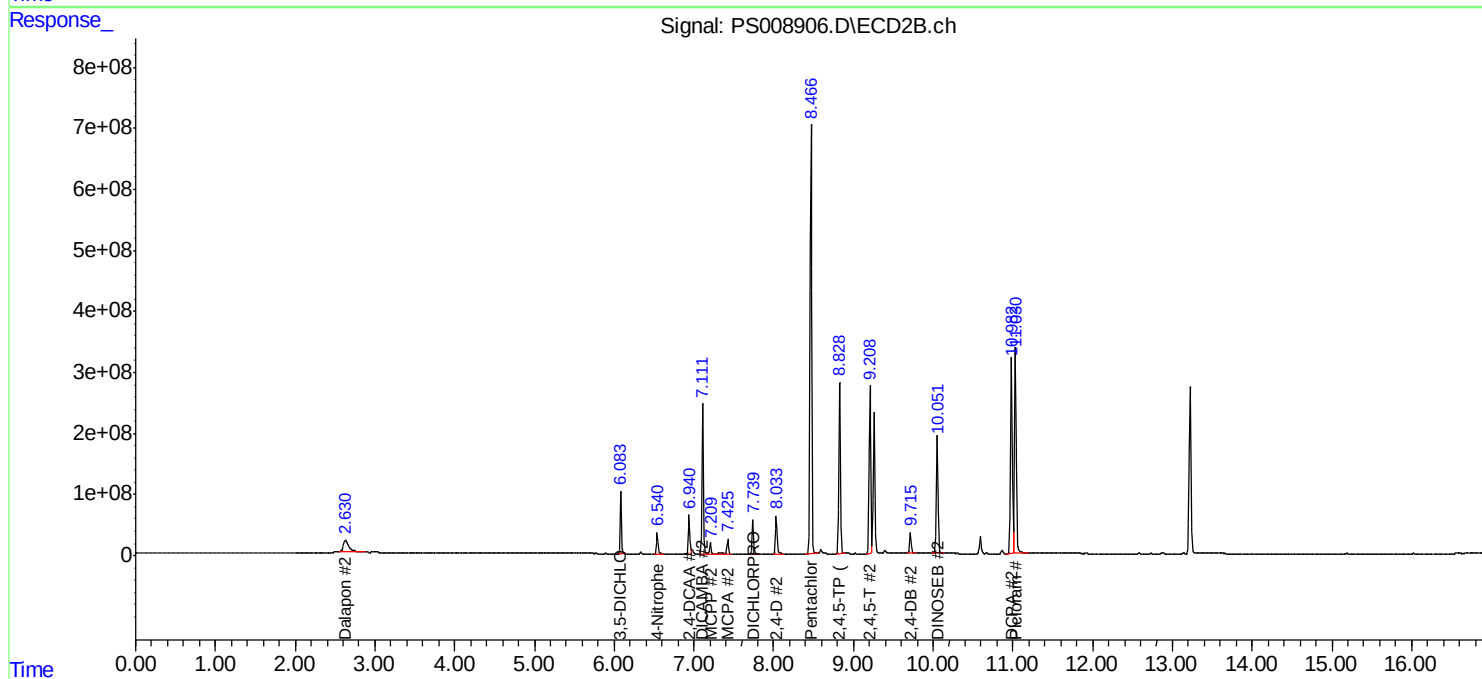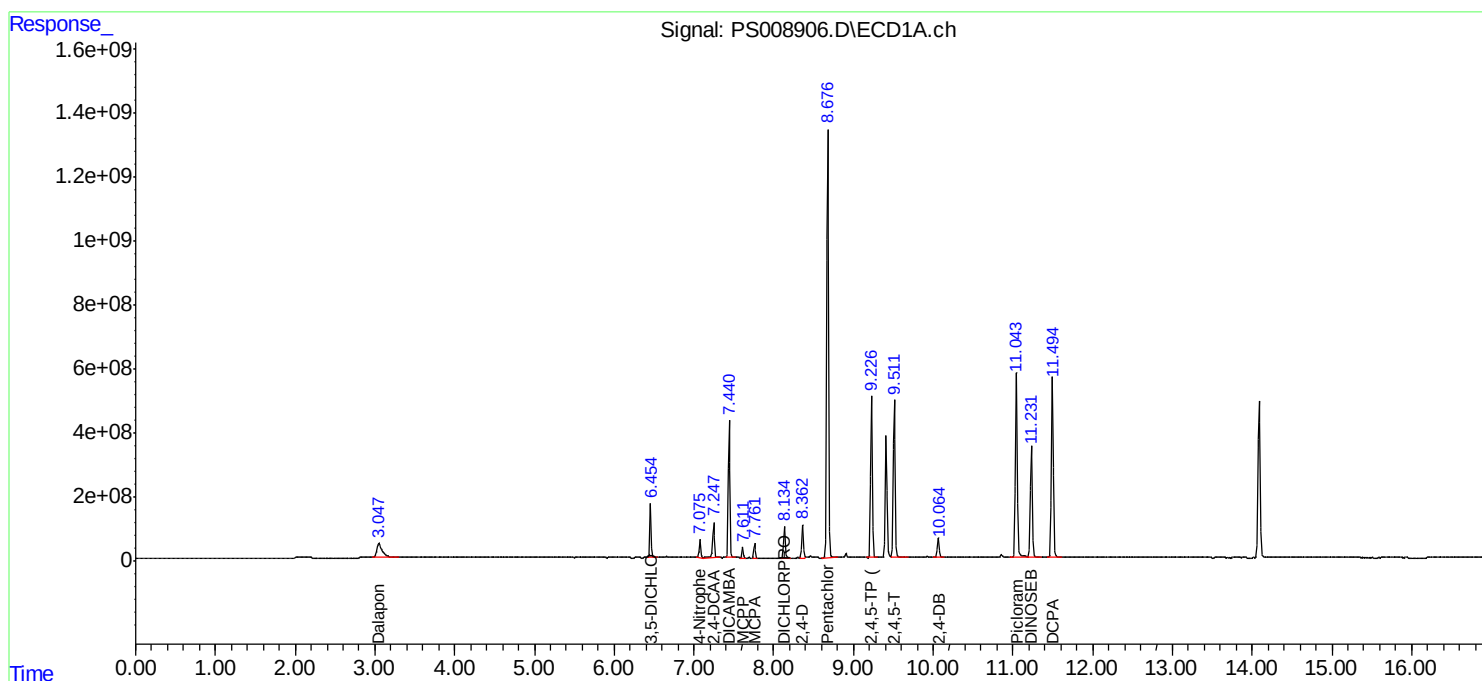


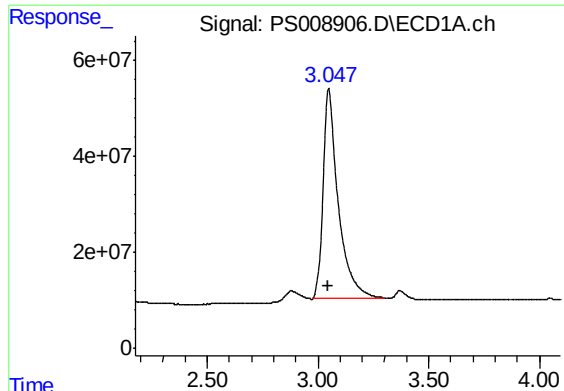

#1 Dalapon


R.T.: 3.048 min
Delta R.T.: 0.000 min
Response: 2077669431
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

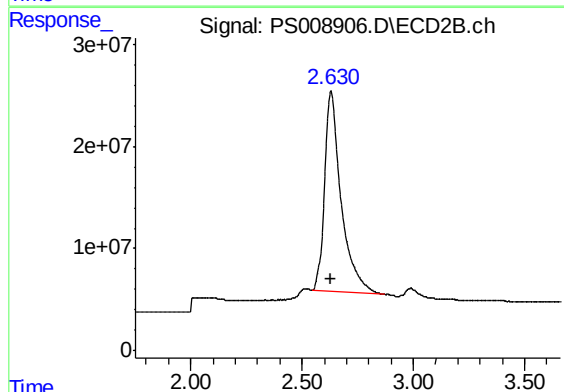


#1 Dalapon

R.T.: 2.630 min
Delta R.T.: 0.000 min
Response: 1021191069
Conc: 682.50 ng/ml

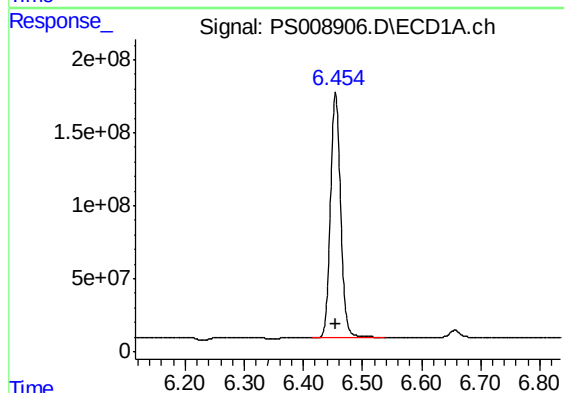


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.455 min
Delta R.T.: 0.000 min
Response: 1991710994
Conc: 697.50 ng/ml

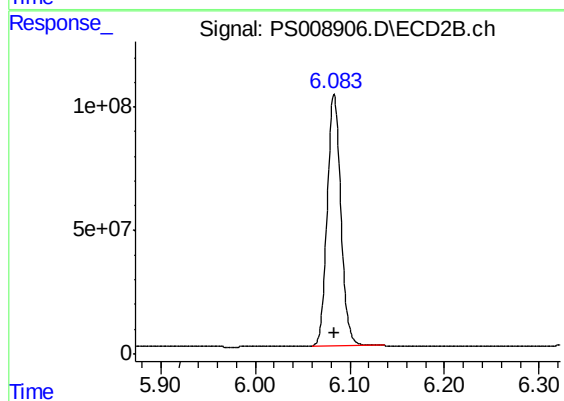

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.083 min
Delta R.T.: 0.000 min
Response: 1020183840
Conc: 697.50 ng/ml

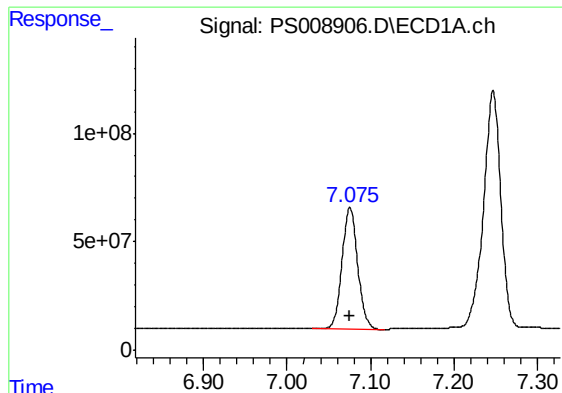

#3 4-Nitrophenol


R.T.: 7.075 min
Delta R.T.: 0.000 min
Response: 734747749
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

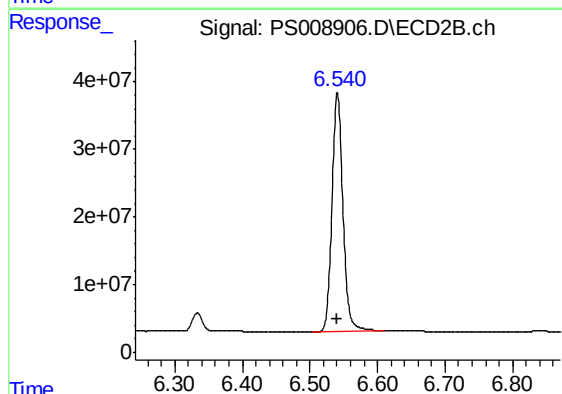


#3 4-Nitrophenol

R.T.: 6.541 min
Delta R.T.: 0.000 min
Response: 396100541
Conc: 682.50 ng/ml

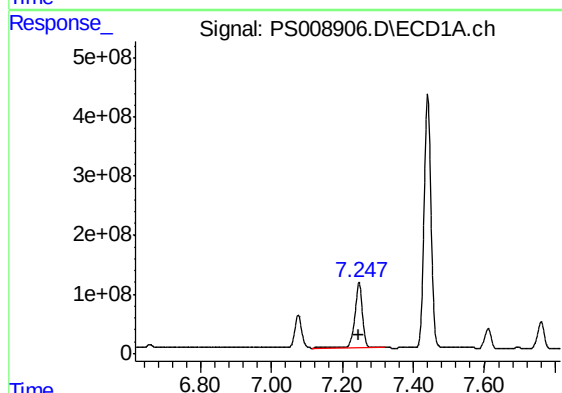


#4 2,4-DCAA

R.T.: 7.247 min
Delta R.T.: 0.000 min
Response: 1627247396
Conc: 750.00 ng/ml

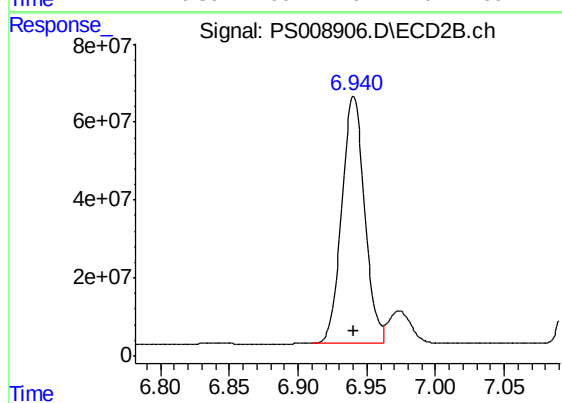

#4 2,4-DCAA


R.T.: 6.940 min
Delta R.T.: 0.000 min
Response: 734216743
Conc: 750.00 ng/ml

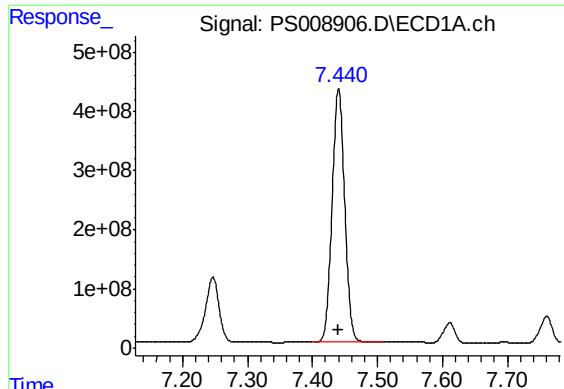

#5 DICAMBA


R.T.: 7.440 min
Delta R.T.: 0.000 min
Response: 5752241964
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

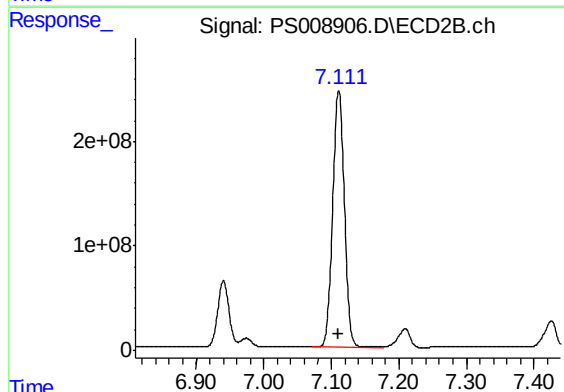


#5 DICAMBA

R.T.: 7.111 min
Delta R.T.: 0.000 min
Response: 2952856795
Conc: 705.00 ng/ml

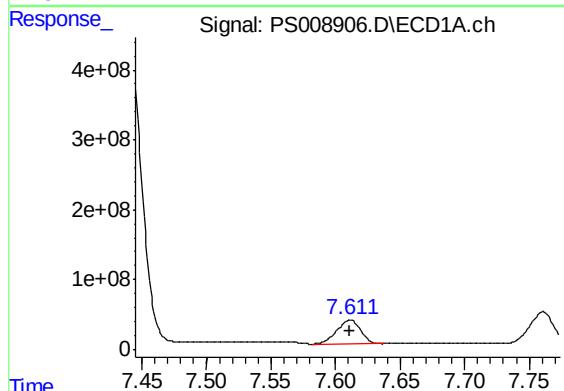


#6 MCPP

R.T.: 7.611 min
Delta R.T.: 0.000 min
Response: 438732862
Conc: 70.50 ug/ml

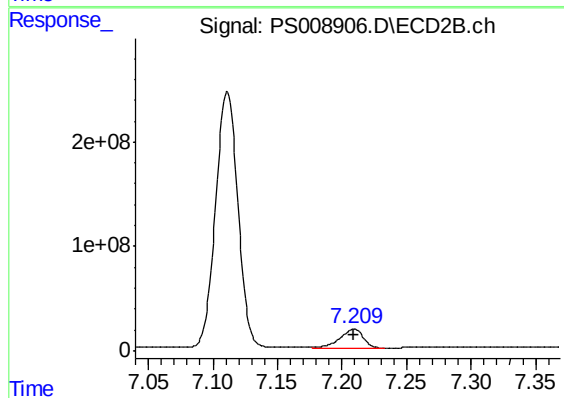

#6 MCPP


R.T.: 7.209 min
Delta R.T.: 0.000 min
Response: 220057626
Conc: 70.50 ug/ml

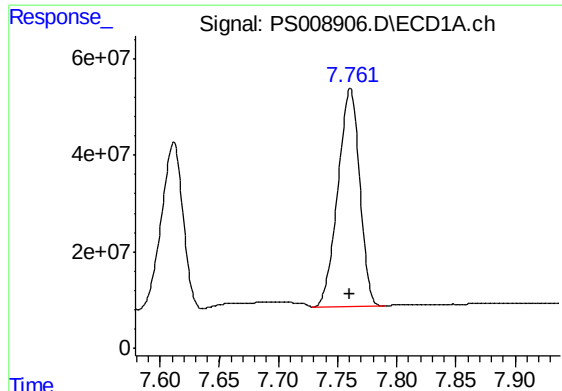

#7 MCPA


R.T.: 7.761 min
Delta R.T.: 0.000 min
Response: 578676398
Conc: 69.75 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

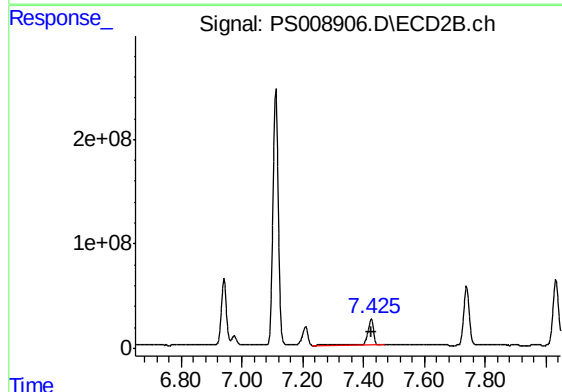


#7 MCPA

R.T.: 7.425 min
Delta R.T.: 0.000 min
Response: 348956490
Conc: 69.75 ug/ml

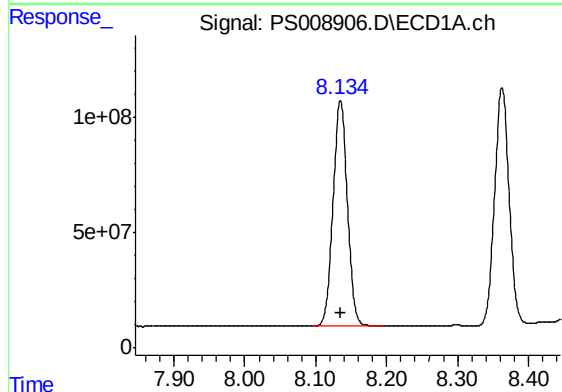


#8 DICHLORPROP

R.T.: 8.135 min
Delta R.T.: 0.000 min
Response: 1366110492
Conc: 705.00 ng/ml

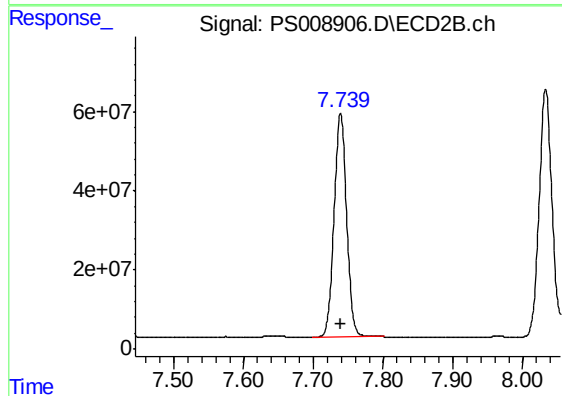

#8 DICHLORPROP


R.T.: 7.739 min
Delta R.T.: 0.000 min
Response: 704899459
Conc: 705.00 ng/ml

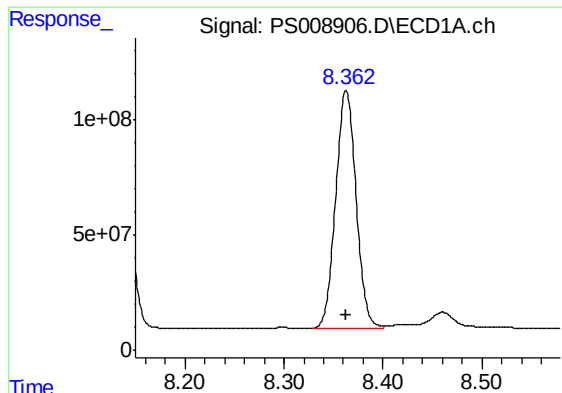

#9 2,4-D


R.T.: 8.363 min
Delta R.T.: 0.000 min
Response: 1474600848
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

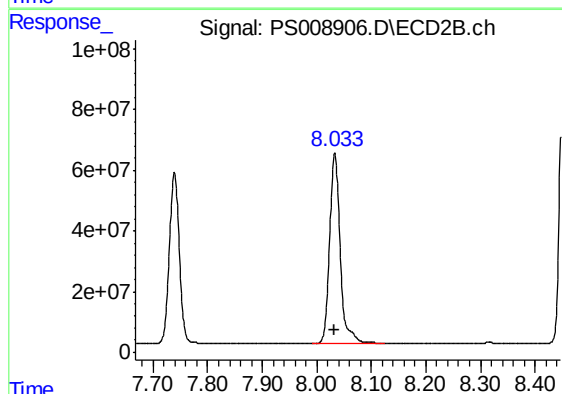


#9 2,4-D

R.T.: 8.033 min
Delta R.T.: 0.000 min
Response: 841863039
Conc: 705.00 ng/ml

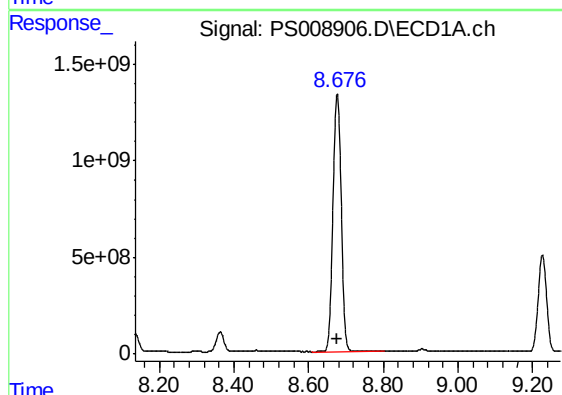


#10 Pentachlorophenol

R.T.: 8.677 min
Delta R.T.: 0.000 min
Response: 20631143582
Conc: 712.50 ng/ml

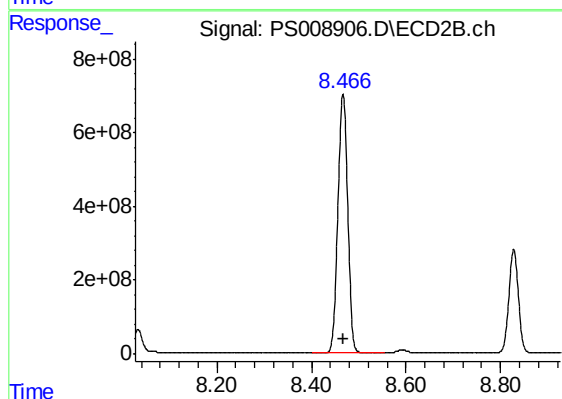

#10 Pentachlorophenol


R.T.: 8.467 min
Delta R.T.: 0.000 min
Response: 10097891960
Conc: 712.50 ng/ml

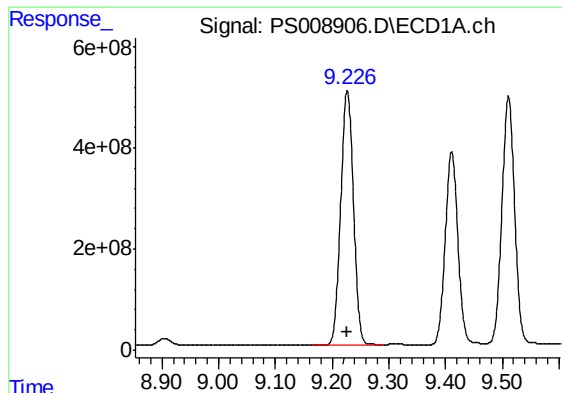

#11 2,4,5-TP (SILVEX)


R.T.: 9.227 min
Delta R.T.: 0.000 min
Response: 7839949468
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

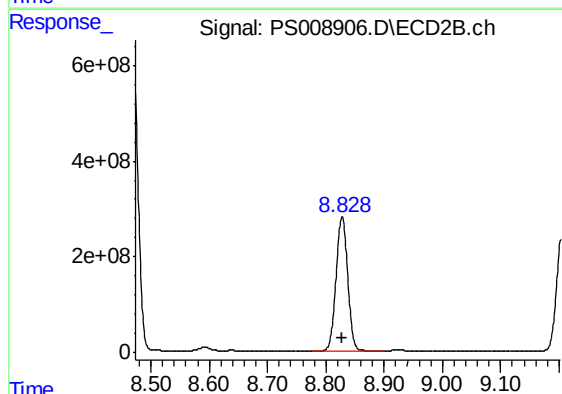


#11 2,4,5-TP (SILVEX)

R.T.: 8.828 min
Delta R.T.: 0.000 min
Response: 3878078340
Conc: 712.50 ng/ml

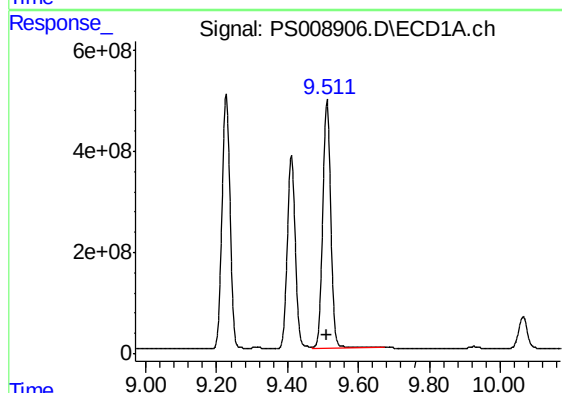


#12 2,4,5-T

R.T.: 9.511 min
Delta R.T.: 0.000 min
Response: 7712231806
Conc: 712.50 ng/ml

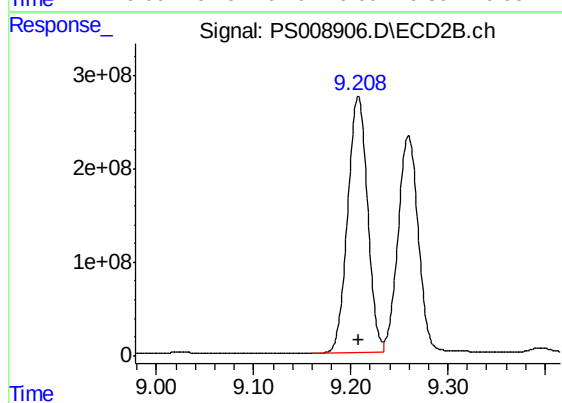

#12 2,4,5-T


R.T.: 9.208 min
Delta R.T.: 0.000 min
Response: 3890083647
Conc: 712.50 ng/ml

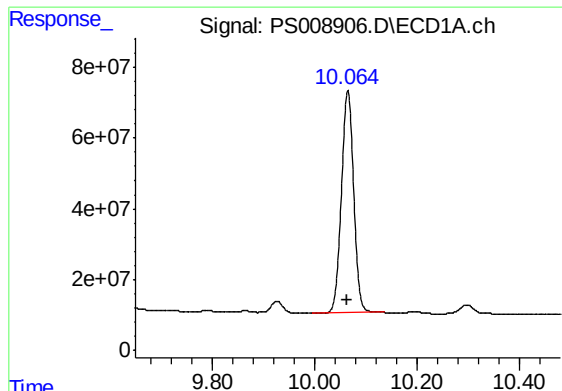

#13 2,4-DB


R.T.: 10.064 min
Delta R.T.: 0.000 min
Response: 1040373818
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

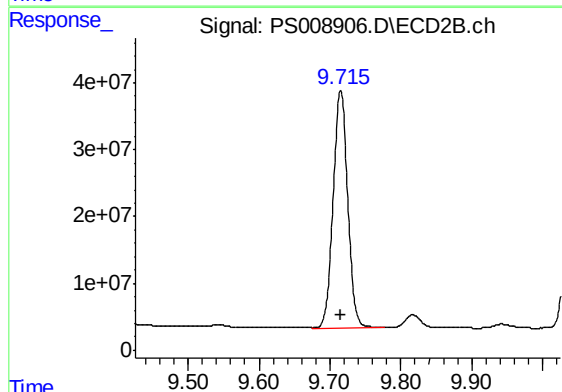


#13 2,4-DB

R.T.: 9.715 min
Delta R.T.: 0.000 min
Response: 505410117
Conc: 712.50 ng/ml

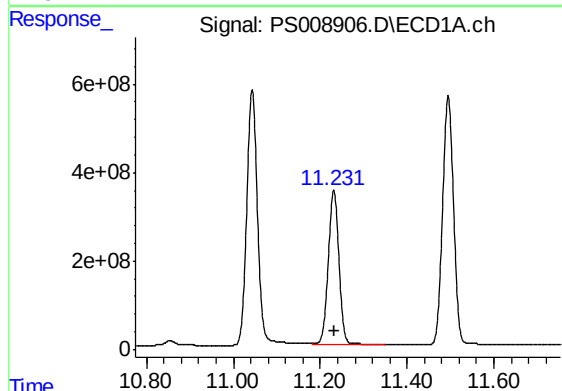


#14 DINOSEB

R.T.: 11.231 min
Delta R.T.: 0.000 min
Response: 5983136802
Conc: 705.00 ng/ml

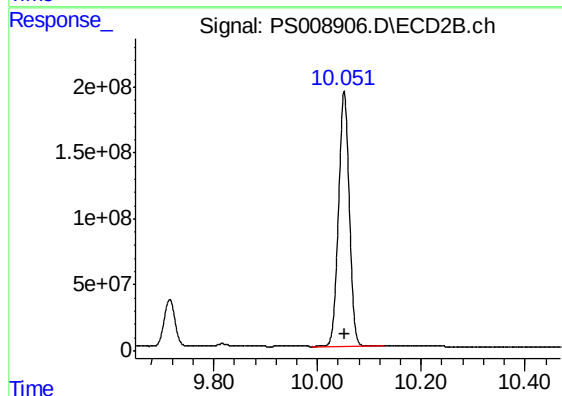

#14 DINOSEB


R.T.: 10.052 min
Delta R.T.: 0.000 min
Response: 2812808083
Conc: 705.00 ng/ml

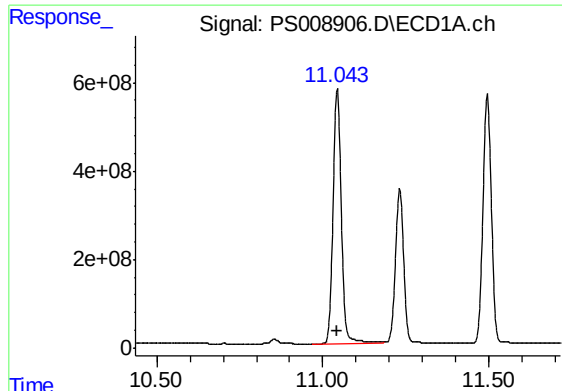

#15 Picloram


R.T.: 11.043 min
Delta R.T.: 0.000 min
Response: 10027948553
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

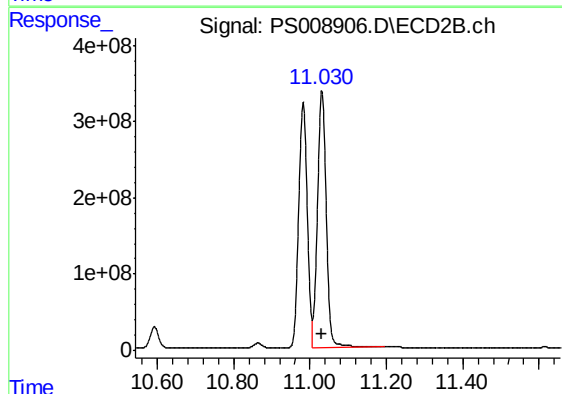


#15 Picloram

R.T.: 11.031 min
Delta R.T.: 0.000 min
Response: 5355297427
Conc: 712.50 ng/ml

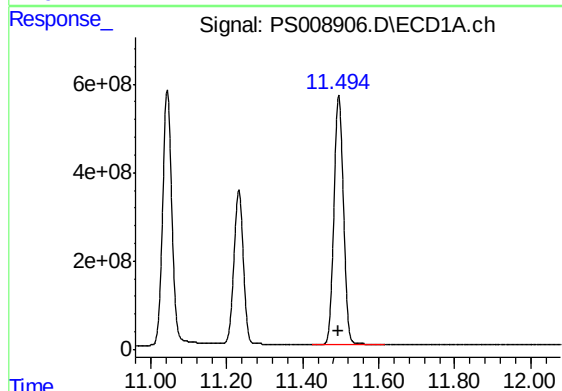

#16 DCPA

R.T.: 11.495 min
Delta R.T.: 0.000 min
Response: 9835125838
Conc: 720.00 ng/ml

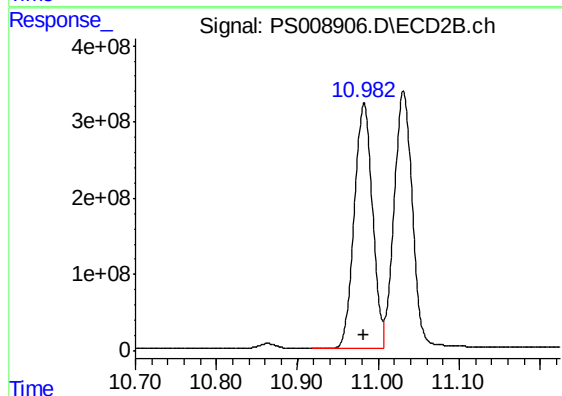

#16 DCPA

R.T.: 10.982 min
Delta R.T.: 0.000 min
Response: 5010408436
Conc: 720.00 ng/ml