

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022020\
 Data File : PS008912.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2020 12:42
 Operator : DD\AJ
 Sample : L1552-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 FK-SF-01-008-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 20 14:01:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.248	6.940	951.6E6	432.5E6	435.213	448.872
Target Compounds							
1) T	Dalapon	0.000	2.594	0	224.8E6	N.D.	153.722
2) T	3,5-DICHL...	0.000	6.114	0	118.5E6	N.D.	81.236
7) T	MCPA	7.800	0.000	58337261	0	7.252	N.D. #
12) T	2,4,5-T	9.456	9.260	60160091	57186930	5.627	10.565 #
15) T	Picloram	11.044	11.031	539.0E6	349.1E6	39.372	48.039
16) T	DCPA	0.000	11.031	0	349.1E6	N.D.	50.449



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022020\
Data File : PS008912.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2020 12:42
Operator : DD\AJ
Sample : L1552-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
FK-SF-01-008-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 20 14:01:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

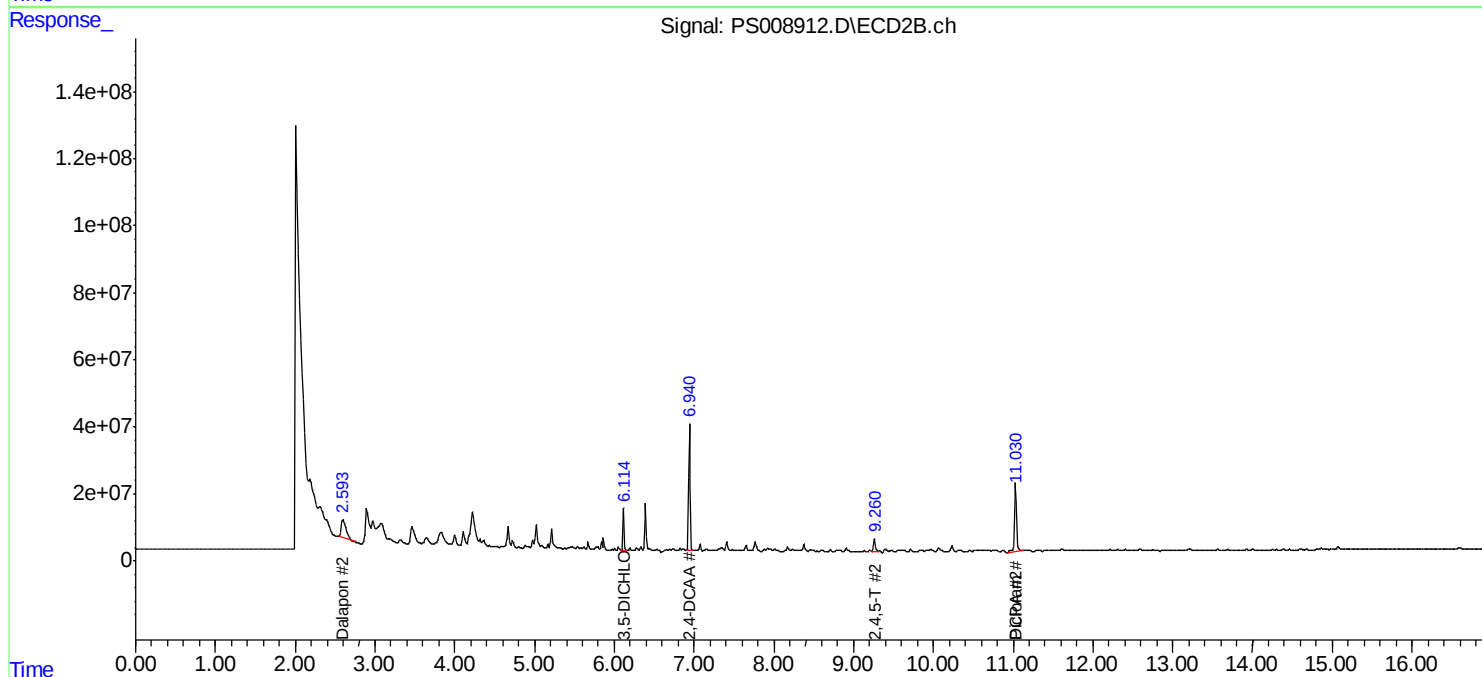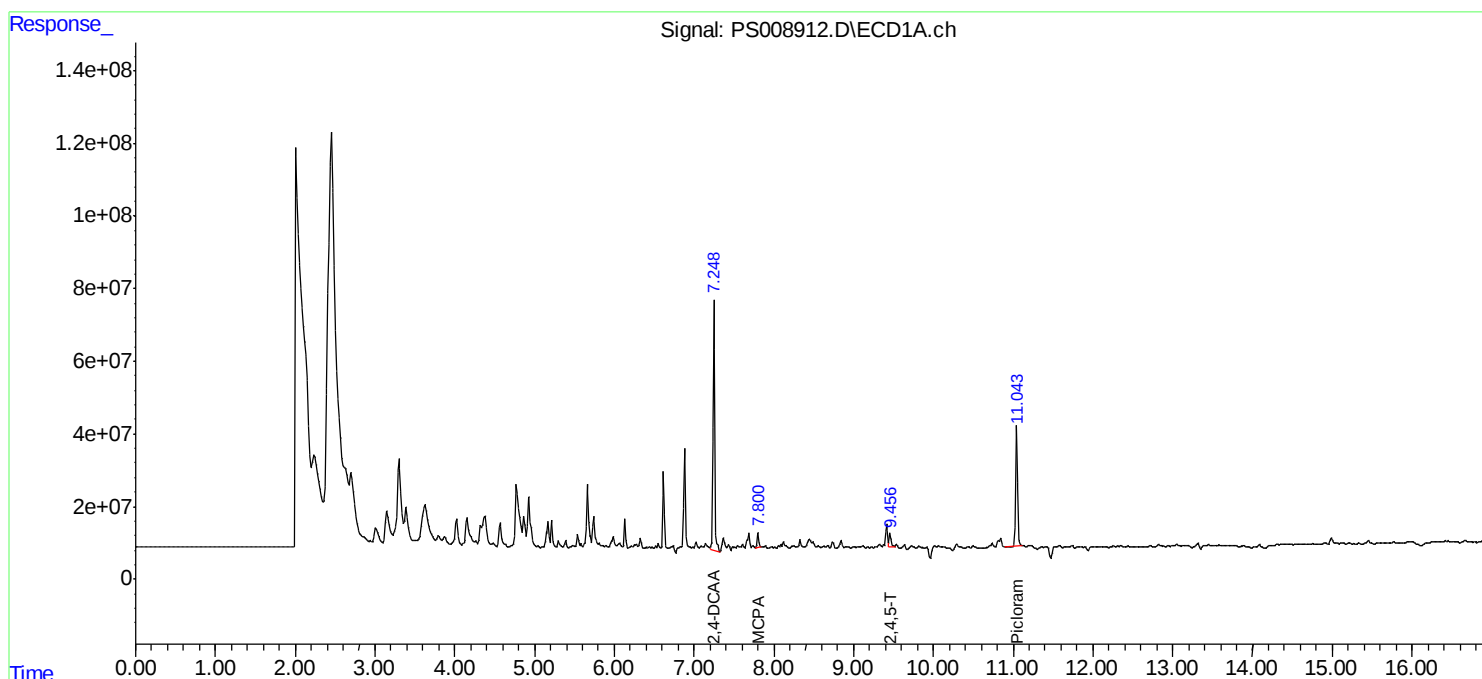


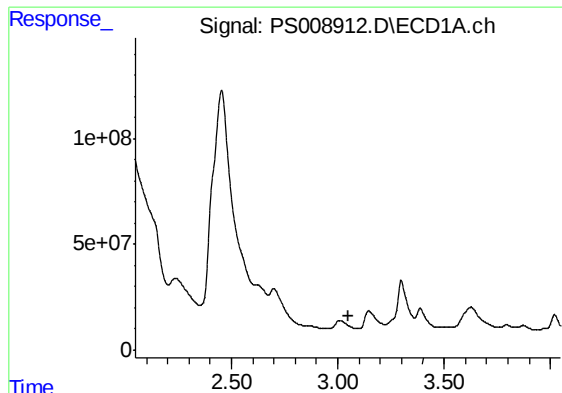

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 3.048 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
FK-SF-01-008-A

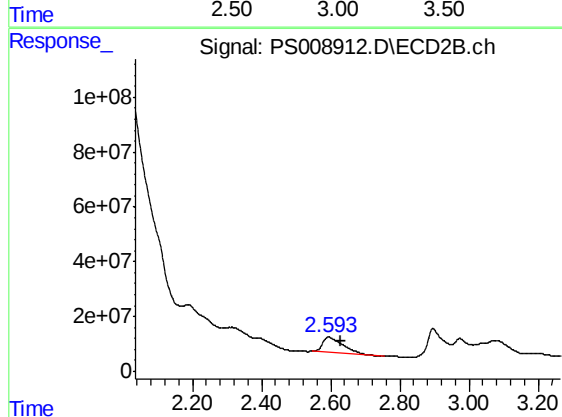


#1 Dalapon

R.T.: 2.594 min
Delta R.T.: -0.036 min
Response: 224775702
Conc: 153.72 ng/ml

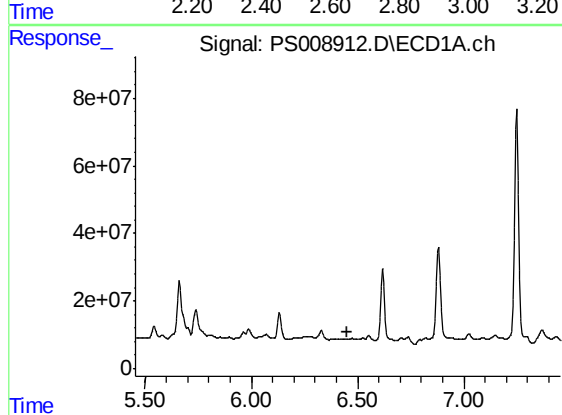


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.455 min
Response: 0
Conc: N.D.

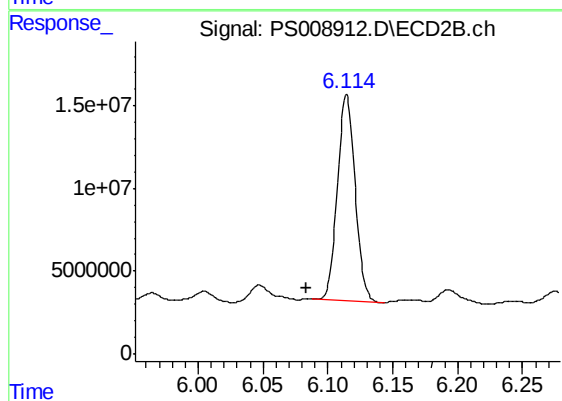

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.114 min
Delta R.T.: 0.031 min
Response: 118545160
Conc: 81.24 ng/ml

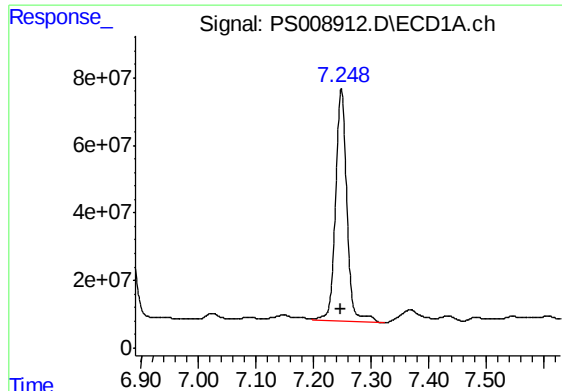

#4 2,4-DCAA


R.T.: 7.248 min
Delta R.T.: 0.001 min
Response: 951633442
Conc: 435.21 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-SF-01-008-A

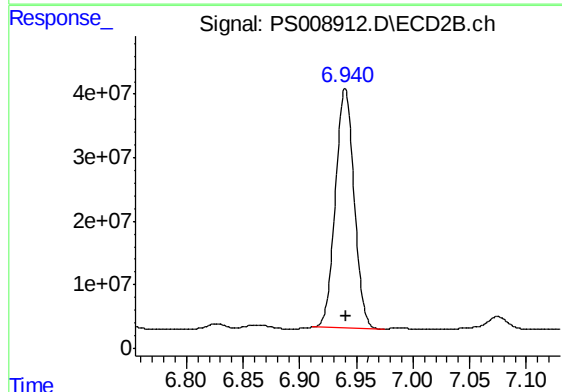


#4 2,4-DCAA

R.T.: 6.940 min
Delta R.T.: 0.000 min
Response: 432512704
Conc: 448.87 ng/ml

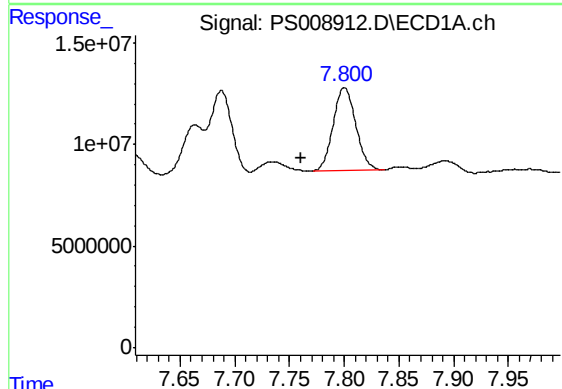


#7 MCPA

R.T.: 7.800 min
Delta R.T.: 0.040 min
Response: 58337261
Conc: 7.25 ug/ml

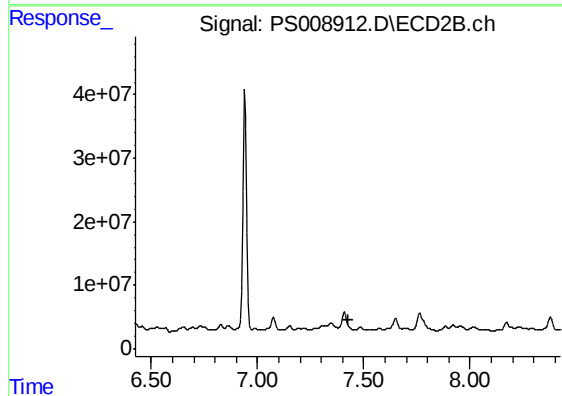

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 7.425 min
Response: 0
Conc: N.D.

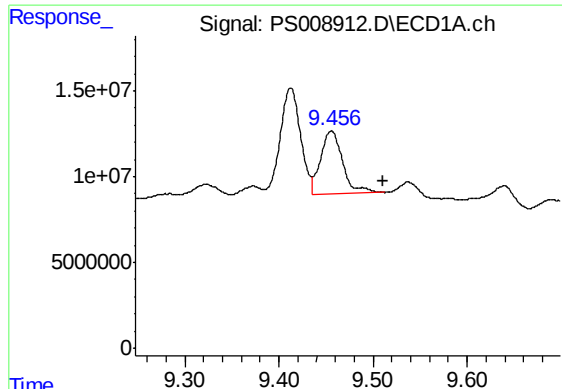

#12 2,4,5-T


R.T.: 9.456 min
Delta R.T.: -0.055 min
Response: 60160091
Conc: 5.63 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-SF-01-008-A

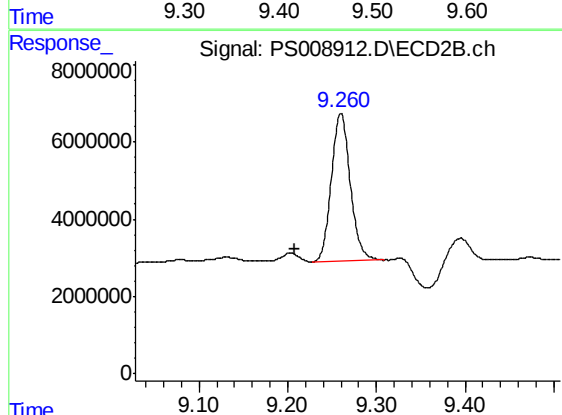


#12 2,4,5-T

R.T.: 9.260 min
Delta R.T.: 0.052 min
Response: 57186930
Conc: 10.56 ng/ml

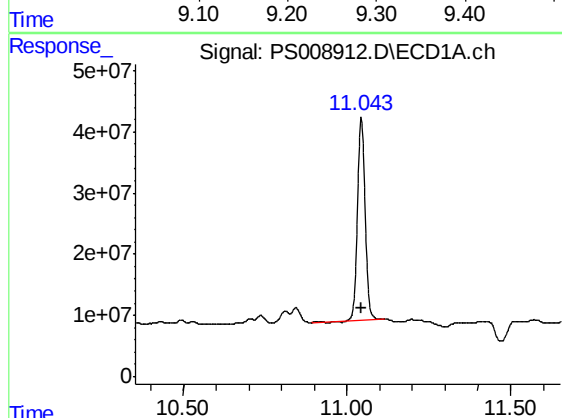


#15 Picloram

R.T.: 11.044 min
Delta R.T.: 0.000 min
Response: 539045166
Conc: 39.37 ng/ml

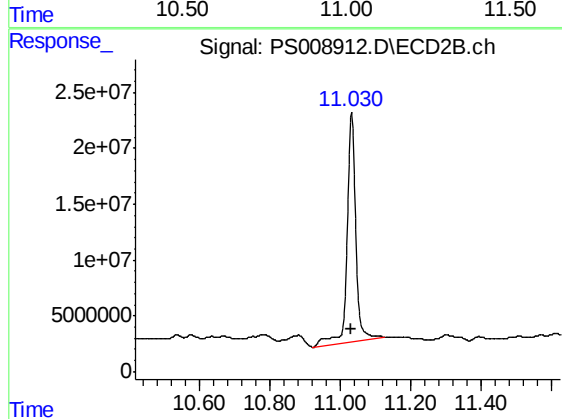

#15 Picloram


R.T.: 11.031 min
Delta R.T.: 0.000 min
Response: 349077770
Conc: 48.04 ng/ml

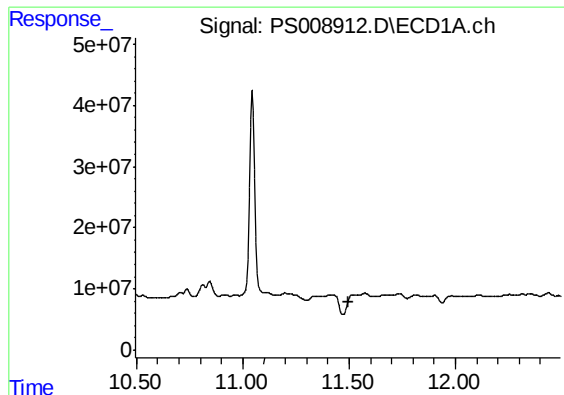

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.495 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
FK-SF-01-008-A

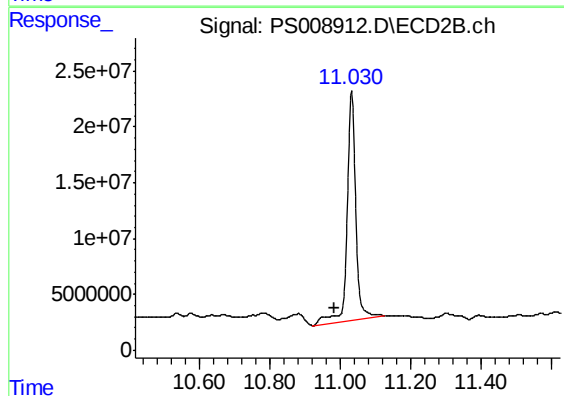

#16 DCPA

R.T.: 11.031 min
Delta R.T.: 0.049 min
Response: 349077770
Conc: 50.45 ng/ml