

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022020\
 Data File : PS008918.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2020 16:29
 Operator : DD\AJ
 Sample : PB126948BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB126948BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 20 17:12:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.247	6.940	1052.7E6	498.8E6	481.442	517.658
Target Compounds							
1) T	Dalapon	0.000	2.591	0	210.0E6	N.D.	143.616
2) T	3,5-DICHL...	0.000	6.114	0	116.7E6	N.D.	79.995
7) T	MCPA	7.800	0.000	62843417	0	7.813	N.D. #
15) T	Picloram	11.043	11.031	230.5E6	153.8E6	16.833	21.160 #
16) T	DCPA	0.000	11.031	0	153.8E6	N.D.	22.221



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022020\
Data File : PS008918.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2020 16:29
Operator : DD\AJ
Sample : PB126948BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB126948BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 20 17:12:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

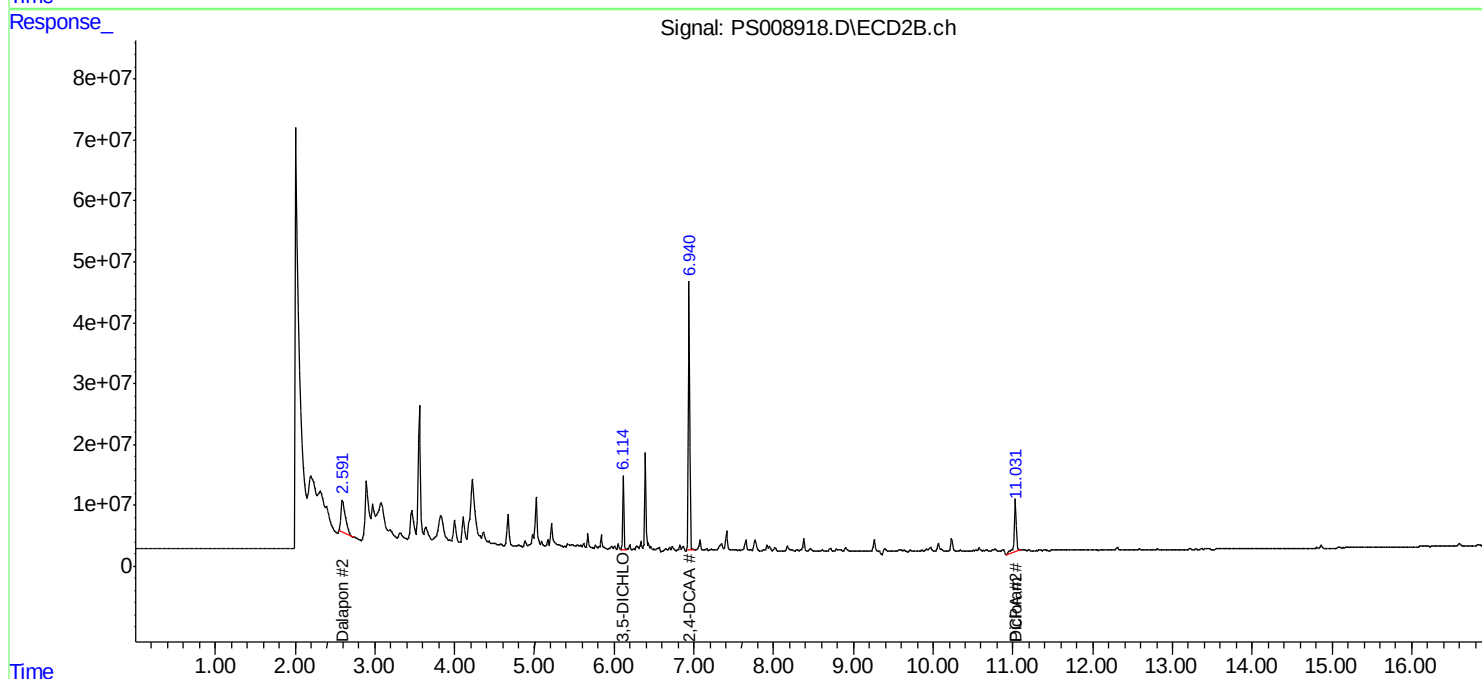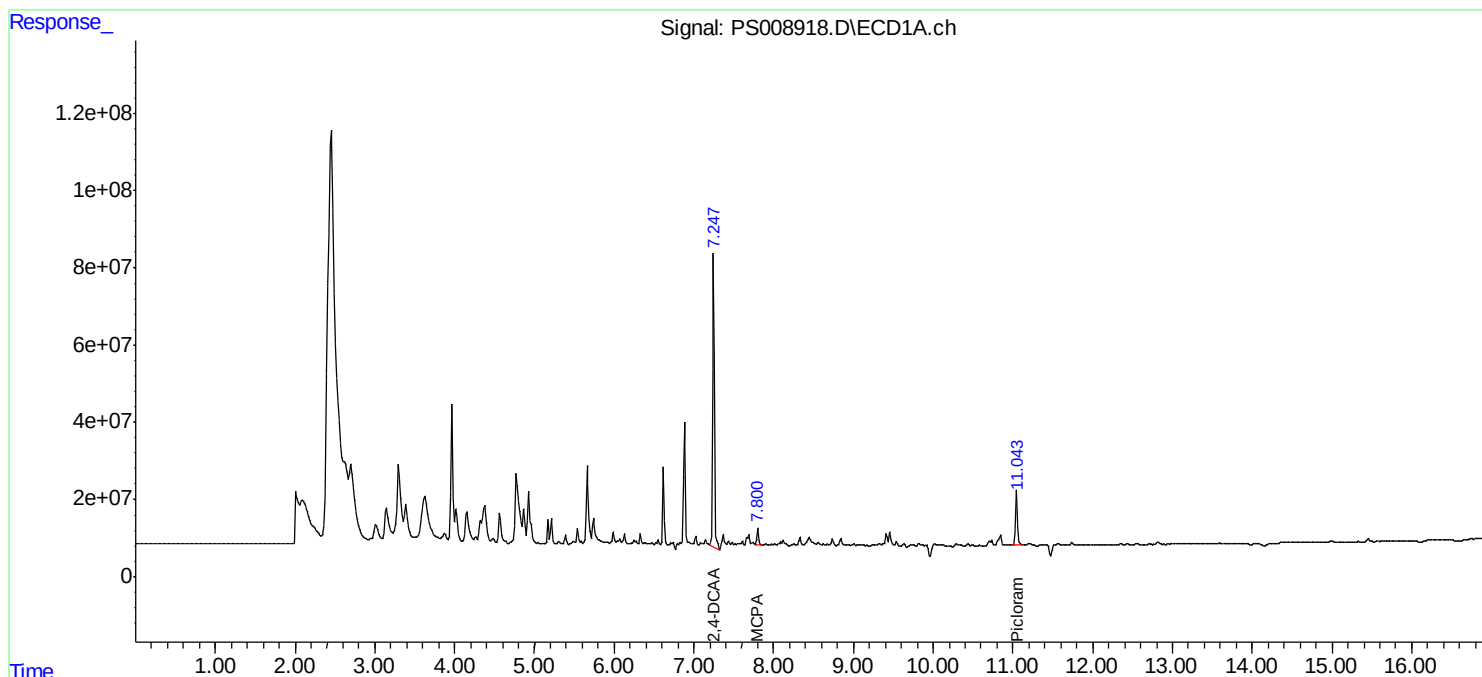


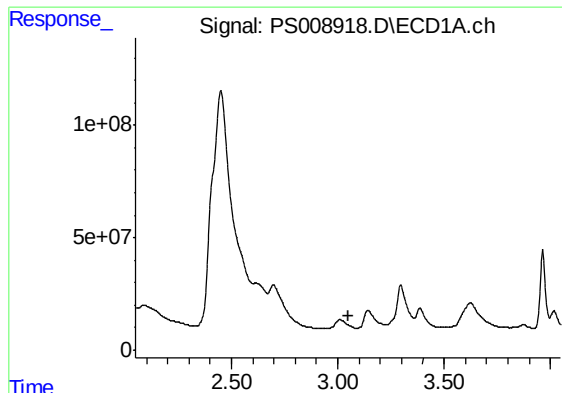

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 3.048 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB126948BL

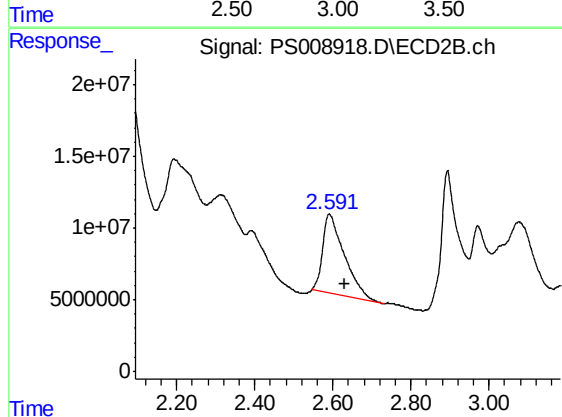


#1 Dalapon

R.T.: 2.591 min
Delta R.T.: -0.039 min
Response: 209998751
Conc: 143.62 ng/ml

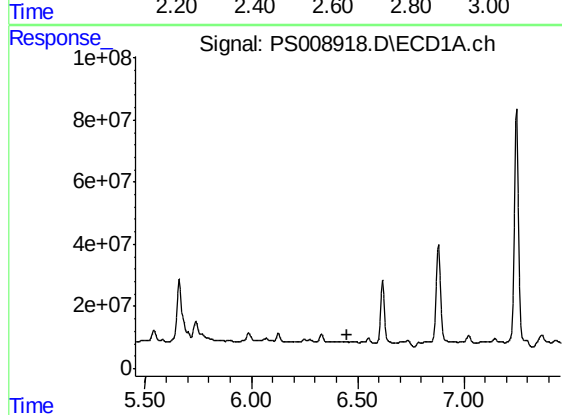


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.455 min
Response: 0
Conc: N.D.

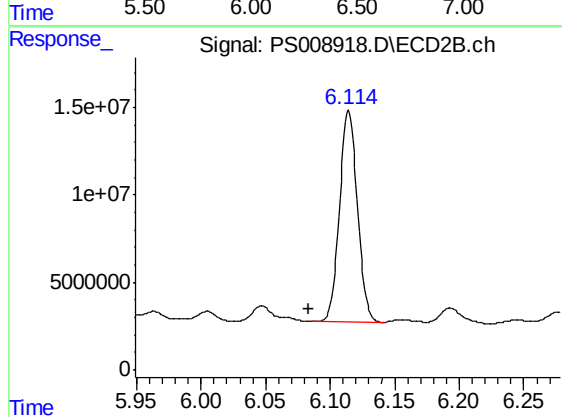

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.114 min
Delta R.T.: 0.031 min
Response: 116735021
Conc: 80.00 ng/ml

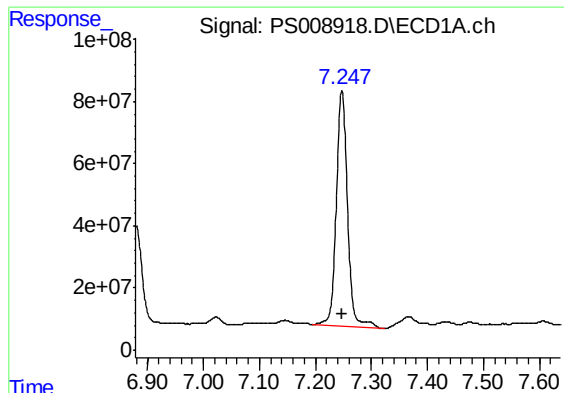

#4 2,4-DCAA


R.T.: 7.247 min
Delta R.T.: 0.000 min
Response: 1052717060
Conc: 481.44 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB126948BL

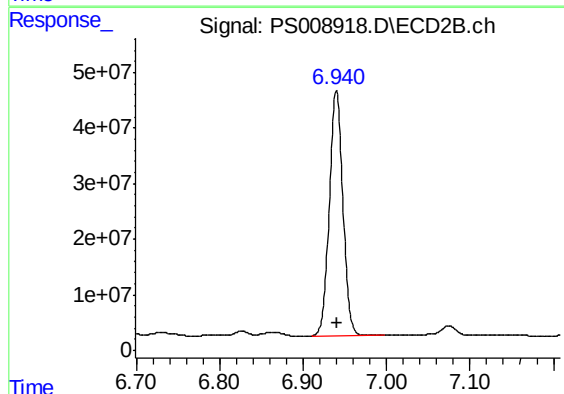


#4 2,4-DCAA

R.T.: 6.940 min
Delta R.T.: 0.000 min
Response: 498791847
Conc: 517.66 ng/ml

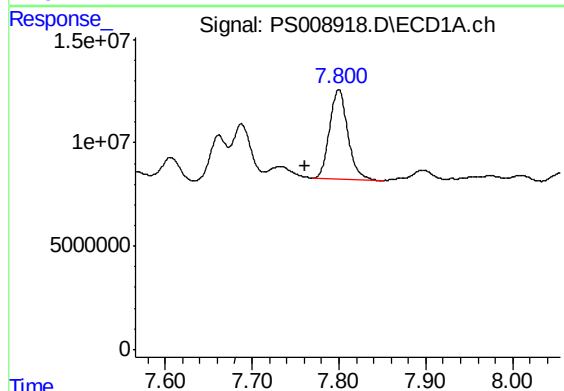


#7 MCPA

R.T.: 7.800 min
Delta R.T.: 0.039 min
Response: 62843417
Conc: 7.81 ug/ml

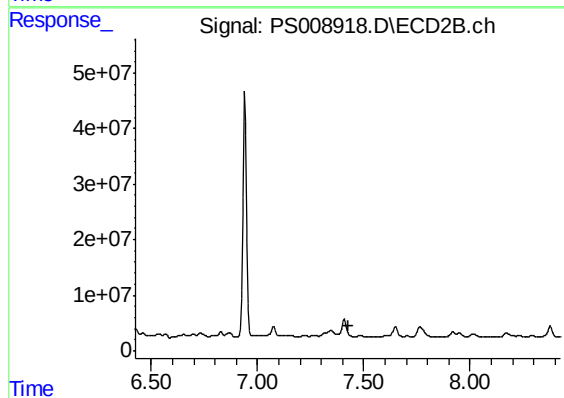

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 7.425 min
Response: 0
Conc: N.D.

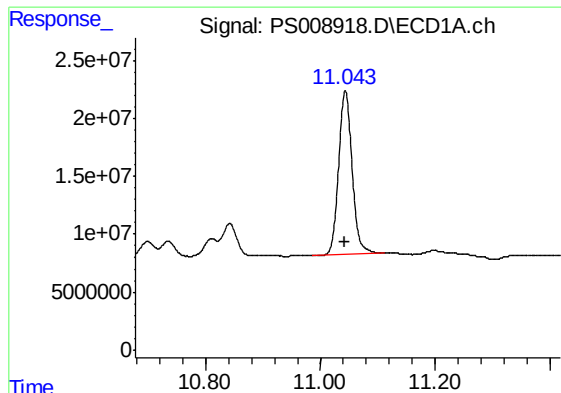

#15 Picloram


R.T.: 11.043 min
Delta R.T.: 0.000 min
Response: 230459169
Conc: 16.83 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB126948BL

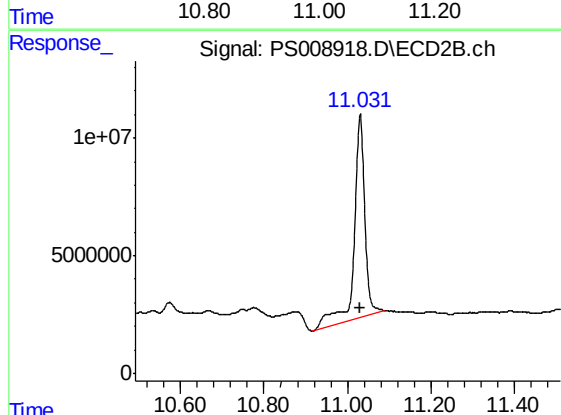


#15 Picloram

R.T.: 11.031 min
Delta R.T.: 0.000 min
Response: 153756958
Conc: 21.16 ng/ml

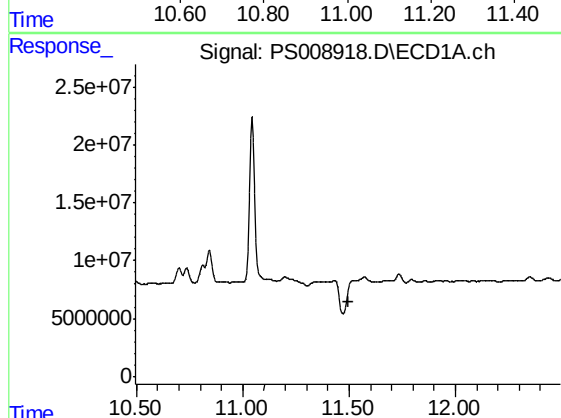

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.495 min
Response: 0
Conc: N.D.

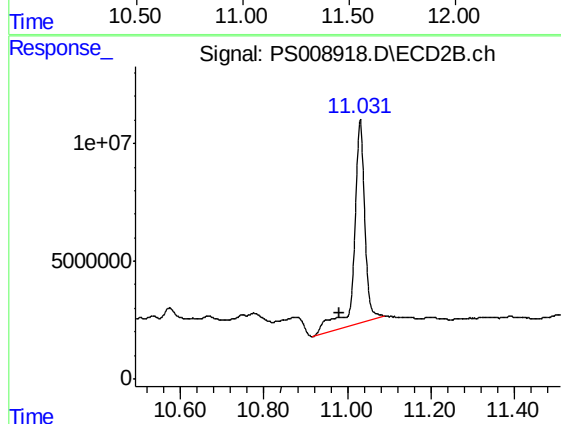

#16 DCPA

R.T.: 11.031 min
Delta R.T.: 0.048 min
Response: 153756958
Conc: 22.22 ng/ml