

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS022020\  
 Data File : PS008921.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 20 Feb 2020 17:38  
 Operator : DD\AJ  
 Sample : L1362-03  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Feb 21 01:25:44 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS022020.M  
 Quant Title : 8080.M  
 QLast Update : Thu Feb 20 11:30:26 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound     | RT#1  | RT#2  | Resp#1   | Resp#2   | ng/ml   | ng/ml   |
|-----------------------------|--------------|-------|-------|----------|----------|---------|---------|
| -----                       |              |       |       |          |          |         |         |
| System Monitoring Compounds |              |       |       |          |          |         |         |
| 4) S                        | 2,4-DCAA     | 7.247 | 6.940 | 980.8E6  | 510.1E6  | 448.539 | 529.360 |
| Target Compounds            |              |       |       |          |          |         |         |
| 1) T                        | Dalapon      | 0.000 | 2.591 | 0        | 252.7E6  | N.D.    | 172.791 |
| 2) T                        | 3,5-DICHL... | 0.000 | 6.115 | 0        | 185.8E6  | N.D.    | 127.291 |
| 5) T                        | DICAMBA      | 0.000 | 7.075 | 0        | 47601357 | N.D.    | 11.500  |
| 6) T                        | MCP          | 7.663 | 0.000 | 25854986 | 0        | 4.299   | N.D. #  |
| 12) T                       | 2,4,5-T      | 9.453 | 0.000 | 104.5E6  | 0        | 9.777   | N.D. #  |
| -----                       |              |       |       |          |          |         |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS022020\  
Data File : PS008921.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 20 Feb 2020 17:38  
Operator : DD\AJ  
Sample : L1362-03  
Misc :  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Feb 21 01:25:44 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS022020.M  
Quant Title : 8080.M  
QLast Update : Thu Feb 20 11:30:26 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

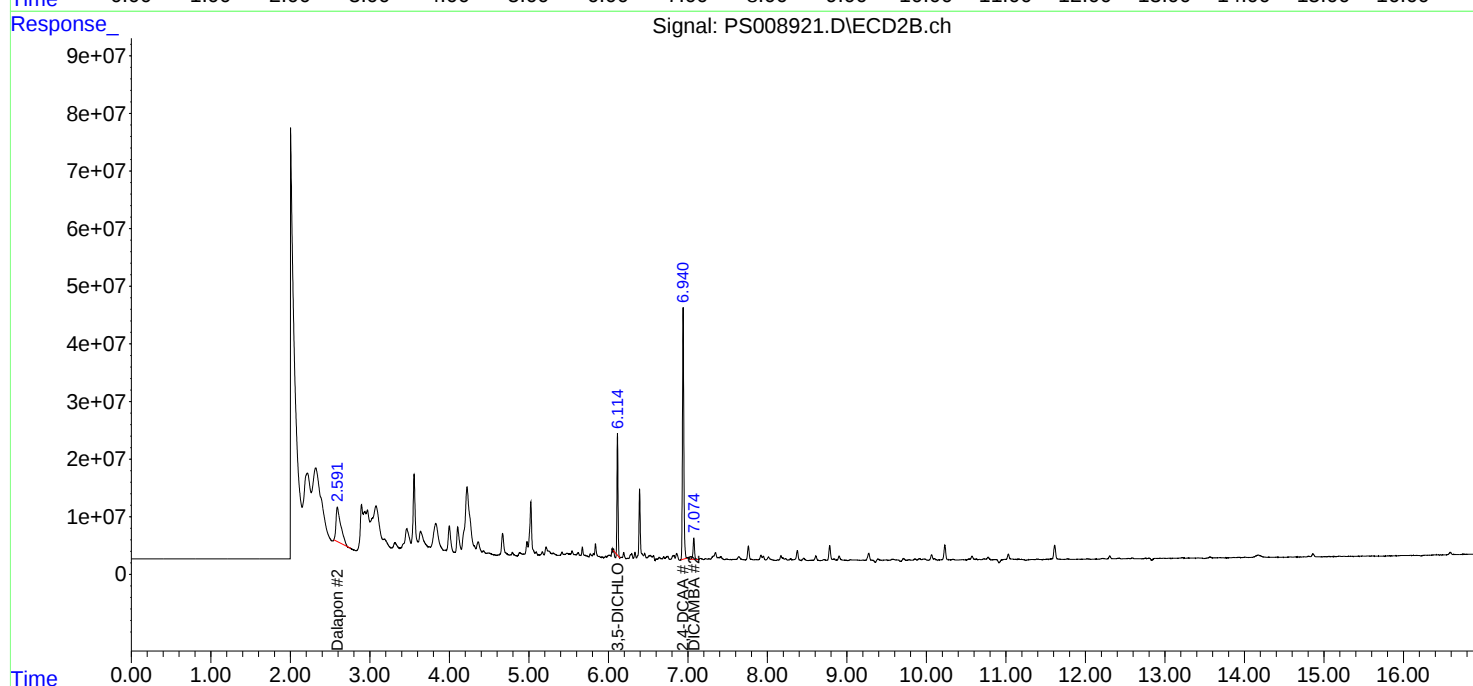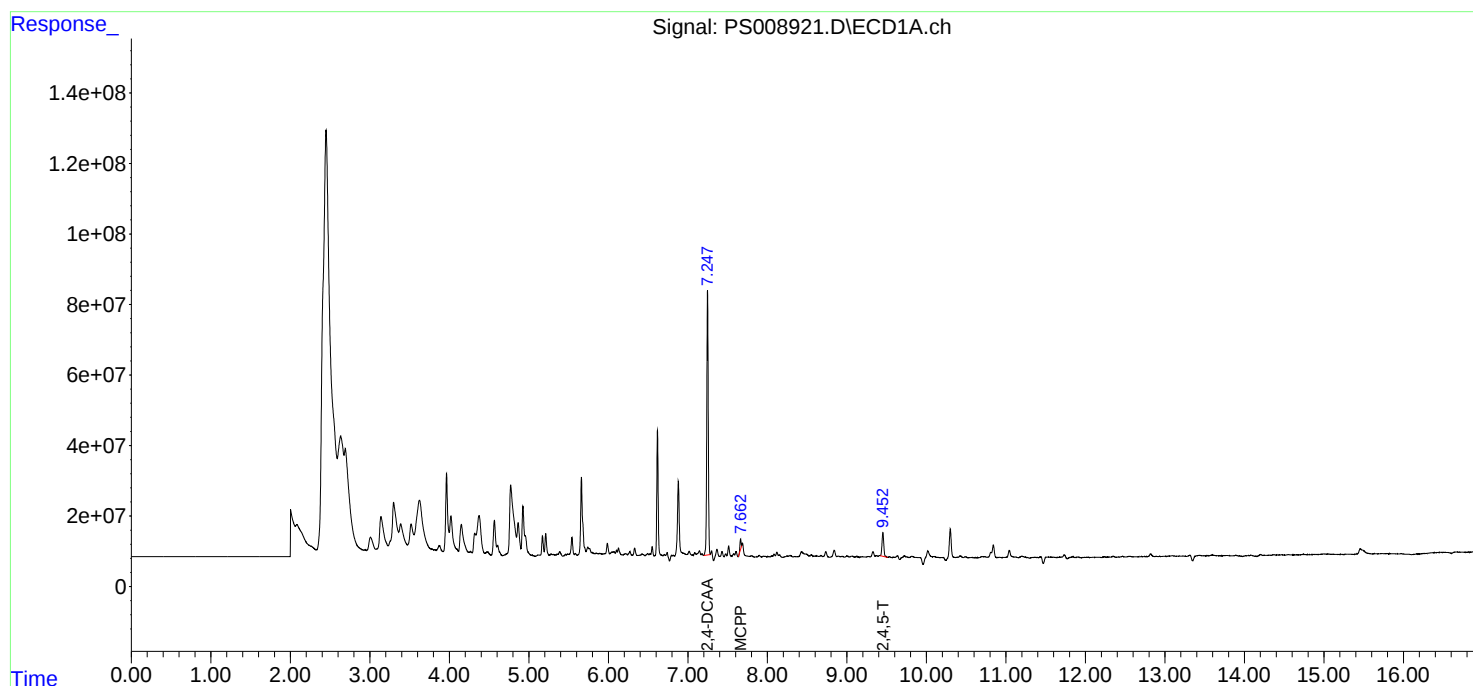


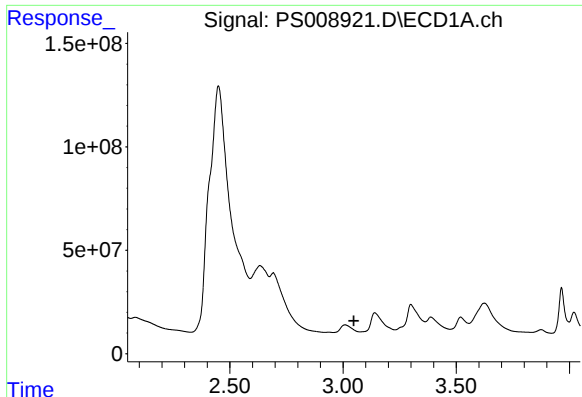

#1 Dalapon


R.T.: 0.000 min  
Exp R.T.: 3.048 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :

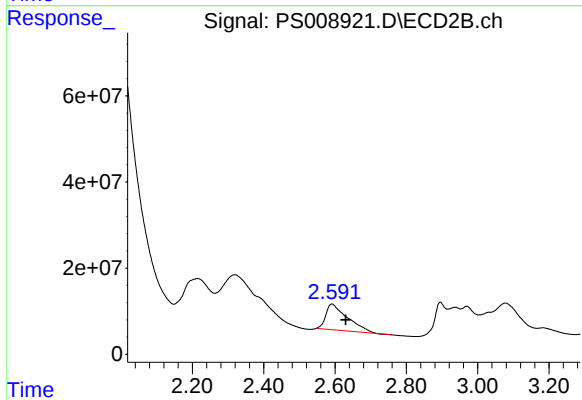


#1 Dalapon

R.T.: 2.591 min  
Delta R.T.: -0.039 min  
Response: 252659227  
Conc: 172.79 ng/ml

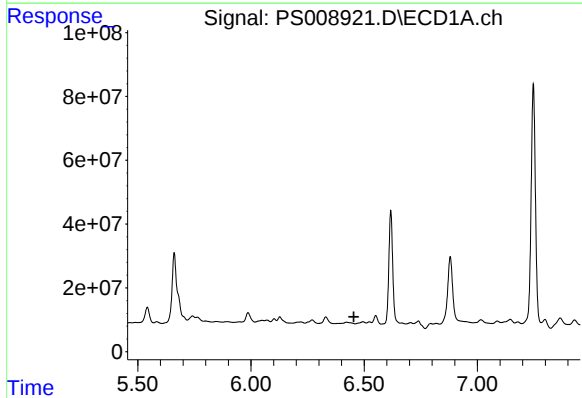


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min  
Exp R.T.: 6.455 min  
Response: 0  
Conc: N.D.

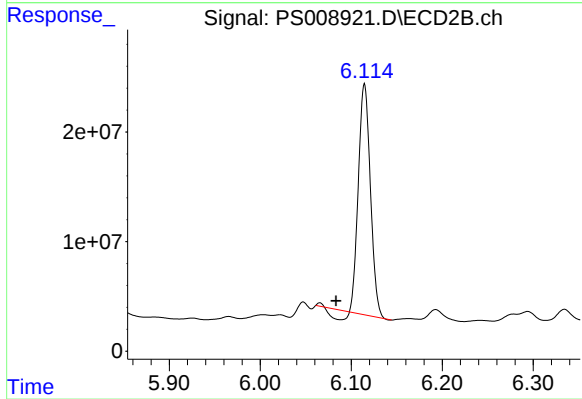

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.115 min  
Delta R.T.: 0.031 min  
Response: 185751394  
Conc: 127.29 ng/ml

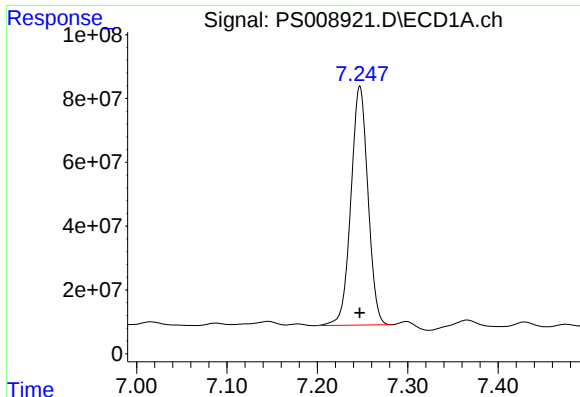

#4 2,4-DCAA


R.T.: 7.247 min  
Delta R.T.: 0.000 min  
Response: 980772419  
Conc: 448.54 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

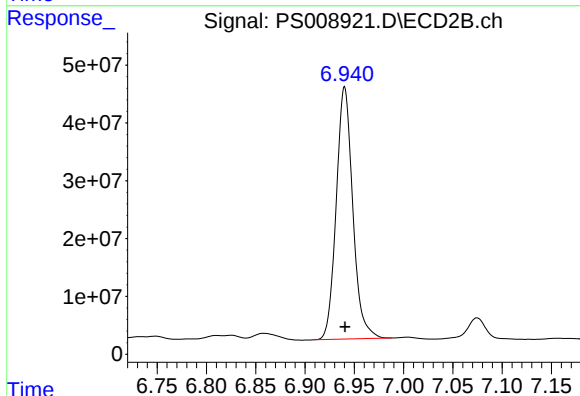


#4 2,4-DCAA

R.T.: 6.940 min  
Delta R.T.: 0.000 min  
Response: 510067629  
Conc: 529.36 ng/ml

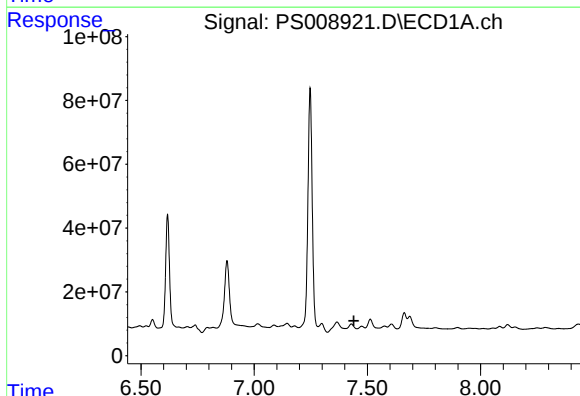


#5 DICAMBA

R.T.: 0.000 min  
Exp R.T. : 7.440 min  
Response: 0  
Conc: N.D.

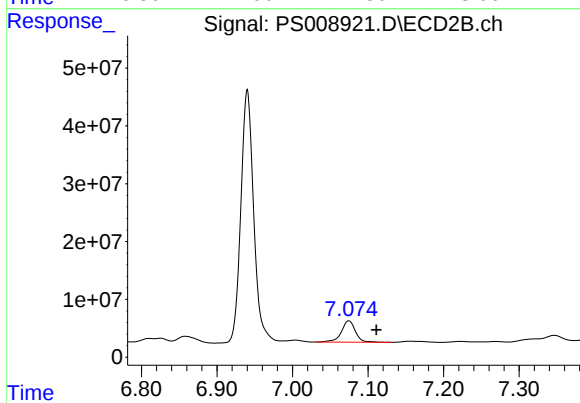

#5 DICAMBA


R.T.: 7.075 min  
Delta R.T.: -0.037 min  
Response: 47601357  
Conc: 11.50 ng/ml

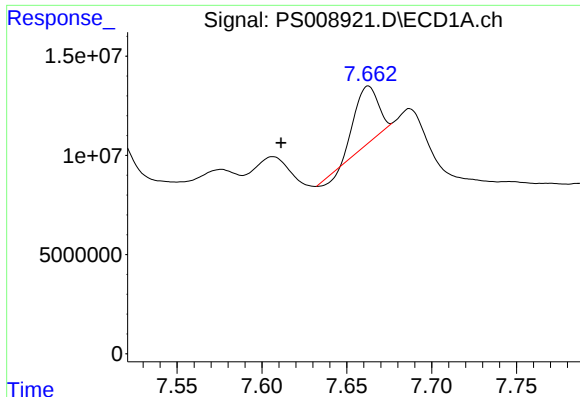

#6 MCP


R.T.: 7.663 min  
Delta R.T.: 0.051 min  
Response: 25854986  
Conc: 4.30 ug/ml

Instrument :  
ECD\_S  
ClientSampleId :

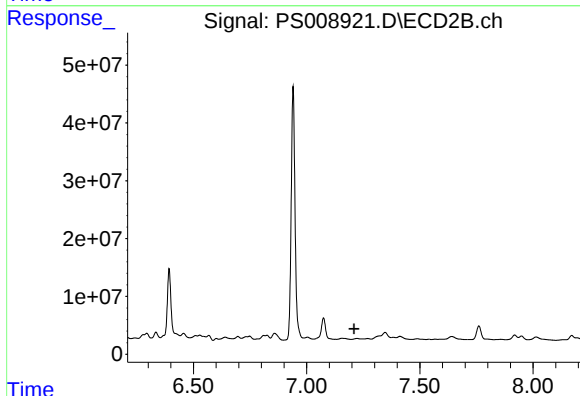


#6 MCP

R.T.: 0.000 min  
Exp R.T. : 7.209 min  
Response: 0  
Conc: N.D.

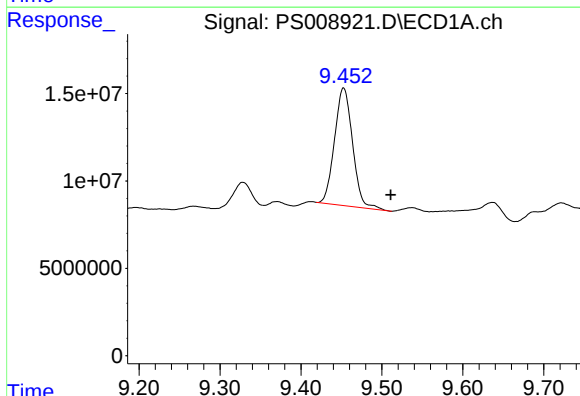

#12 2,4,5-T

R.T.: 9.453 min  
Delta R.T.: -0.058 min  
Response: 104539164  
Conc: 9.78 ng/ml

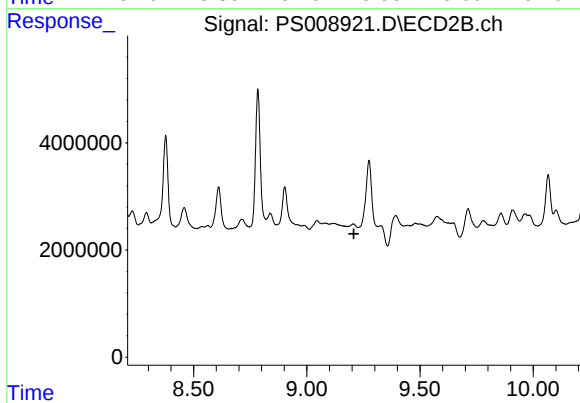

#12 2,4,5-T

R.T.: 0.000 min  
Exp R.T. : 9.208 min  
Response: 0  
Conc: N.D.