

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022020\
 Data File : PS008924.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2020 18:46
 Operator : DD\AJ
 Sample : L1573-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 01:26:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.247	6.940	1051.2E6	533.6E6	480.750	553.756
Target Compounds							
1) T	Dalapon	0.000	2.591	0	259.8E6	N.D.	177.647
2) T	3,5-DICHL...	0.000	6.115	0	187.7E6	N.D.	128.615
5) T	DICAMBA	0.000	7.074	0	45280261	N.D.	10.939
6) T	MCP	7.662	0.000	22954047	0	3.816	N.D. #
11) T	2,4,5-TP ...	0.000	8.784	0	49810268	N.D.	9.195
12) T	2,4,5-T	9.452	0.000	126.8E6	0	11.862	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022020\
Data File : PS008924.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2020 18:46
Operator : DD\AJ
Sample : L1573-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 01:26:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

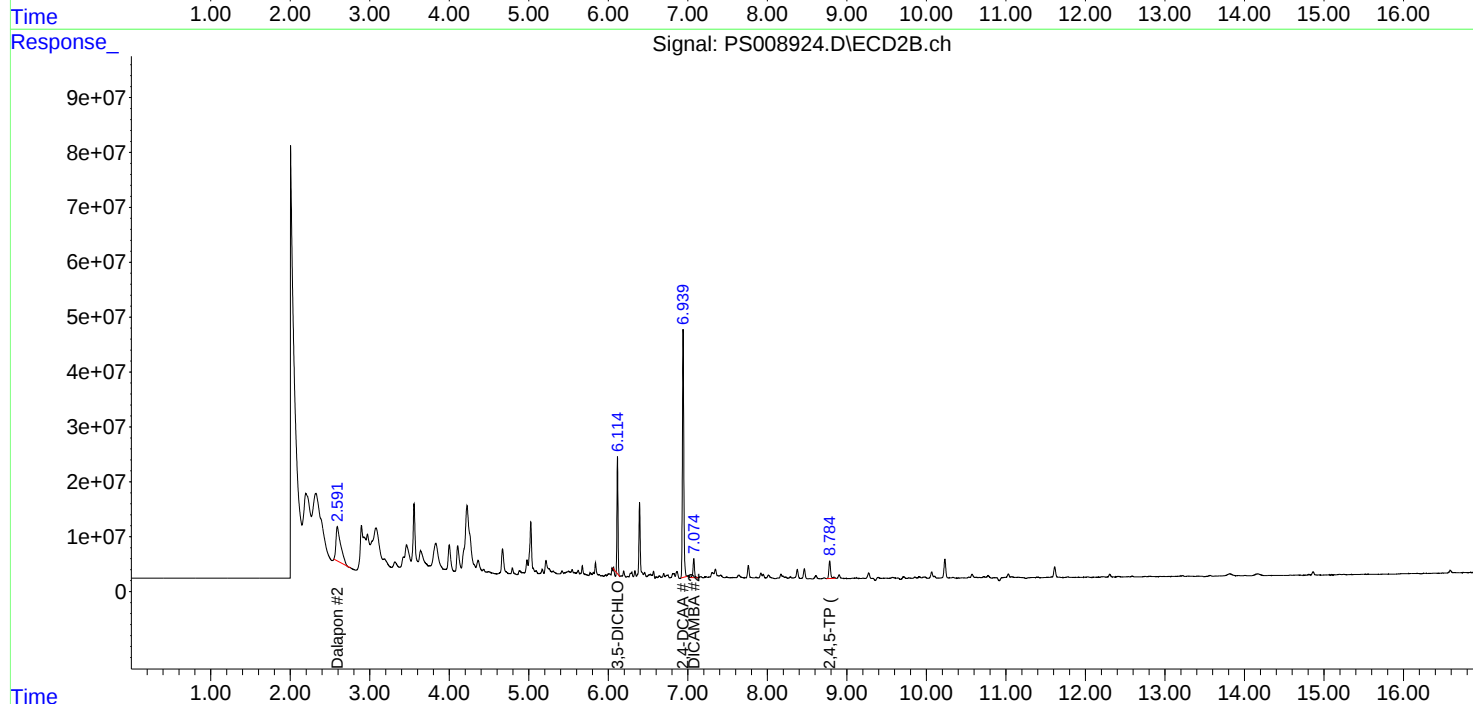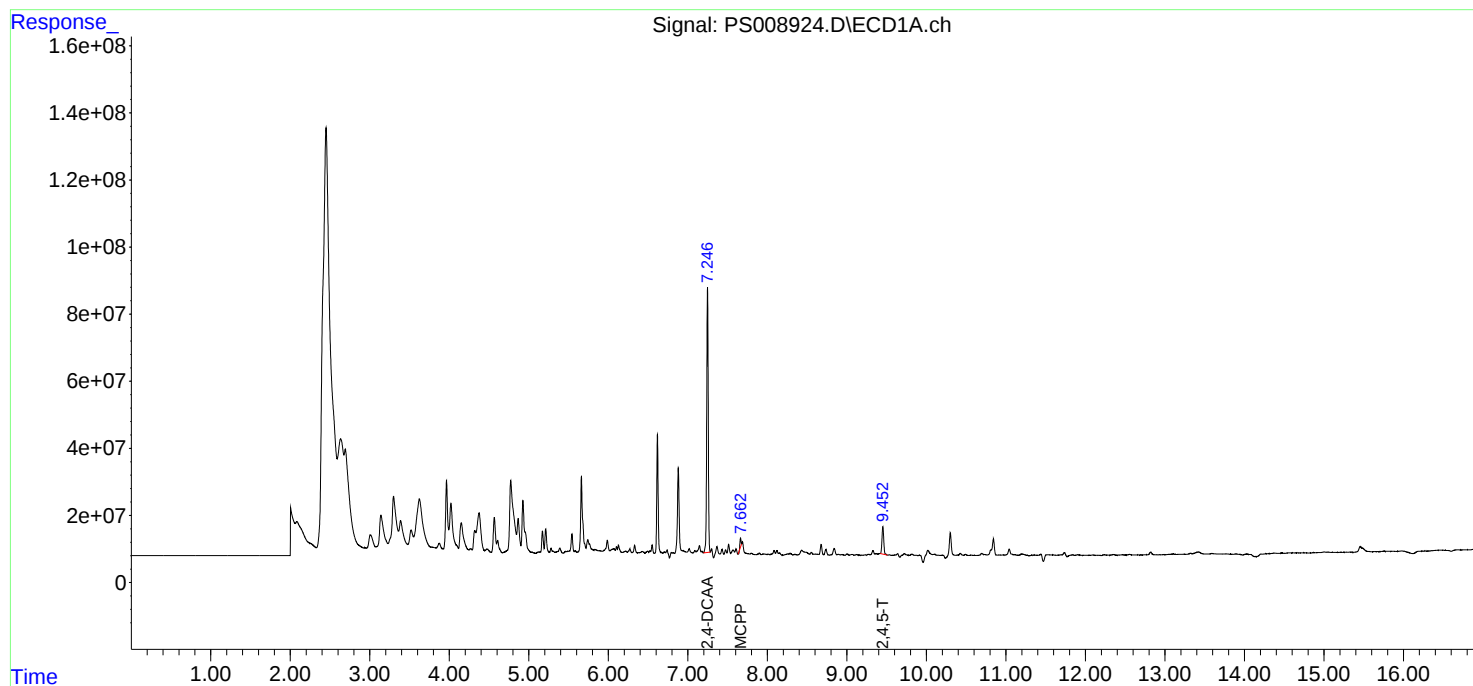


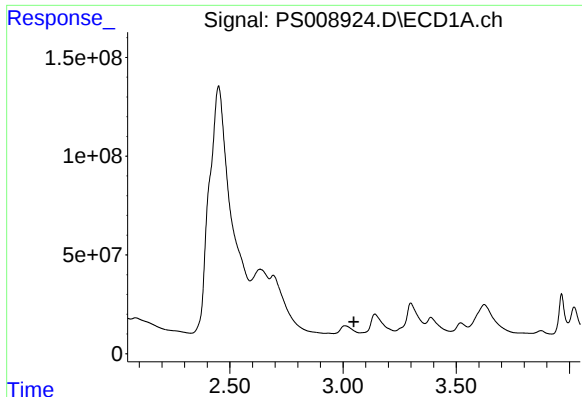

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.048 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

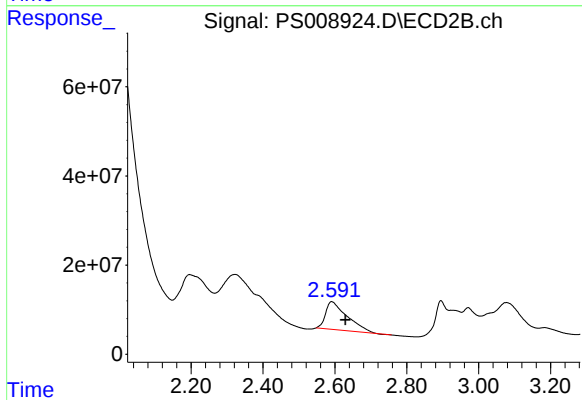


#1 Dalapon

R.T.: 2.591 min
Delta R.T.: -0.038 min
Response: 259759781
Conc: 177.65 ng/ml

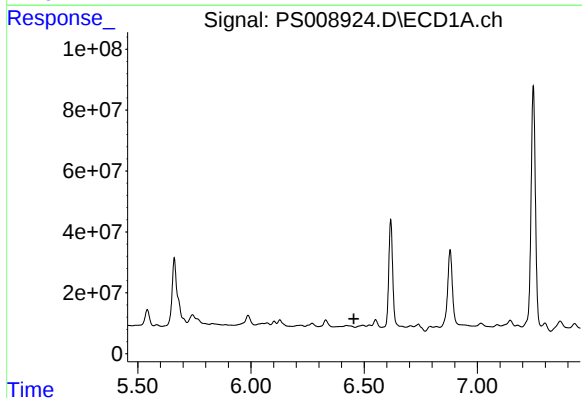


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

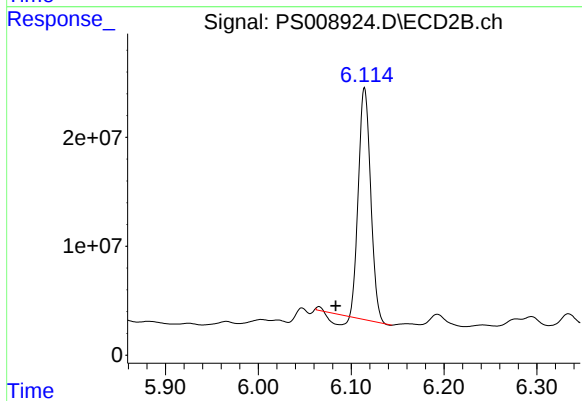

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.115 min
Delta R.T.: 0.031 min
Response: 187683368
Conc: 128.61 ng/ml

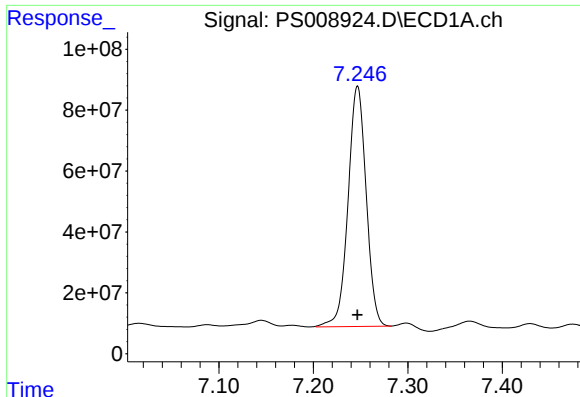

#4 2,4-DCAA


R.T.: 7.247 min
Delta R.T.: 0.000 min
Response: 1051203138
Conc: 480.75 ng/ml

Instrument :
ECD_S
ClientSampleId :

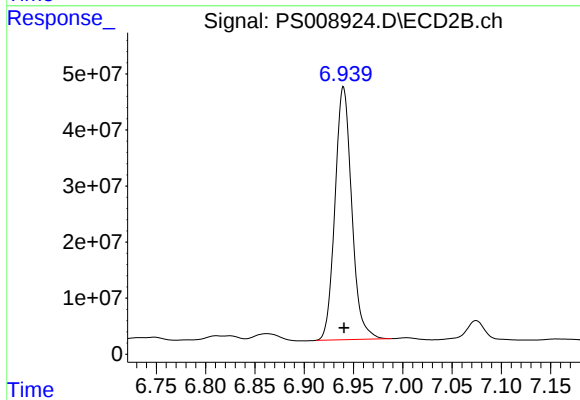


#4 2,4-DCAA

R.T.: 6.940 min
Delta R.T.: 0.000 min
Response: 533574507
Conc: 553.76 ng/ml

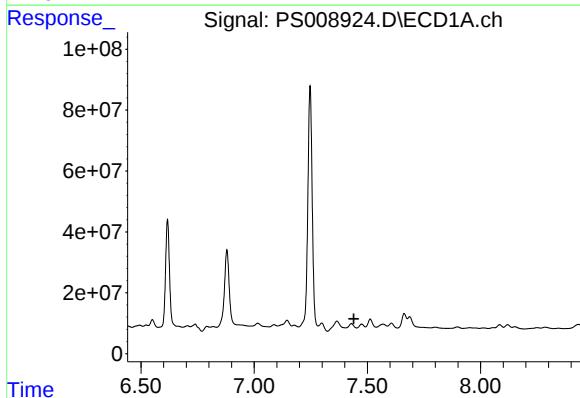


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.440 min
Response: 0
Conc: N.D.

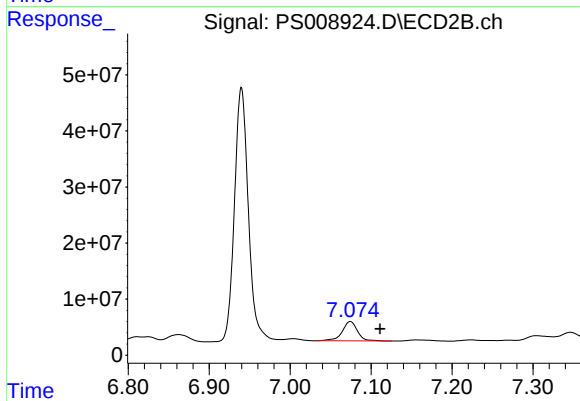

#5 DICAMBA


R.T.: 7.074 min
Delta R.T.: -0.037 min
Response: 45280261
Conc: 10.94 ng/ml

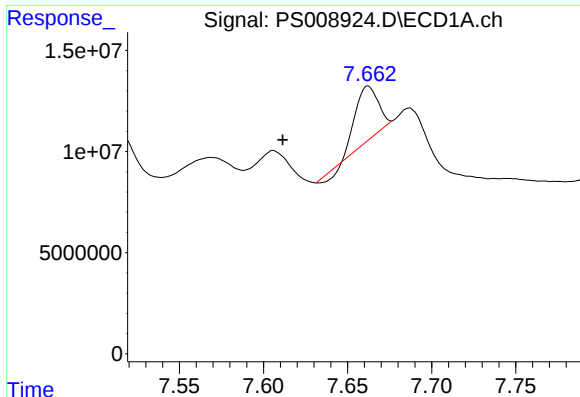

#6 MCP


R.T.: 7.662 min
Delta R.T.: 0.051 min
Response: 22954047
Conc: 3.82 ug/ml

Instrument :
ECD_S
ClientSampleId :

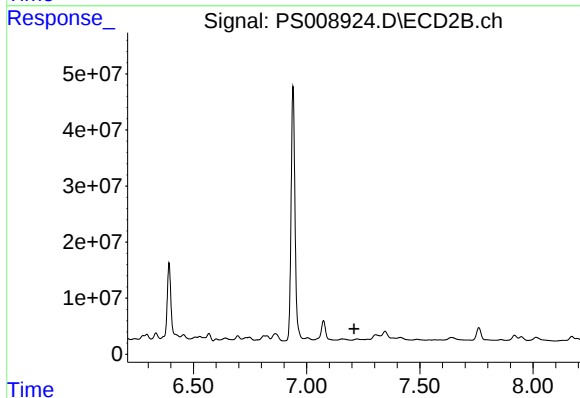


#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.209 min
Response: 0
Conc: N.D.

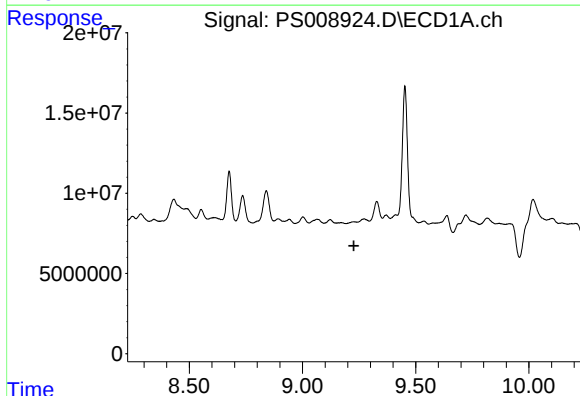


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.227 min
Response: 0
Conc: N.D.

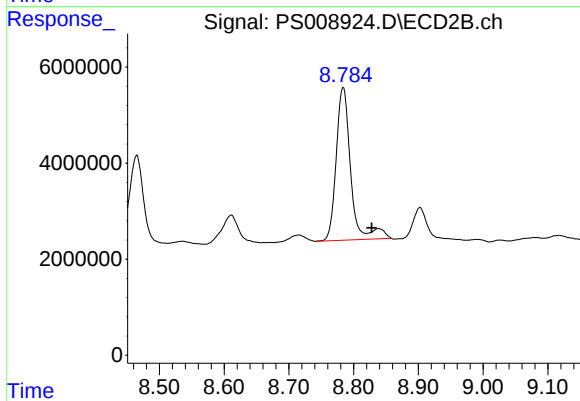

#11 2,4,5-TP (SILVEX)


R.T.: 8.784 min
Delta R.T.: -0.044 min
Response: 49810268
Conc: 9.20 ng/ml

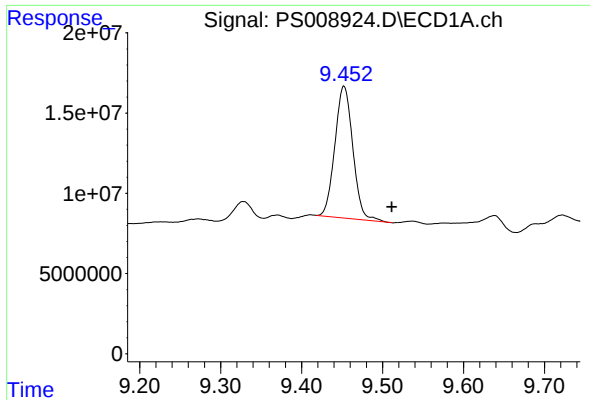

#12 2,4,5-T

R.T.: 9.452 min
Delta R.T.: -0.059 min
Response: 126829271
Conc: 11.86 ng/ml

Instrument :
ECD_S
ClientSampleId :

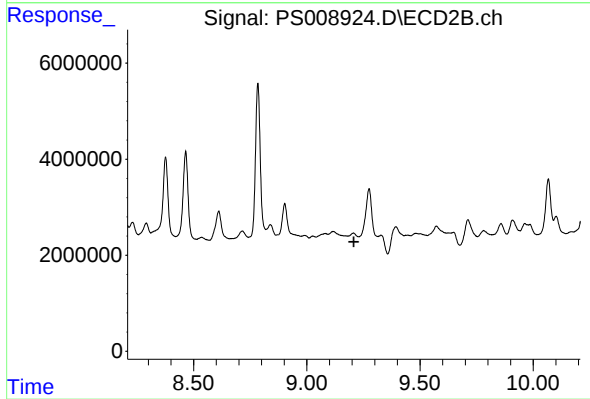

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.208 min
Response: 0
Conc: N.D.