

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022023\
 Data File : PS022197.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2023 10:35
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 20 16:05:37 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022023.M
 Quant Title : 8080.M
 QLast Update : Mon Feb 20 13:26:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	6.304	0.000	438314	0	<MDL	N.D.	#
Target Compounds								
1) T	Dalapon	2.452f	2.526f	1062494	732552	<MDL	<MDL	#
2) T	3,5-DICHL...	5.697	0.000	5346958	0	1.438	N.D.	#
3) T	4-Nitroph...	6.192f	0.000	409146	0	<MDL	N.D.	#
5) T	DICAMBA	0.000	6.951f	0	5784866	N.D.	<MDL	#
6) T	MCPD	6.517f	6.951	159750	5784866	<MDL	<MDL	#
7) T	MCPA	0.000	7.168	0	6909481	N.D.	<MDL	#
8) T	DICHLORPROP	7.011	0.000	74904	0	<MDL	N.D.	#
10) T	Pentachlo...	7.464	0.000	2467355	0	<MDL	N.D.	#
11) T	2,4,5-TP ...	7.962	0.000	275310	0	<MDL	N.D.	#
12) T	2,4,5-T	8.218	0.000	120964	0	<MDL	N.D.	#
13) T	2,4-DB	8.701	0.000	45073	0	<MDL	N.D.	#
14) T	DINOSEB	9.780	0.000	413888	0	<MDL	N.D.	#


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022023\
Data File : PS022197.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2023 10:35
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 20 16:05:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022023.M
Quant Title : 8080.M
QLast Update : Mon Feb 20 13:26:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

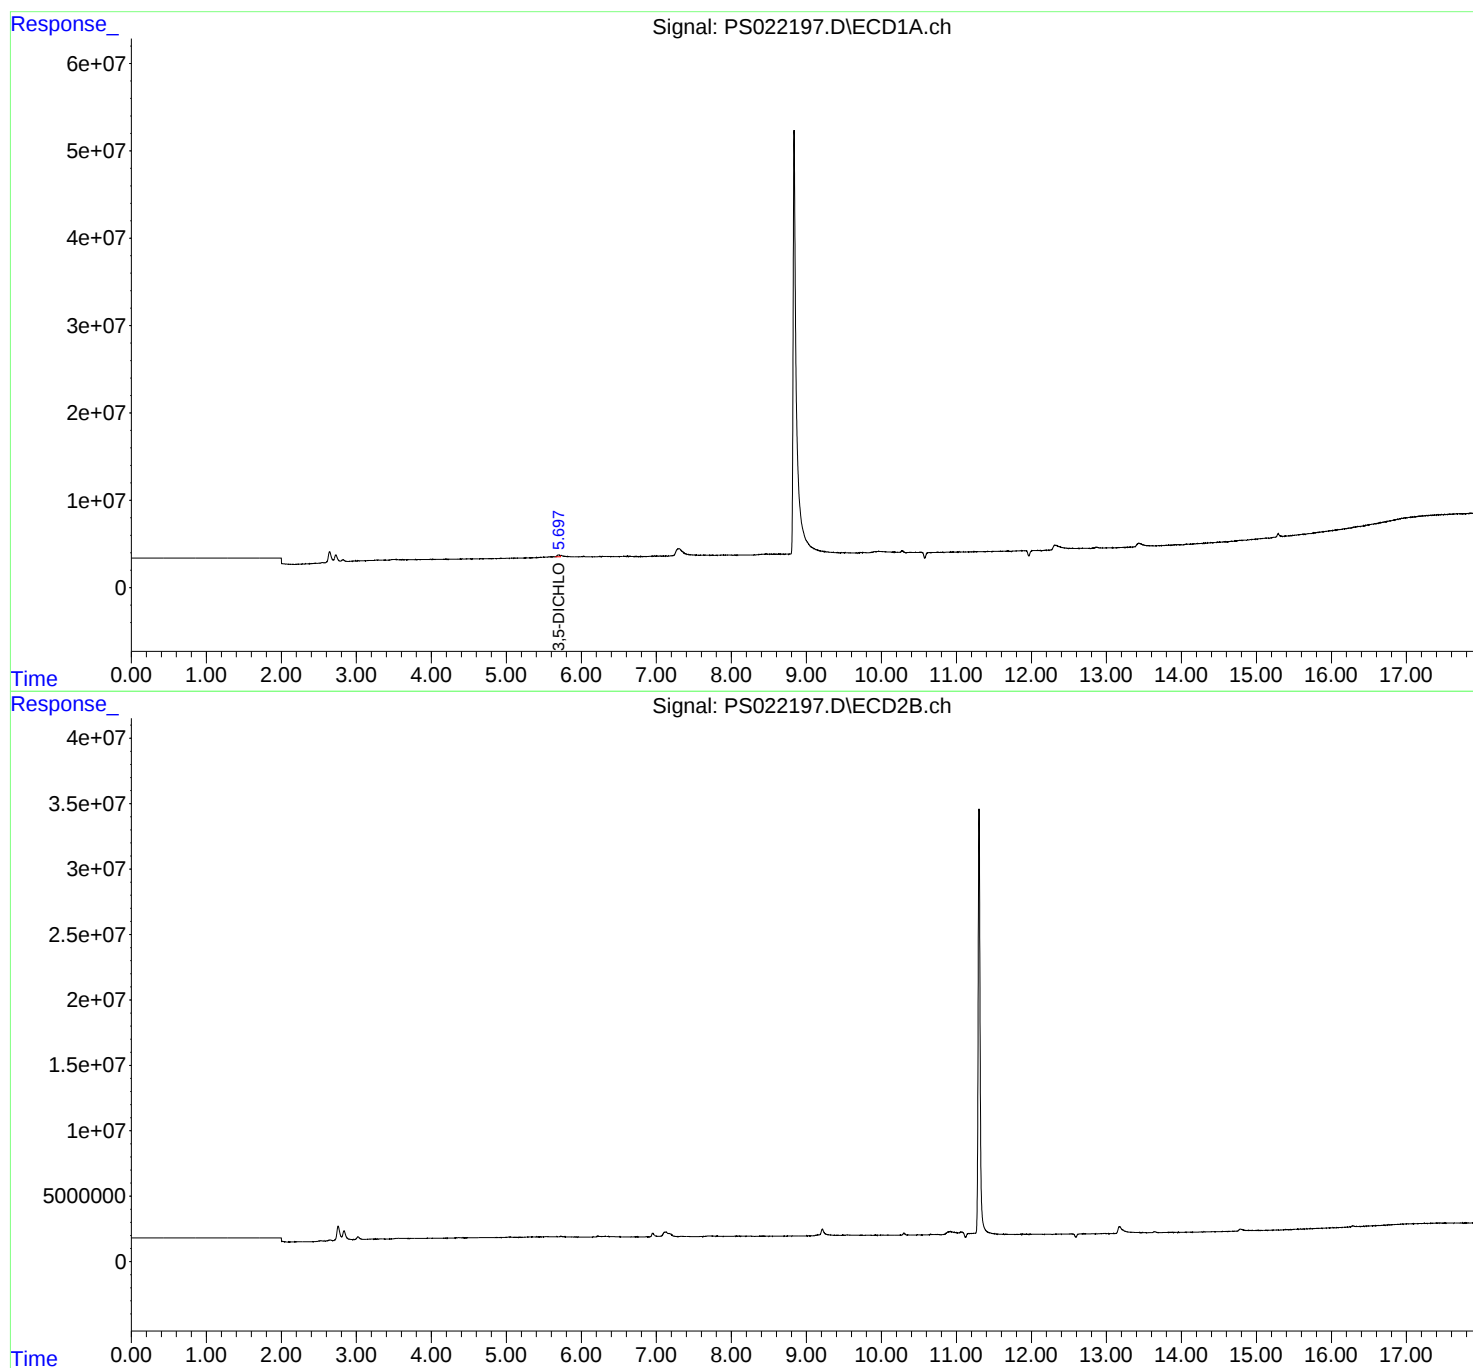


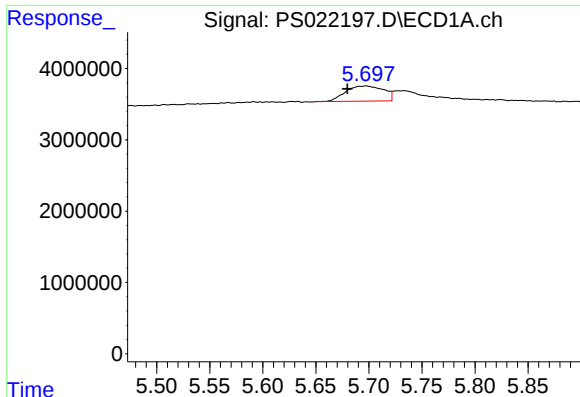

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.697 min
Delta R.T.: 0.018 min
Response: 5346958
Conc: 1.44 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

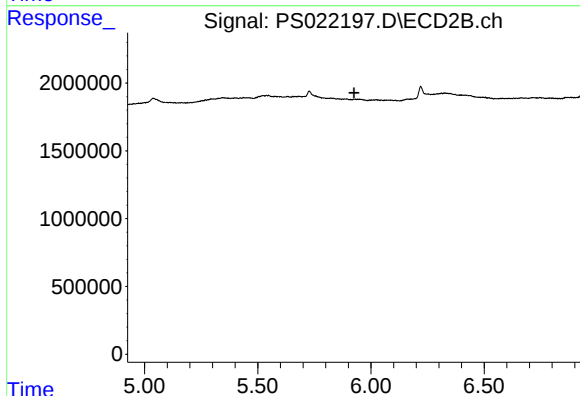


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.925 min
Response: 0
Conc: N.D.

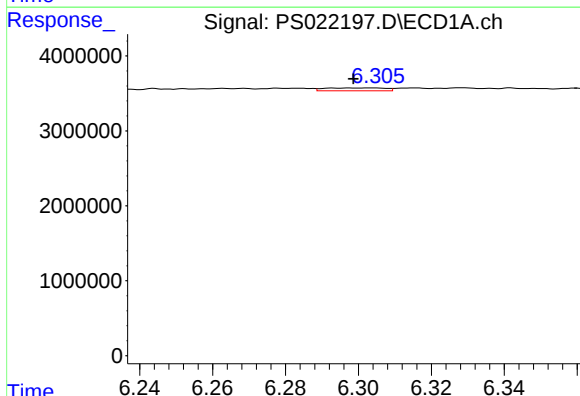

#4 2,4-DCAA

R.T.: 6.304 min
Delta R.T.: 0.005 min
Response: 438314
Conc: N.D.

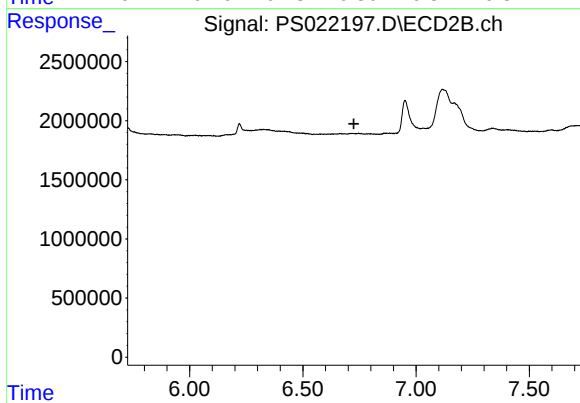

#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.726 min
Response: 0
Conc: N.D.