

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022023\
 Data File : PS022198.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2023 10:59
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 20 16:06:26 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022023.M
 Quant Title : 8080.M
 QLast Update : Mon Feb 20 13:26:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.306	6.729	1226.6E6	1175.0E6	494.866	559.807
Target Compounds							
1) T	Dalapon	2.457f	2.522	1016791	1224990	<MDL	<MDL #
2) T	3,5-DICHL...	5.692	0.000	490240	0	<MDL	N.D. #
3) T	4-Nitroph...	6.128	0.000	473154	0	<MDL	N.D. #
7) T	MCPA	0.000	7.166	0	13758030	N.D.	1.350
9) T	2,4-D	7.289f	0.000	25856013	0	7.886	N.D. #
10) T	Pentachlo...	7.470	8.226	6836315	6704301	<MDL	<MDL #
11) T	2,4,5-TP ...	7.983	8.625f	957963	2350510	<MDL	<MDL #
12) T	2,4,5-T	8.191	0.000	923625	0	<MDL	N.D. #
14) T	DINOSEB	9.794	9.794	2036554	2944871	<MDL	<MDL #
15) T	Picloram	9.623	10.711	549939	3876481	<MDL	<MDL #
16) T	DCPA	10.057	10.711	5364426	3876481	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022023\
Data File : PS022198.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2023 10:59
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 20 16:06:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022023.M
Quant Title : 8080.M
QLast Update : Mon Feb 20 13:26:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

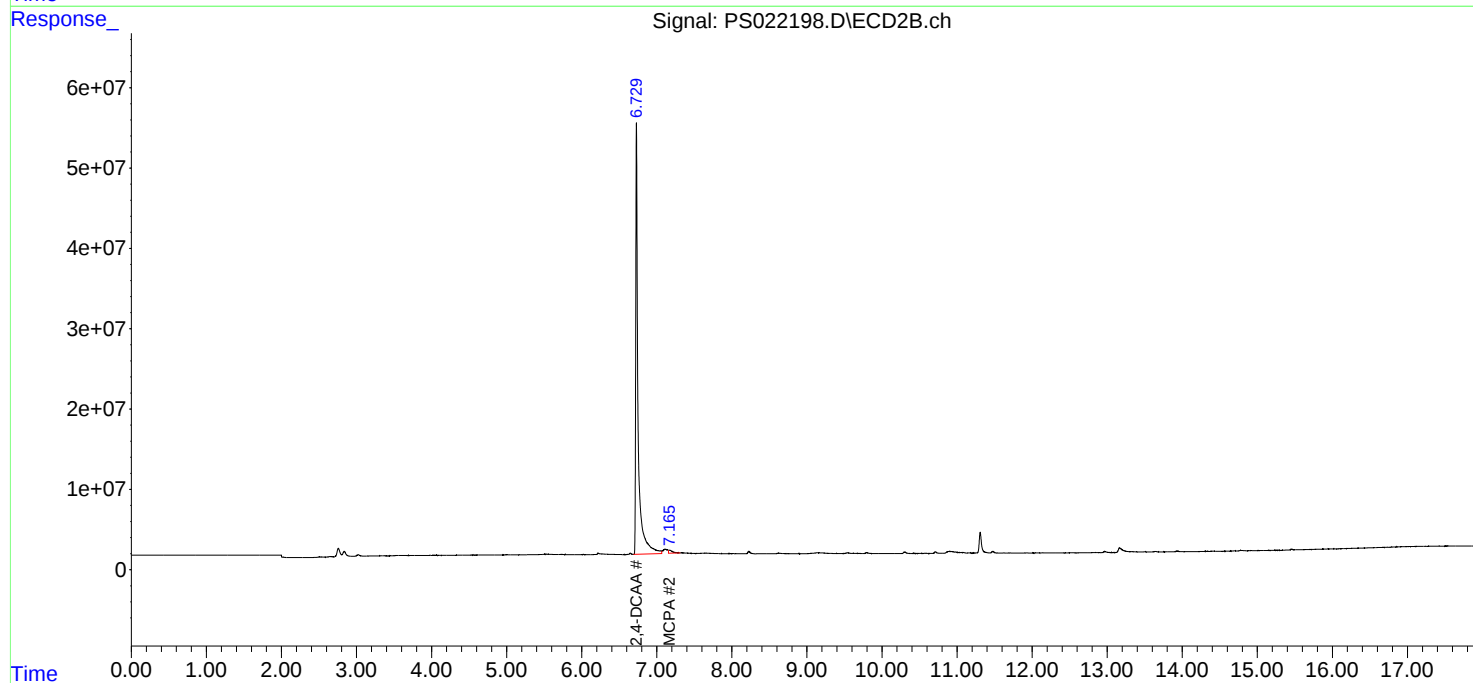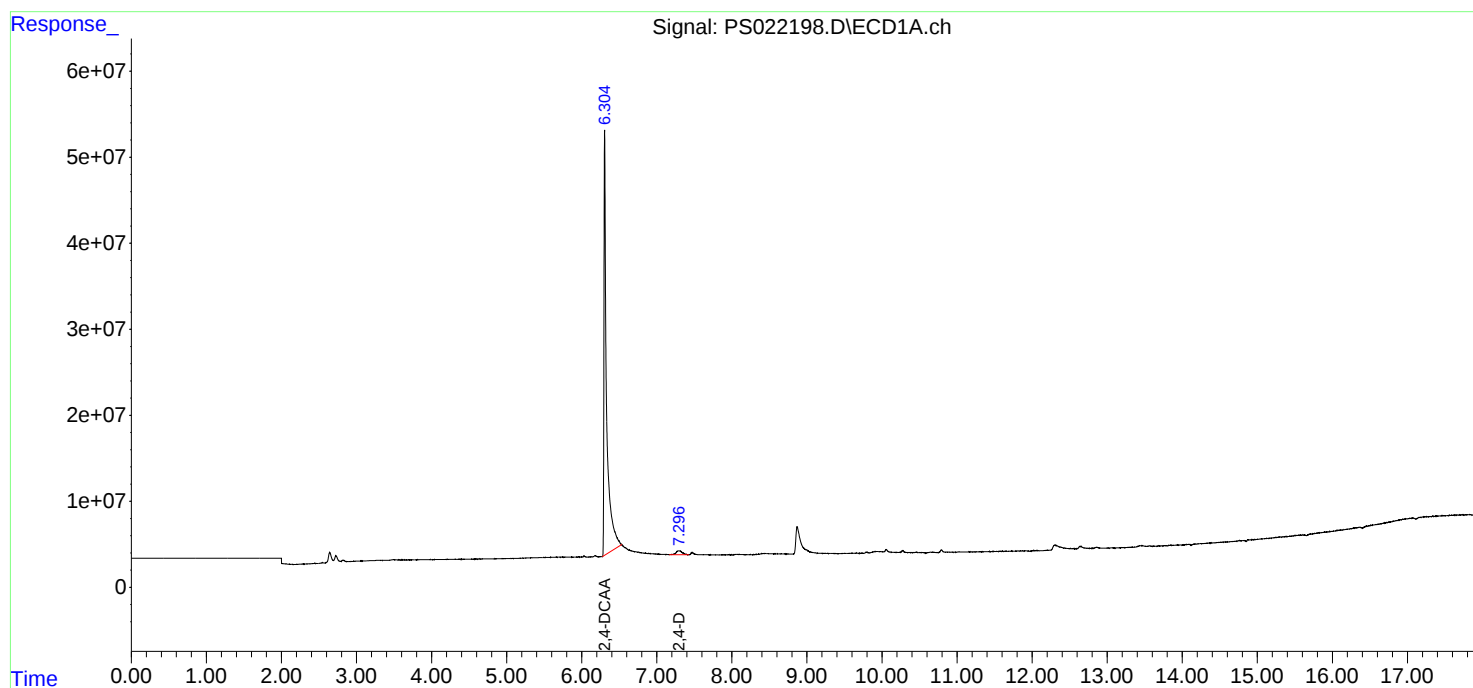


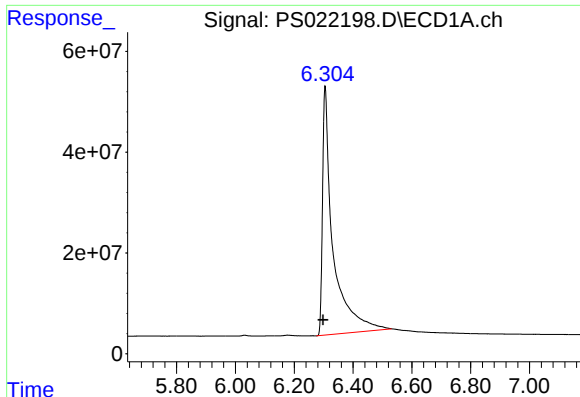

#4 2,4-DCAA


R.T.: 6.306 min
Delta R.T.: 0.007 min
Response: 1226619648
Conc: 494.87 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

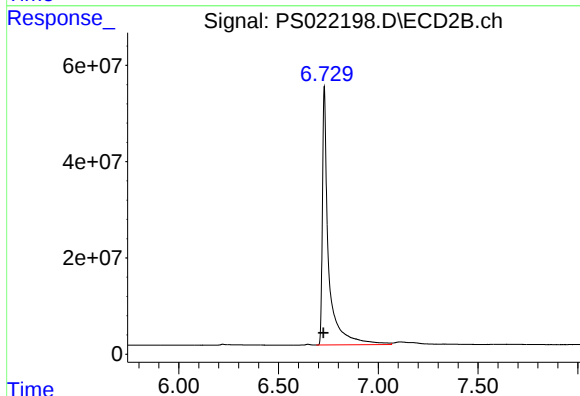


#4 2,4-DCAA

R.T.: 6.729 min
Delta R.T.: 0.004 min
Response: 1175013174
Conc: 559.81 ng/ml

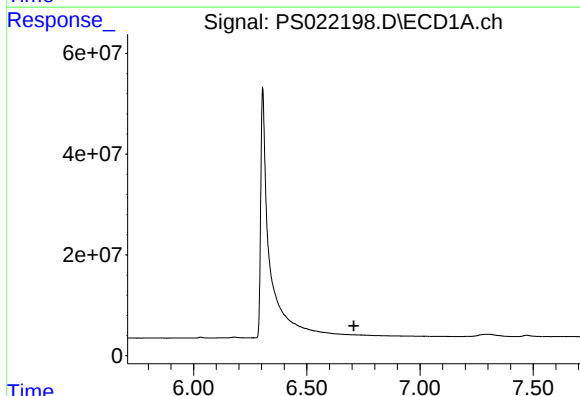


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 6.708 min
Response: 0
Conc: N.D.

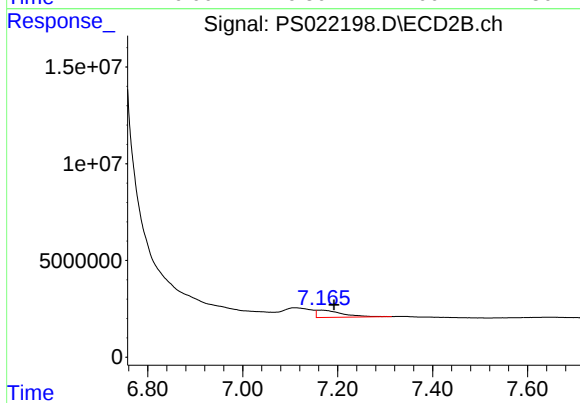

#7 MCPA

R.T.: 7.166 min
Delta R.T.: -0.027 min
Response: 13758030
Conc: 1.35 ug/ml

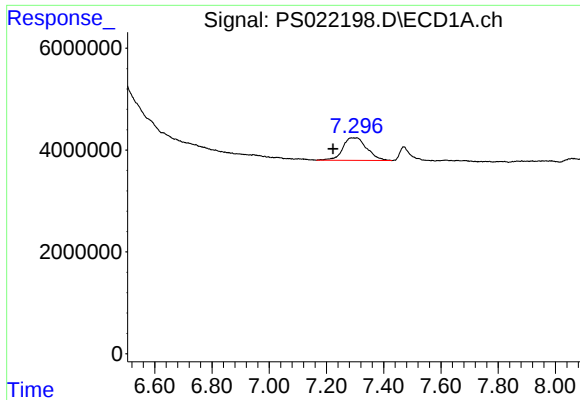

#9 2,4-D


R.T.: 7.289 min

Delta R.T.: 0.067 min

Response: 25856013

Conc: 7.89 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

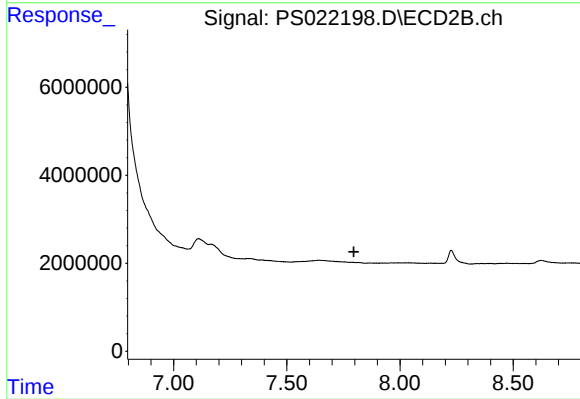

#9 2,4-D

R.T.: 0.000 min

Exp R.T. : 7.796 min

Response: 0

Conc: N.D.