

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022023\
 Data File : PS022208.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2023 16:03
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 20 17:39:43 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022023.M
 Quant Title : 8080.M
 QLast Update : Mon Feb 20 13:26:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.305	6.727	1254.2E6	1156.5E6	505.991	550.963
Target Compounds							
1) T	Dalapon	2.455f	2.527f	1229306	1333137	<MDL	<MDL #
2) T	3,5-DICHL...	5.683	0.000	1779806	0	<MDL	N.D. #
3) T	4-Nitroph...	6.172	0.000	4144692	0	3.257	N.D. #
5) T	DICAMBA	0.000	6.941f	0	25344890	N.D.	2.623
6) T	MCPD	0.000	6.941f	0	25344890	N.D.	3.320
7) T	MCPA	0.000	7.132f	0	32084935	N.D.	3.148
8) T	DICHLORPROP	7.079f	0.000	536392	0	<MDL	N.D. #
10) T	Pentachlo...	7.464	8.223	11954131	9699155	<MDL	<MDL #
11) T	2,4,5-TP ...	7.916f	8.609	241497	4029019	<MDL	<MDL #
14) T	DINOSEB	9.839f	9.791	25251003	4172456	1.837	<MDL #
15) T	Picloram	9.619	10.709f	410892	11469338	<MDL	<MDL #
16) T	DCPA	10.056	10.709	7574003	11469338	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022023\
Data File : PS022208.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2023 16:03
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 20 17:39:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022023.M
Quant Title : 8080.M
QLast Update : Mon Feb 20 13:26:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

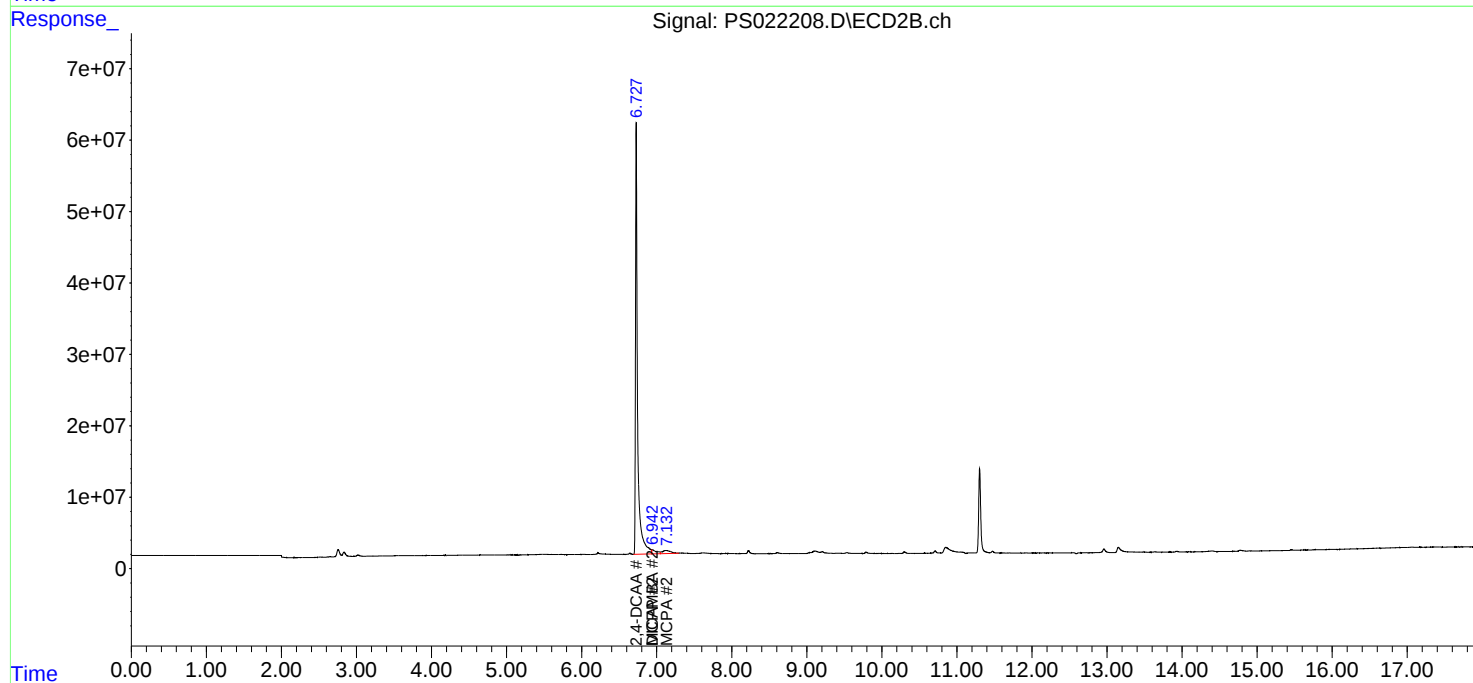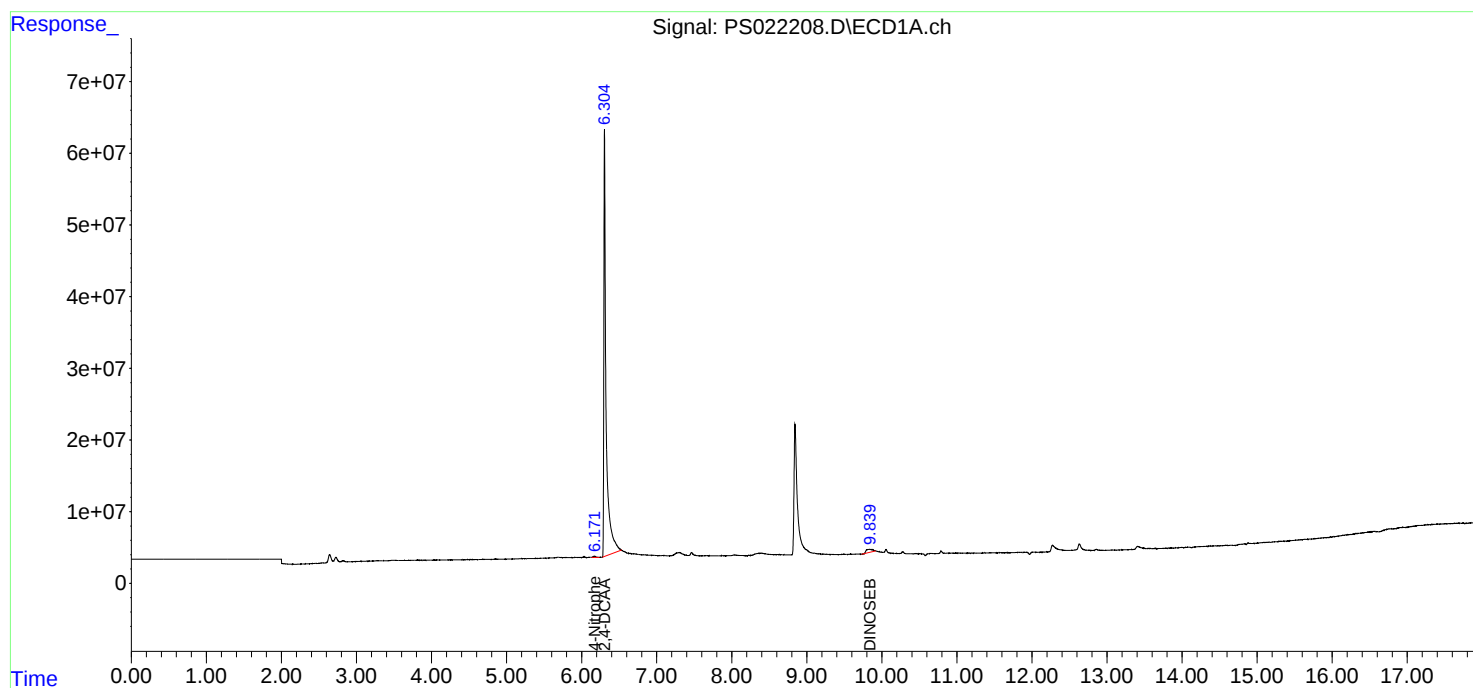


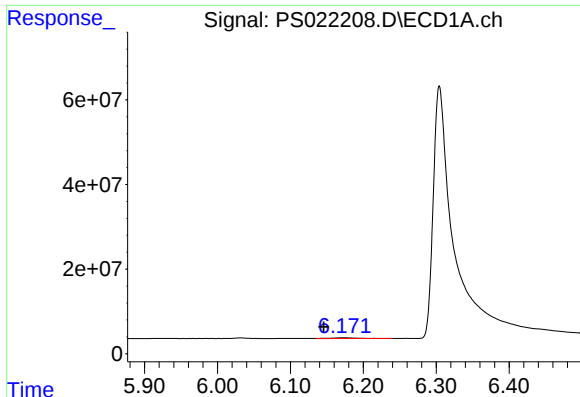

#3 4-Nitrophenol


R.T.: 6.172 min
Delta R.T.: 0.026 min
Response: 4144692
Conc: 3.26 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

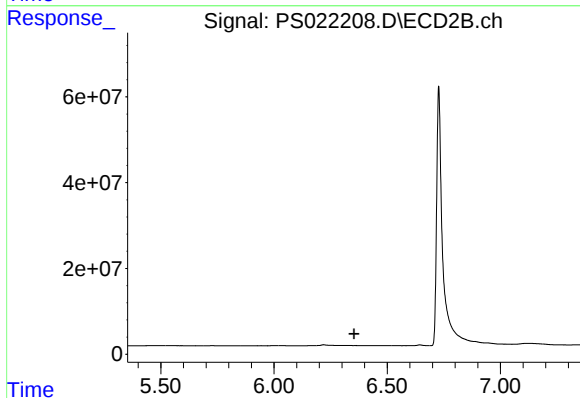


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.353 min
Response: 0
Conc: N.D.

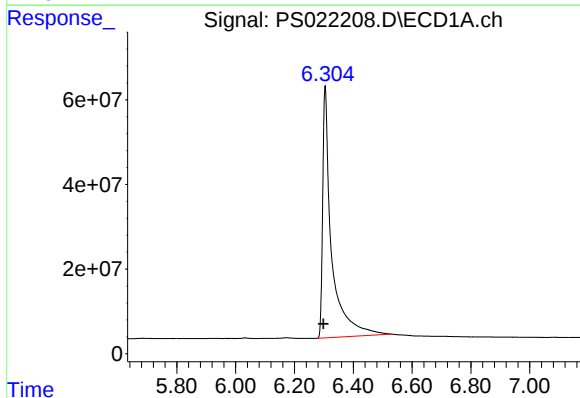


#4 2,4-DCAA

R.T.: 6.305 min
Delta R.T.: 0.006 min
Response: 1254194284
Conc: 505.99 ng/ml

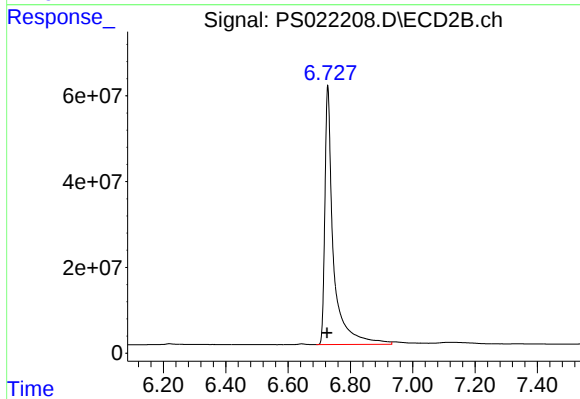

#4 2,4-DCAA


R.T.: 6.727 min
Delta R.T.: 0.002 min
Response: 1156451102
Conc: 550.96 ng/ml

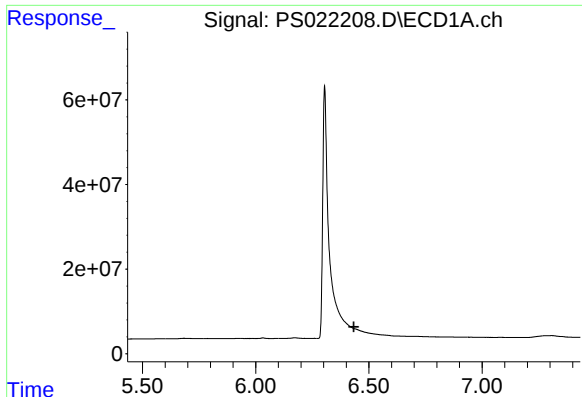

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

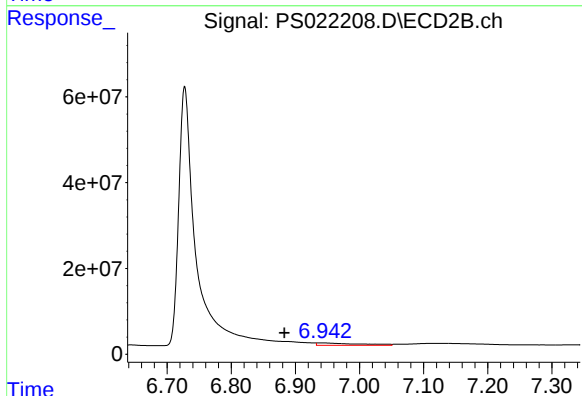


#5 DICAMBA

R.T.: 6.941 min
Delta R.T.: 0.058 min
Response: 25344890
Conc: 2.62 ng/ml

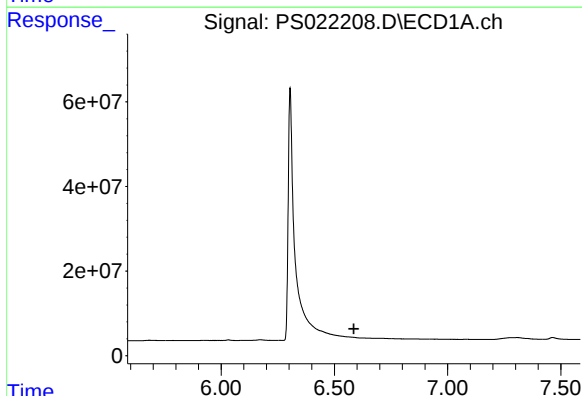


#6 MCP

R.T.: 0.000 min
Exp R.T.: 6.586 min
Response: 0
Conc: N.D.

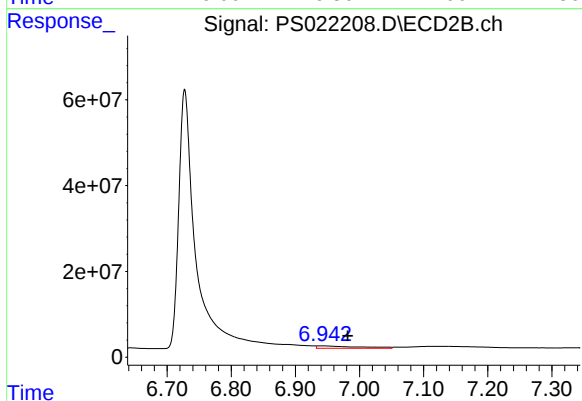

#6 MCP


R.T.: 6.941 min
Delta R.T.: -0.041 min
Response: 25344890
Conc: 3.32 ug/ml

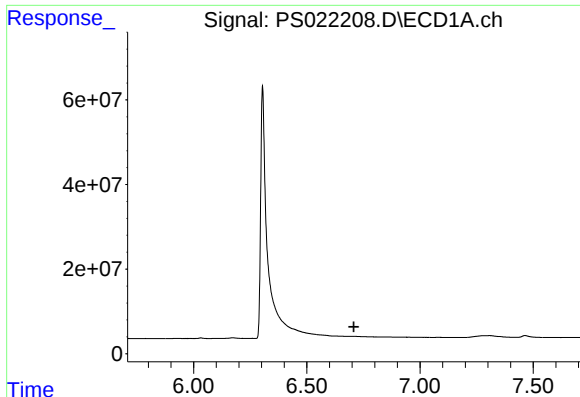

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.708 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

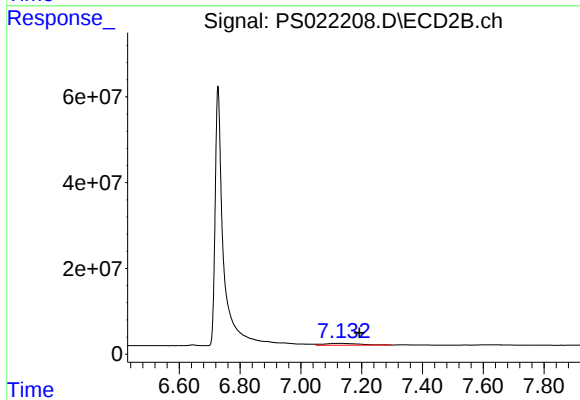


#7 MCPA

R.T.: 7.132 min
Delta R.T.: -0.060 min
Response: 32084935
Conc: 3.15 ug/ml

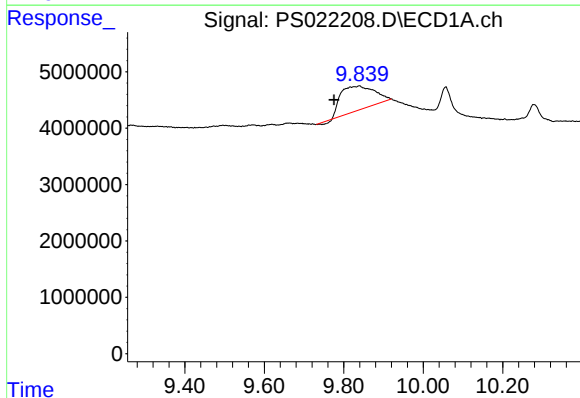

#14 DINOSEB

R.T.: 9.839 min
Delta R.T.: 0.063 min
Response: 25251003
Conc: 1.84 ng/ml

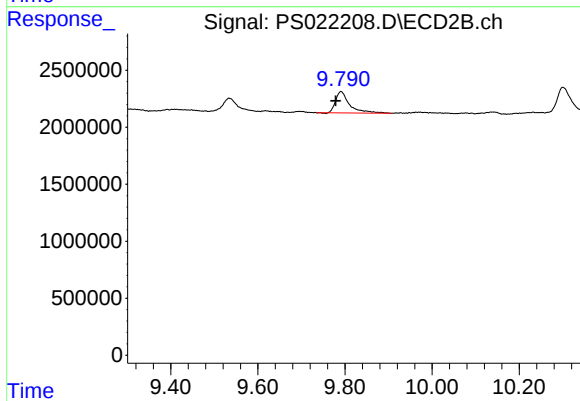

#14 DINOSEB

R.T.: 9.791 min
Delta R.T.: 0.012 min
Response: 4172456
Conc: N.D.