

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022119\
 Data File : PS003295.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2019 18:39
 Operator : EI\SJ
 Sample : PB117278TB
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB117278TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 23:58:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.291	10.790	138.0E6	147.5E6	363.486	344.879
Target Compounds							
6) T	MCP	11.976	0.000	9962973	0	8.315	N.D. #
12) T	2,4,5-T	0.000	14.416	0	4868001	N.D.	2.544 #
15) T	Picloram	0.000	16.726	0	11443357	N.D.	3.806 #
16) T	DCPA	0.000	16.650	0	3055255	N.D.	0.986 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022119\
Data File : PS003295.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2019 18:39
Operator : EI\SJ
Sample : PB117278TB
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB117278TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 23:58:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

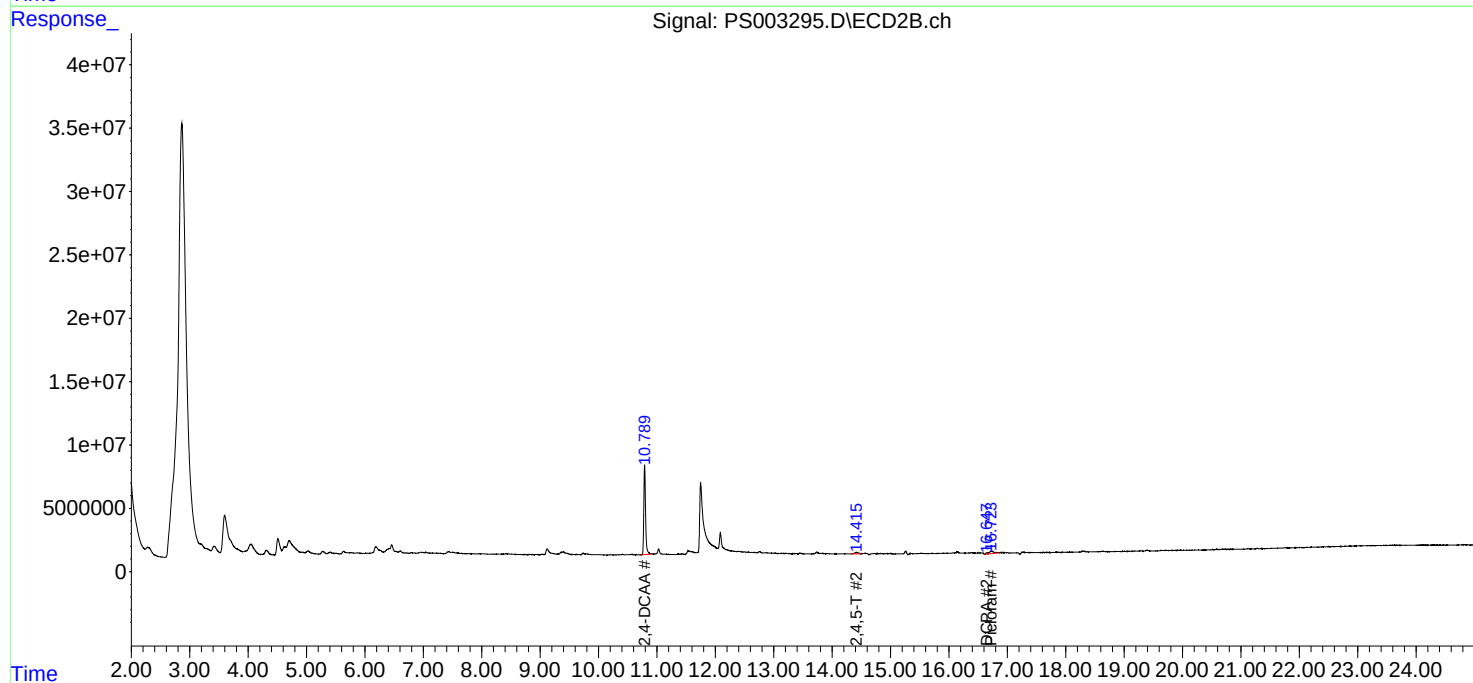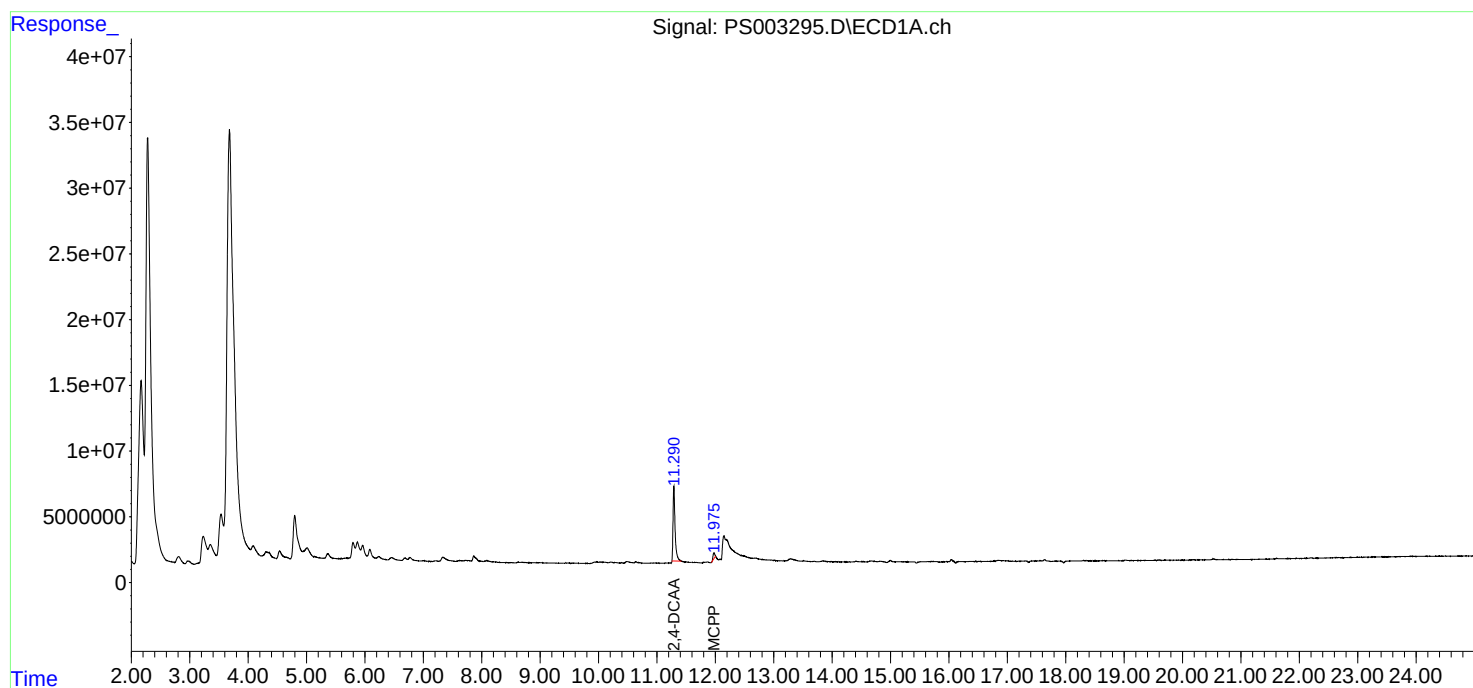


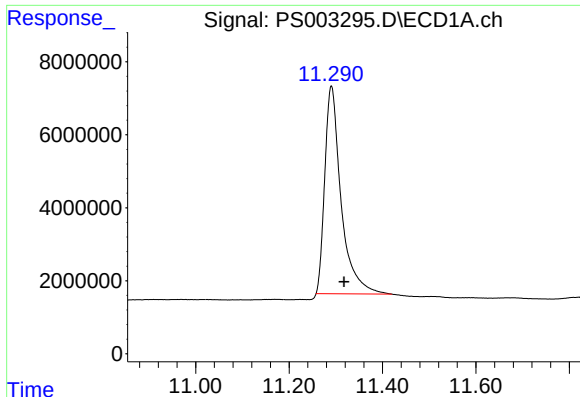

#4 2,4-DCAA


R.T.: 11.291 min
Delta R.T.: -0.027 min
Response: 137994090
Conc: 363.49 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB117278TB

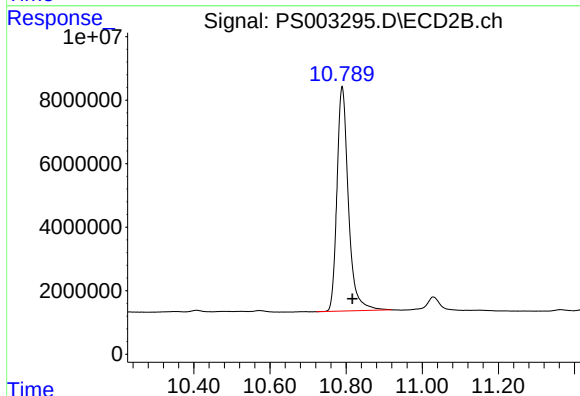


#4 2,4-DCAA

R.T.: 10.790 min
Delta R.T.: -0.027 min
Response: 147451403
Conc: 344.88 ng/ml

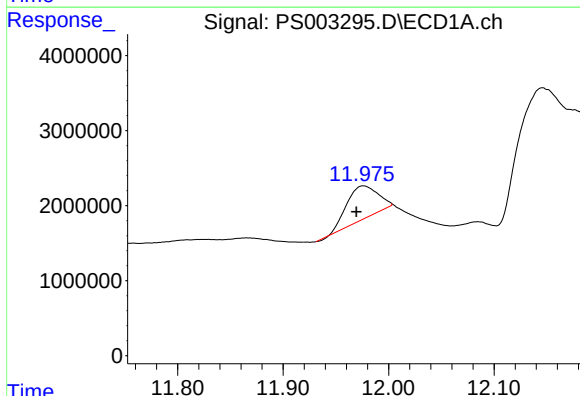


#6 MCP

R.T.: 11.976 min
Delta R.T.: 0.007 min
Response: 9962973
Conc: 8.32 ug/ml

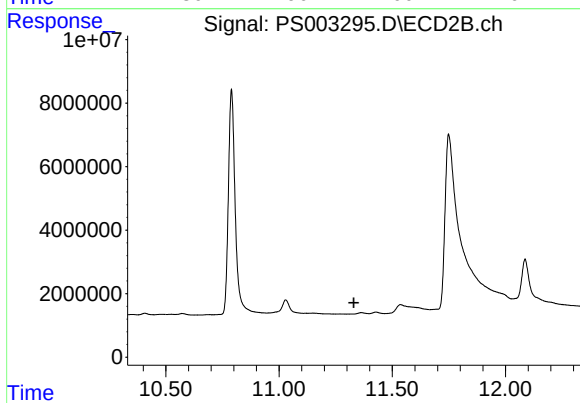

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.330 min
Response: 0
Conc: N.D.

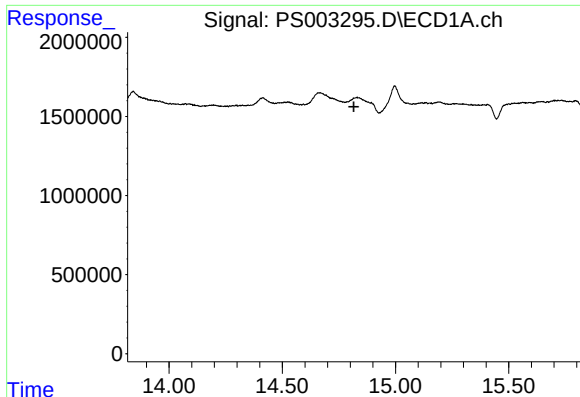

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.817 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB117278TB

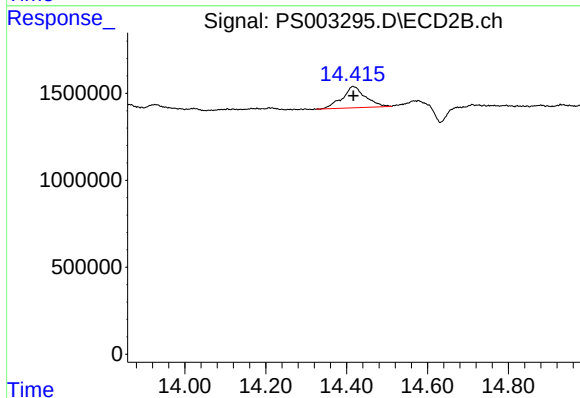


#12 2,4,5-T

R.T.: 14.416 min
Delta R.T.: -0.001 min
Response: 4868001
Conc: 2.54 ng/ml

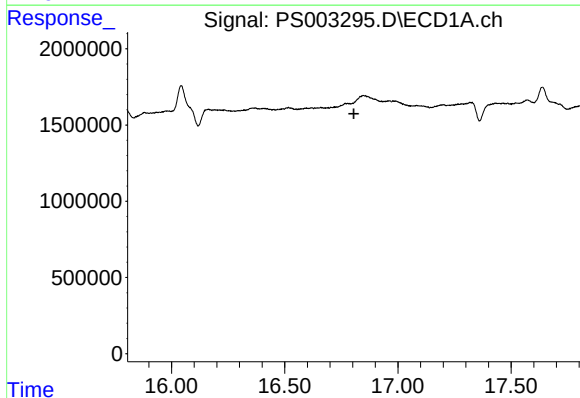


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.806 min
Response: 0
Conc: N.D.

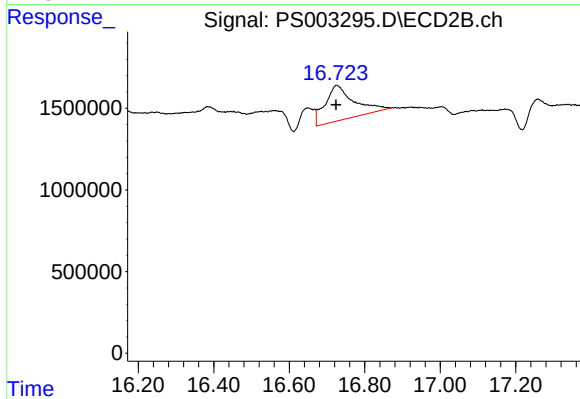

#15 Picloram


R.T.: 16.726 min
Delta R.T.: 0.002 min
Response: 11443357
Conc: 3.81 ng/ml

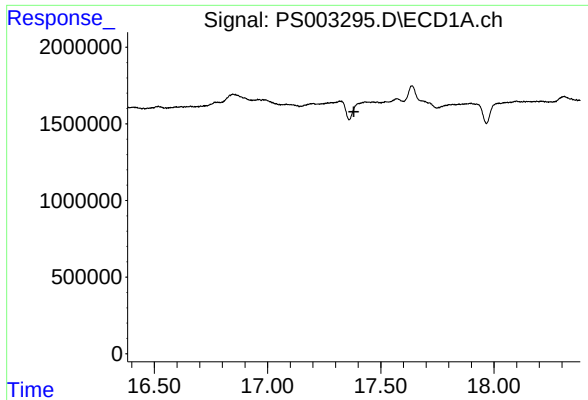

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB117278TB

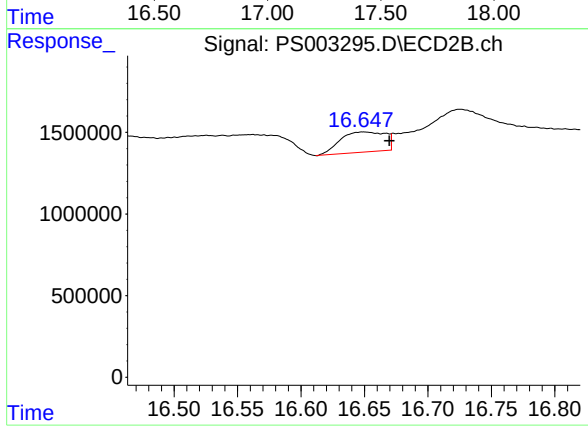

#16 DCPA

R.T.: 16.650 min
Delta R.T.: -0.020 min
Response: 3055255
Conc: 0.99 ng/ml