

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022119\
 Data File : PS003300.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2019 21:14
 Operator : EI\SJ
 Sample : K1345-04
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HD-01-022019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 00:00:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.290	10.789	108.2E6	112.7E6	285.009	263.709
Target Compounds							
1) T	Dalapon	0.000	2.285	0	1539327	N.D.	2.872 #
5) T	DICAMBA	11.693	11.027	2240986	628535	1.398	0.396 #
6) T	MCP	11.975	0.000	11399282	0	9.514	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022119\
Data File : PS003300.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2019 21:14
Operator : EI\SJ
Sample : K1345-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HD-01-022019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 00:00:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

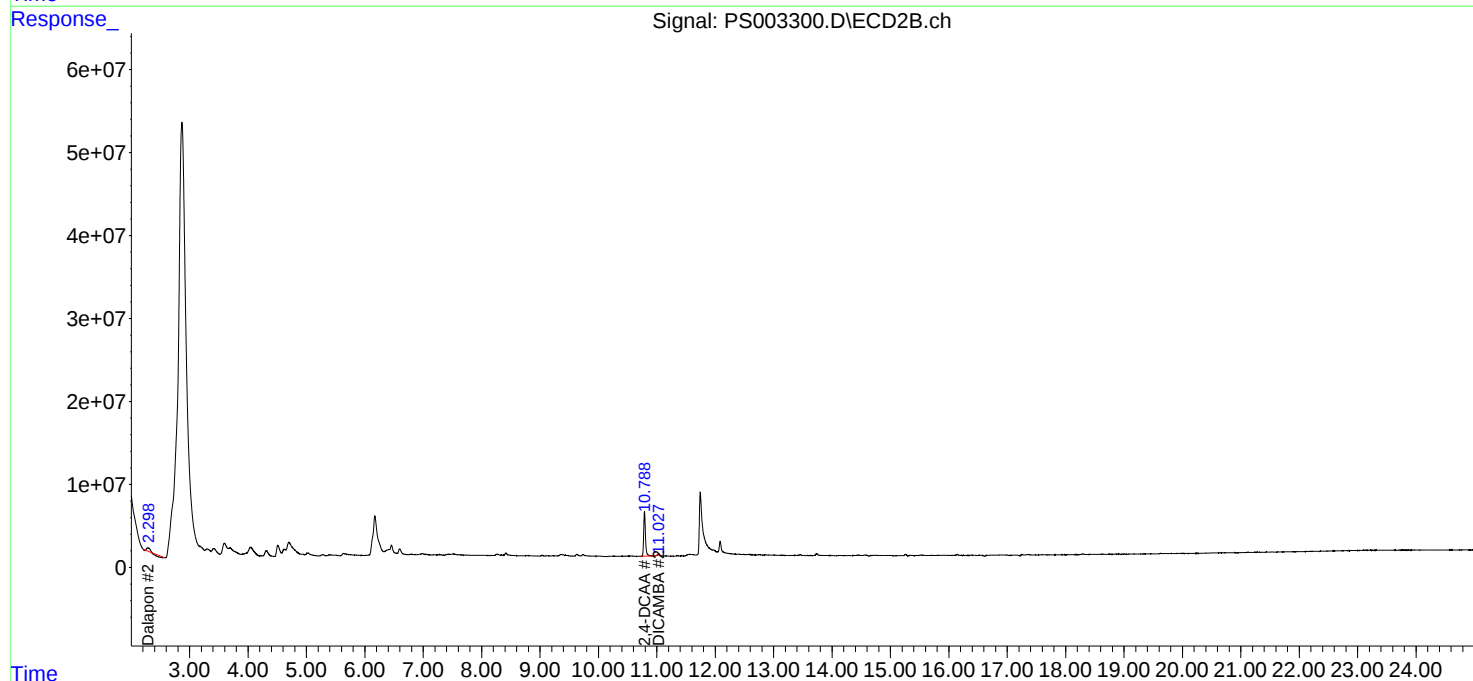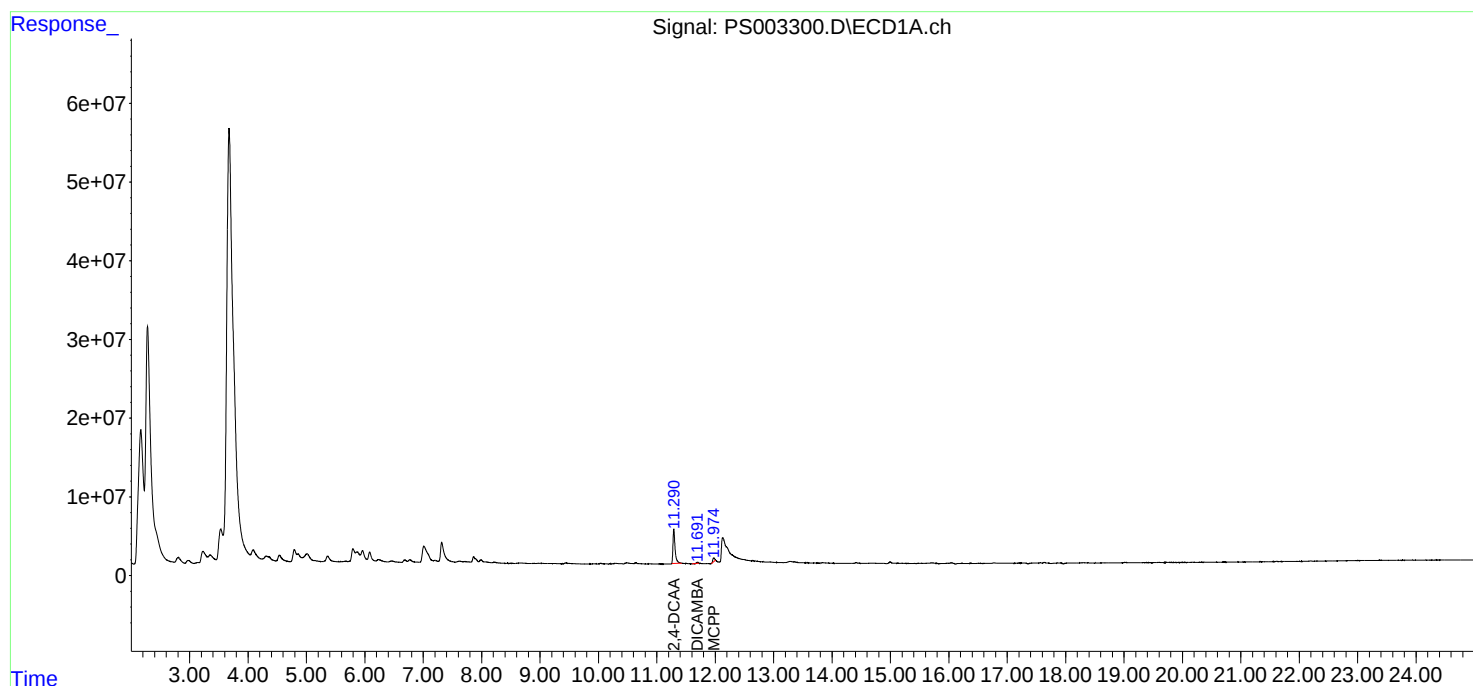


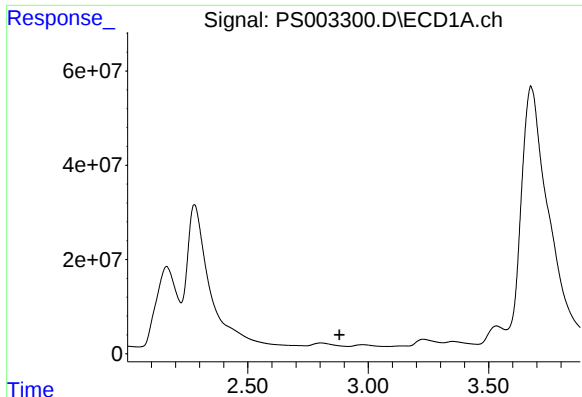

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.880 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HD-01-022019

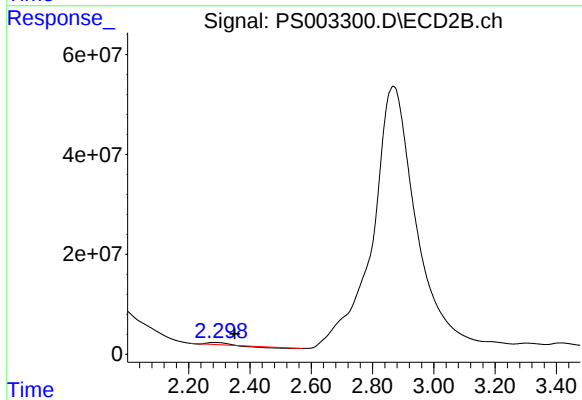


#1 Dalapon

R.T.: 2.285 min
Delta R.T.: -0.065 min
Response: 1539327
Conc: 2.87 ng/ml

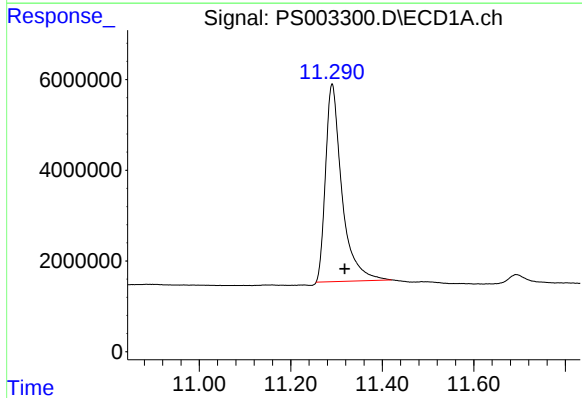


#4 2,4-DCAA

R.T.: 11.290 min
Delta R.T.: -0.027 min
Response: 108200900
Conc: 285.01 ng/ml

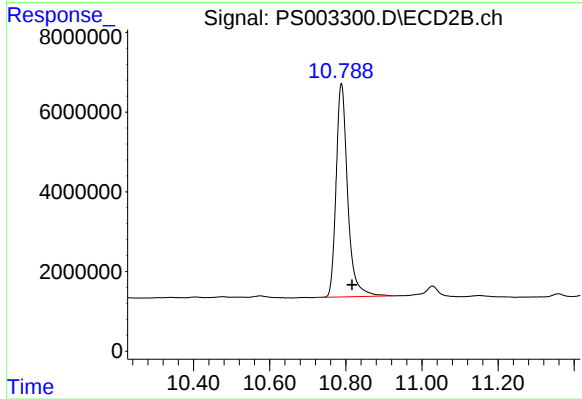

#4 2,4-DCAA


R.T.: 10.789 min
Delta R.T.: -0.028 min
Response: 112747653
Conc: 263.71 ng/ml

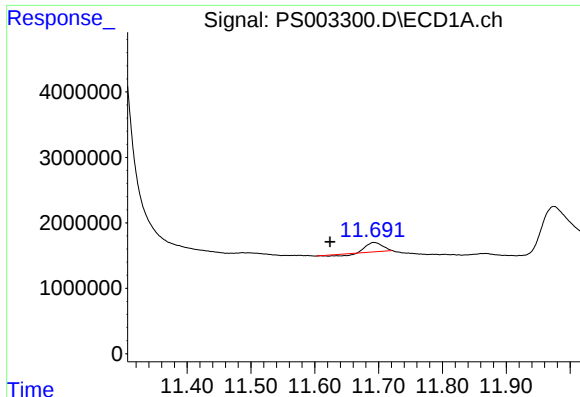

#5 DICAMBA


R.T.: 11.693 min
Delta R.T.: 0.069 min
Response: 2240986
Conc: 1.40 ng/ml

Instrument :
ECD_S
ClientSampleId :
HD-01-022019

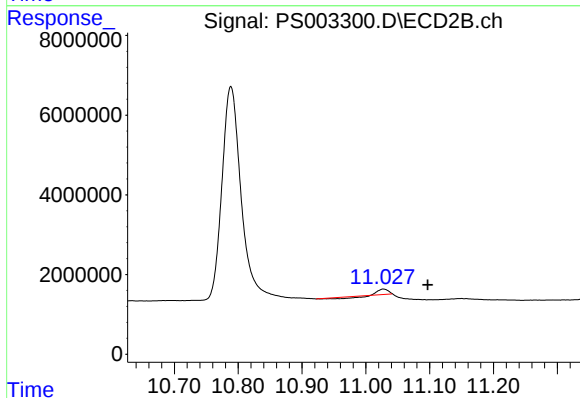


#5 DICAMBA

R.T.: 11.027 min
Delta R.T.: -0.070 min
Response: 628535
Conc: 0.40 ng/ml

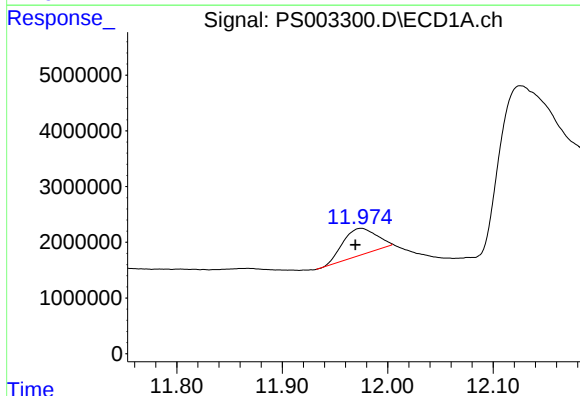

#6 MCP

R.T.: 11.975 min
Delta R.T.: 0.005 min
Response: 11399282
Conc: 9.51 ug/ml

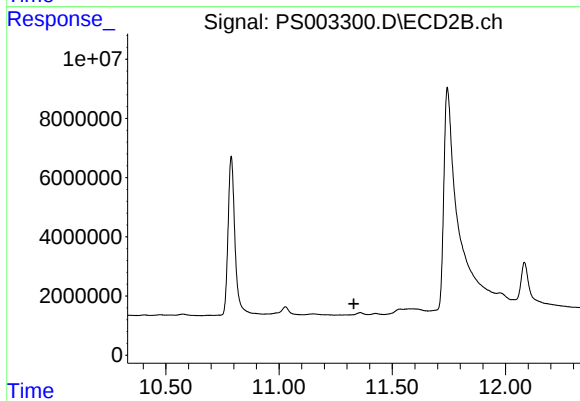

#6 MCP

R.T.: 0.000 min
Exp R.T.: 11.330 min
Response: 0
Conc: N.D.