

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022119\
 Data File : PS003306.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Feb 2019 00:21
 Operator : EI\SJ
 Sample : K1349-12
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 OR-02-021919-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 02:28:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.294	10.793	124.2E6	125.5E6	327.162	293.531
Target Compounds							
6) T	MCP	11.977	0.000	7912862	0	6.604	N.D. #
11) T	2,4,5-TP ...	14.415	0.000	3635069	0	1.443	N.D. #
12) T	2,4,5-T	0.000	14.416	0	5604868	N.D.	2.929 #
15) T	Picloram	0.000	16.724	0	6586304	N.D.	2.191 #
16) T	DCPA	0.000	16.650	0	2223398	N.D.	0.718 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022119\
Data File : PS003306.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Feb 2019 00:21
Operator : EI\SJ
Sample : K1349-12
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
OR-02-021919-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 02:28:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

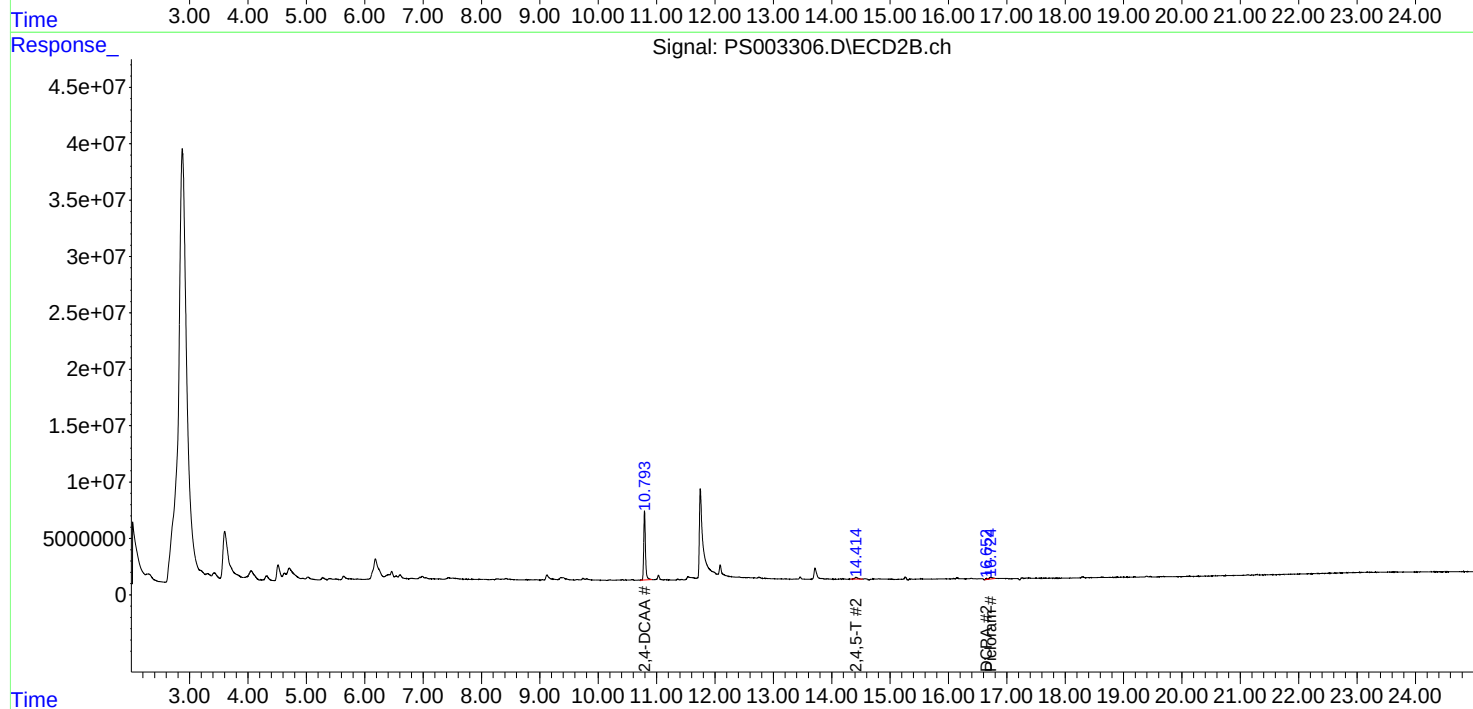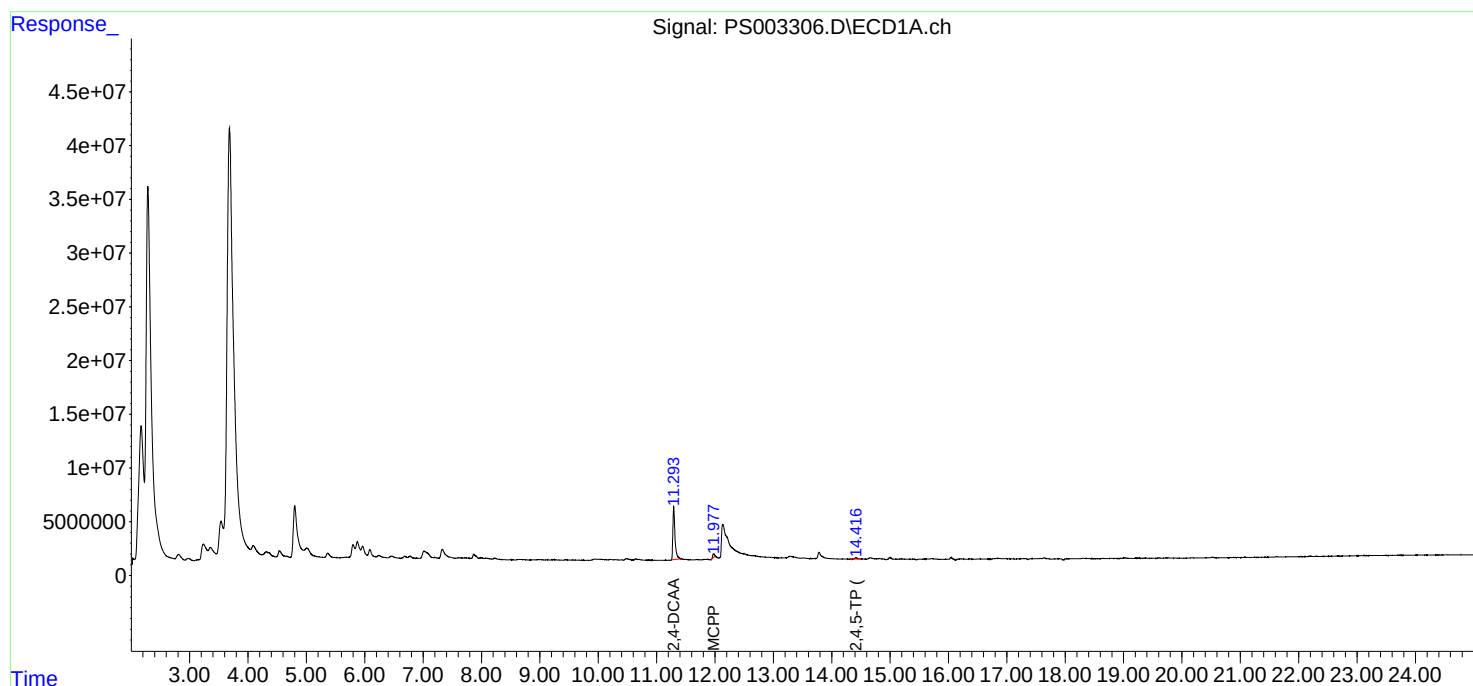


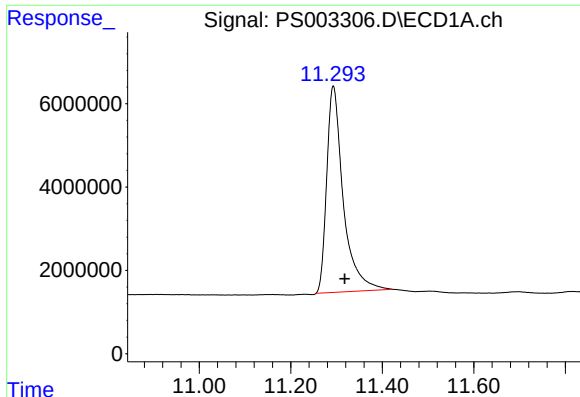

#4 2,4-DCAA


R.T.: 11.294 min
Delta R.T.: -0.024 min
Response: 124204134
Conc: 327.16 ng/ml

Instrument :
ECD_S
ClientSampleId :
OR-02-021919-B

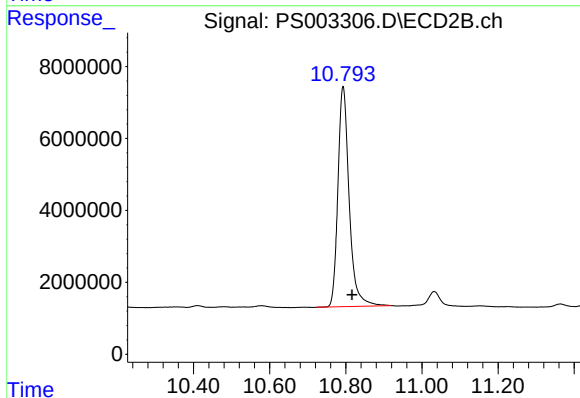


#4 2,4-DCAA

R.T.: 10.793 min
Delta R.T.: -0.024 min
Response: 125497792
Conc: 293.53 ng/ml

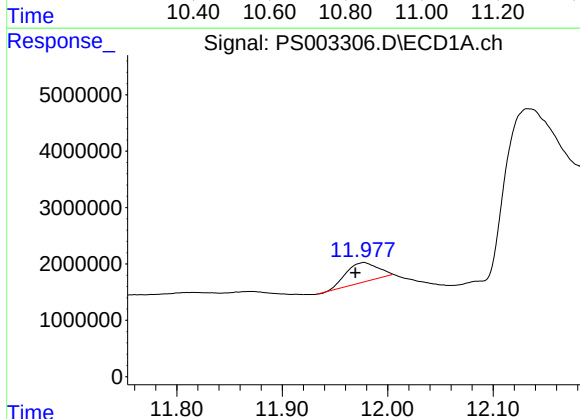


#6 MCP

R.T.: 11.977 min
Delta R.T.: 0.008 min
Response: 7912862
Conc: 6.60 ug/ml

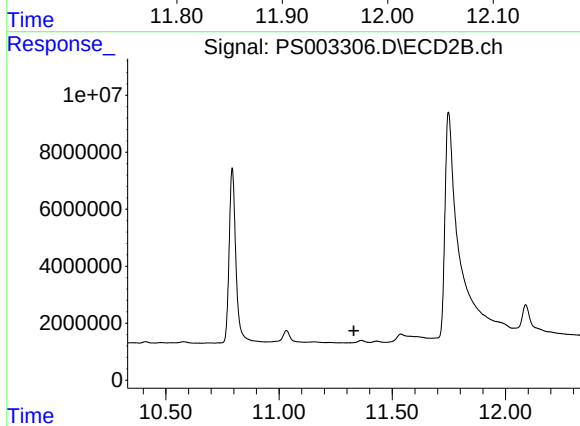

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.330 min
Response: 0
Conc: N.D.

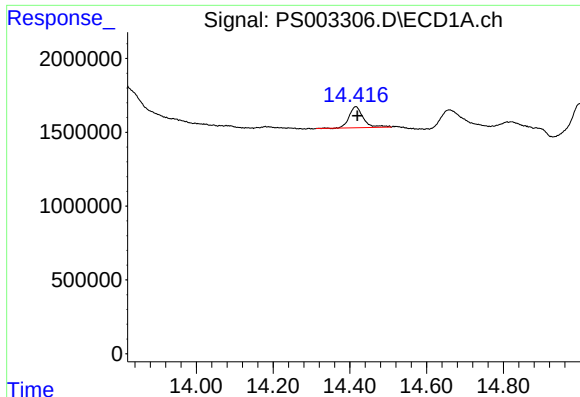

#11 2,4,5-TP (SILVEX)


R.T.: 14.415 min
Delta R.T.: -0.004 min
Response: 3635069
Conc: 1.44 ng/ml

Instrument :
ECD_S
ClientSampleId :
OR-02-021919-B

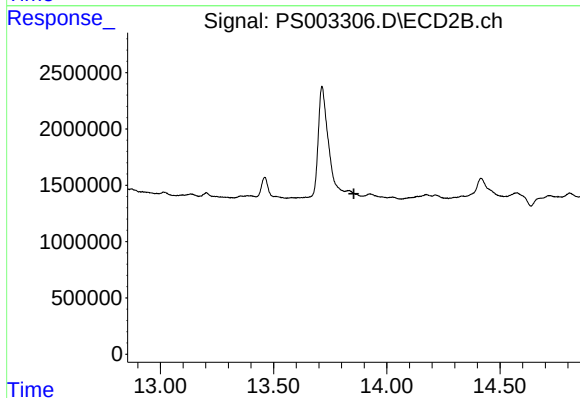


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 13.854 min
Response: 0
Conc: N.D.

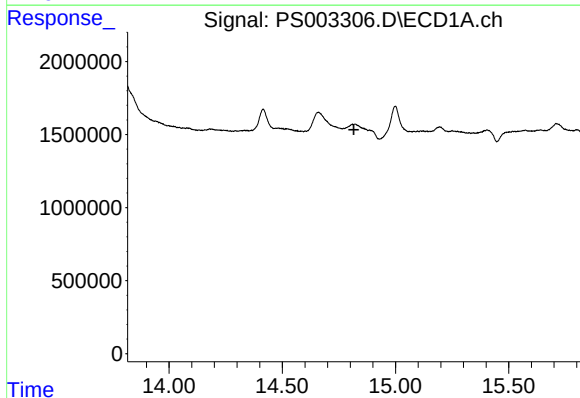


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 14.817 min
Response: 0
Conc: N.D.

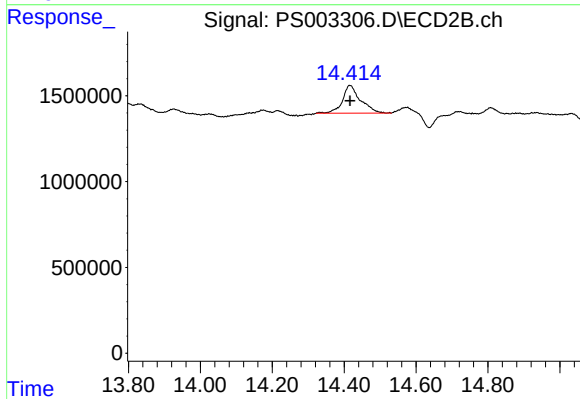

#12 2,4,5-T


R.T.: 14.416 min
Delta R.T.: 0.000 min
Response: 5604868
Conc: 2.93 ng/ml

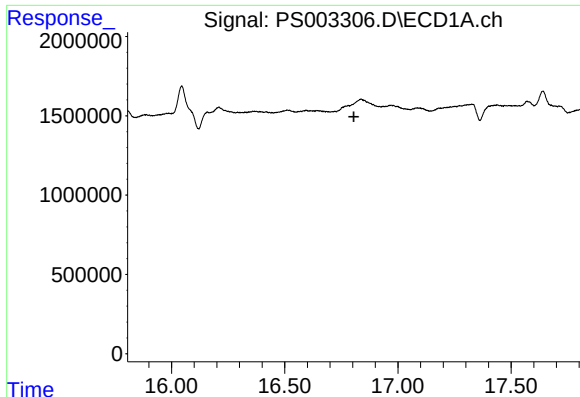

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 16.806 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
OR-02-021919-B

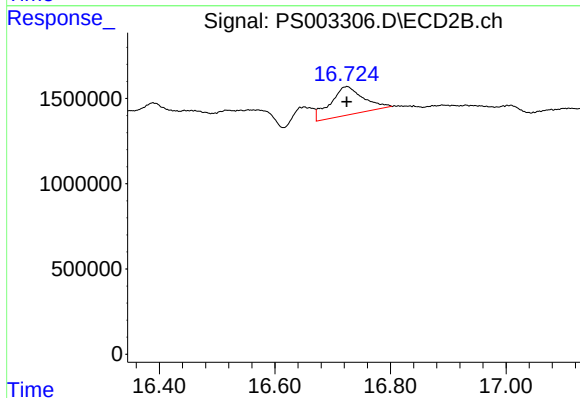


#15 Picloram

R.T.: 16.724 min
Delta R.T.: 0.000 min
Response: 6586304
Conc: 2.19 ng/ml

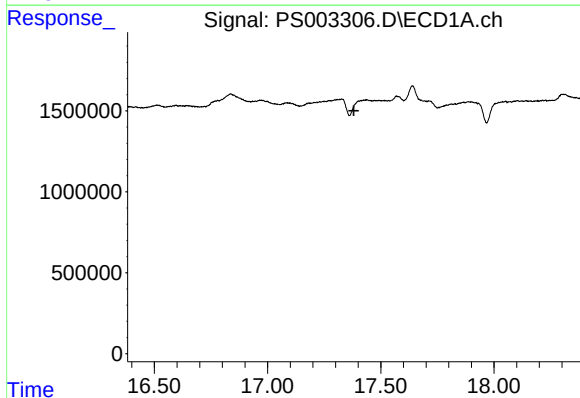

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.382 min
Response: 0
Conc: N.D.

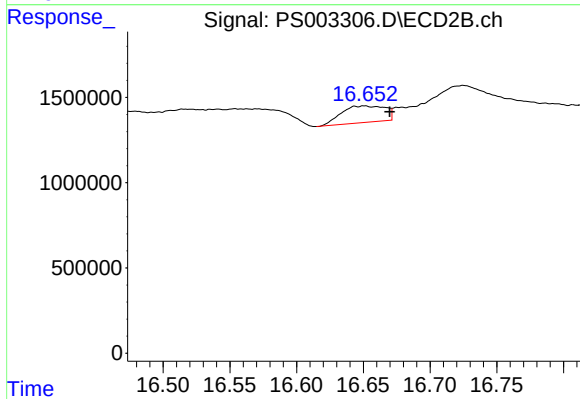

#16 DCPA

R.T.: 16.650 min
Delta R.T.: -0.019 min
Response: 2223398
Conc: 0.72 ng/ml