

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022119\
 Data File : PS003309.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Feb 2019 01:54
 Operator : EI\SJ
 Sample : K1538-04
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 M-11-A-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 02:29:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.284	10.785	127.5E6	146.7E6	335.845	343.183
Target Compounds							
1) T	Dalapon	0.000	2.285	0	13168162	N.D.	24.571 #
6) T	MCP	11.971	0.000	4935588	0	4.119	N.D. #
15) T	Picloram	0.000	16.740	0	5824349	N.D.	1.937 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022119\
Data File : PS003309.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Feb 2019 01:54
Operator : EI\SJ
Sample : K1538-04
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
M-11-A-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 02:29:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

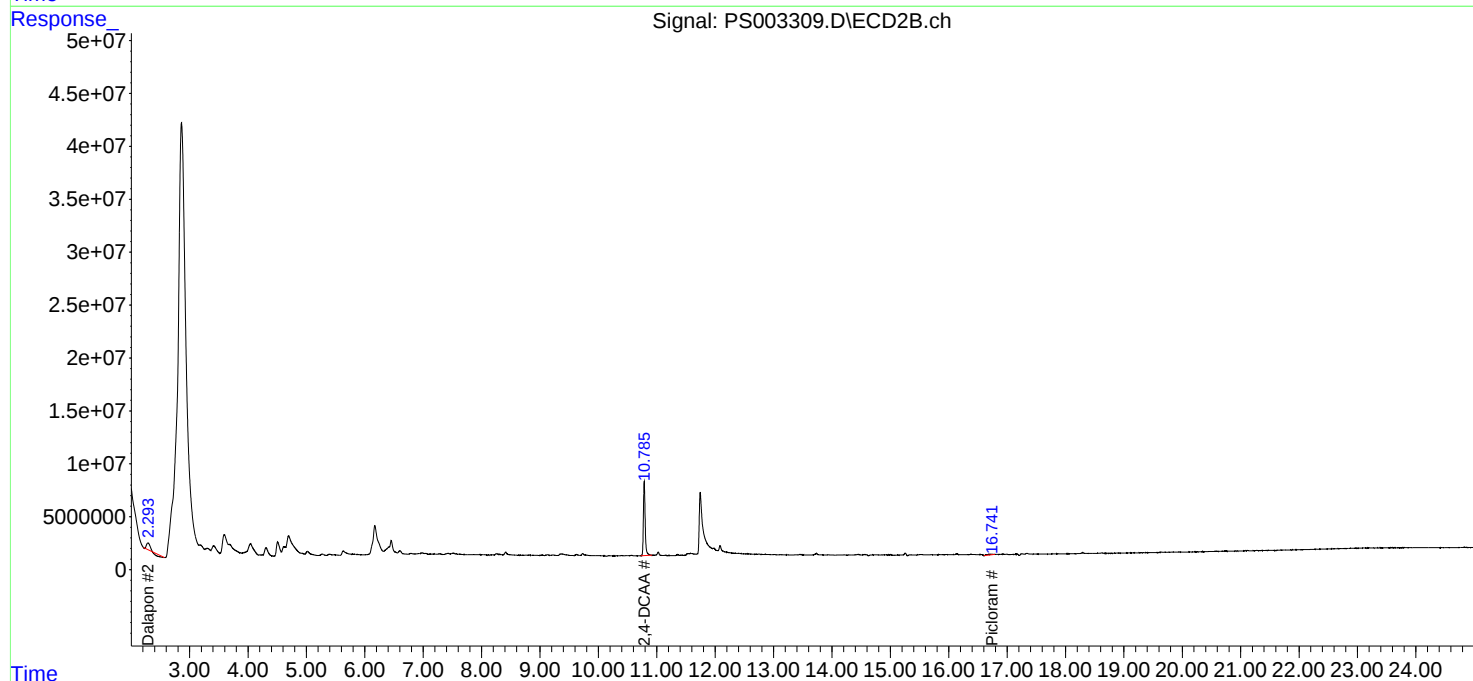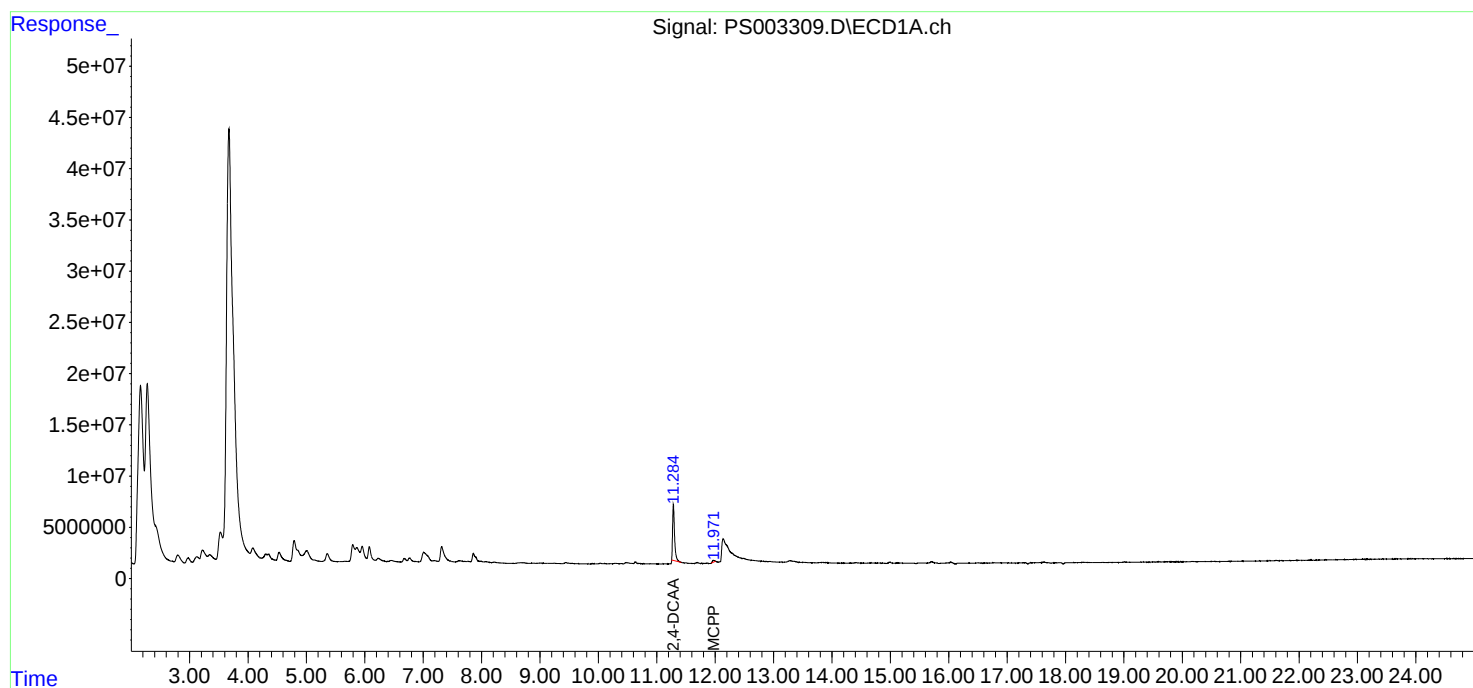


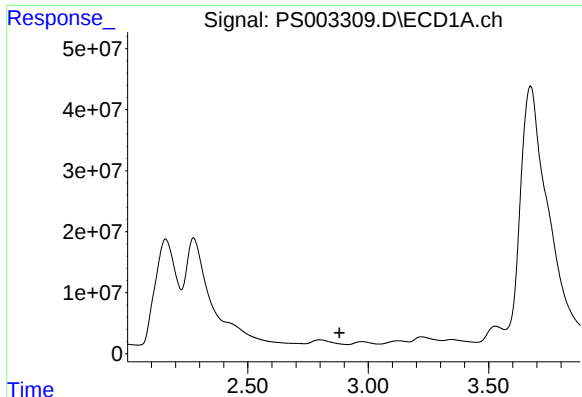

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.880 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
M-11-A-S

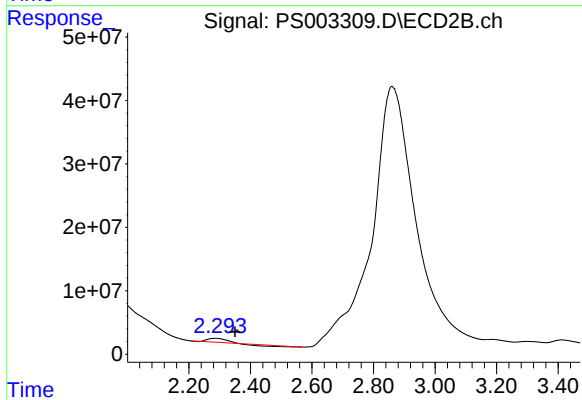


#1 Dalapon

R.T.: 2.285 min
Delta R.T.: -0.066 min
Response: 13168162
Conc: 24.57 ng/ml

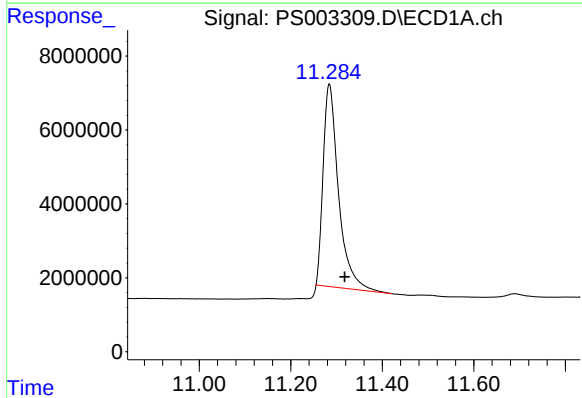


#4 2,4-DCAA

R.T.: 11.284 min
Delta R.T.: -0.034 min
Response: 127500368
Conc: 335.84 ng/ml

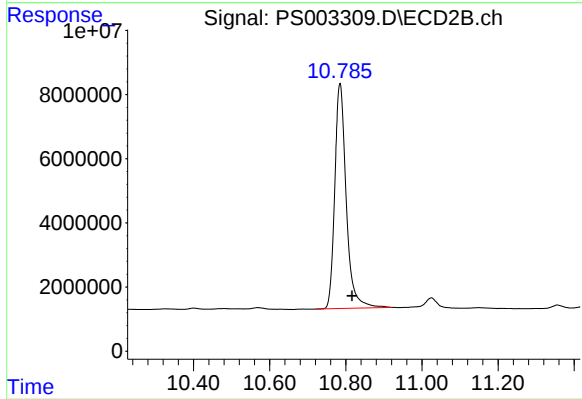

#4 2,4-DCAA


R.T.: 10.785 min
Delta R.T.: -0.032 min
Response: 146726340
Conc: 343.18 ng/ml

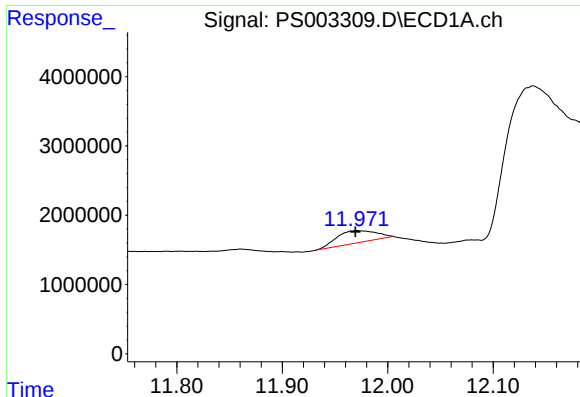

#6 MCP


R.T.: 11.971 min
Delta R.T.: 0.002 min
Response: 4935588
Conc: 4.12 ug/ml

Instrument :
ECD_S
ClientSampleId :
M-11-A-S

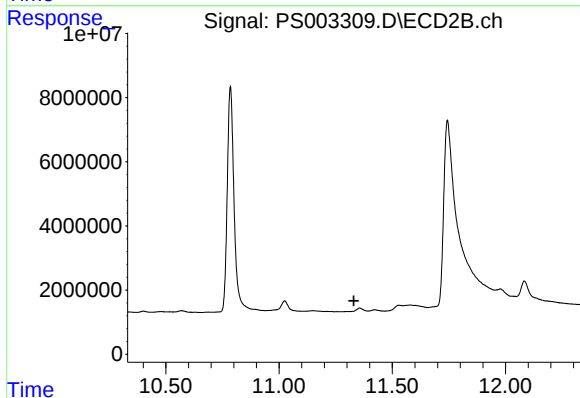


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.330 min
Response: 0
Conc: N.D.

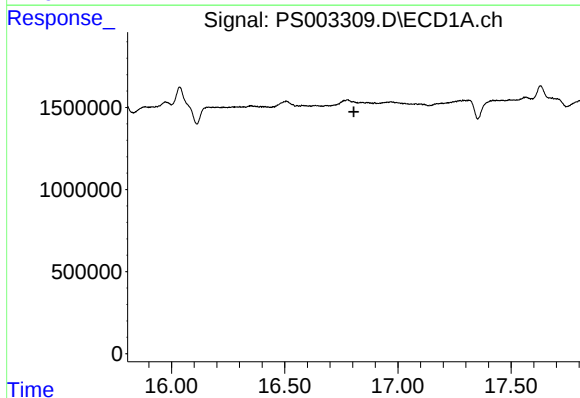

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.806 min
Response: 0
Conc: N.D.

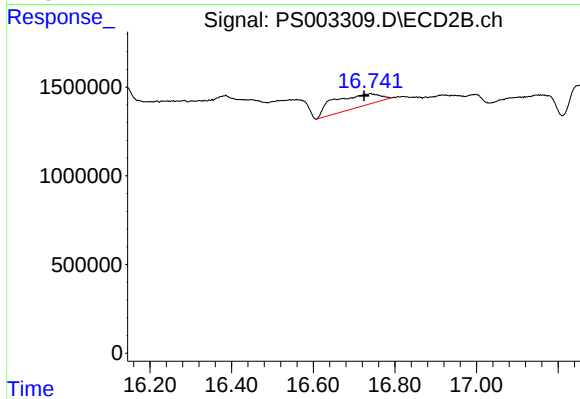

#15 Picloram

R.T.: 16.740 min
Delta R.T.: 0.016 min
Response: 5824349
Conc: 1.94 ng/ml