

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022119\
 Data File : PS003312.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Feb 2019 03:27
 Operator : EI\SJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 04:49:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.276	10.778	74150170	307.2E6	195.317	718.507 #
Target Compounds							
1) T	Dalapon	2.842	2.312	64161409	375.8E6	116.309	701.175 #
2) T	3,5-DICHL...	0.000	8.938	0	10919447	N.D.	19.376 #
3) T	4-Nitroph...	10.873	9.930	89193964	145.2E6	460.857	694.665 #
8) T	DICHLORPROP	0.000	12.182	0	267.6E6	N.D.	699.965 #
9) T	2,4-D	0.000	12.655	0	211.1E6	N.D.	421.004 #
11) T	2,4,5-TP ...	14.374	13.814	1819.6E6	1736.9E6	722.528	700.271
12) T	2,4,5-T	14.775	14.379	1758.0E6	289.0E6	720.675	151.020 #
14) T	DINOSEB	16.984	0.000	1392.8E6	0	740.308	N.D. #
15) T	Picloram	16.765	16.686	1929.2E6	1808.4E6	609.806	601.502
16) T	DCPA	0.000	16.686	0	1808.4E6	N.D.	583.795 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022119\
Data File : PS003312.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Feb 2019 03:27
Operator : EI\SJ
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 04:49:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

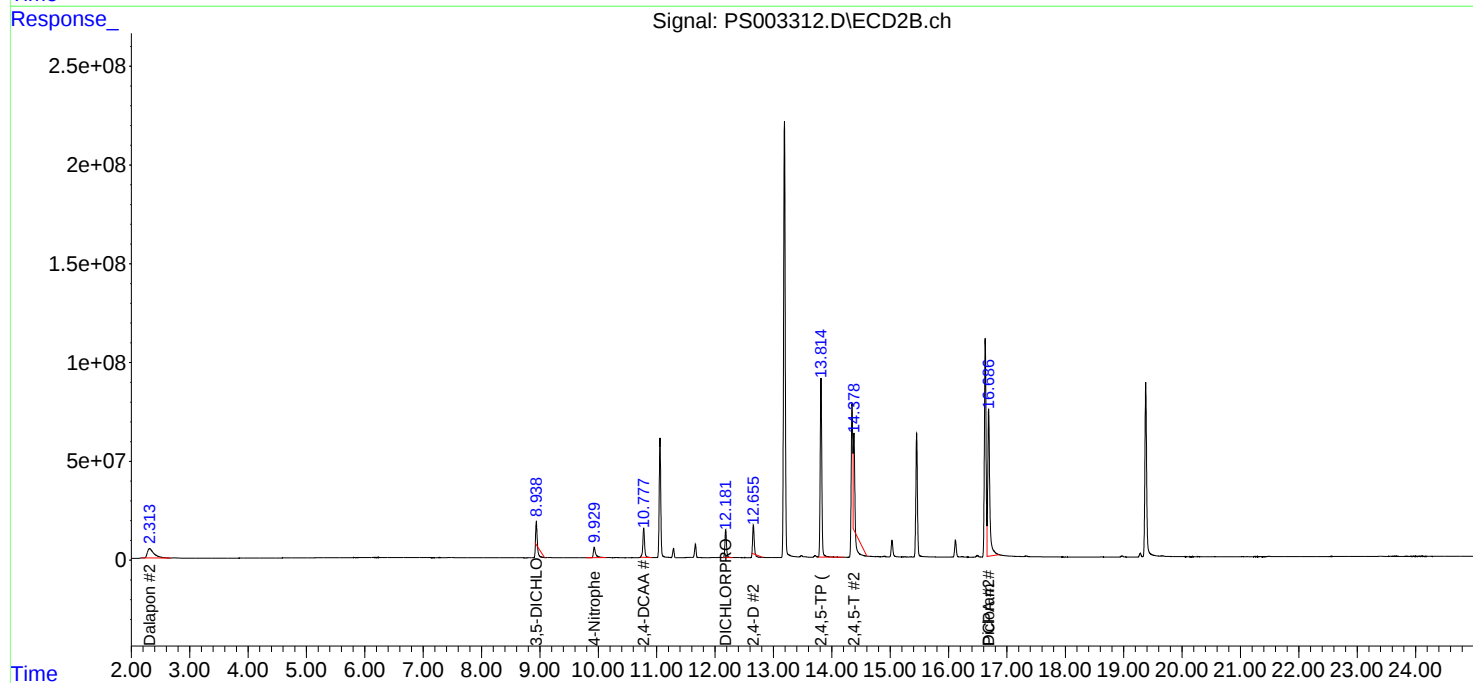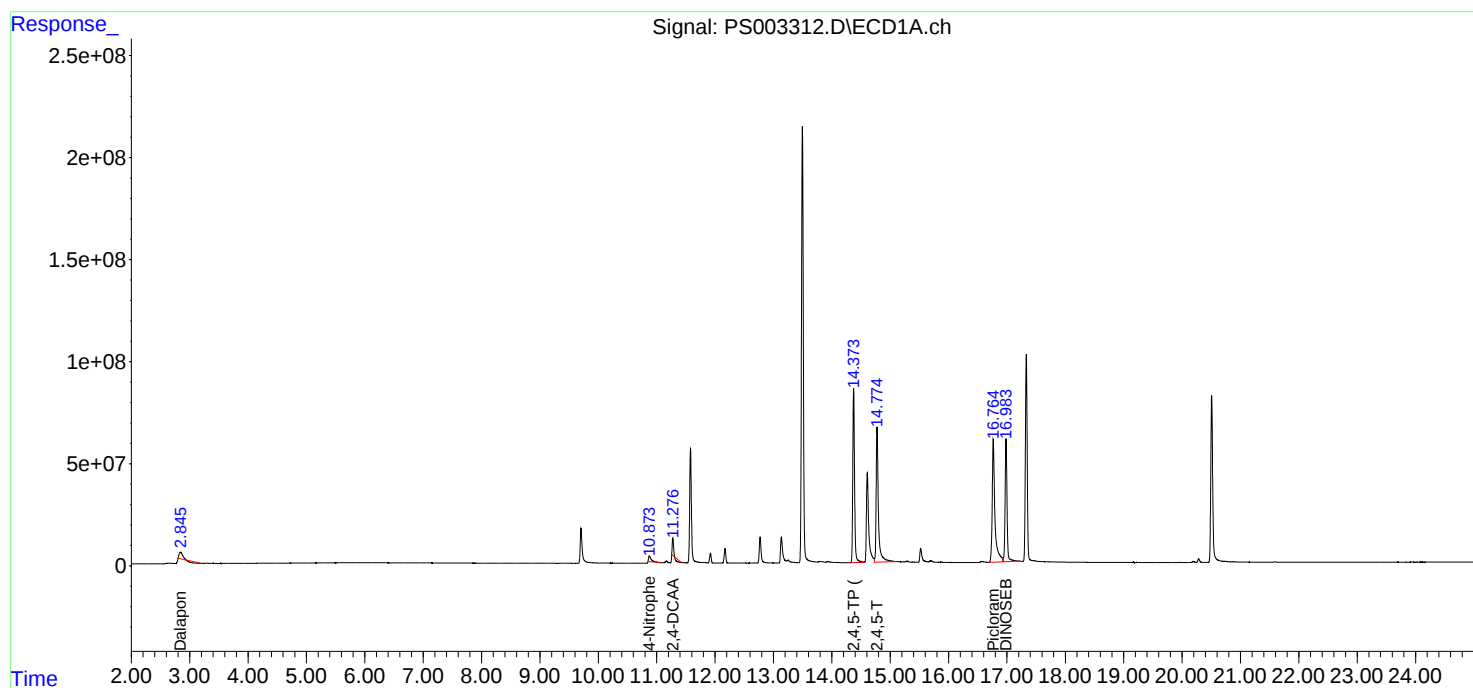


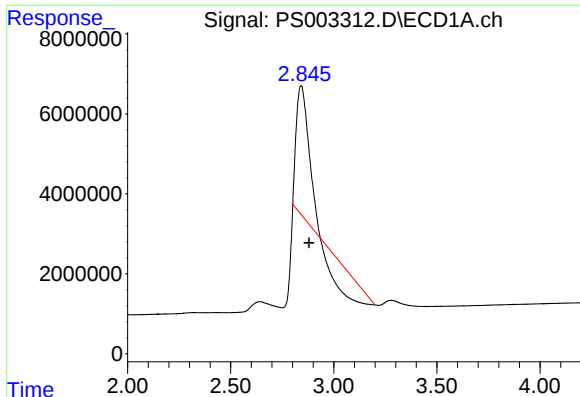

#1 Dalapon


R.T.: 2.842 min
Delta R.T.: -0.038 min
Response: 64161409
Conc: 116.31 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

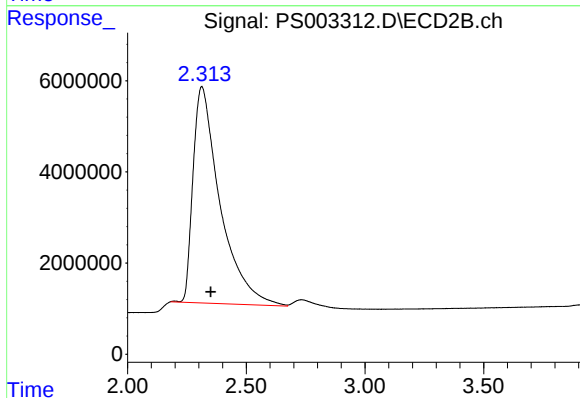


#1 Dalapon

R.T.: 2.312 min
Delta R.T.: -0.038 min
Response: 375774910
Conc: 701.18 ng/ml

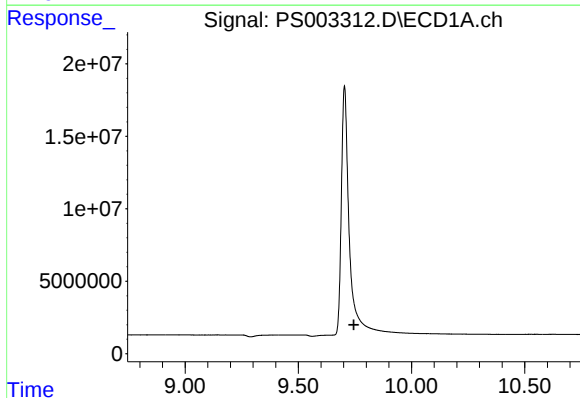


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.745 min
Response: 0
Conc: N.D.

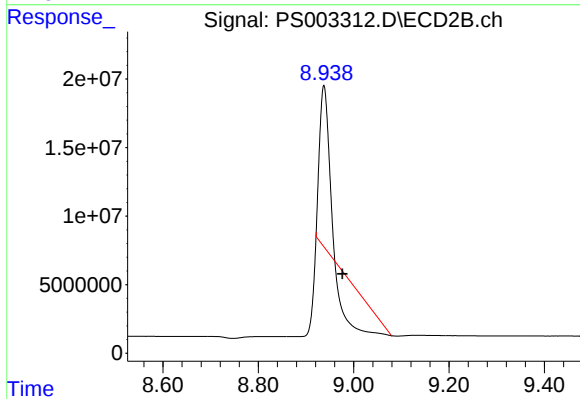

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.938 min
Delta R.T.: -0.039 min
Response: 10919447
Conc: 19.38 ng/ml

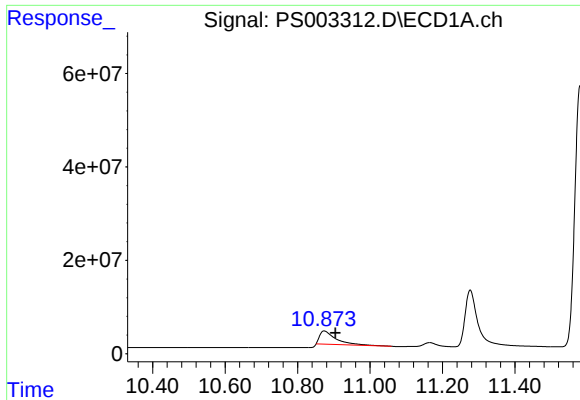

#3 4-Nitrophenol


R.T.: 10.873 min
Delta R.T.: -0.031 min
Response: 89193964
Conc: 460.86 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

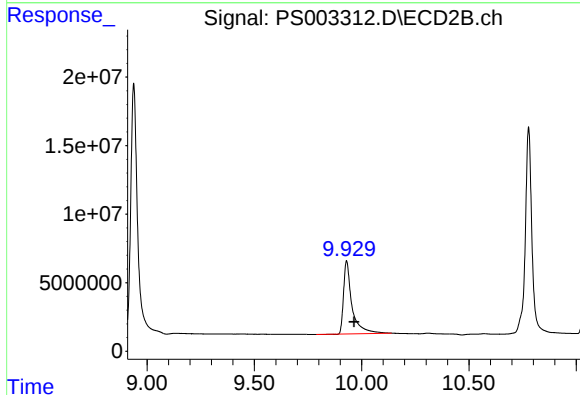


#3 4-Nitrophenol

R.T.: 9.930 min
Delta R.T.: -0.036 min
Response: 145200653
Conc: 694.67 ng/ml

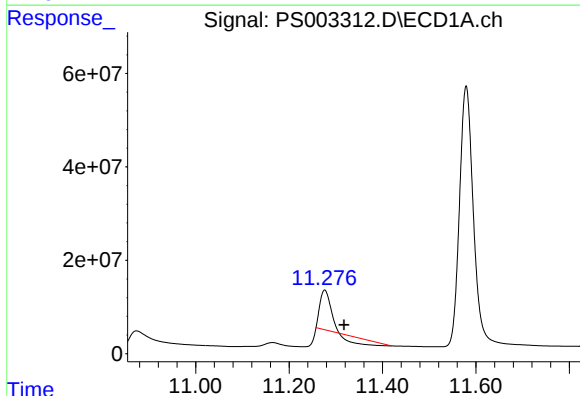


#4 2,4-DCAA

R.T.: 11.276 min
Delta R.T.: -0.041 min
Response: 74150170
Conc: 195.32 ng/ml

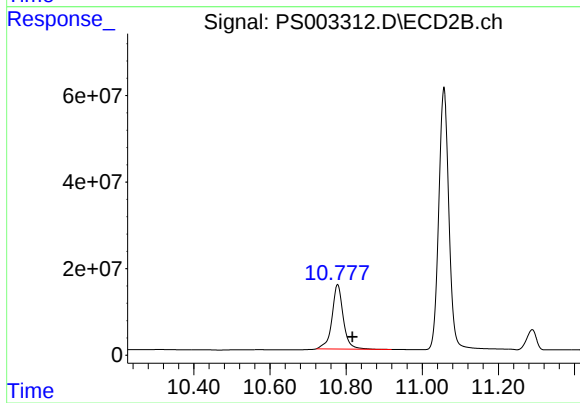

#4 2,4-DCAA


R.T.: 10.778 min
Delta R.T.: -0.039 min
Response: 307194699
Conc: 718.51 ng/ml

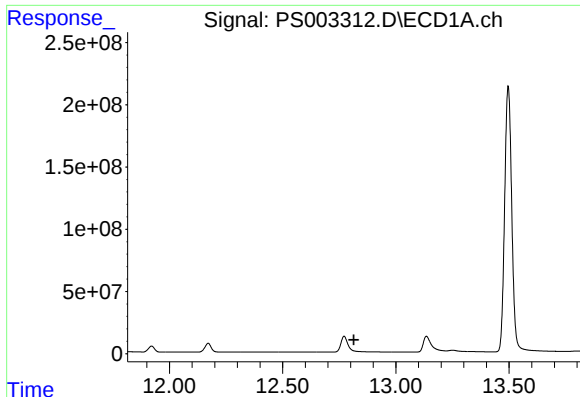

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.815 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

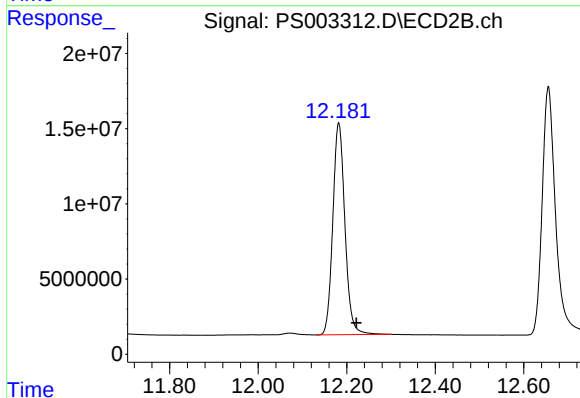


#8 DICHLORPROP

R.T.: 12.182 min
Delta R.T.: -0.040 min
Response: 267625286
Conc: 699.96 ng/ml

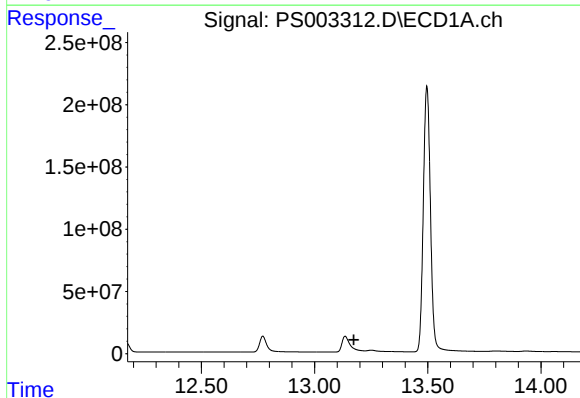


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 13.173 min
Response: 0
Conc: N.D.

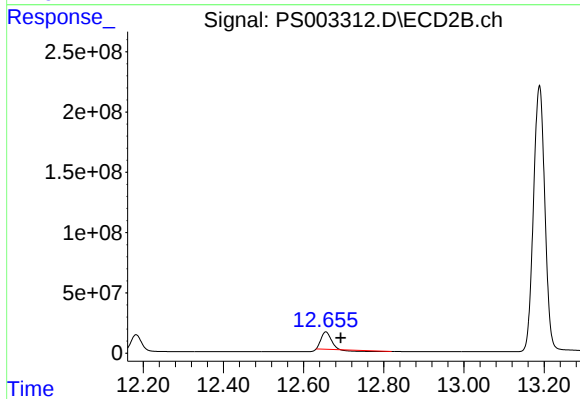

#9 2,4-D


R.T.: 12.655 min
Delta R.T.: -0.037 min
Response: 211085340
Conc: 421.00 ng/ml

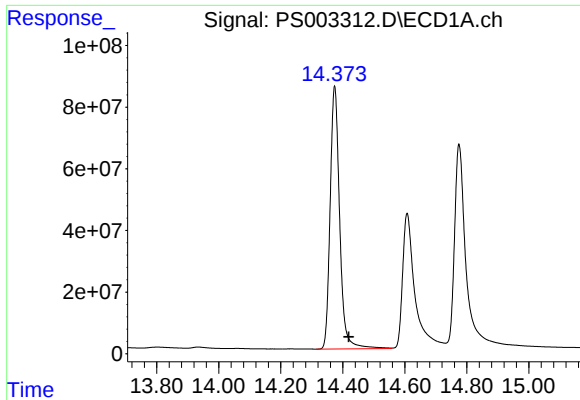

#11 2,4,5-TP (SILVEX)


R.T.: 14.374 min
Delta R.T.: -0.046 min
Response: 1819596145
Conc: 722.53 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

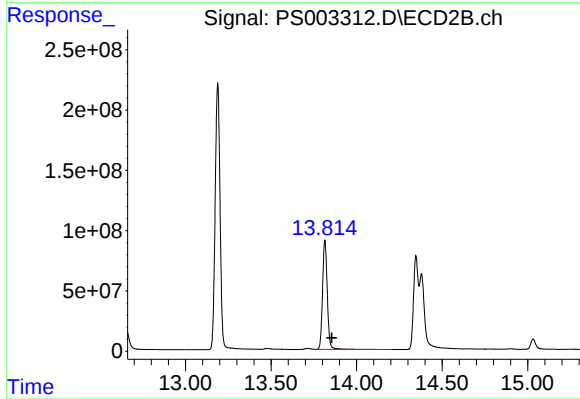


#11 2,4,5-TP (SILVEX)

R.T.: 13.814 min
Delta R.T.: -0.040 min
Response: 1736920560
Conc: 700.27 ng/ml

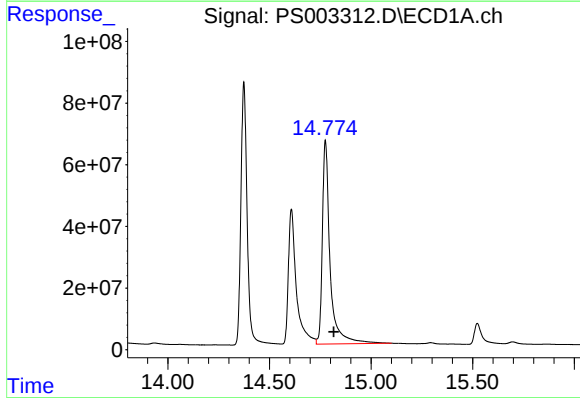


#12 2,4,5-T

R.T.: 14.775 min
Delta R.T.: -0.042 min
Response: 1758017285
Conc: 720.67 ng/ml

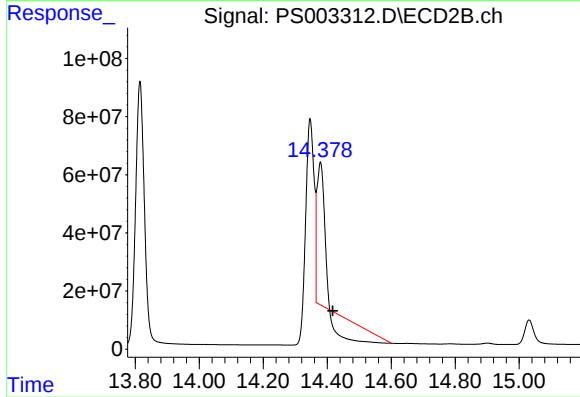

#12 2,4,5-T


R.T.: 14.379 min
Delta R.T.: -0.038 min
Response: 288975300
Conc: 151.02 ng/ml

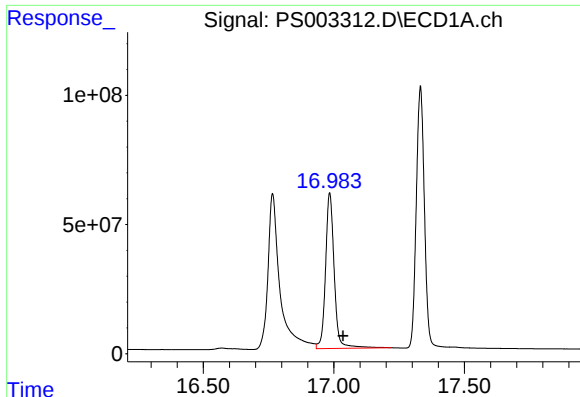

#14 DINOSEB


R.T.: 16.984 min
Delta R.T.: -0.051 min
Response: 1392760975
Conc: 740.31 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

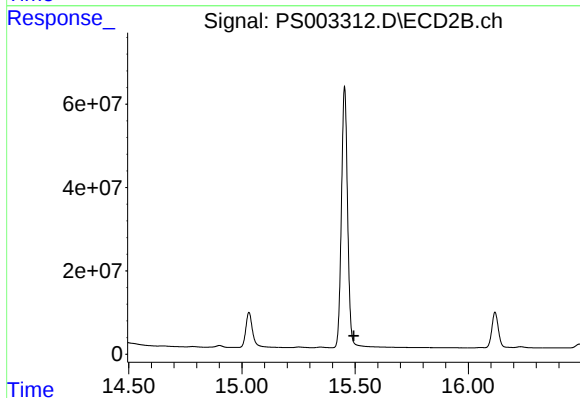


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 15.495 min
Response: 0
Conc: N.D.

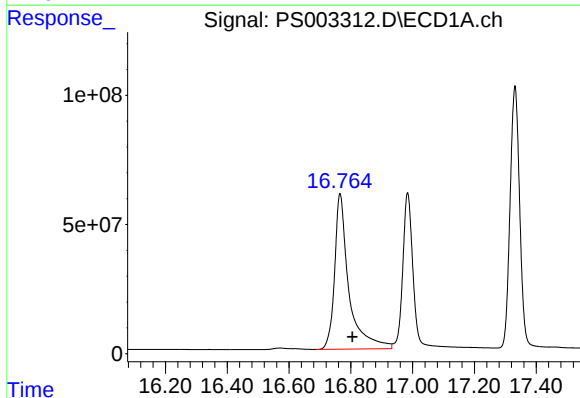


#15 Picloram

R.T.: 16.765 min
Delta R.T.: -0.040 min
Response: 1929203378
Conc: 609.81 ng/ml

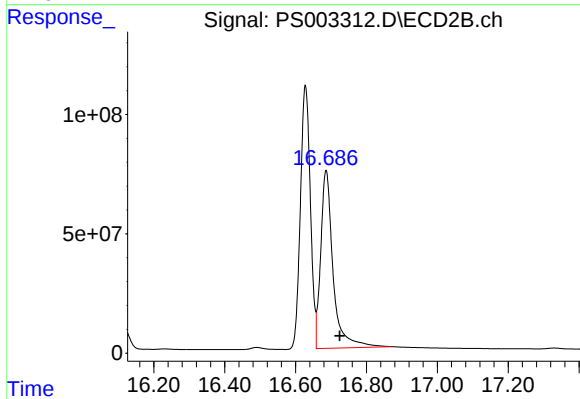

#15 Picloram


R.T.: 16.686 min
Delta R.T.: -0.038 min
Response: 1808358263
Conc: 601.50 ng/ml

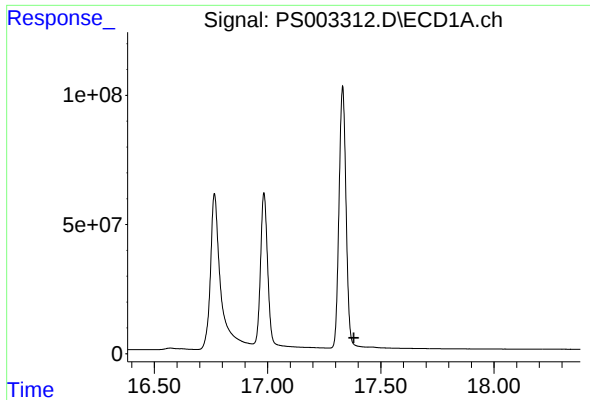

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

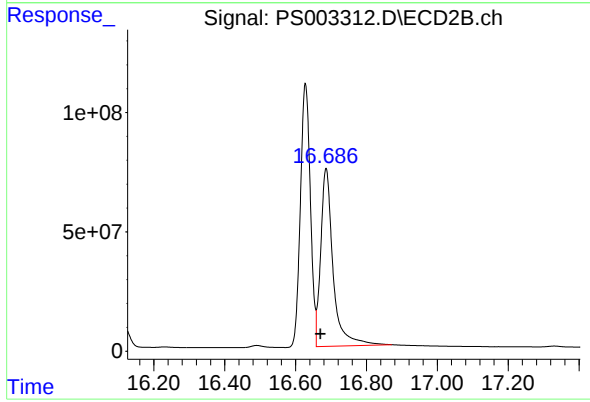

#16 DCPA

R.T.: 16.686 min
Delta R.T.: 0.016 min
Response: 1808358263
Conc: 583.80 ng/ml