

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022119\
 Data File : PS003313.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Feb 2019 03:58
 Operator : EI\SJ
 Sample : K1544-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CHRT-20420

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 04:50:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.286	10.785	139.3E6	152.8E6	366.957	357.366
Target Compounds							
6) T	MCP	11.967	0.000	10994942	0	9.177	N.D. #
12) T	2,4,5-T	0.000	14.407	0	6679458	N.D.	3.491 #
14) T	DINOSEB	0.000	15.527	0	4444229	N.D.	2.535 #
15) T	Picloram	16.822	16.713	4651036	12835810	1.470	4.269 #
16) T	DCPA	0.000	16.713	0	12835810	N.D.	4.144 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022119\
Data File : PS003313.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Feb 2019 03:58
Operator : EI\SJ
Sample : K1544-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
CHRT-20420

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 04:50:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

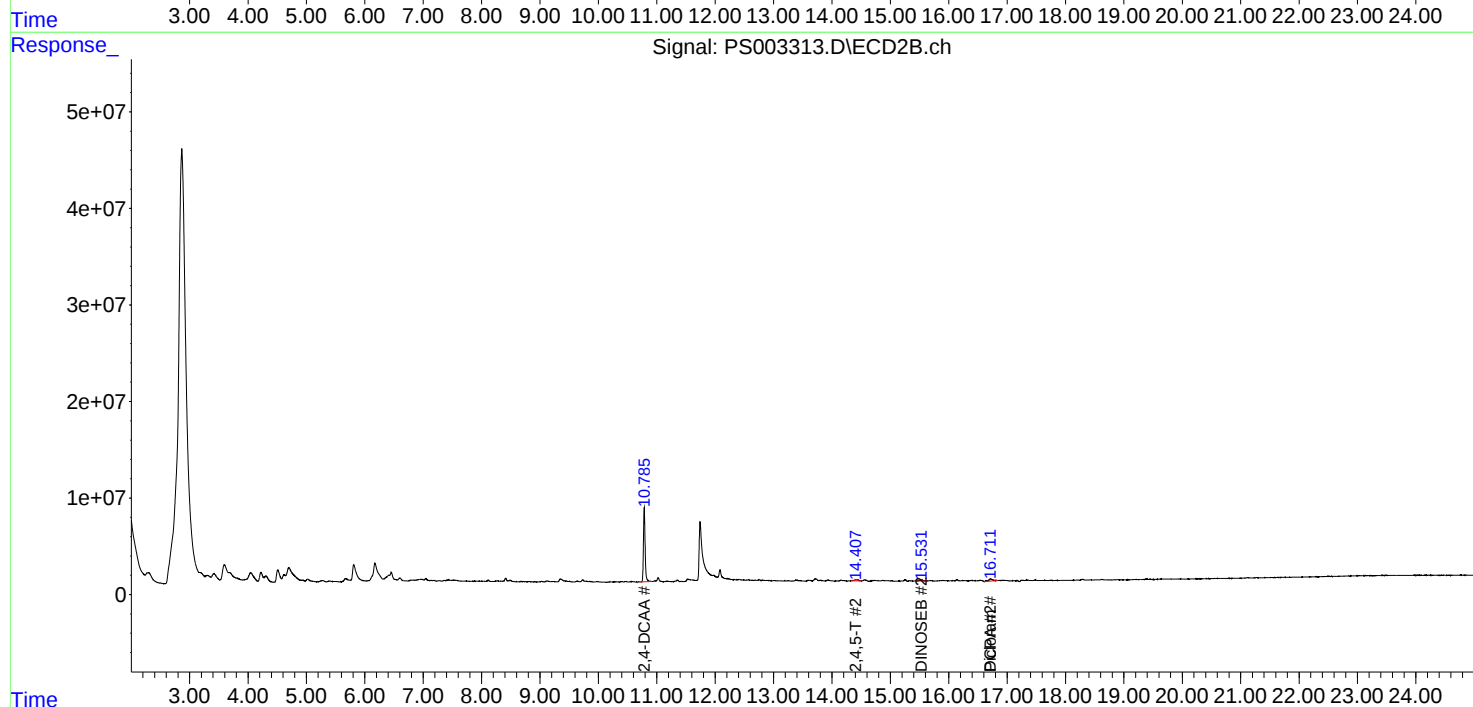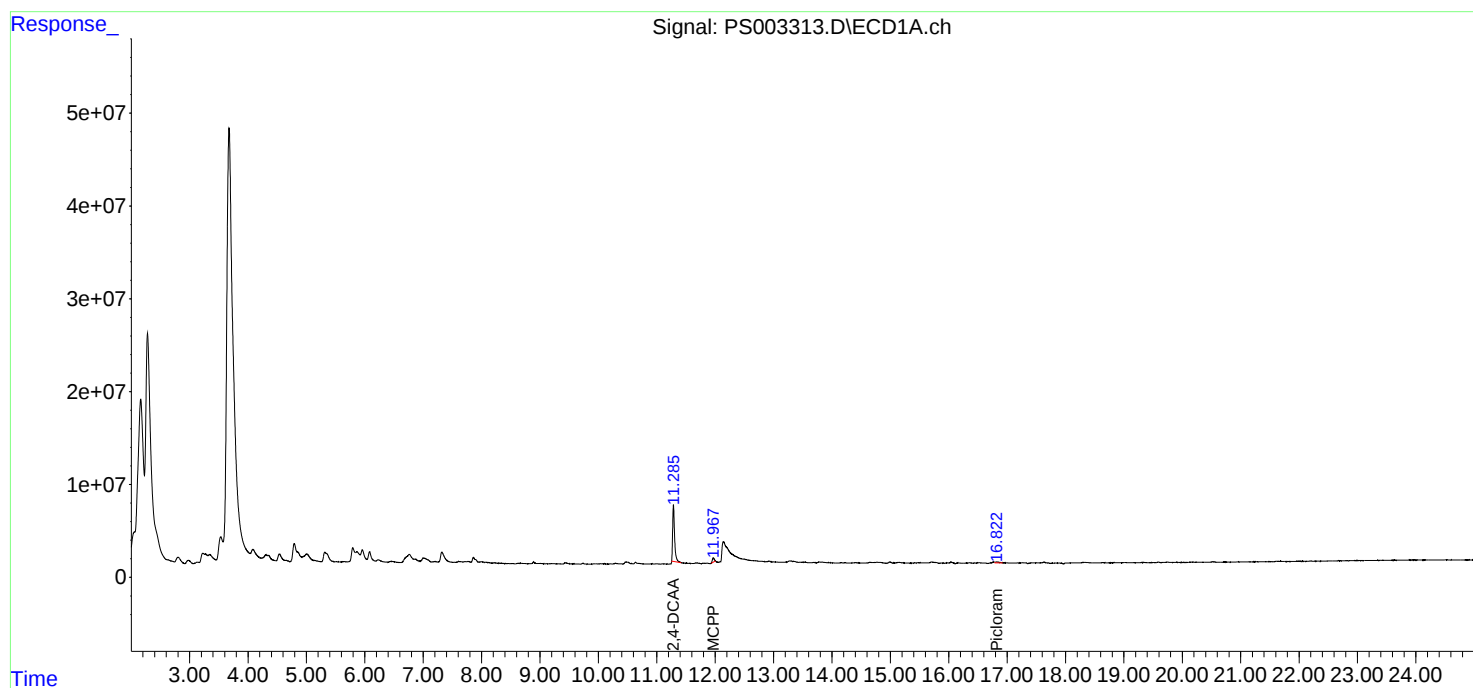


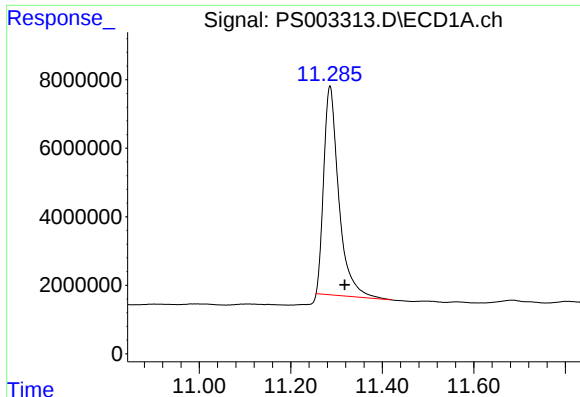

#4 2,4-DCAA


R.T.: 11.286 min
Delta R.T.: -0.032 min
Response: 139312020
Conc: 366.96 ng/ml

Instrument :
ECD_S
ClientSampleId :
CHRT-20420

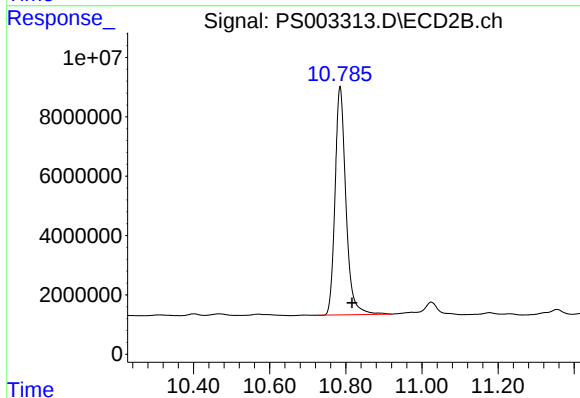


#4 2,4-DCAA

R.T.: 10.785 min
Delta R.T.: -0.031 min
Response: 152790150
Conc: 357.37 ng/ml

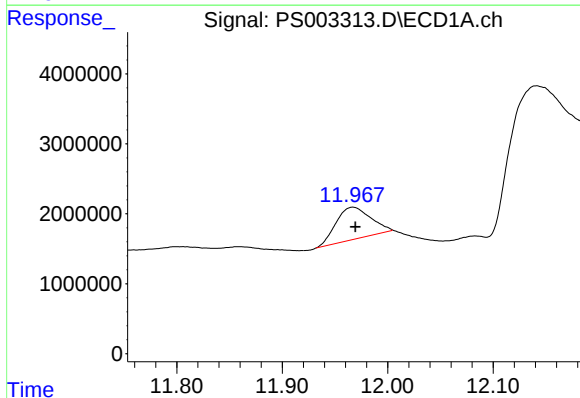


#6 MCP

R.T.: 11.967 min
Delta R.T.: -0.002 min
Response: 10994942
Conc: 9.18 ug/ml

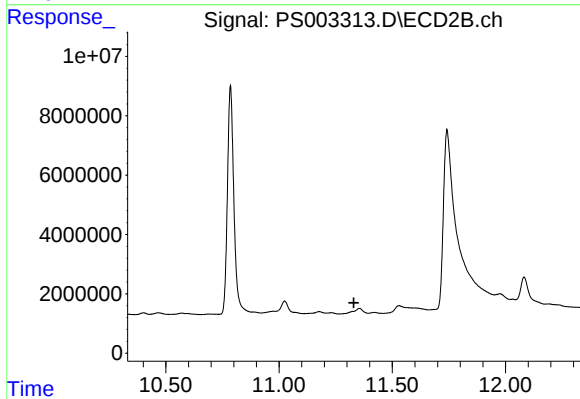

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.330 min
Response: 0
Conc: N.D.

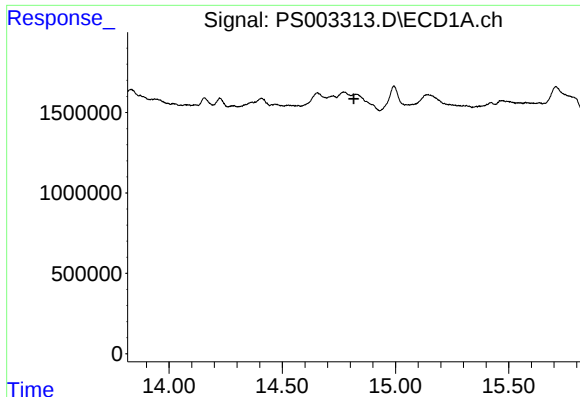

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.817 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CHRT-20420

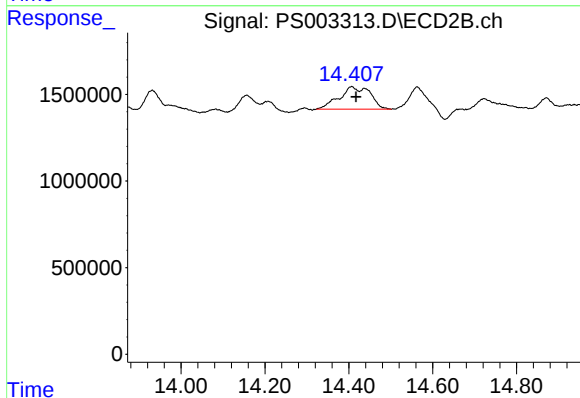


#12 2,4,5-T

R.T.: 14.407 min
Delta R.T.: -0.010 min
Response: 6679458
Conc: 3.49 ng/ml

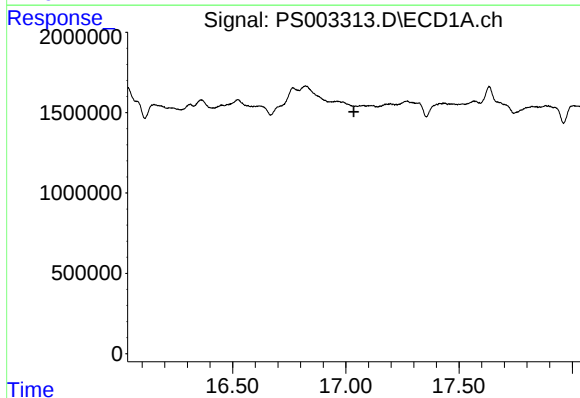


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 17.035 min
Response: 0
Conc: N.D.

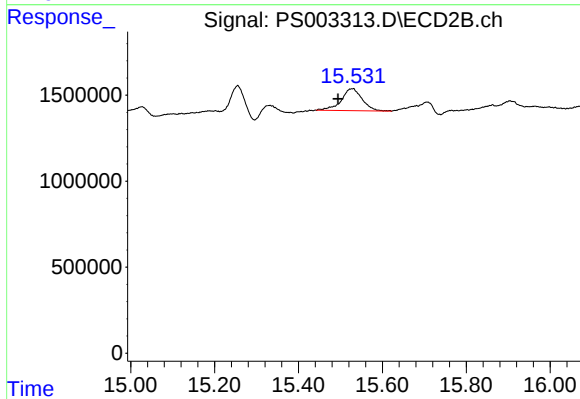

#14 DINOSEB


R.T.: 15.527 min
Delta R.T.: 0.032 min
Response: 4444229
Conc: 2.54 ng/ml

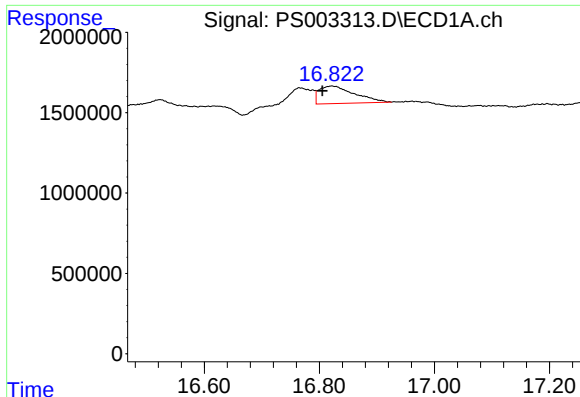

#15 Picloram


R.T.: 16.822 min
Delta R.T.: 0.016 min
Response: 4651036
Conc: 1.47 ng/ml

Instrument :
ECD_S
ClientSampleId :
CHRT-20420

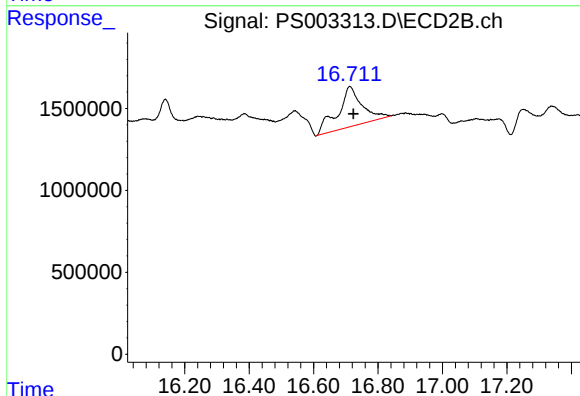


#15 Picloram

R.T.: 16.713 min
Delta R.T.: -0.011 min
Response: 12835810
Conc: 4.27 ng/ml

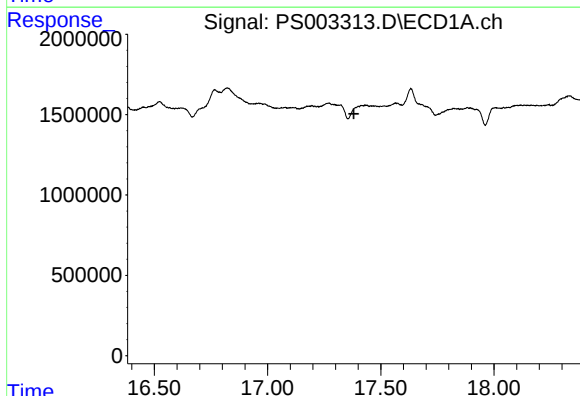

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.382 min
Response: 0
Conc: N.D.

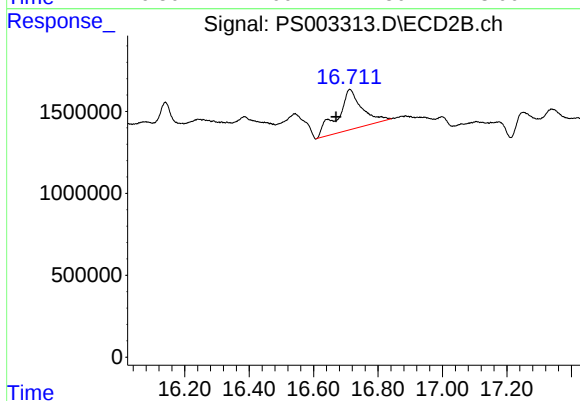

#16 DCPA

R.T.: 16.713 min
Delta R.T.: 0.043 min
Response: 12835810
Conc: 4.14 ng/ml