

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022119\
 Data File : PS003315.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Feb 2019 05:00
 Operator : EI\SJ
 Sample : K1546-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 RT-3422

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 05:41:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.309	10.810	142.1E6	142.9E6	374.230	334.350
Target Compounds							
1) T	Dalapon	2.826	2.305	7359013	7958924	13.340	14.851
6) T	MCPD	11.992	0.000	637776	0	0.532	N.D. #
7) T	MCPA	0.000	11.762	0	193.5E6	N.D.	122.990 #
15) T	Picloram	0.000	16.740	0	5816119	N.D.	1.935 #
16) T	DCPA	0.000	16.740	0	5816119	N.D.	1.878 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022119\
Data File : PS003315.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Feb 2019 05:00
Operator : EI\SJ
Sample : K1546-06
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
RT-3422

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 05:41:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

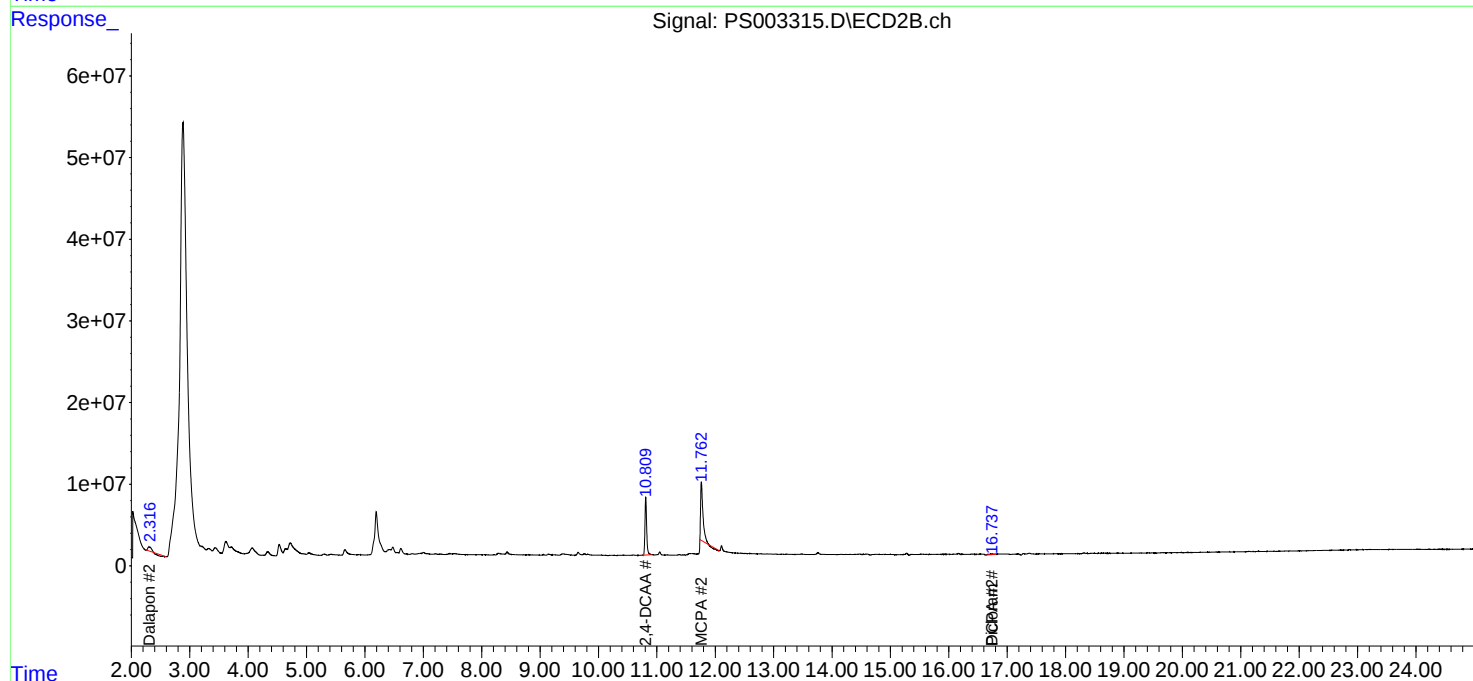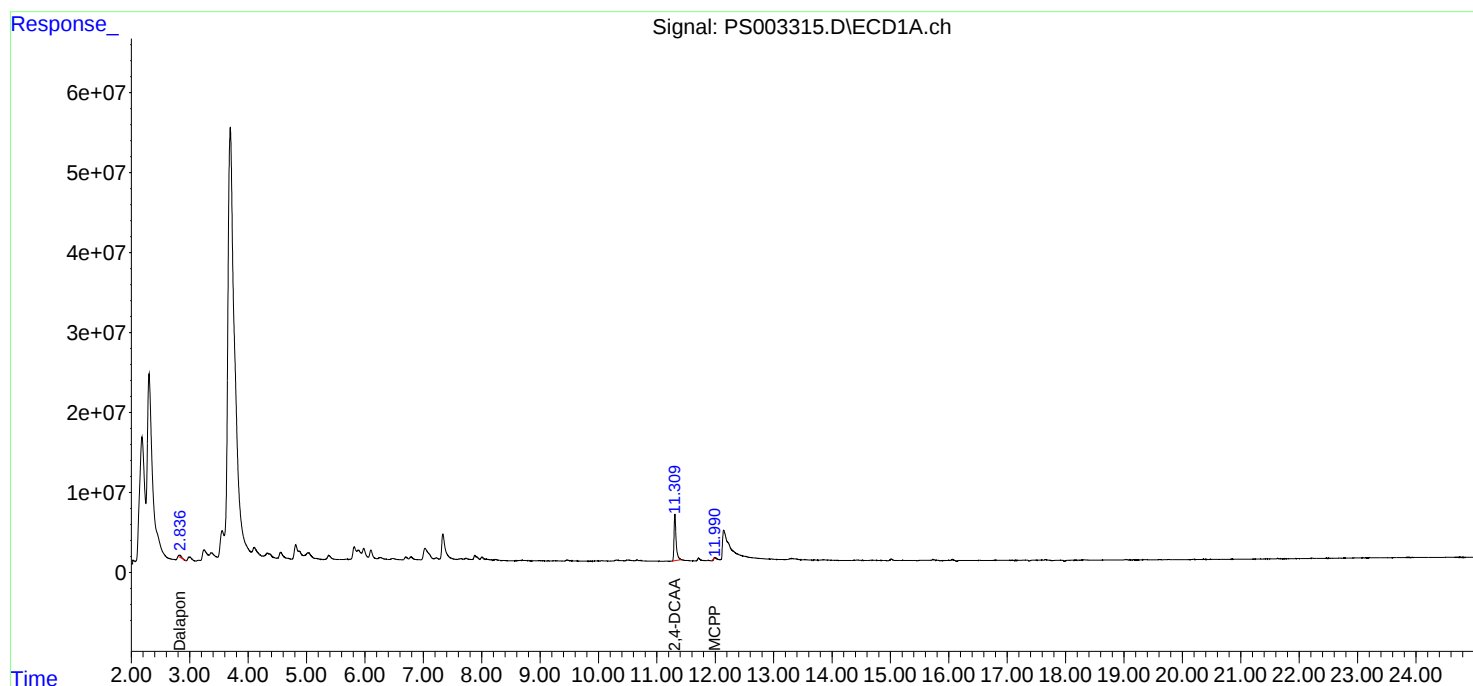


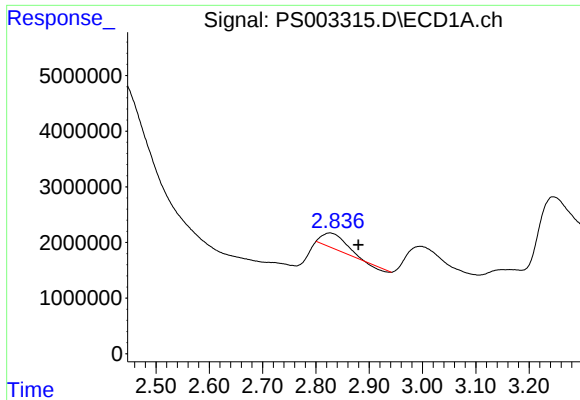

#1 Dalapon


R.T.: 2.826 min
Delta R.T.: -0.054 min
Response: 7359013
Conc: 13.34 ng/ml

Instrument :
ECD_S
ClientSampleId :
RT-3422

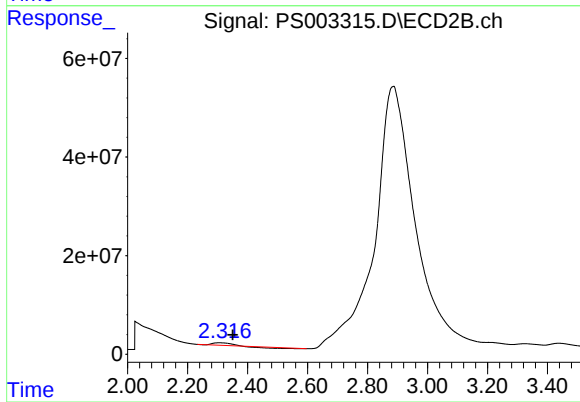


#1 Dalapon

R.T.: 2.305 min
Delta R.T.: -0.046 min
Response: 7958924
Conc: 14.85 ng/ml

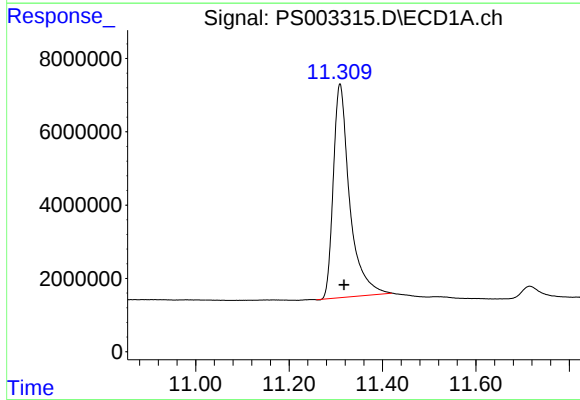


#4 2,4-DCAA

R.T.: 11.309 min
Delta R.T.: -0.009 min
Response: 142073060
Conc: 374.23 ng/ml

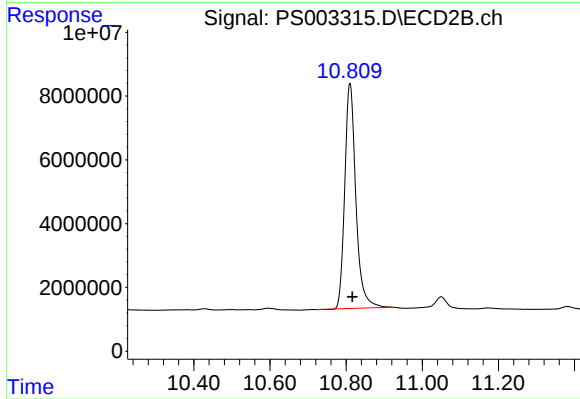

#4 2,4-DCAA


R.T.: 10.810 min
Delta R.T.: -0.007 min
Response: 142949909
Conc: 334.35 ng/ml

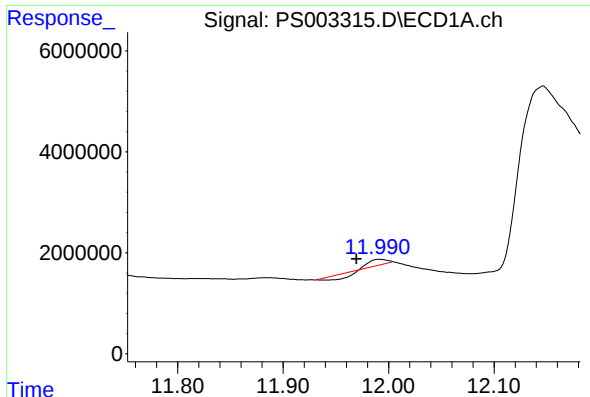

#6 MCPP


R.T.: 11.992 min
Delta R.T.: 0.022 min
Response: 637776
Conc: 0.53 ug/ml

Instrument :
ECD_S
ClientSampleId :
RT-3422

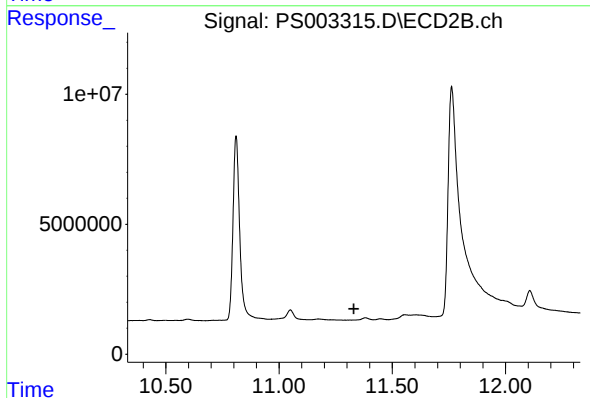


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.330 min
Response: 0
Conc: N.D.

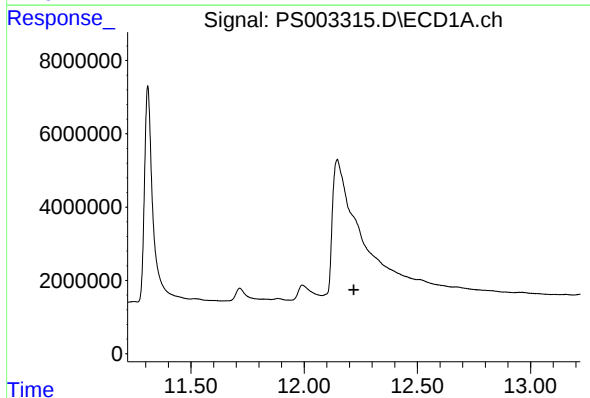


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.219 min
Response: 0
Conc: N.D.

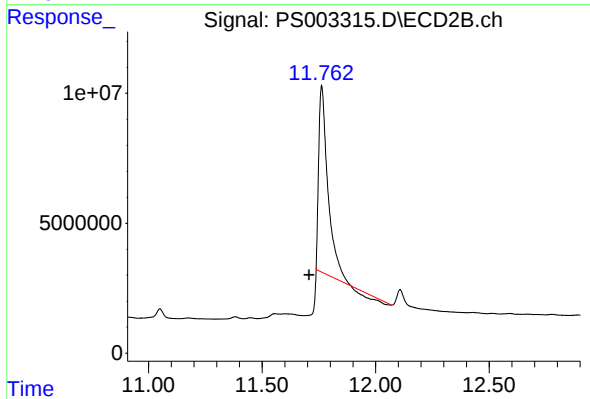

#7 MCPA


R.T.: 11.762 min
Delta R.T.: 0.056 min
Response: 193470639
Conc: 122.99 ug/ml

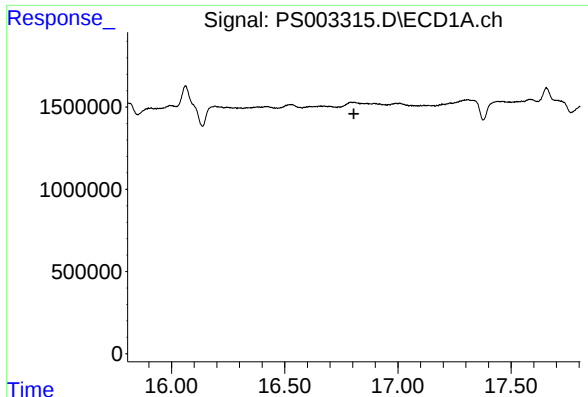

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.806 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
RT-3422

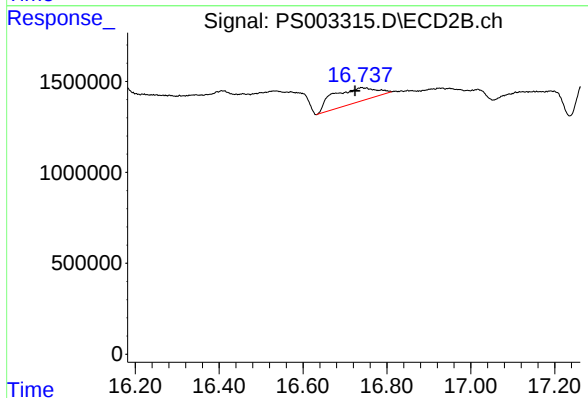


#15 Picloram

R.T.: 16.740 min
Delta R.T.: 0.015 min
Response: 5816119
Conc: 1.93 ng/ml

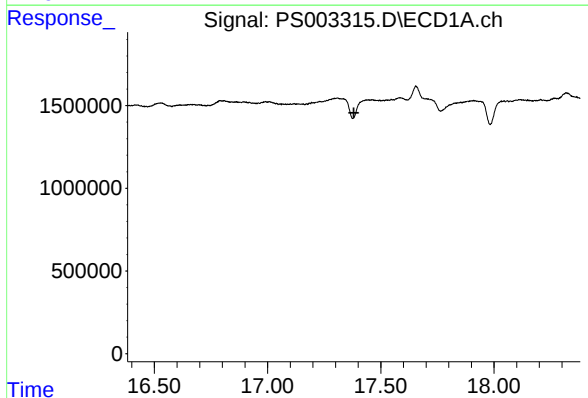

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.382 min
Response: 0
Conc: N.D.

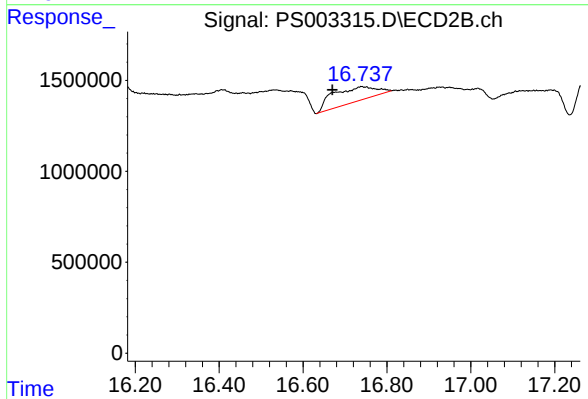

#16 DCPA

R.T.: 16.740 min
Delta R.T.: 0.070 min
Response: 5816119
Conc: 1.88 ng/ml