

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022119\
 Data File : PS003316.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Feb 2019 05:31
 Operator : EI\SJ
 Sample : K1546-09
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 07:10:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.282	10.781	76754900	110.1E6	202.178	257.602 #
Target Compounds							
2) T	3,5-DICHL...	0.000	9.031	0	1858289	N.D.	3.297 #
5) T	DICAMBA	11.682	0.000	22903493	0	14.289	N.D. #
6) T	MCP	11.965	0.000	18375705	0	15.337	N.D. #
15) T	Picloram	16.757	0.000	4798140	0	1.517	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022119\
Data File : PS003316.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Feb 2019 05:31
Operator : EI\SJ
Sample : K1546-09
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 07:10:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

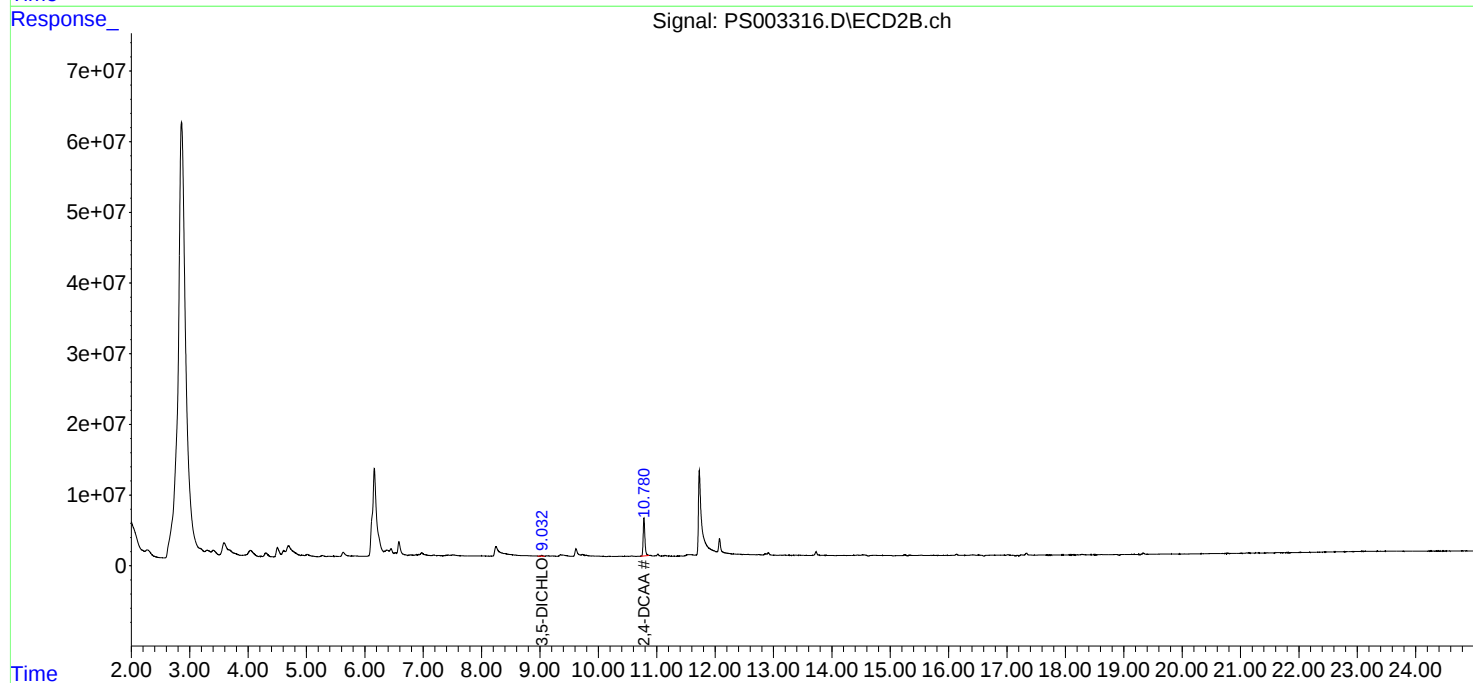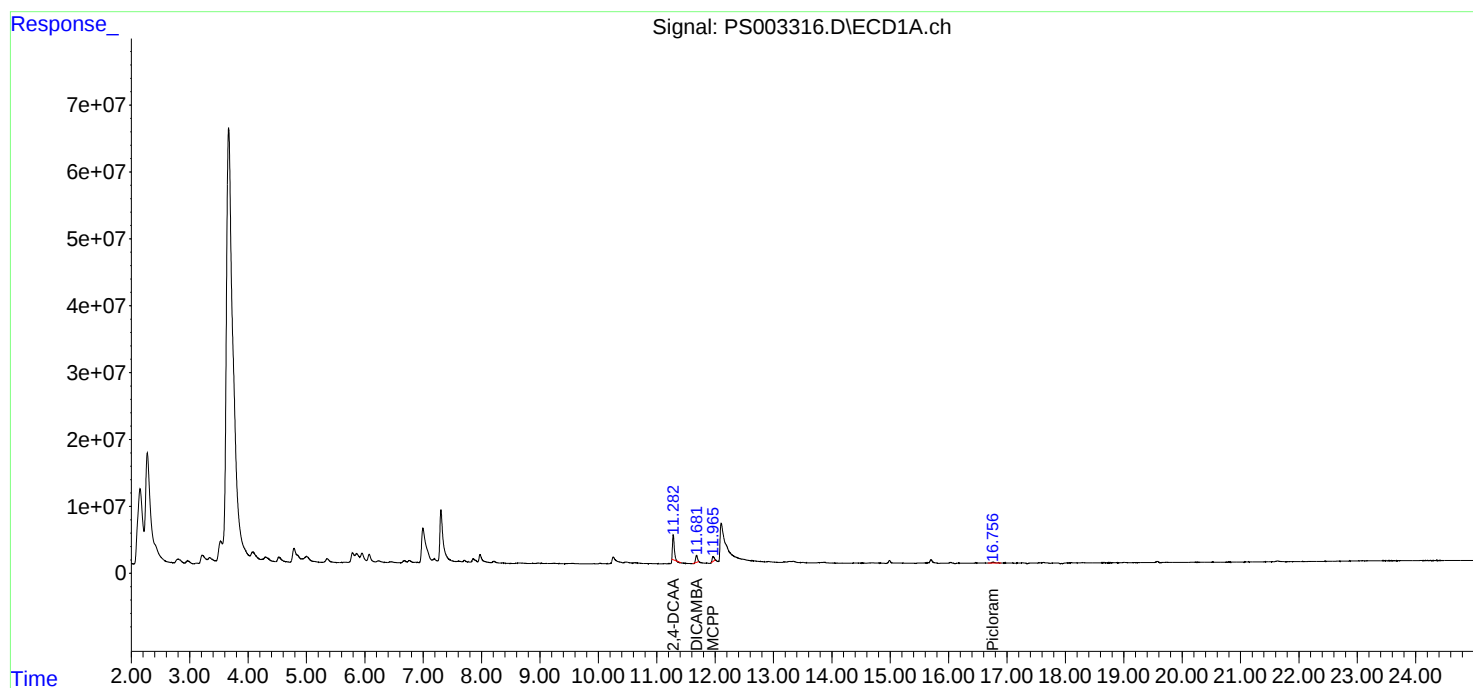


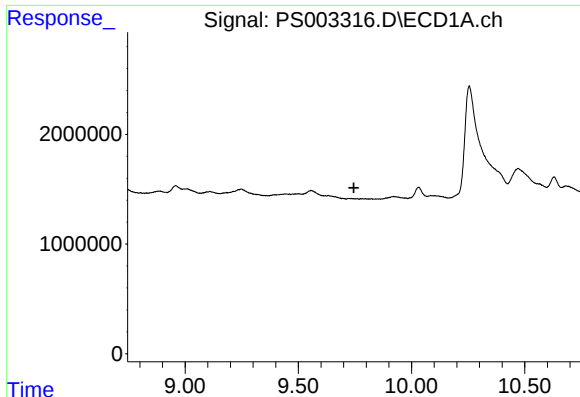

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.745 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

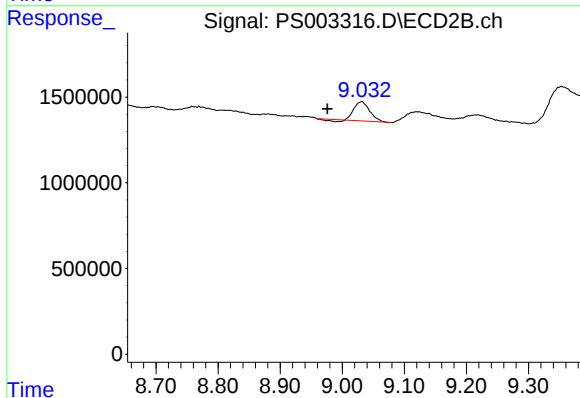


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.031 min
Delta R.T.: 0.054 min
Response: 1858289
Conc: 3.30 ng/ml

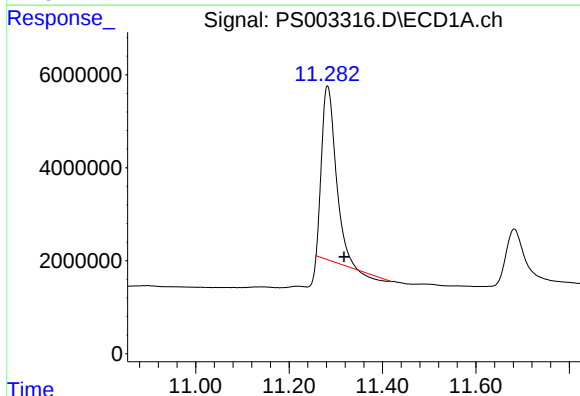


#4 2,4-DCAA

R.T.: 11.282 min
Delta R.T.: -0.035 min
Response: 76754900
Conc: 202.18 ng/ml

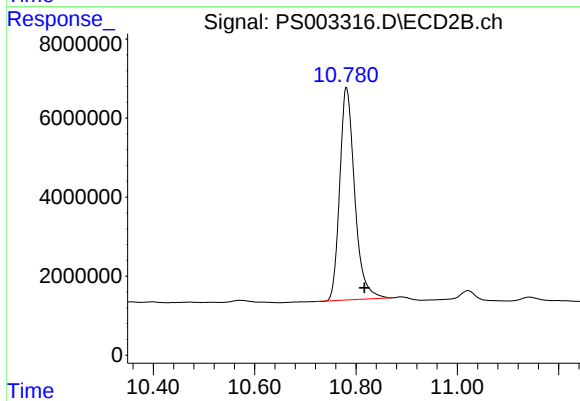

#4 2,4-DCAA


R.T.: 10.781 min
Delta R.T.: -0.035 min
Response: 110136540
Conc: 257.60 ng/ml

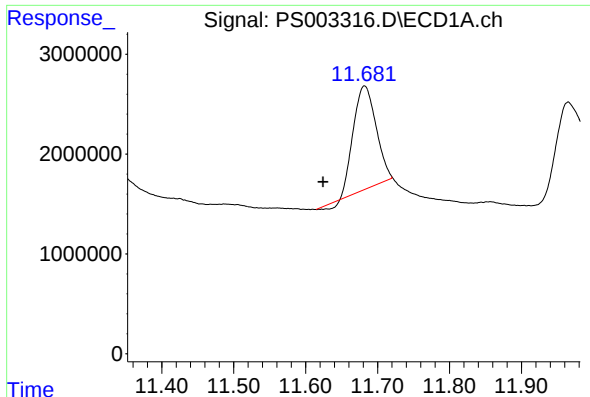

#5 DICAMBA


R.T.: 11.682 min
Delta R.T.: 0.058 min
Response: 22903493
Conc: 14.29 ng/ml

Instrument :
ECD_S
ClientSampleId :

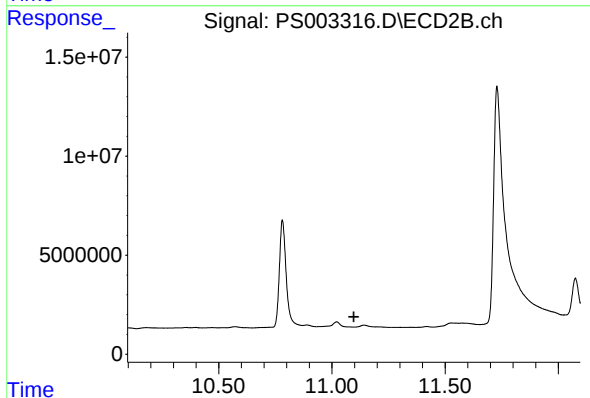


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.097 min
Response: 0
Conc: N.D.

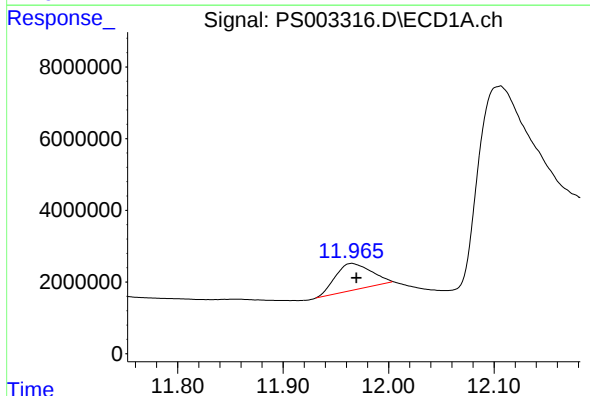


#6 MCP

R.T.: 11.965 min
Delta R.T.: -0.004 min
Response: 18375705
Conc: 15.34 ug/ml

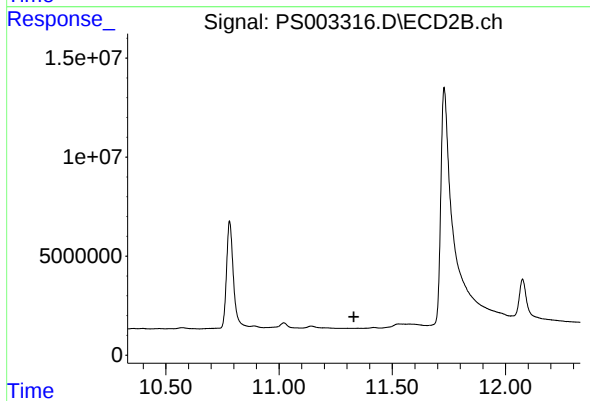

#6 MCP


R.T.: 0.000 min
Exp R.T. : 11.330 min
Response: 0
Conc: N.D.

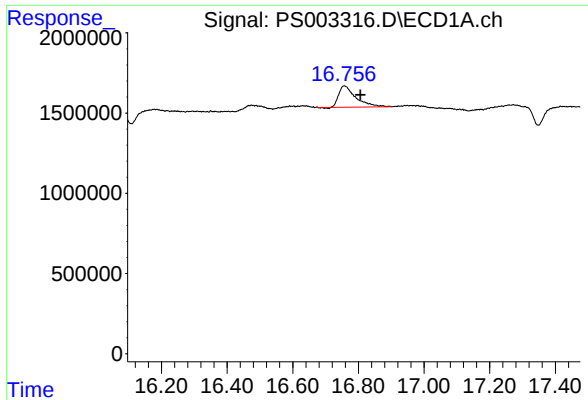

#15 Picloram

R.T.: 16.757 min
Delta R.T.: -0.049 min
Response: 4798140
Conc: 1.52 ng/ml

Instrument :
ECD_S
ClientSampleId :

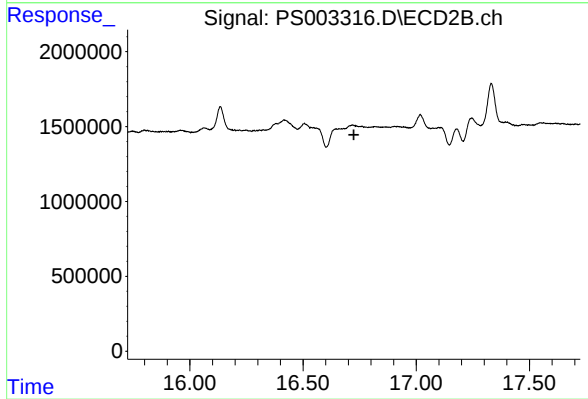

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.724 min
Response: 0
Conc: N.D.