

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022119\
 Data File : PS003319.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Feb 2019 07:04
 Operator : EI\SJ
 Sample : K1546-15
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 11:42:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.280	10.780	133.9E6	191.6E6	352.610	448.108 #
Target Compounds							
5) T	DICAMBA	11.691	0.000	3593225	0	2.242	N.D. #
6) T	MCPD	11.967	0.000	4898928	0	4.089	N.D. #
15) T	Picloram	0.000	16.722	0	3822366	N.D.	1.271 #
16) T	DCPA	0.000	16.722	0	3822366	N.D.	1.234 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022119\
Data File : PS003319.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Feb 2019 07:04
Operator : EI\SJ
Sample : K1546-15
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 11:42:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

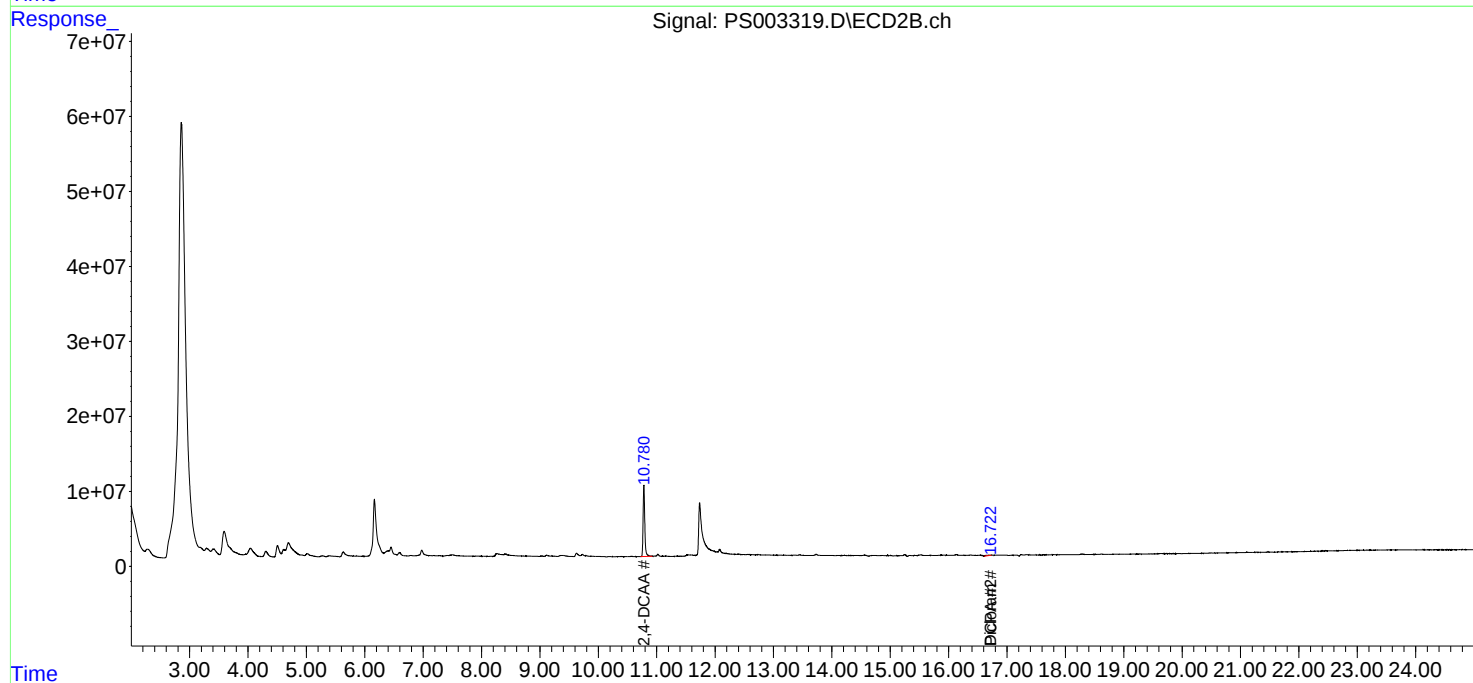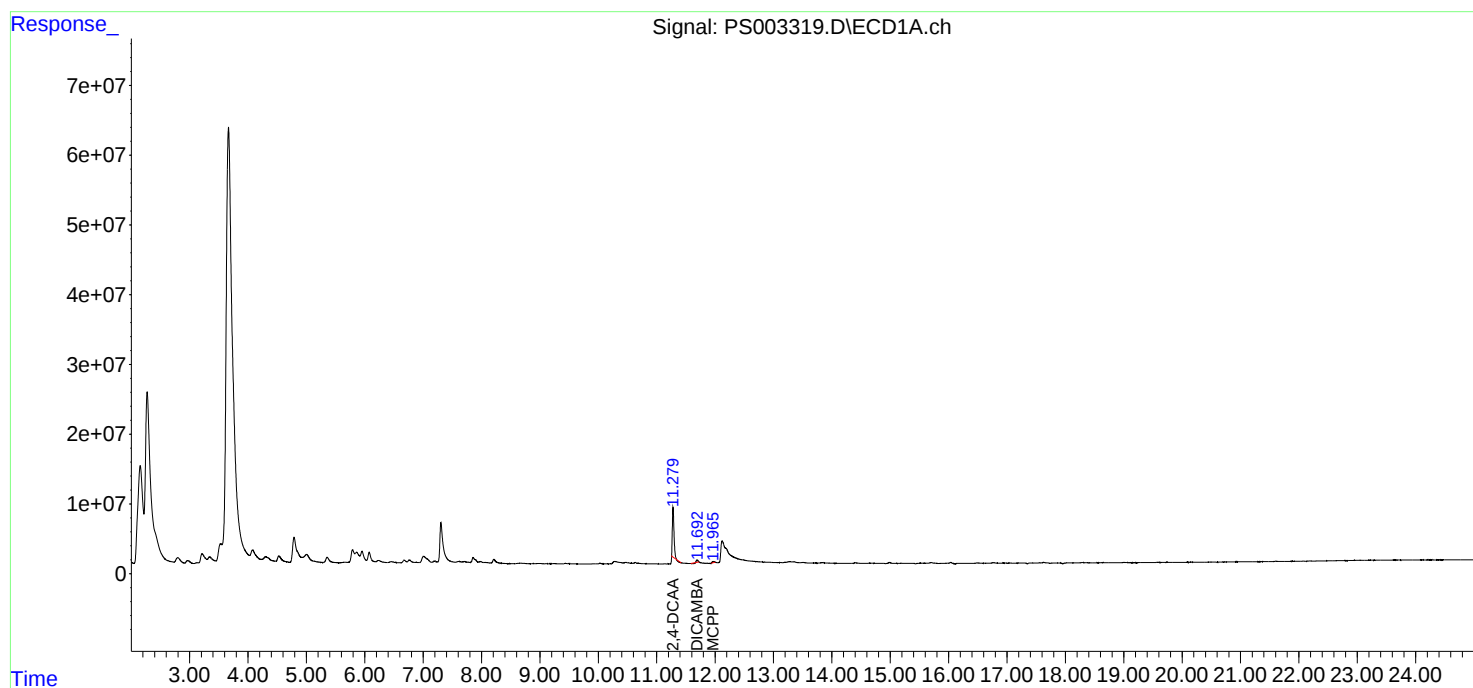


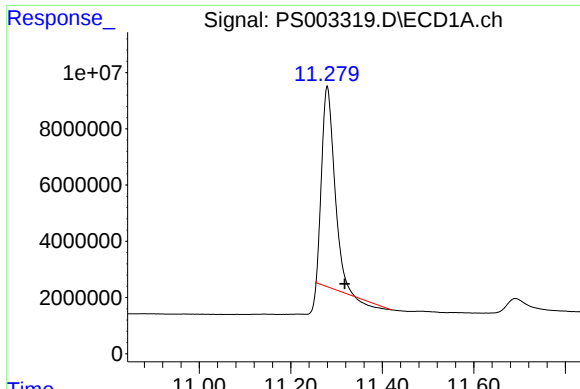

#4 2,4-DCAA


R.T.: 11.280 min
Delta R.T.: -0.038 min
Response: 133865229
Conc: 352.61 ng/ml

Instrument :
ECD_S
ClientSampleId :

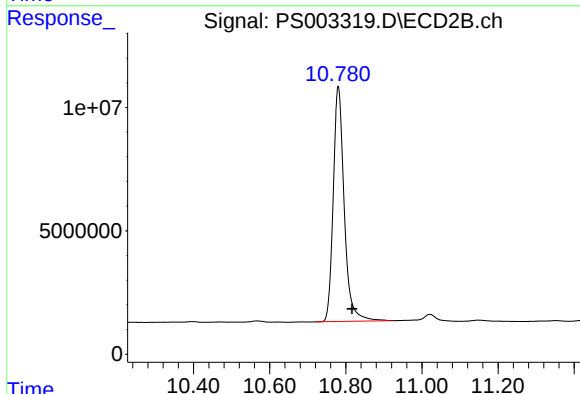


#4 2,4-DCAA

R.T.: 10.780 min
Delta R.T.: -0.036 min
Response: 191586483
Conc: 448.11 ng/ml

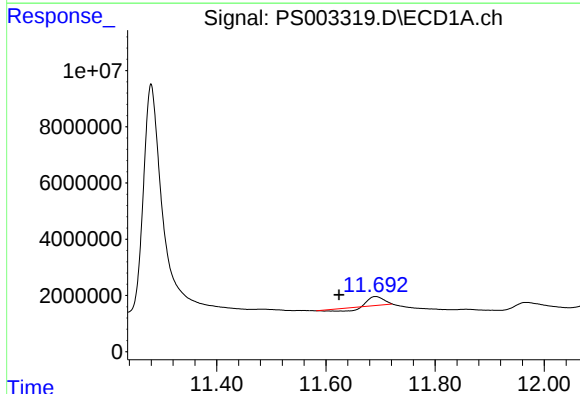


#5 DICAMBA

R.T.: 11.691 min
Delta R.T.: 0.067 min
Response: 3593225
Conc: 2.24 ng/ml

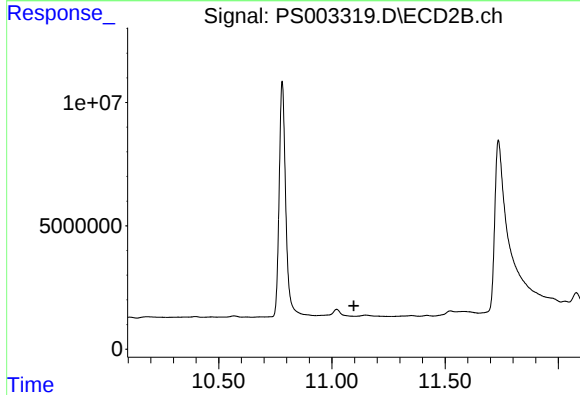

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.097 min
Response: 0
Conc: N.D.

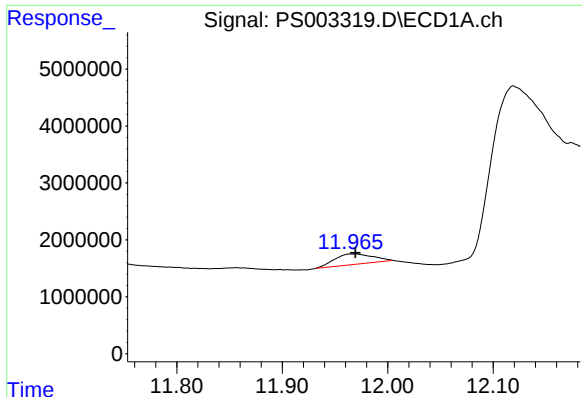

#6 MCPP


R.T.: 11.967 min
Delta R.T.: -0.002 min
Response: 4898928
Conc: 4.09 ug/ml

Instrument :
ECD_S
ClientSampleId :

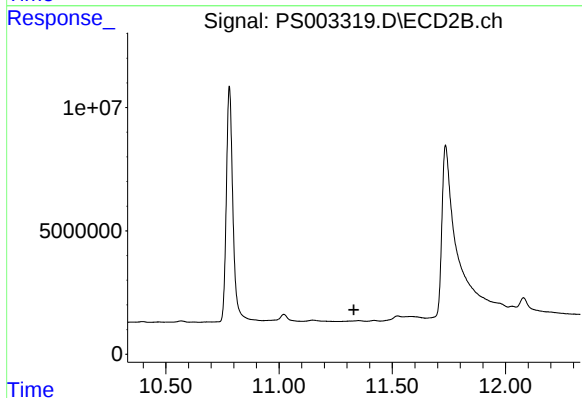


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.330 min
Response: 0
Conc: N.D.

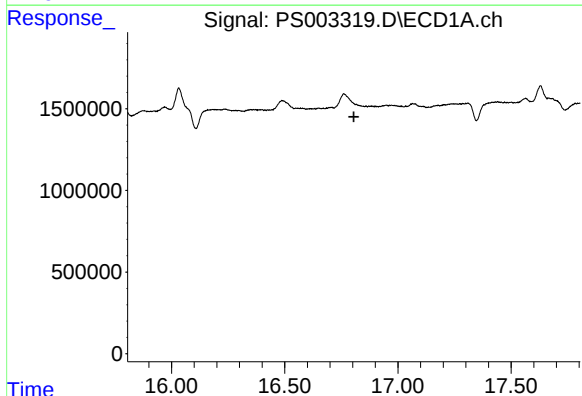


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.806 min
Response: 0
Conc: N.D.

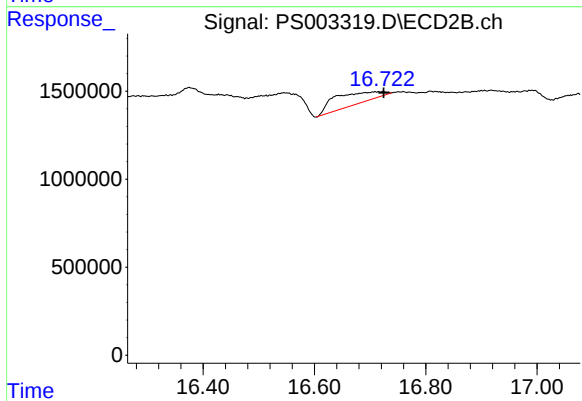

#15 Picloram


R.T.: 16.722 min
Delta R.T.: -0.002 min
Response: 3822366
Conc: 1.27 ng/ml

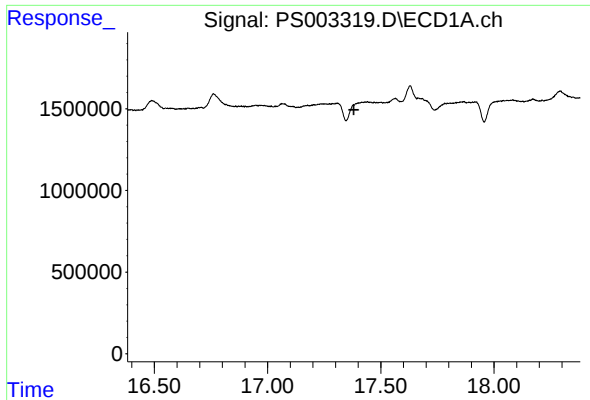

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

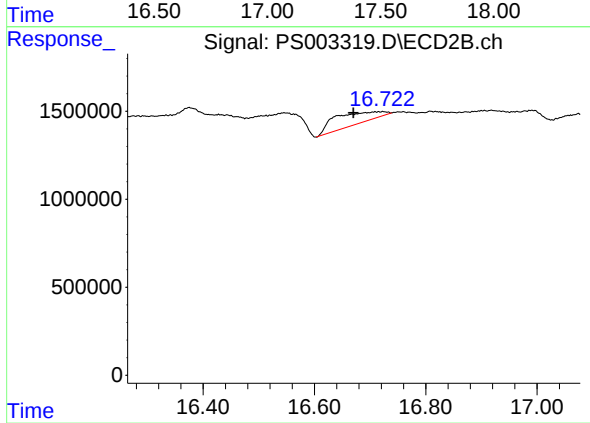

#16 DCPA

R.T.: 16.722 min
Delta R.T.: 0.053 min
Response: 3822366
Conc: 1.23 ng/ml