

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022120\
 Data File : PS008934.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2020 17:21
 Operator : DD\AJ
 Sample : PB126982BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 23:28:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.247	6.940	1125.7E6	552.4E6	514.800	573.313
Target Compounds							
1) T	Dalapon	0.000	2.591	0	267.2E6	N.D.	182.730
2) T	3,5-DICHL...	0.000	6.114	0	68504662	N.D.	46.944
7) T	MCPA	7.799	7.407	66116019	42528233	8.219	9.613
15) T	Picloram	11.043	11.030	347.4E6	195.7E6	25.378	26.932
16) T	DCPA	0.000	11.030	0	195.7E6	N.D.	28.283



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022120\
Data File : PS008934.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2020 17:21
Operator : DD\AJ
Sample : PB126982BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 23:28:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

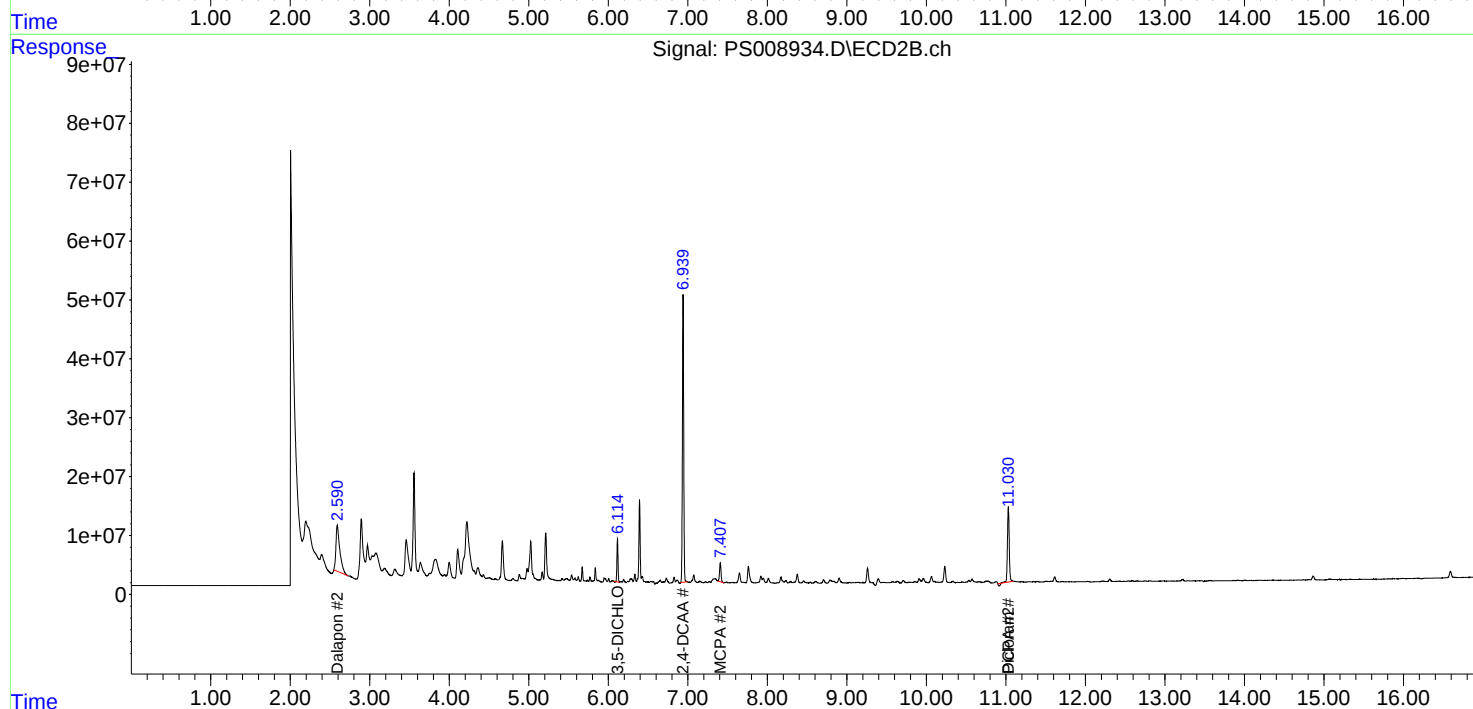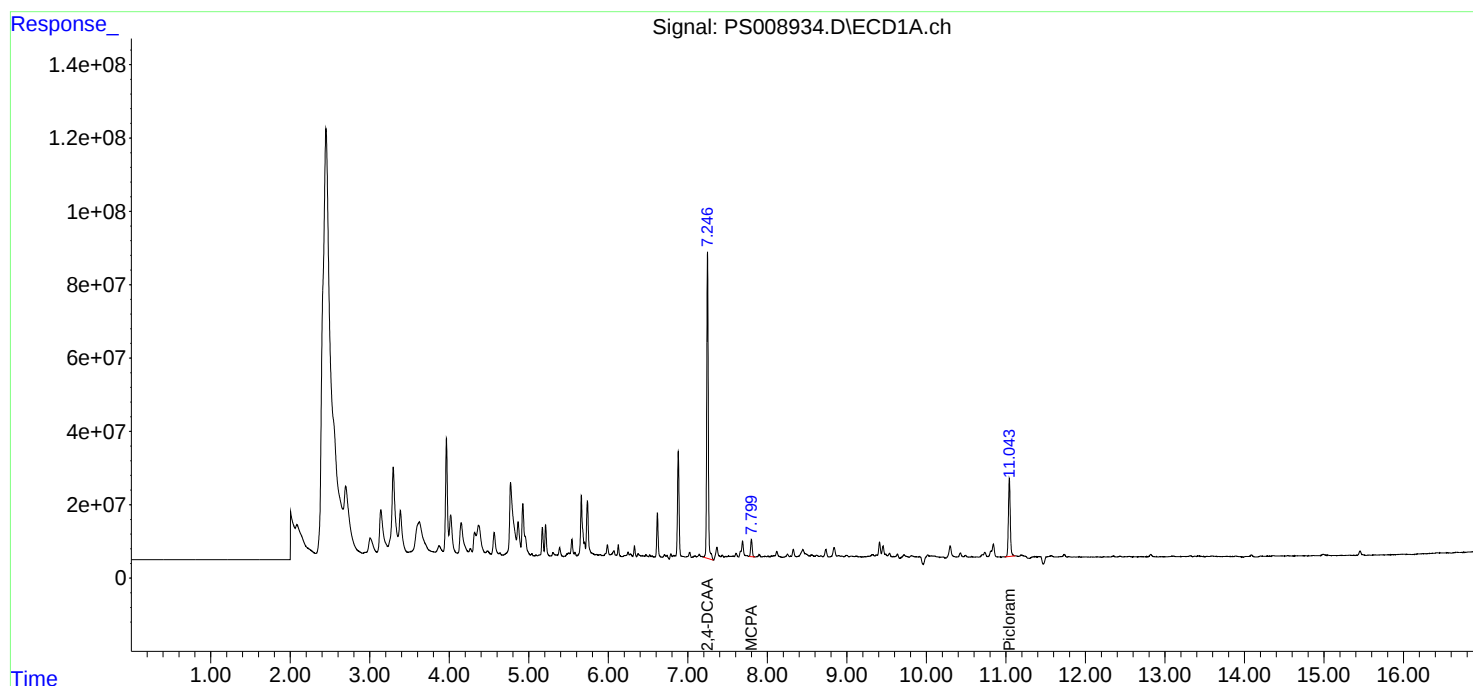


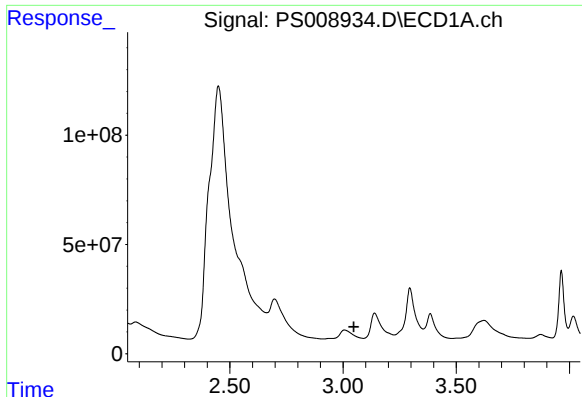

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.048 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

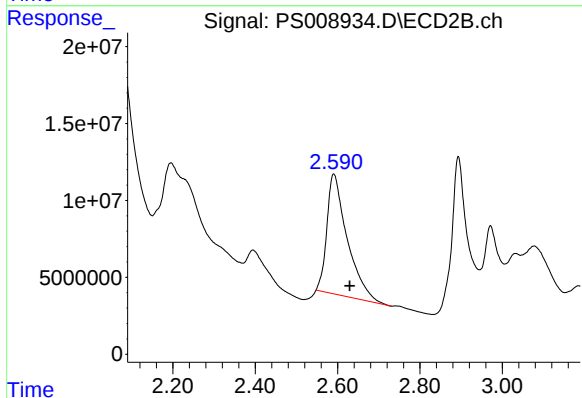


#1 Dalapon

R.T.: 2.591 min
Delta R.T.: -0.039 min
Response: 267191822
Conc: 182.73 ng/ml

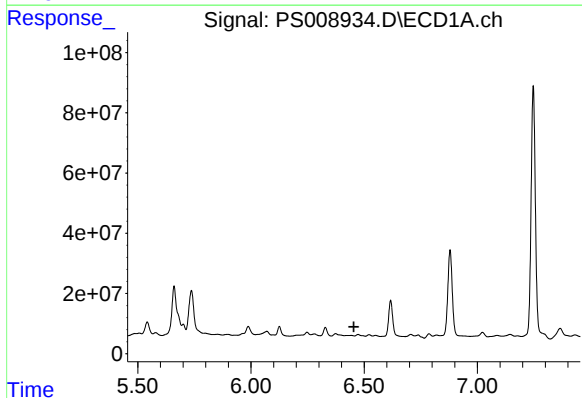


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

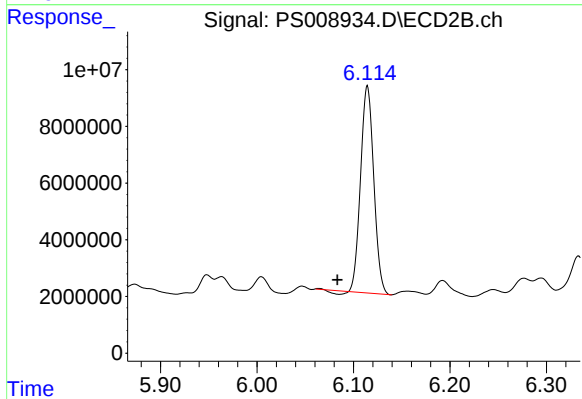

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.114 min
Delta R.T.: 0.031 min
Response: 68504662
Conc: 46.94 ng/ml

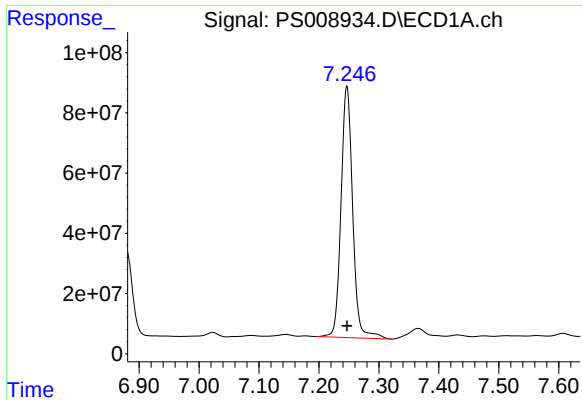

#4 2,4-DCAA


R.T.: 7.247 min
Delta R.T.: 0.000 min
Response: 1125656940
Conc: 514.80 ng/ml

Instrument :
ECD_S
ClientSampleId :

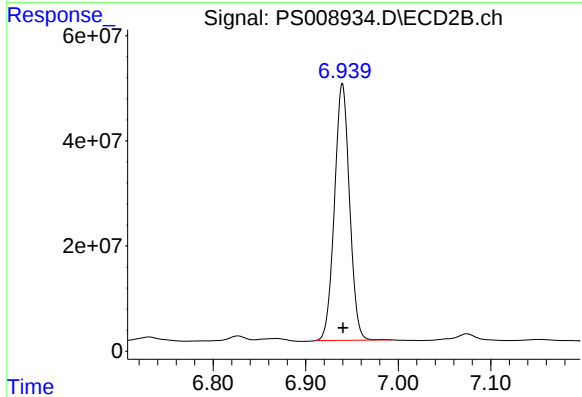


#4 2,4-DCAA

R.T.: 6.940 min
Delta R.T.: 0.000 min
Response: 552419306
Conc: 573.31 ng/ml

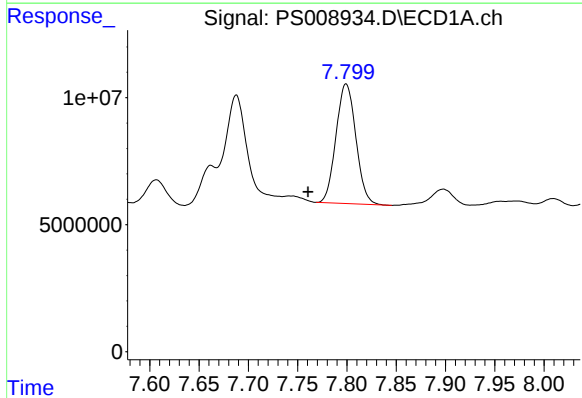


#7 MCPA

R.T.: 7.799 min
Delta R.T.: 0.039 min
Response: 66116019
Conc: 8.22 ug/ml

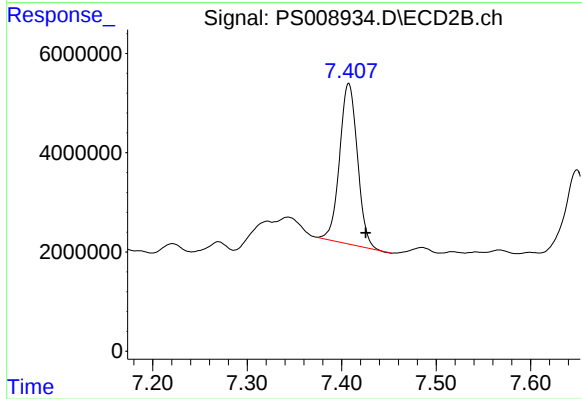

#7 MCPA


R.T.: 7.407 min
Delta R.T.: -0.018 min
Response: 42528233
Conc: 9.61 ug/ml

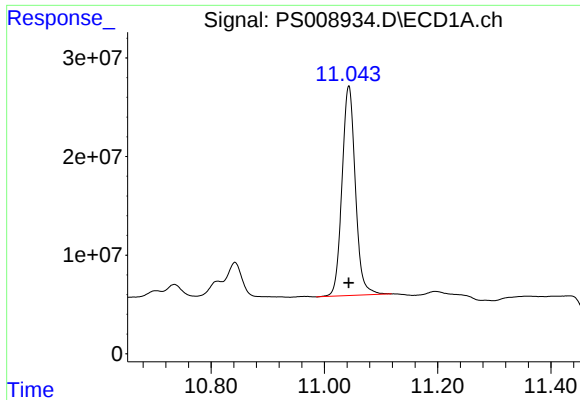

#15 Picloram


R.T.: 11.043 min
Delta R.T.: 0.000 min
Response: 347447588
Conc: 25.38 ng/ml

Instrument :
ECD_S
ClientSampleId :

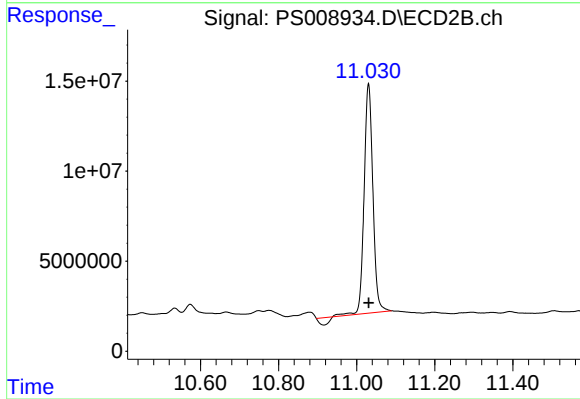


#15 Picloram

R.T.: 11.030 min
Delta R.T.: 0.000 min
Response: 195703251
Conc: 26.93 ng/ml

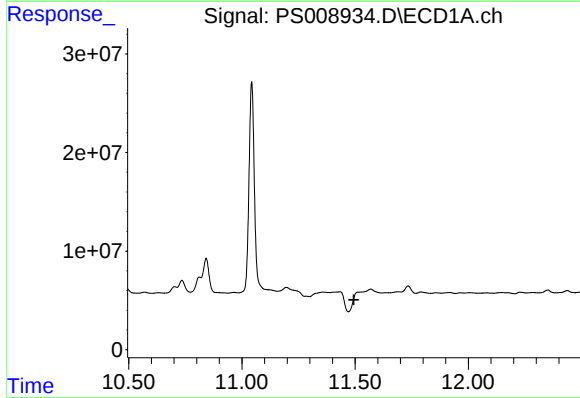

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.495 min
Response: 0
Conc: N.D.

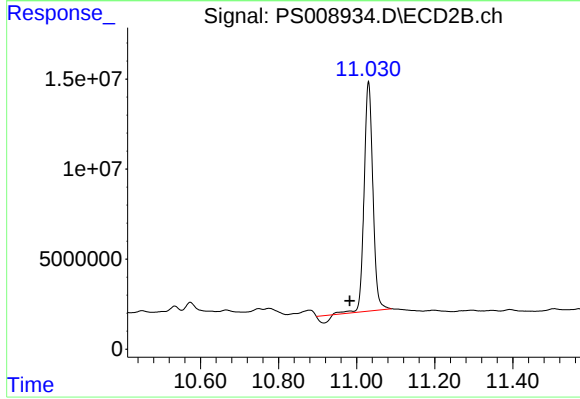

#16 DCPA

R.T.: 11.030 min
Delta R.T.: 0.048 min
Response: 195703251
Conc: 28.28 ng/ml