

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022122\
 Data File : PS018384.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2022 11:19
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 00:47:53 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 22 00:27:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
9) T	2,4-D	8.189f	7.685	5470817	4770898	2.682 5.097 #
10) T	Pentachlo...	8.371f	0.000	5439720	0	<MDL N.D. #
11) T	2,4,5-TP ...	0.000	8.430	0	12129592	N.D. 2.938
12) T	2,4,5-T	9.203f	0.000	31261508	0	3.108 N.D. #
13) T	2,4-DB	0.000	9.278f	0	5948804	N.D. 11.011
15) T	Picloram	10.814	10.671	125.4E6	72176830	9.873 12.481 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022122\
Data File : PS018384.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2022 11:19
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 00:47:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
Quant Title : 8080.M
QLast Update : Tue Feb 22 00:27:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

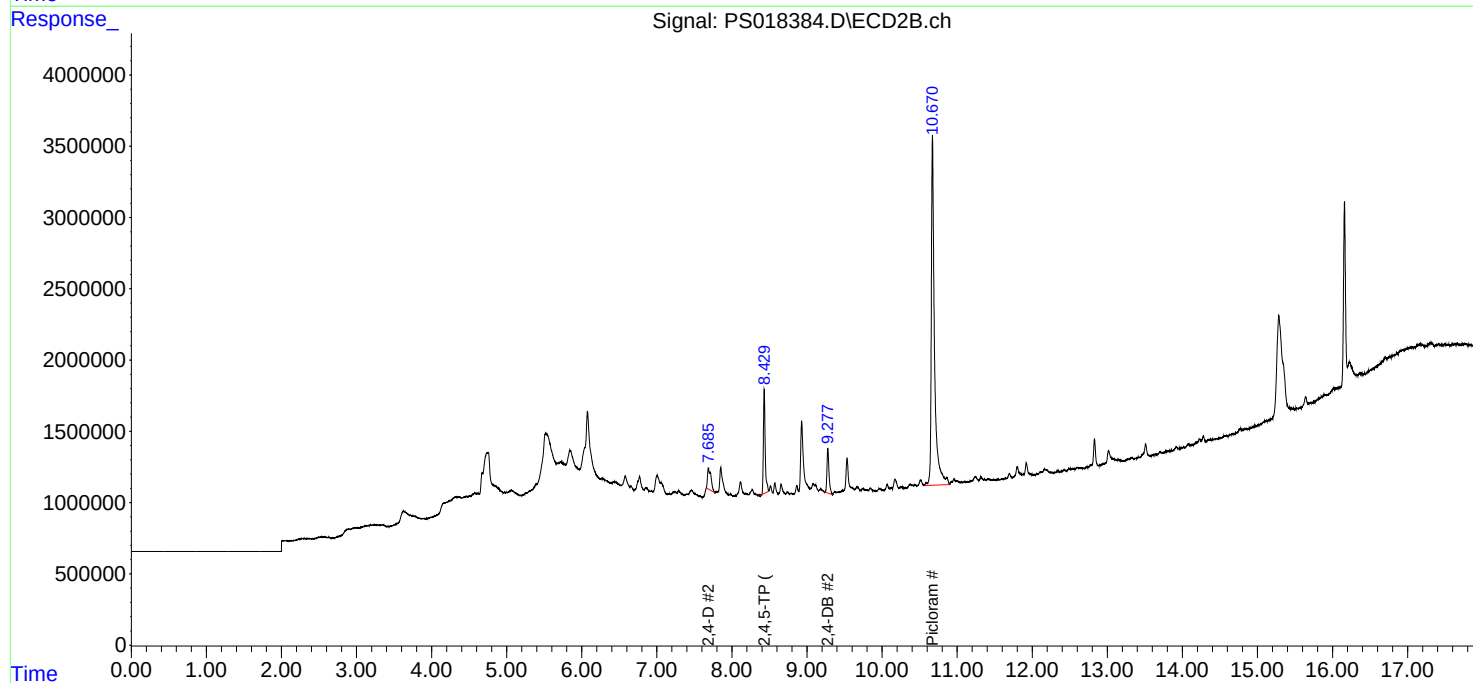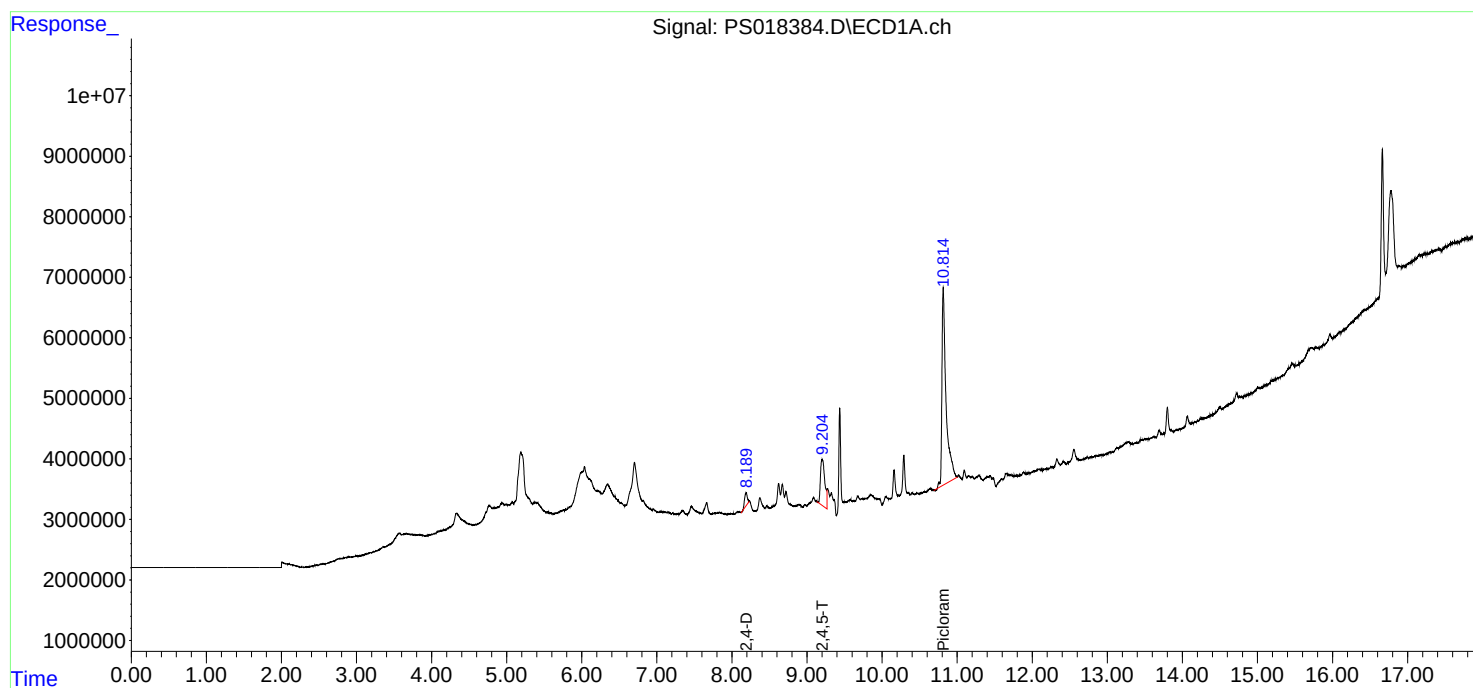

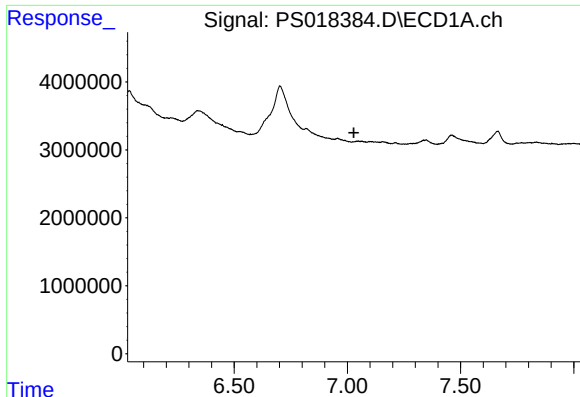

#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 7.029 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 6.640 min
Response: 0
Conc: N.D.

#9 2,4-D

R.T.: 8.189 min
Delta R.T.: 0.057 min
Response: 5470817
Conc: 2.68 ng/ml

#9 2,4-D


R.T.: 7.685 min
Delta R.T.: -0.012 min
Response: 4770898
Conc: 5.10 ng/ml

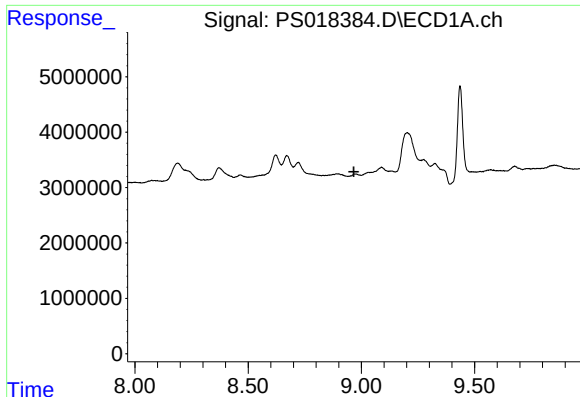

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 8.967 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

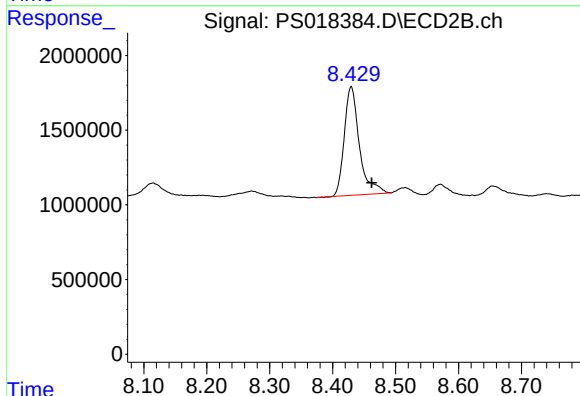


#11 2,4,5-TP (SILVEX)

R.T.: 8.430 min
Delta R.T.: -0.032 min
Response: 12129592
Conc: 2.94 ng/ml

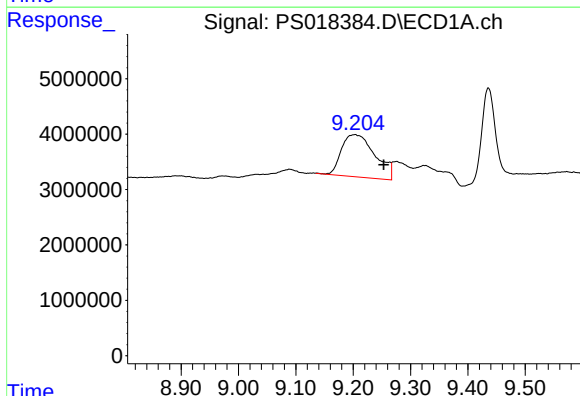


#12 2,4,5-T

R.T.: 9.203 min
Delta R.T.: -0.050 min
Response: 31261508
Conc: 3.11 ng/ml

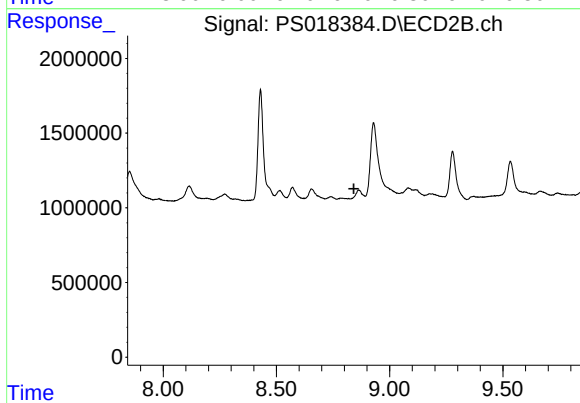

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 8.842 min
Response: 0
Conc: N.D.

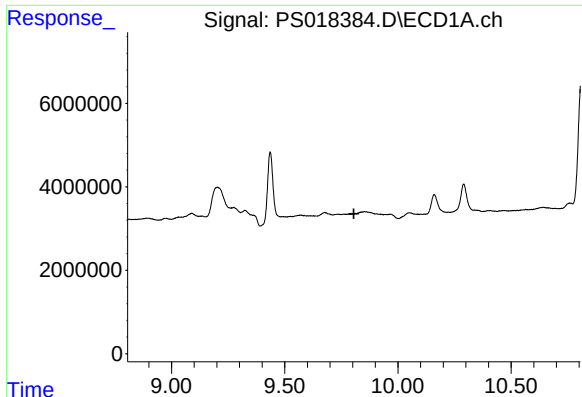

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 9.806 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

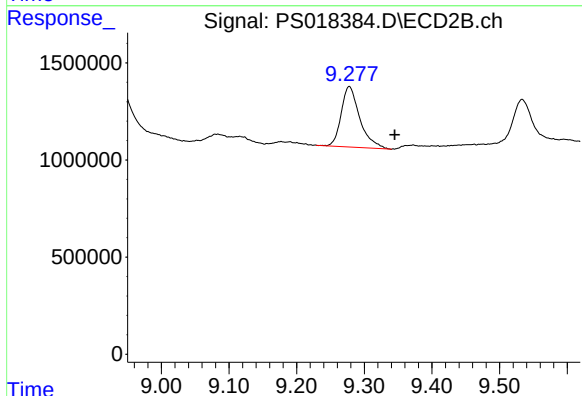


#13 2,4-DB

R.T.: 9.278 min
Delta R.T.: -0.067 min
Response: 5948804
Conc: 11.01 ng/ml

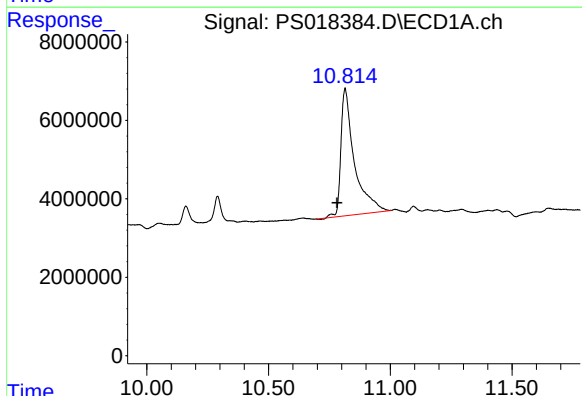

#15 Picloram

R.T.: 10.814 min
Delta R.T.: 0.033 min
Response: 125441162
Conc: 9.87 ng/ml

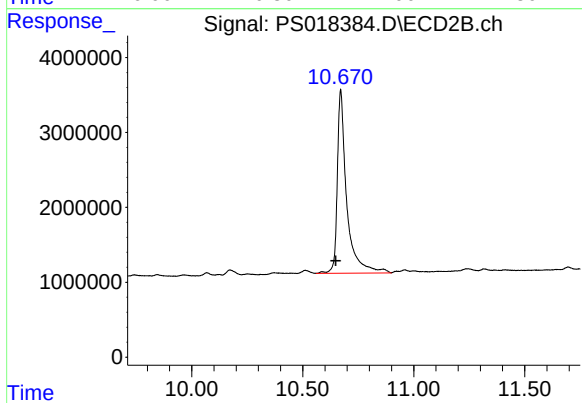

#15 Picloram

R.T.: 10.671 min
Delta R.T.: 0.022 min
Response: 72176830
Conc: 12.48 ng/ml