

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022122\
 Data File : PS018385.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2022 11:43
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 00:48:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 22 00:27:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.027	6.639	654.8E6	328.6E6	393.505	493.184 #
Target Compounds							
7) T	MCPA	0.000	7.025f	0	3906832	N.D.	1.166
9) T	2,4-D	8.188f	7.688	13259242	768683	6.500	<MDL #
11) T	2,4,5-TP ...	0.000	8.431	0	15120873	N.D.	3.662
12) T	2,4,5-T	9.205f	0.000	14544853	0	1.446	N.D. #
13) T	2,4-DB	0.000	9.280f	0	5604622	N.D.	10.374
15) T	Picloram	10.821f	10.673	113.1E6	62058688	8.901	10.731


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022122\
Data File : PS018385.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2022 11:43
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 00:48:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
Quant Title : 8080.M
QLast Update : Tue Feb 22 00:27:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

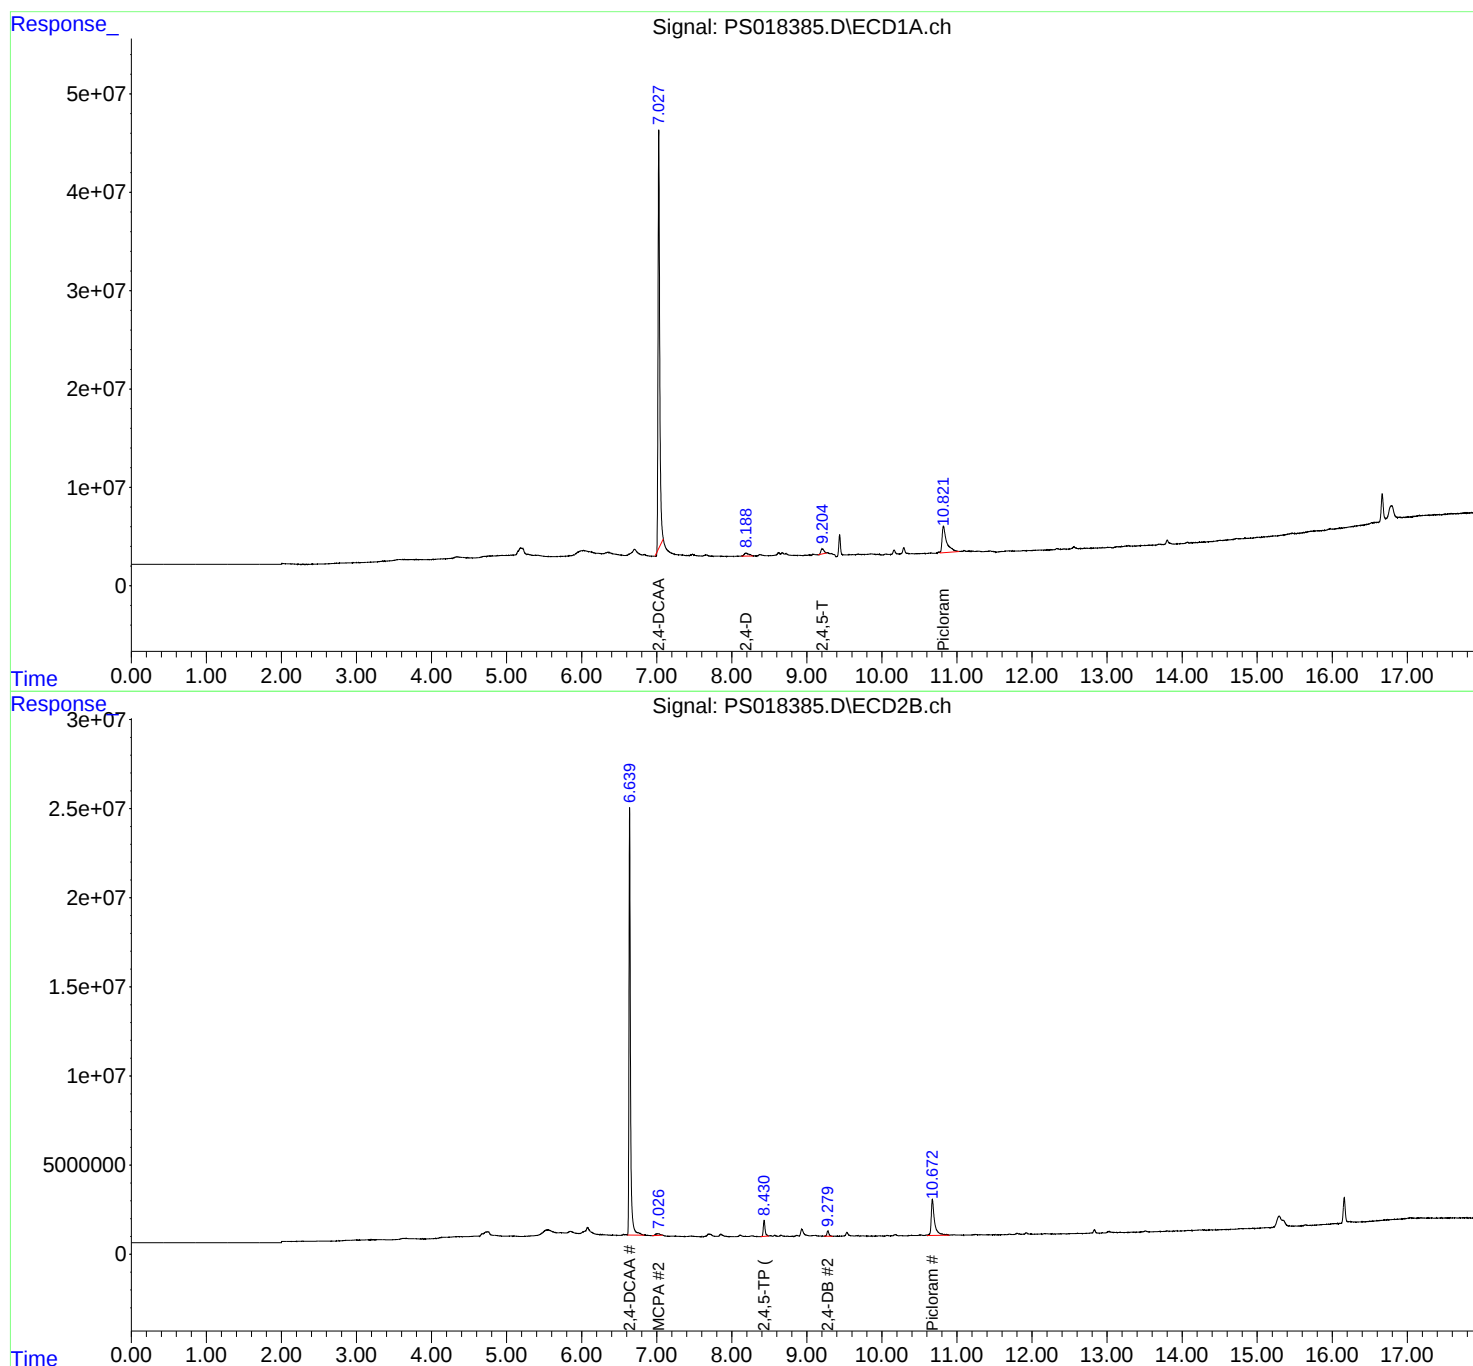


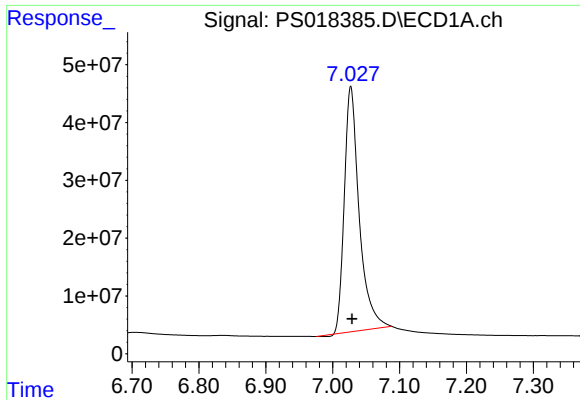

#4 2,4-DCAA


R.T.: 7.027 min
Delta R.T.: -0.002 min
Response: 654811293
Conc: 393.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

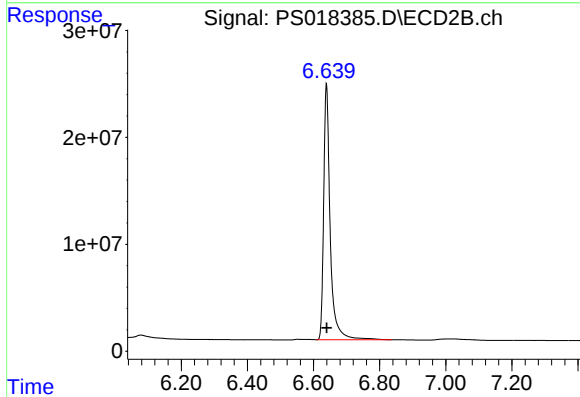


#4 2,4-DCAA

R.T.: 6.639 min
Delta R.T.: 0.000 min
Response: 328629628
Conc: 493.18 ng/ml

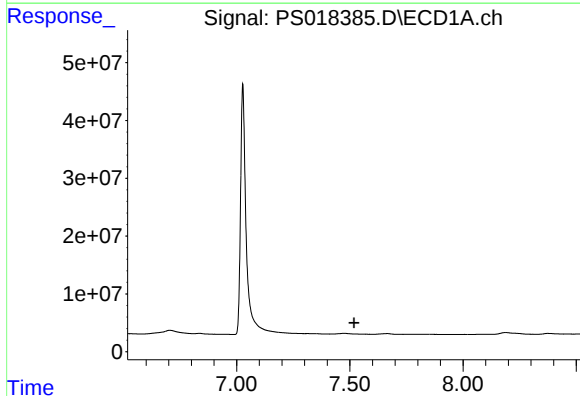


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.518 min
Response: 0
Conc: N.D.

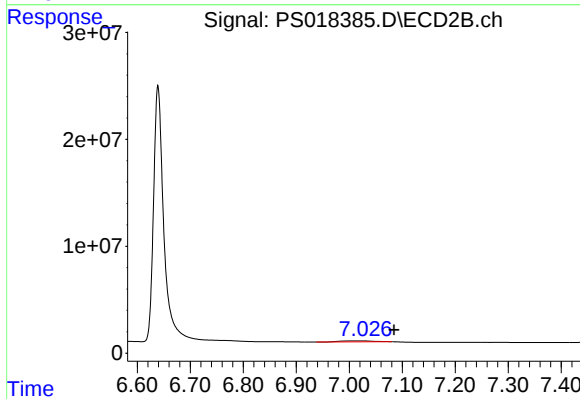

#7 MCPA


R.T.: 7.025 min
Delta R.T.: -0.060 min
Response: 3906832
Conc: 1.17 ug/ml

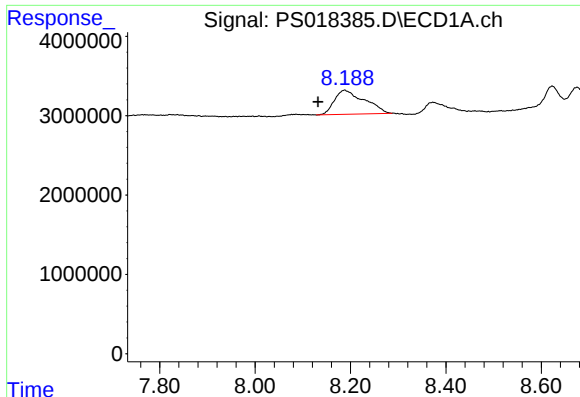

#9 2,4-D


R.T.: 8.188 min
Delta R.T.: 0.055 min
Response: 13259242
Conc: 6.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

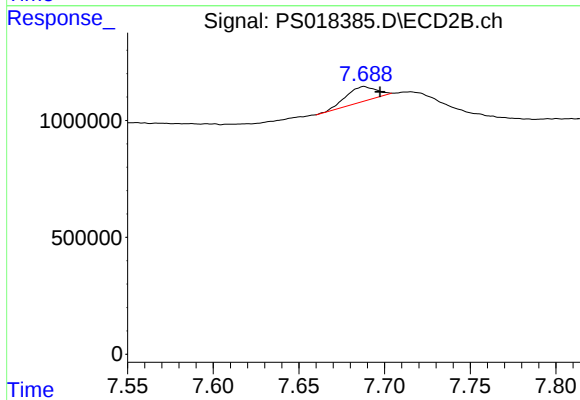


#9 2,4-D

R.T.: 7.688 min
Delta R.T.: -0.009 min
Response: 768683
Conc: N.D.

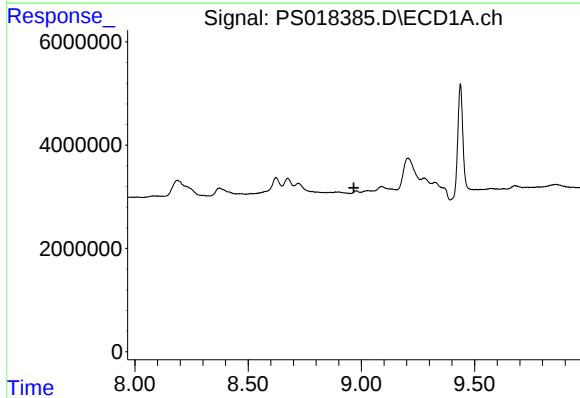


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 8.967 min
Response: 0
Conc: N.D.

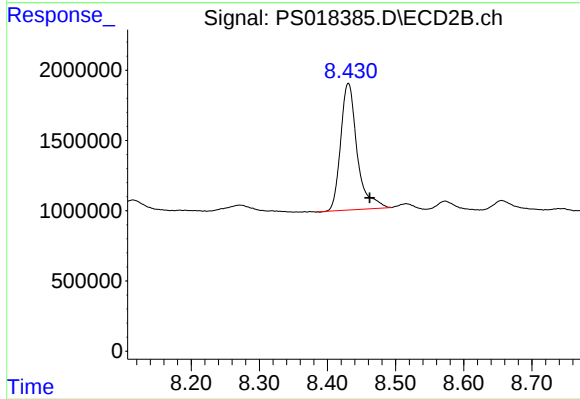

#11 2,4,5-TP (SILVEX)


R.T.: 8.431 min
Delta R.T.: -0.031 min
Response: 15120873
Conc: 3.66 ng/ml

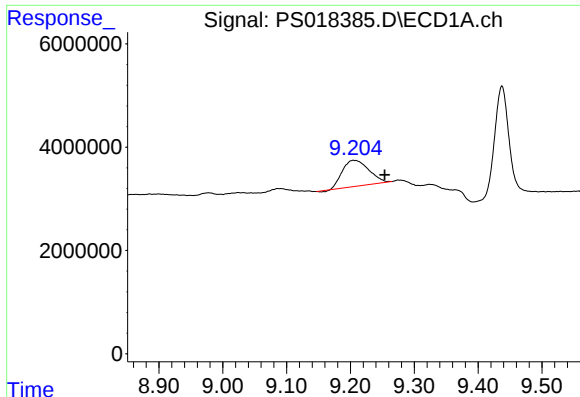

#12 2,4,5-T


R.T.: 9.205 min
Delta R.T.: -0.049 min
Response: 14544853
Conc: 1.45 ng/ml

Instrument :
ECD_S
ClientSampleId :

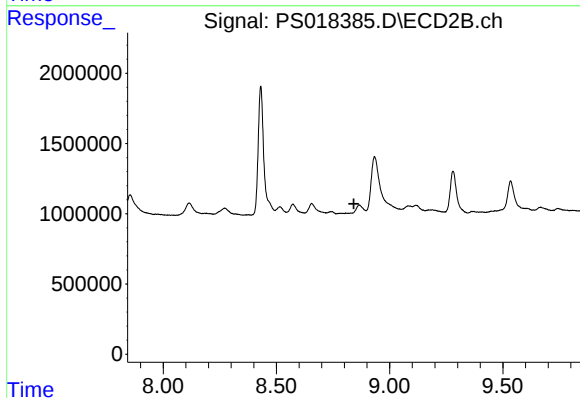


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 8.842 min
Response: 0
Conc: N.D.

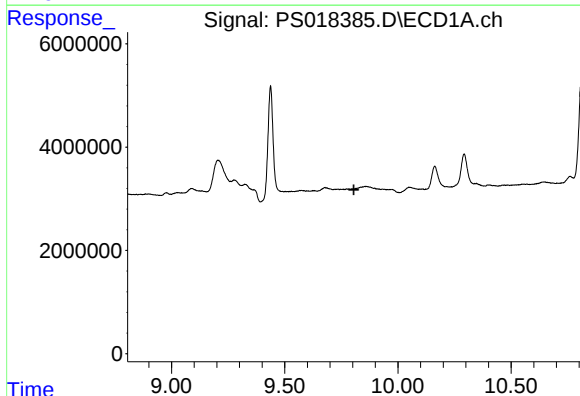


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.806 min
Response: 0
Conc: N.D.

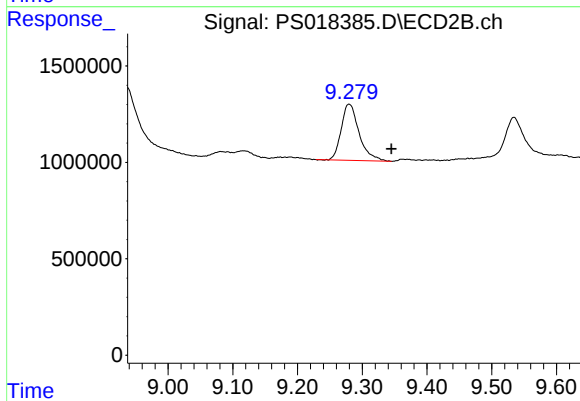

#13 2,4-DB


R.T.: 9.280 min
Delta R.T.: -0.065 min
Response: 5604622
Conc: 10.37 ng/ml

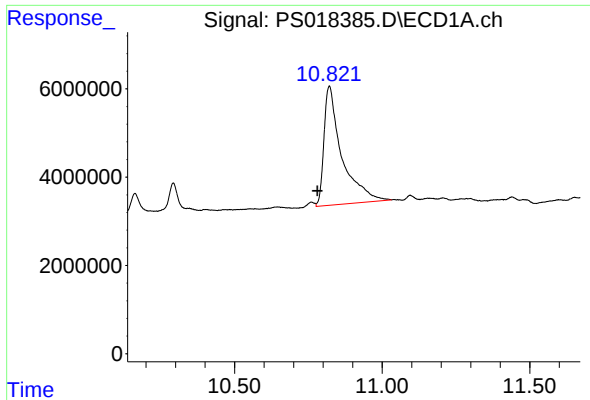

#15 Picloram

R.T.: 10.821 min
Delta R.T.: 0.040 min
Response: 113094269
Conc: 8.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

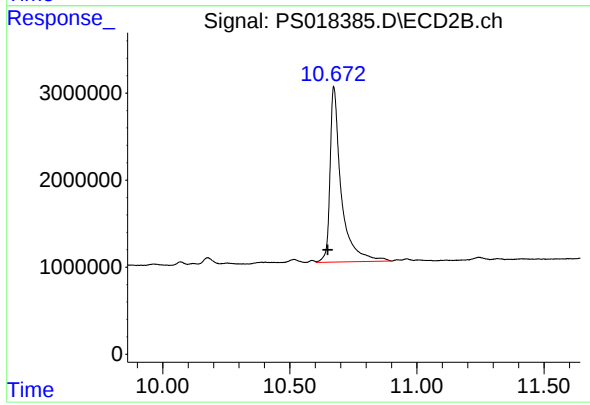

#15 Picloram

R.T.: 10.673 min
Delta R.T.: 0.024 min
Response: 62058688
Conc: 10.73 ng/ml