

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022123\
 Data File : PS022210.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2023 09:46
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 01:32:47 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022023.M
 Quant Title : 8080.M
 QLast Update : Mon Feb 20 13:26:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	6.287	0.000	1173881	0	<MDL	N.D.	#
Target Compounds								
1) T	Dalapon	2.447	2.521	892512	919835	<MDL	<MDL	#
2) T	3,5-DICHL...	5.680	0.000	10605666	0	2.853	N.D.	#
3) T	4-Nitroph...	6.161	0.000	2153952	0	1.693	N.D.	#
5) T	DICAMBA	6.377f	6.945f	172104	7471229	<MDL	<MDL	#
6) T	MCP	0.000	6.945	0	7471229	N.D.	<MDL	
8) T	DICHLORPROP	6.958f	0.000	256390	0	<MDL	N.D.	#
9) T	2,4-D	7.255	0.000	52486009	0	16.008	N.D.	#
10) T	Pentachlo...	7.467	0.000	3026760	0	<MDL	N.D.	#
11) T	2,4,5-TP ...	7.991	0.000	753531	0	<MDL	N.D.	#
12) T	2,4,5-T	8.163f	0.000	97707	0	<MDL	N.D.	#
15) T	Picloram	0.000	10.712	0	6400351	N.D.	<MDL	
16) T	DCPA	0.000	10.712	0	6400351	N.D.	<MDL	


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022123\
Data File : PS022210.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2023 09:46
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 01:32:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022023.M
Quant Title : 8080.M
QLast Update : Mon Feb 20 13:26:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

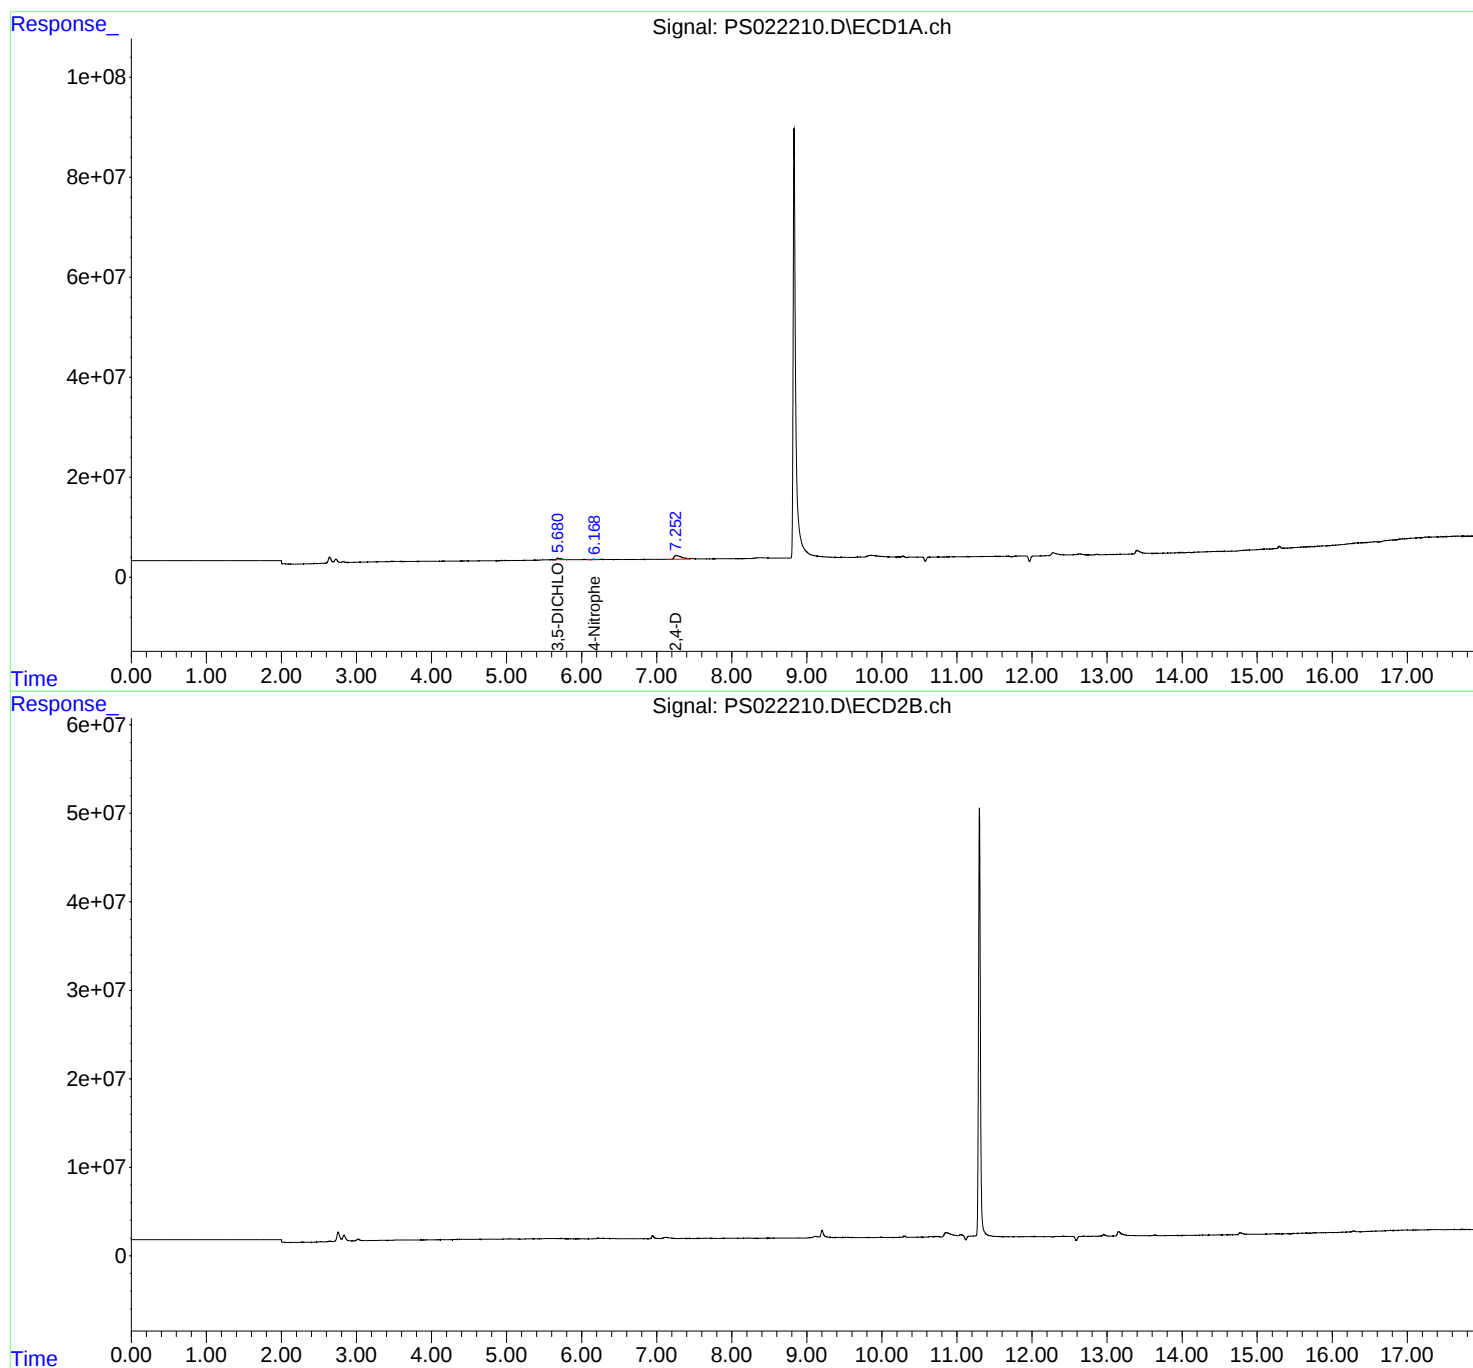


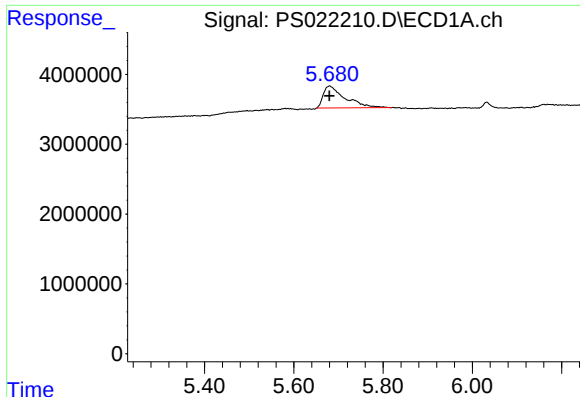

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.680 min
Delta R.T.: 0.000 min
Response: 10605666
Conc: 2.85 ng/ml

Instrument :
ECD_S
ClientSampleId :

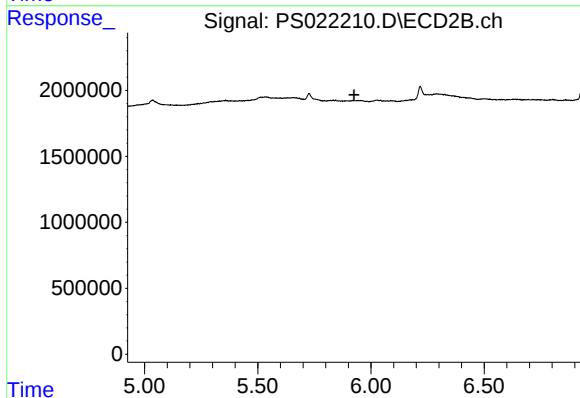


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.925 min
Response: 0
Conc: N.D.

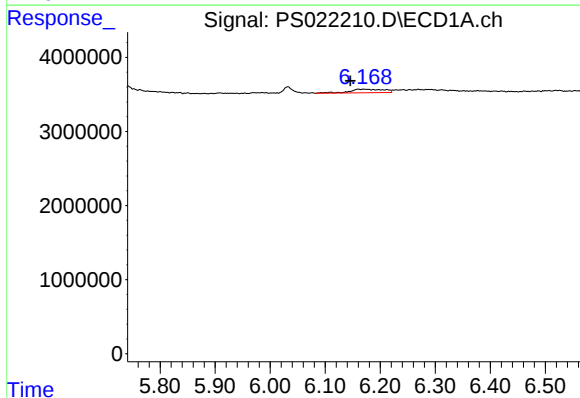


#3 4-Nitrophenol

R.T.: 6.161 min
Delta R.T.: 0.015 min
Response: 2153952
Conc: 1.69 ng/ml

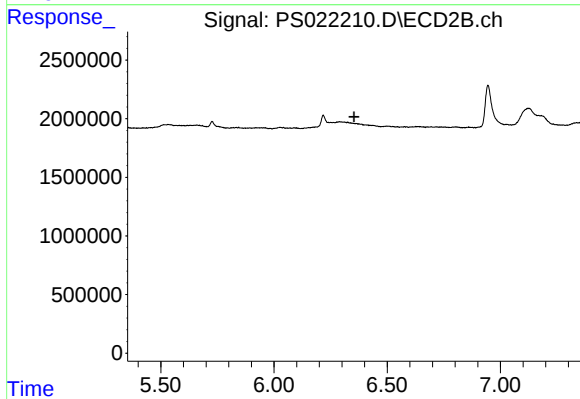

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.353 min
Response: 0
Conc: N.D.

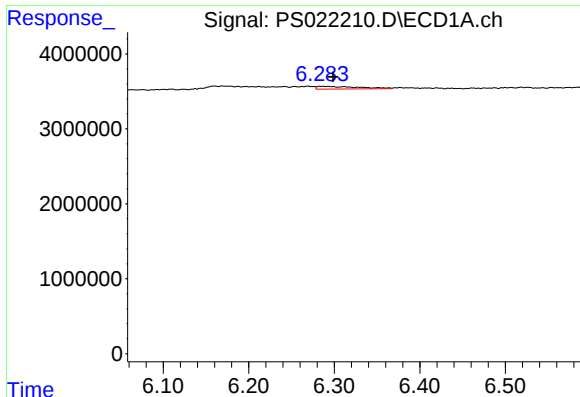

#4 2,4-DCAA


R.T.: 6.287 min
Delta R.T.: -0.012 min
Response: 1173881
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

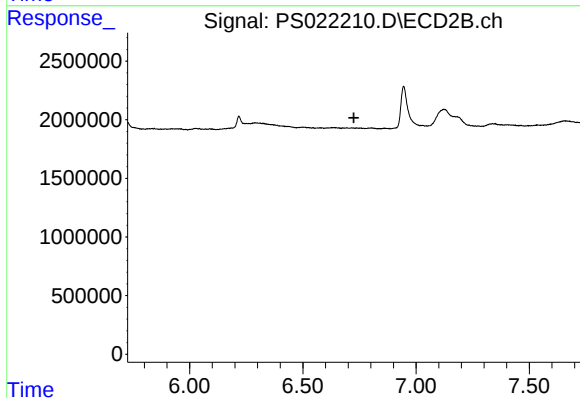


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.726 min
Response: 0
Conc: N.D.

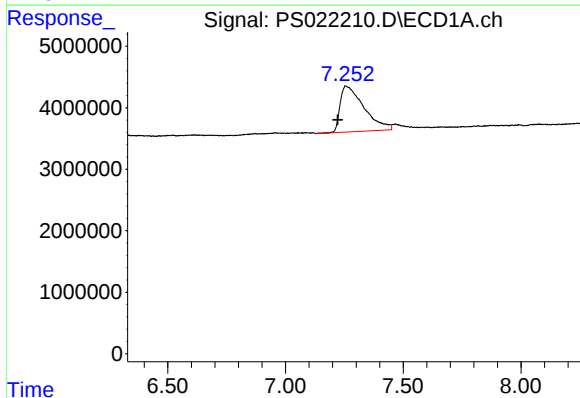

#9 2,4-D

R.T.: 7.255 min
Delta R.T.: 0.032 min
Response: 52486009
Conc: 16.01 ng/ml

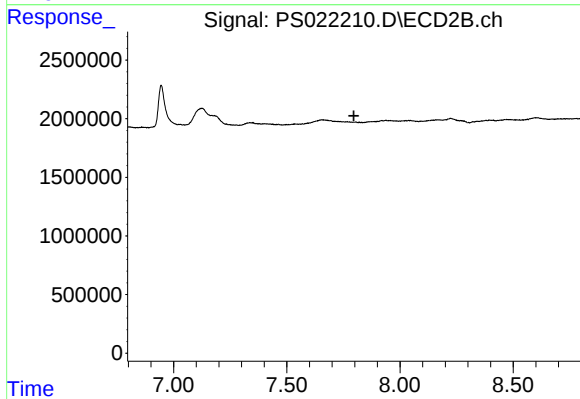

#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.796 min
Response: 0
Conc: N.D.