

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022123\
 Data File : PS022211.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2023 10:10
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 01:33:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022023.M
 Quant Title : 8080.M
 QLast Update : Mon Feb 20 13:26:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.305	6.727	1266.9E6	1170.1E6	511.098	557.479
Target Compounds							
1) T	Dalapon	2.454f	2.518	1085509	973106	<MDL	<MDL #
2) T	3,5-DICHL...	5.681	0.000	4980728	0	1.340	N.D. #
3) T	4-Nitroph...	6.123	0.000	1093226	0	<MDL	N.D. #
5) T	DICAMBA	0.000	6.941f	0	23480211	N.D.	2.430
6) T	MCPD	0.000	7.013	0	9610936	N.D.	1.259
9) T	2,4-D	7.283f	0.000	38114380	0	11.625	N.D. #
10) T	Pentachlo...	7.464	8.223	9214788	7612140	<MDL	<MDL #
11) T	2,4,5-TP ...	0.000	8.611	0	2667099	N.D.	<MDL
12) T	2,4,5-T	8.177f	0.000	67266	0	<MDL	N.D. #
14) T	DINOSEB	0.000	9.791	0	2940052	N.D.	<MDL
15) T	Picloram	9.613	10.709f	130319	8671506	<MDL	<MDL #
16) T	DCPA	10.056	10.709	5281857	8671506	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022123\
Data File : PS022211.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2023 10:10
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 01:33:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022023.M
Quant Title : 8080.M
QLast Update : Mon Feb 20 13:26:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

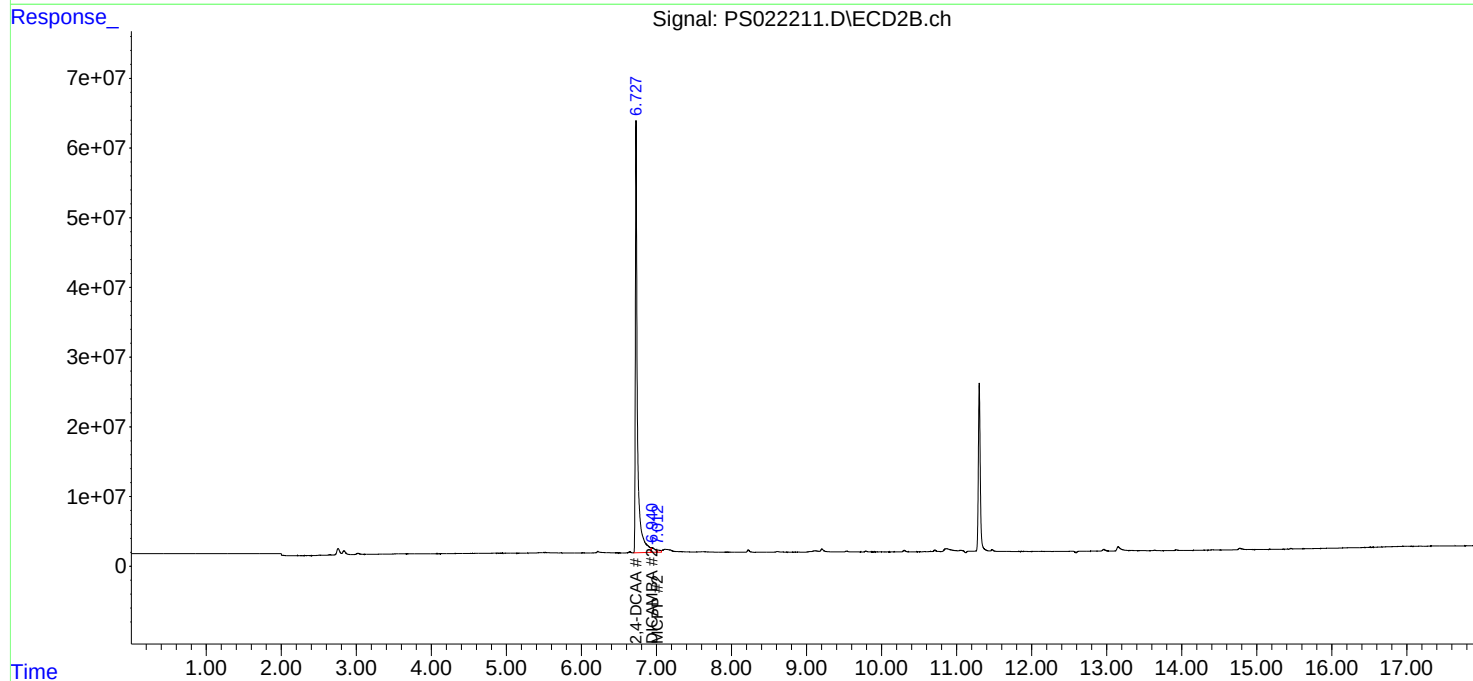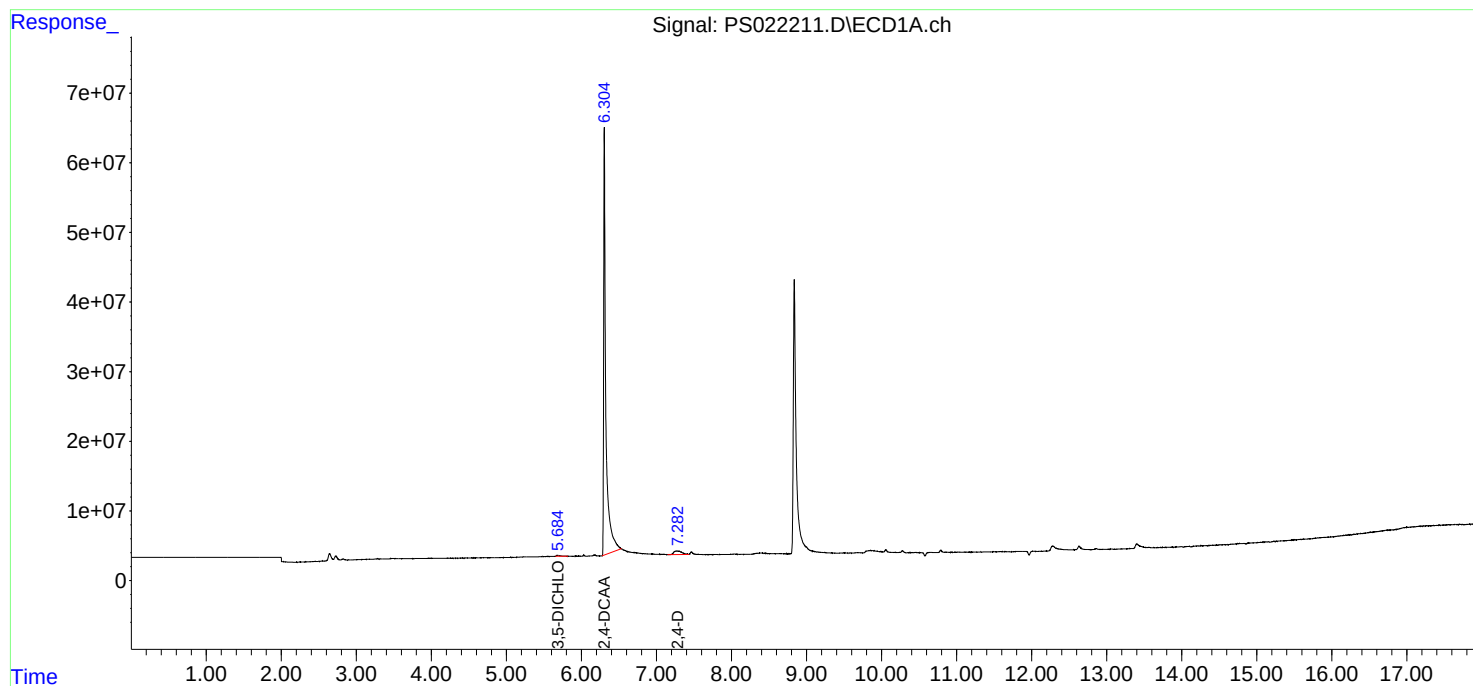


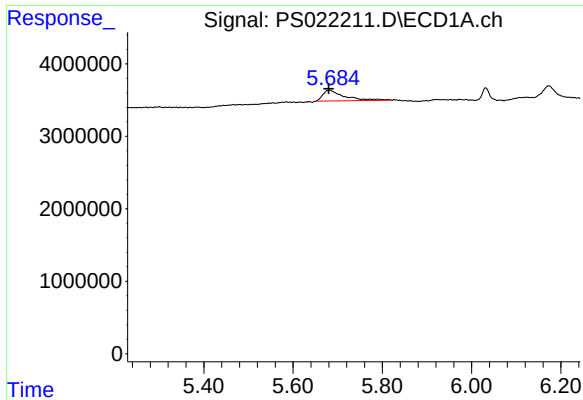

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.681 min
Delta R.T.: 0.002 min
Response: 4980728
Conc: 1.34 ng/ml

Instrument :
ECD_S
ClientSampleId :

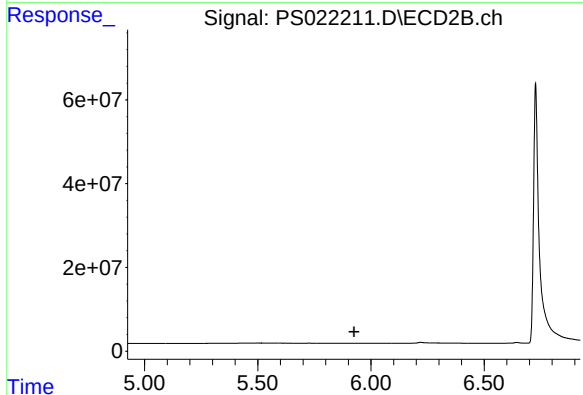


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.925 min
Response: 0
Conc: N.D.

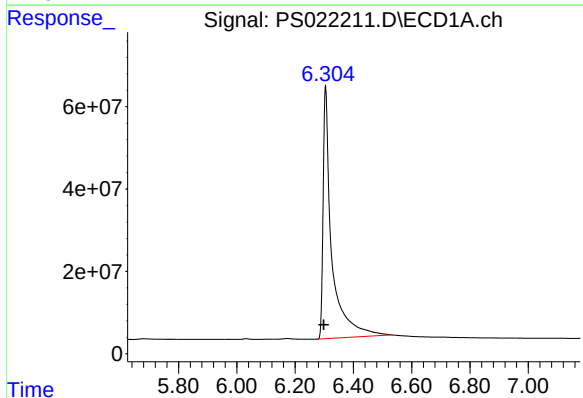


#4 2,4-DCAA

R.T.: 6.305 min
Delta R.T.: 0.006 min
Response: 1266854536
Conc: 511.10 ng/ml

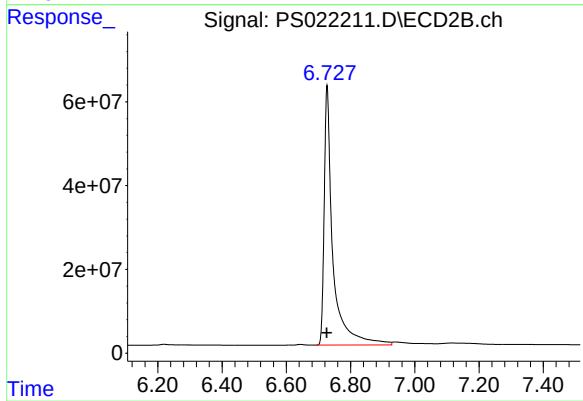

#4 2,4-DCAA


R.T.: 6.727 min
Delta R.T.: 0.001 min
Response: 1170128046
Conc: 557.48 ng/ml

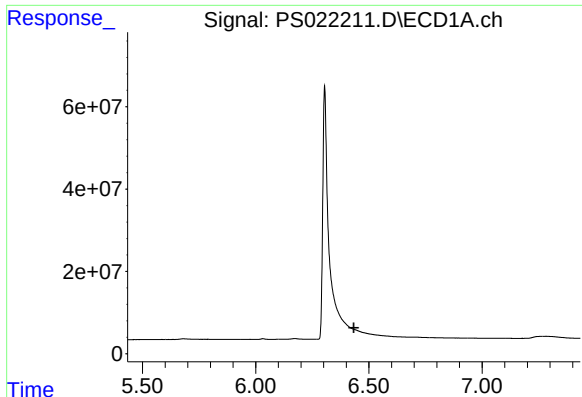

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

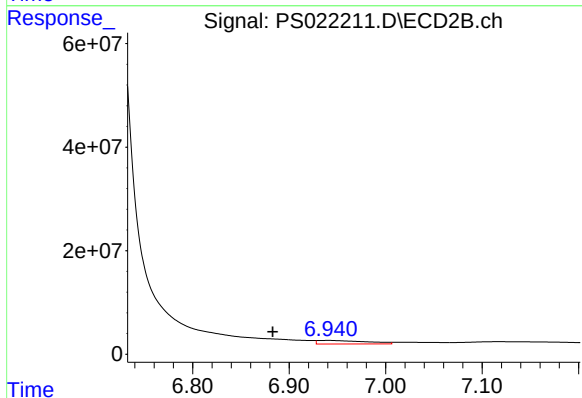


#5 DICAMBA

R.T.: 6.941 min
Delta R.T.: 0.058 min
Response: 23480211
Conc: 2.43 ng/ml

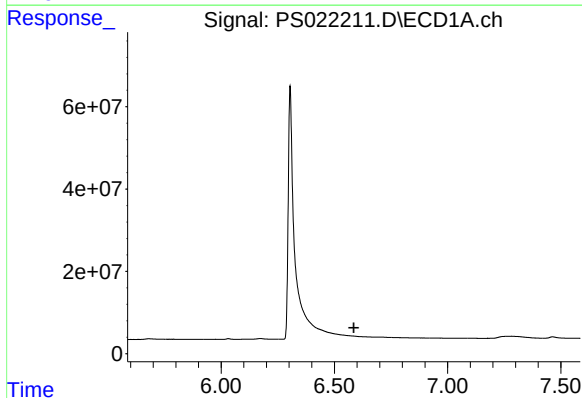


#6 MCP

R.T.: 0.000 min
Exp R.T.: 6.586 min
Response: 0
Conc: N.D.

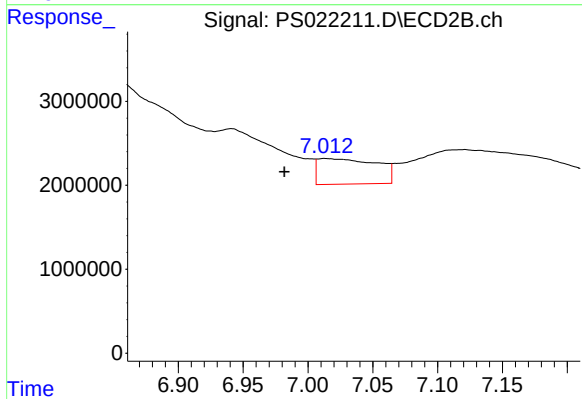

#6 MCP

R.T.: 7.013 min
Delta R.T.: 0.031 min
Response: 9610936
Conc: 1.26 ug/ml

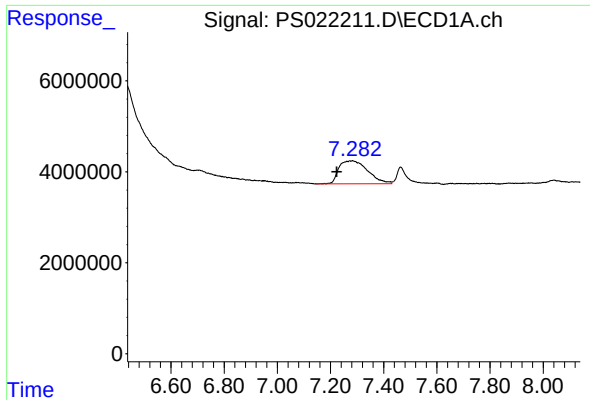

#9 2,4-D


R.T.: 7.283 min

Delta R.T.: 0.060 min

Response: 38114380

Conc: 11.62 ng/ml

Instrument :
ECD_S
ClientSampleId :

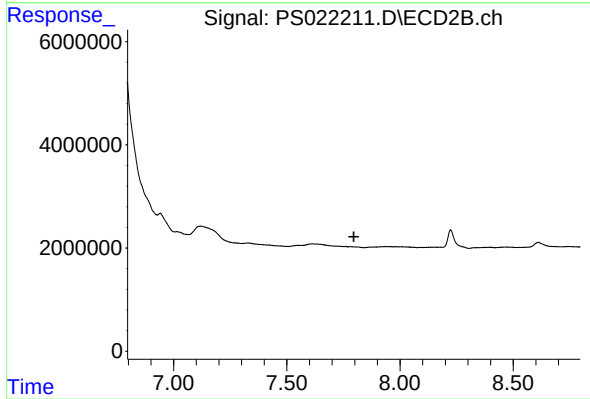

#9 2,4-D

R.T.: 0.000 min

Exp R.T. : 7.796 min

Response: 0

Conc: N.D.