

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022223\
 Data File : PS022235.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Feb 2023 08:48
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 20:06:32 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022023.M
 Quant Title : 8080.M
 QLast Update : Mon Feb 20 13:26:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	6.273	0.000	1162552	0	<MDL	N.D.	#
Target Compounds								
1) T	Dalapon	2.386	2.522	134759	1112500	<MDL	<MDL	#
2) T	3,5-DICHL...	5.678	0.000	19198061	0	5.164	N.D.	#
3) T	4-Nitroph...	6.163	0.000	2037770	0	1.601	N.D.	#
5) T	DICAMBA	6.391f	6.944f	396579	14624835	<MDL	1.513	#
6) T	MCPD	0.000	6.944	0	14624835	N.D.	1.916	
7) T	MCPA	0.000	7.123f	0	9598569	N.D.	<MDL	
9) T	2,4-D	7.243	0.000	84457595	0	25.759	N.D.	#
10) T	Pentachlo...	7.461	0.000	5897380	0	<MDL	N.D.	#
11) T	2,4,5-TP ...	7.995	8.600	736596	3500551	<MDL	<MDL	#
14) T	DINOSEB	9.808	0.000	40332324	0	2.935	N.D.	#
15) T	Picloram	9.674f	10.705f	4425816	19895396	<MDL	1.015	#
16) T	DCPA	0.000	10.705	0	19895396	N.D.	1.272	



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022223\
Data File : PS022235.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Feb 2023 08:48
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 20:06:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022023.M
Quant Title : 8080.M
QLast Update : Mon Feb 20 13:26:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

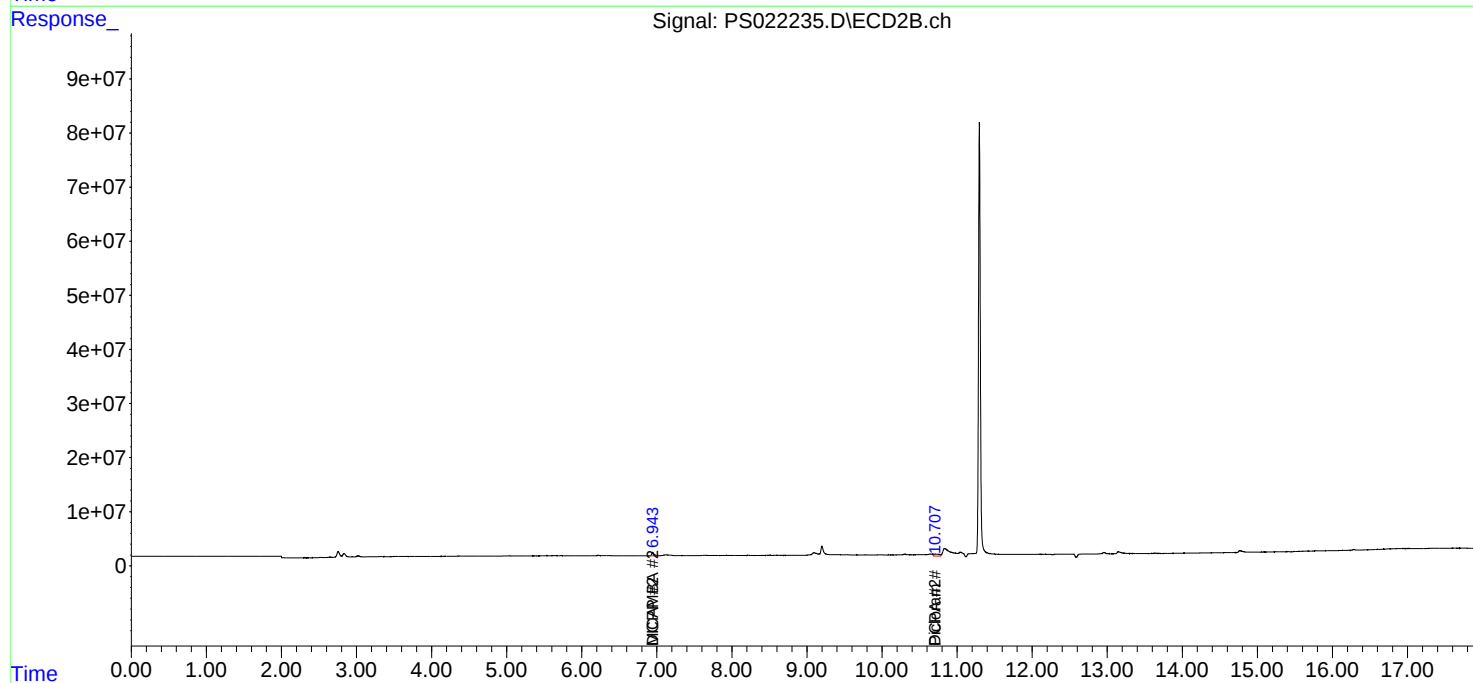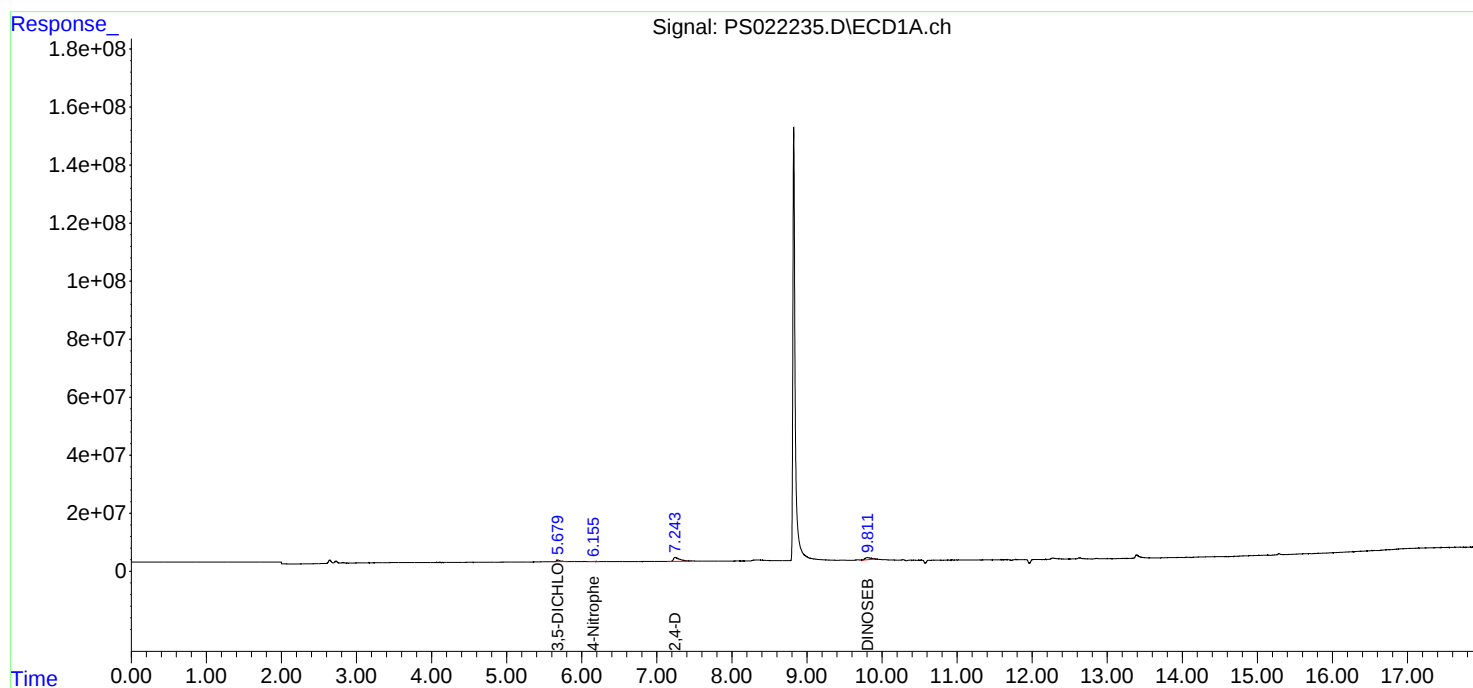


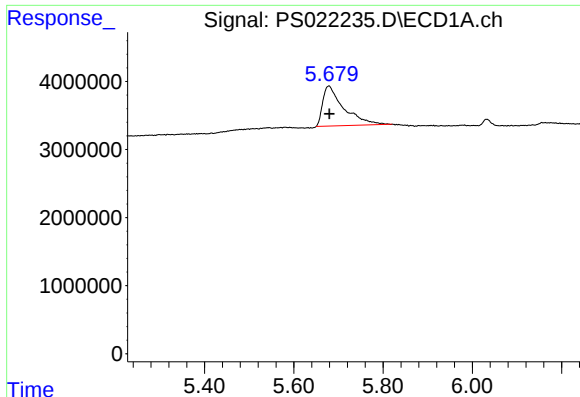

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.678 min
Delta R.T.: -0.001 min
Response: 19198061
Conc: 5.16 ng/ml

Instrument :
ECD_S
ClientSampleId :

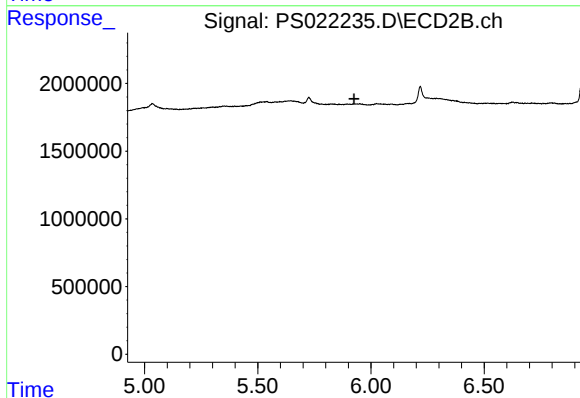


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.925 min
Response: 0
Conc: N.D.

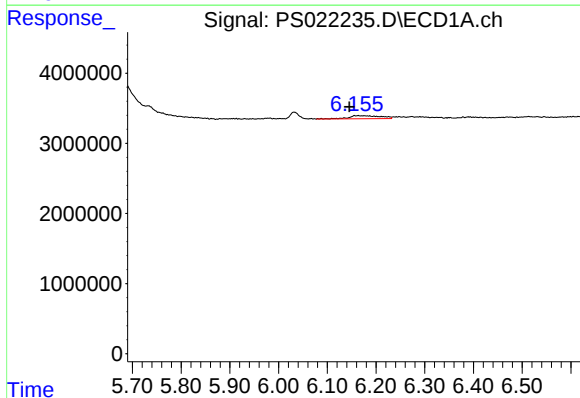


#3 4-Nitrophenol

R.T.: 6.163 min
Delta R.T.: 0.017 min
Response: 2037770
Conc: 1.60 ng/ml

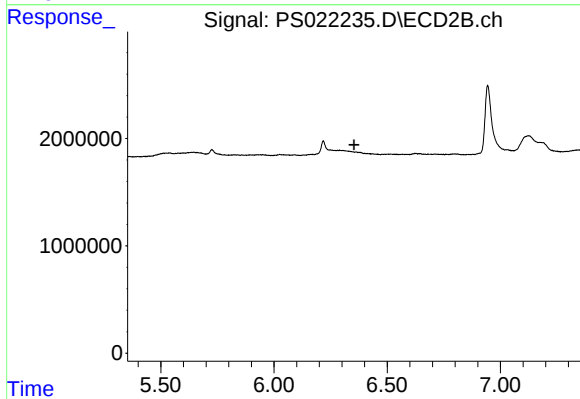

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.353 min
Response: 0
Conc: N.D.

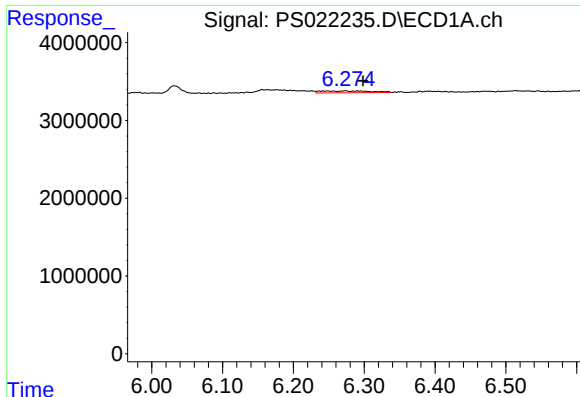

#4 2,4-DCAA


R.T.: 6.273 min
Delta R.T.: -0.026 min
Response: 1162552
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

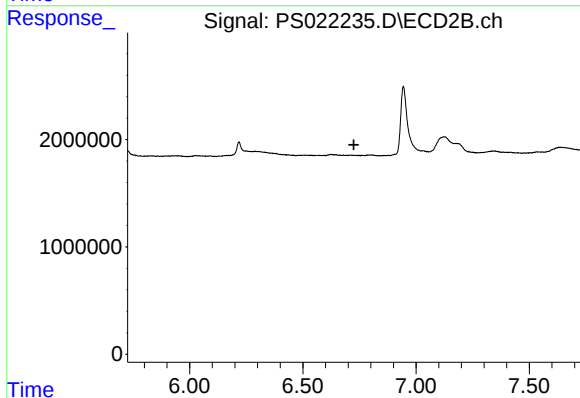


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.726 min
Response: 0
Conc: N.D.

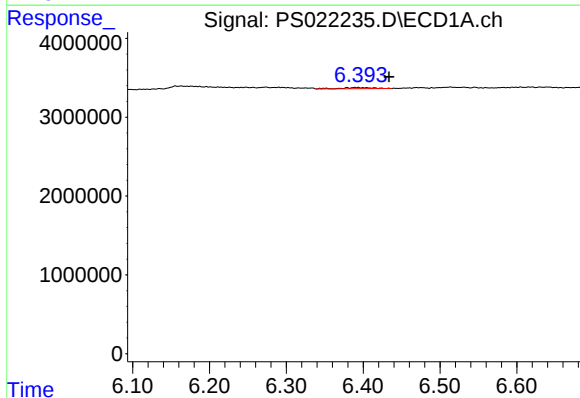


#5 DICAMBA

R.T.: 6.391 min
Delta R.T.: -0.043 min
Response: 396579
Conc: N.D.

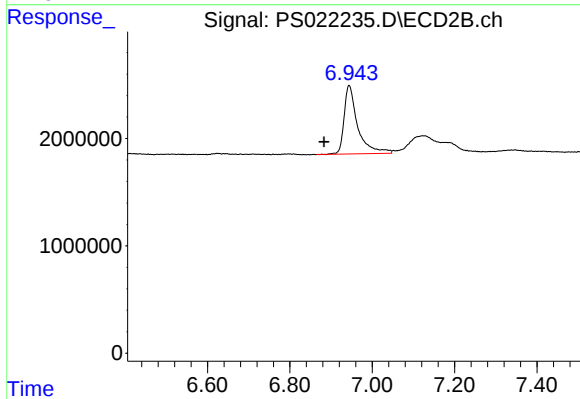

#5 DICAMBA


R.T.: 6.944 min
Delta R.T.: 0.061 min
Response: 14624835
Conc: 1.51 ng/ml

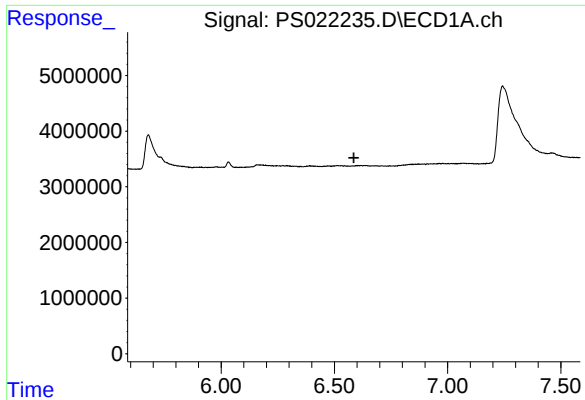

#6 MCP


R.T.: 0.000 min
Exp R.T.: 6.586 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

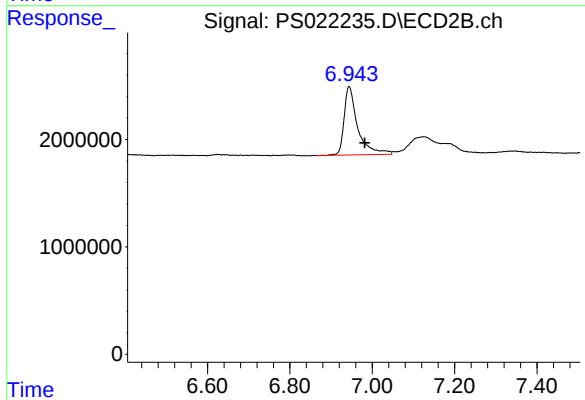


#6 MCP

R.T.: 6.944 min
Delta R.T.: -0.038 min
Response: 14624835
Conc: 1.92 ug/ml

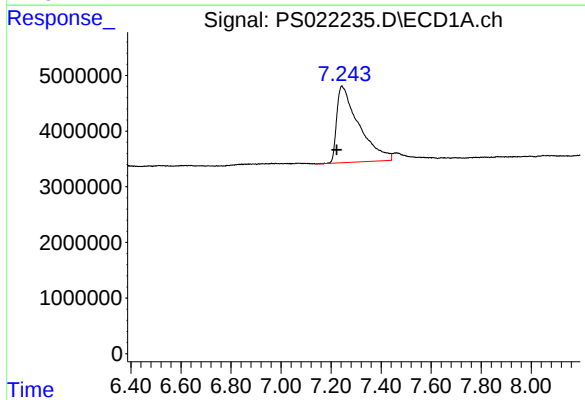


#9 2,4-D

R.T.: 7.243 min
Delta R.T.: 0.020 min
Response: 84457595
Conc: 25.76 ng/ml

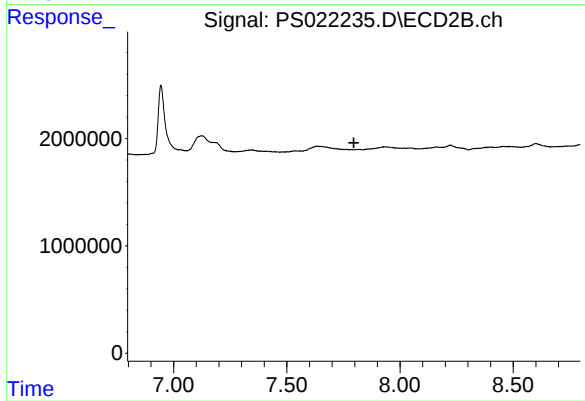

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.796 min
Response: 0
Conc: N.D.

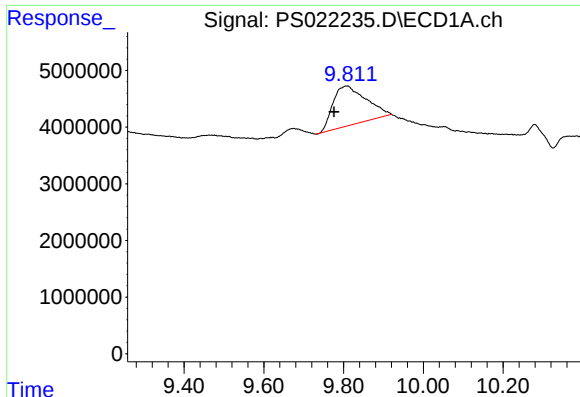

#14 DINOSEB


R.T.: 9.808 min
Delta R.T.: 0.032 min
Response: 40332324
Conc: 2.93 ng/ml

Instrument :
ECD_S
ClientSampleId :

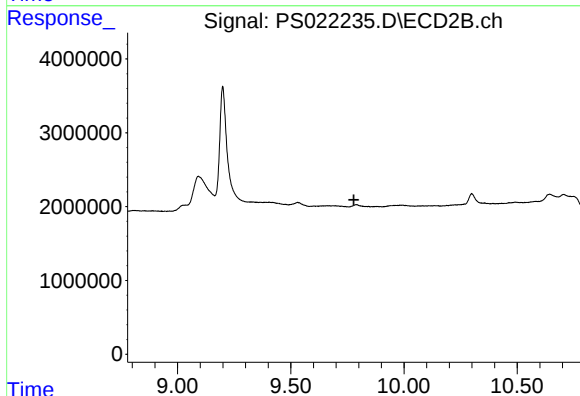


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.779 min
Response: 0
Conc: N.D.

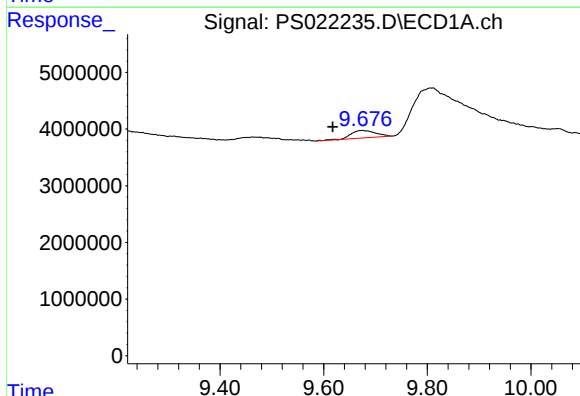


#15 Picloram

R.T.: 9.674 min
Delta R.T.: 0.057 min
Response: 4425816
Conc: N.D.

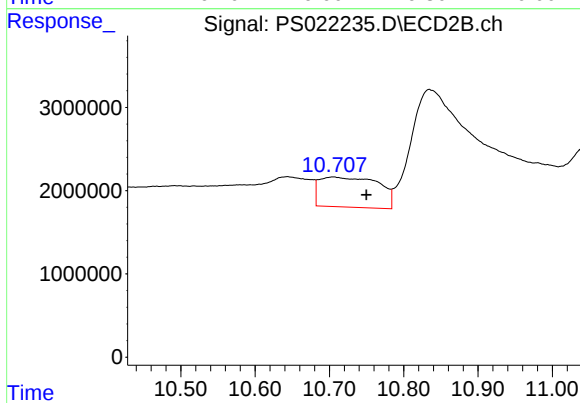

#15 Picloram


R.T.: 10.705 min
Delta R.T.: -0.045 min
Response: 19895396
Conc: 1.01 ng/ml

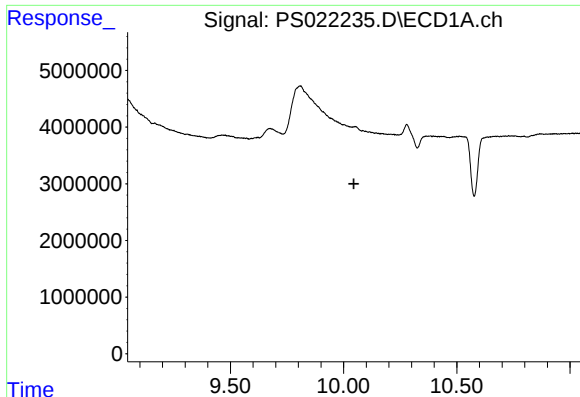

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.045 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

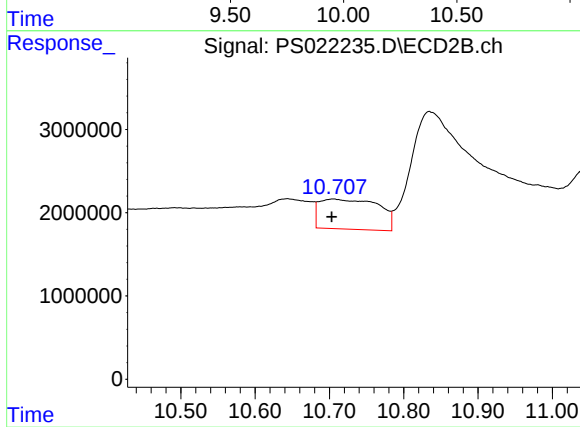

#16 DCPA

R.T.: 10.705 min
Delta R.T.: 0.002 min
Response: 19895396
Conc: 1.27 ng/ml