

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022223\
 Data File : PS022236.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Feb 2023 09:12
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 20:07:25 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022023.M
 Quant Title : 8080.M
 QLast Update : Mon Feb 20 13:26:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.303	6.726	1274.3E6	1176.2E6	514.101	560.388
Target Compounds							
1) T	Dalapon	2.450f	2.520	1439677	1165429	<MDL	<MDL #
2) T	3,5-DICHL...	5.678	0.000	3818833	0	1.027	N.D. #
3) T	4-Nitroph...	6.171	0.000	4558427	0	3.582	N.D. #
5) T	DICAMBA	0.000	6.941f	0	22496213	N.D.	2.328
6) T	MCPD	0.000	6.941f	0	22496213	N.D.	2.947
7) T	MCPA	6.696	7.142f	783850	23468199	<MDL	2.302 #
8) T	DICHLORPROP	7.072f	0.000	413058	0	<MDL	N.D. #
9) T	2,4-D	7.241	0.000	29866141	0	9.109	N.D. #
10) T	Pentachlo...	7.462	8.221	8650554	7329206	<MDL	<MDL #
11) T	2,4,5-TP ...	7.951	8.601	308642	3217389	<MDL	<MDL #
12) T	2,4,5-T	8.193	0.000	58514	0	<MDL	N.D. #
13) T	2,4-DB	8.749	0.000	179964	0	<MDL	N.D. #
14) T	DINOSEB	9.795	9.786	39817027	3494347	2.897	<MDL #
15) T	Picloram	9.615	10.707f	497185	14051963	<MDL	<MDL #
16) T	DCPA	10.055	10.707	5452858	14051963	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022223\
Data File : PS022236.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Feb 2023 09:12
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 20:07:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022023.M
Quant Title : 8080.M
QLast Update : Mon Feb 20 13:26:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

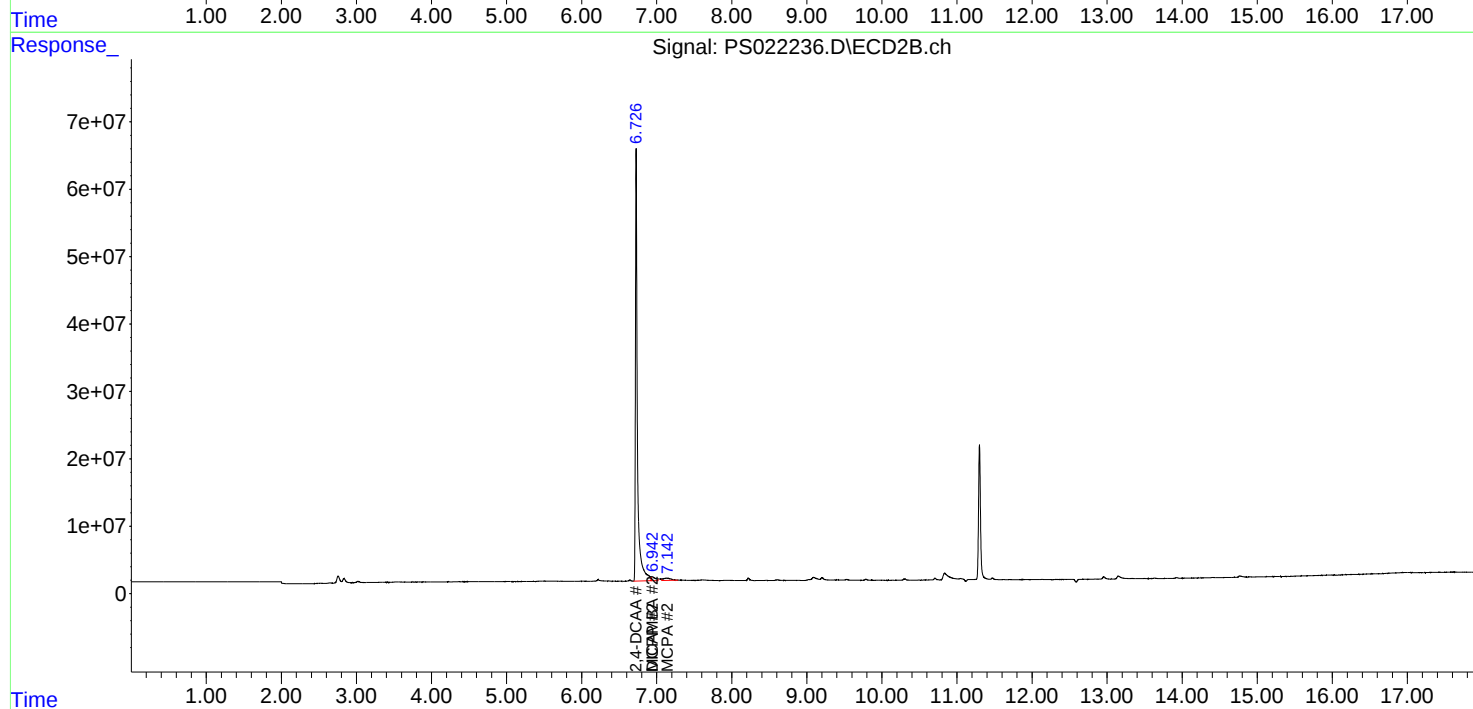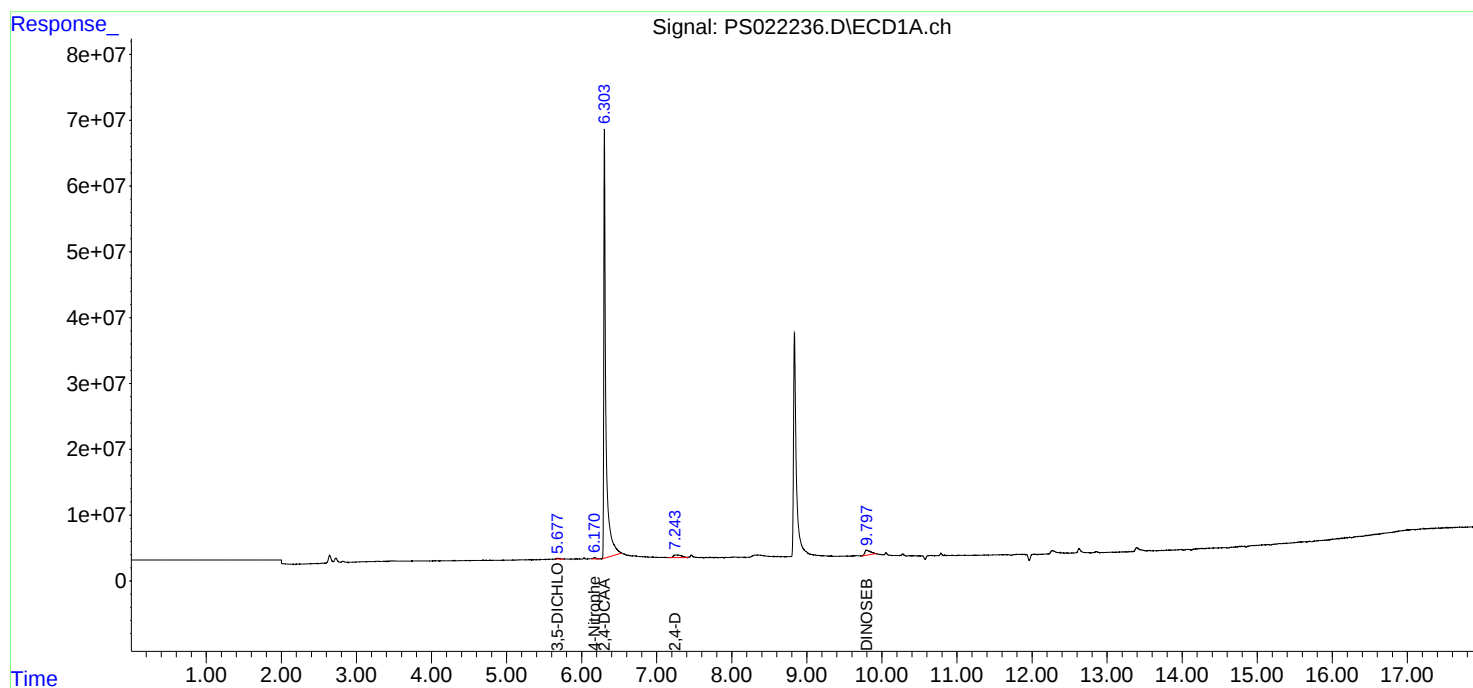


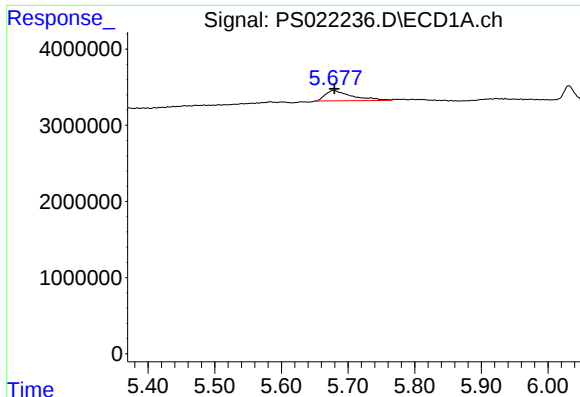

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.678 min
Delta R.T.: -0.001 min
Response: 3818833
Conc: 1.03 ng/ml

Instrument :
ECD_S
ClientSampleId :

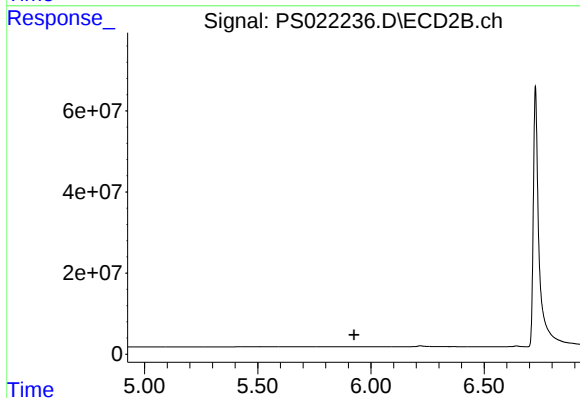


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.925 min
Response: 0
Conc: N.D.

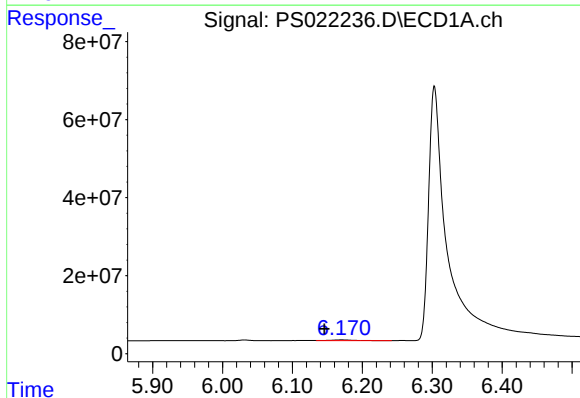


#3 4-Nitrophenol

R.T.: 6.171 min
Delta R.T.: 0.025 min
Response: 4558427
Conc: 3.58 ng/ml

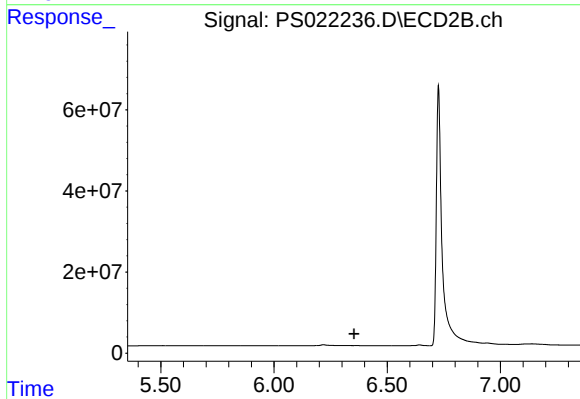

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.353 min
Response: 0
Conc: N.D.

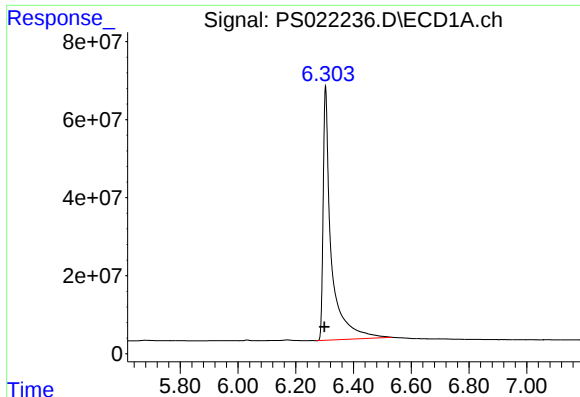

#4 2,4-DCAA


R.T.: 6.303 min
Delta R.T.: 0.005 min
Response: 1274297266
Conc: 514.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

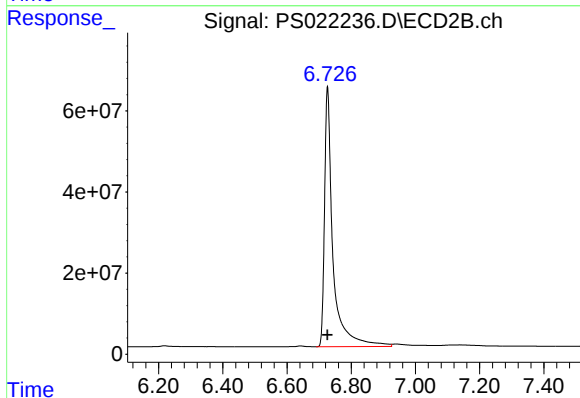


#4 2,4-DCAA

R.T.: 6.726 min
Delta R.T.: 0.000 min
Response: 1176233761
Conc: 560.39 ng/ml

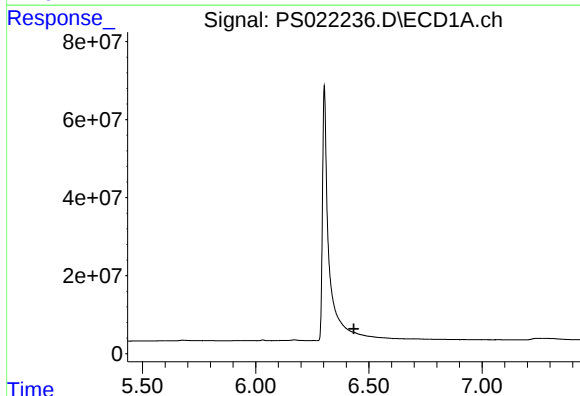


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 6.434 min
Response: 0
Conc: N.D.

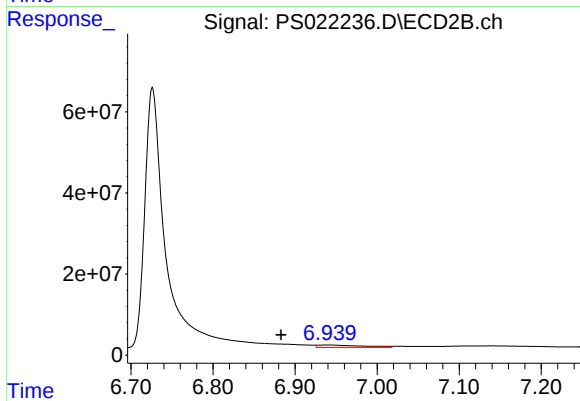

#5 DICAMBA


R.T.: 6.941 min
Delta R.T.: 0.058 min
Response: 22496213
Conc: 2.33 ng/ml

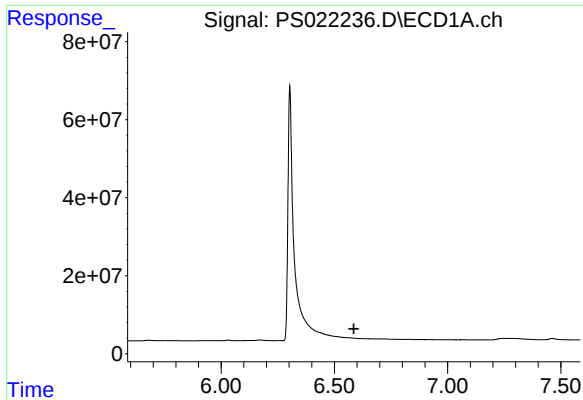

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 6.586 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

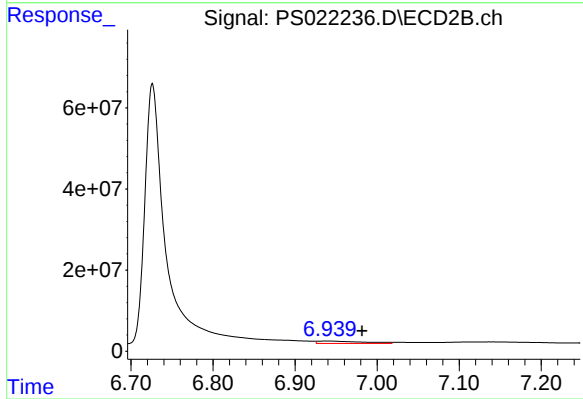


#6 MCPP

R.T.: 6.941 min
Delta R.T.: -0.041 min
Response: 22496213
Conc: 2.95 ug/ml

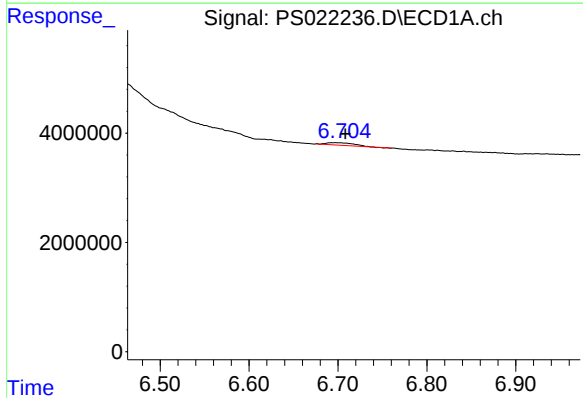


#7 MCPA

R.T.: 6.696 min
Delta R.T.: -0.012 min
Response: 783850
Conc: N.D.

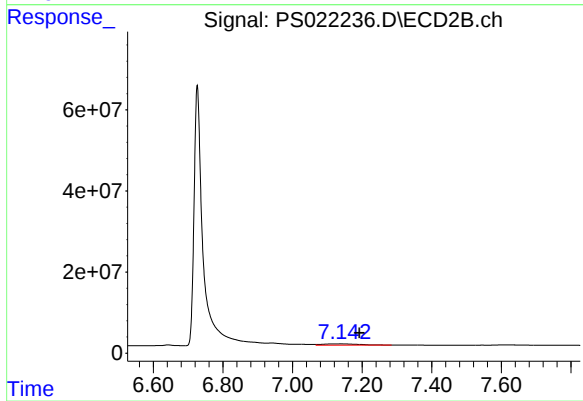

#7 MCPA


R.T.: 7.142 min
Delta R.T.: -0.051 min
Response: 23468199
Conc: 2.30 ug/ml

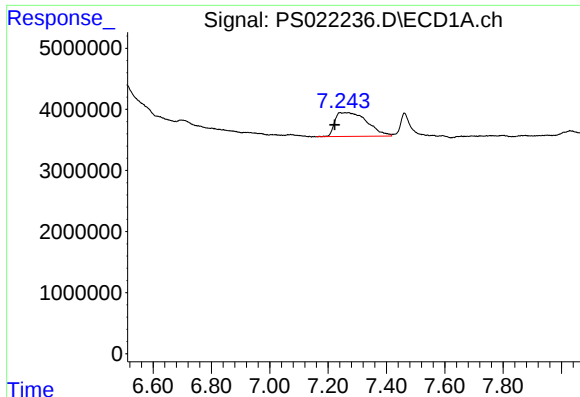

#9 2,4-D


R.T.: 7.241 min
Delta R.T.: 0.019 min
Response: 29866141
Conc: 9.11 ng/ml

Instrument :
ECD_S
ClientSampleId :

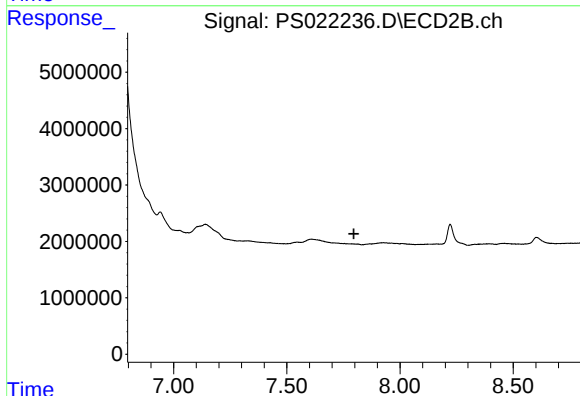


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.796 min
Response: 0
Conc: N.D.

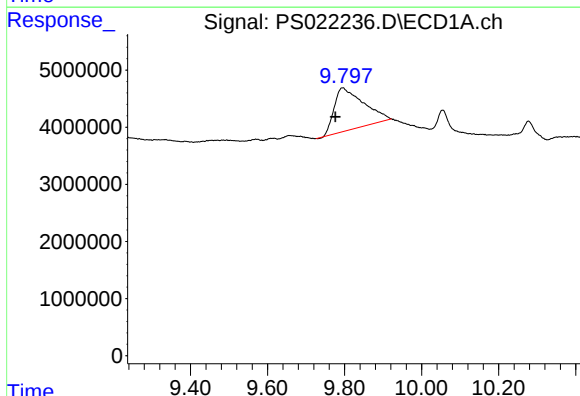

#14 DINOSEB

R.T.: 9.795 min
Delta R.T.: 0.019 min
Response: 39817027
Conc: 2.90 ng/ml

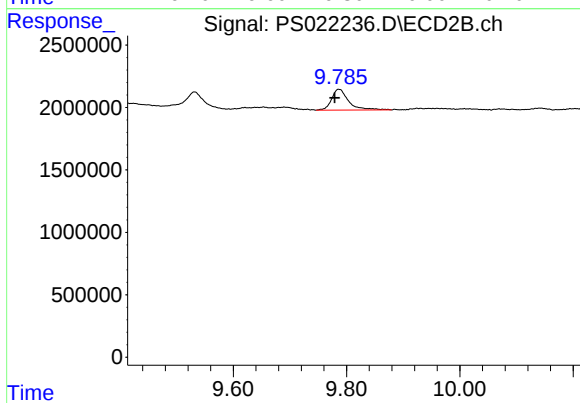

#14 DINOSEB

R.T.: 9.786 min
Delta R.T.: 0.007 min
Response: 3494347
Conc: N.D.