

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022322\
 Data File : PS018402.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Feb 2022 22:50
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 24 01:07:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 22 00:27:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
5) T	DICAMBA	7.214	6.790	4051560	1500520	<MDL	<MDL #
9) T	2,4-D	8.150	7.706	12464474	2336859	6.110	2.496 #
10) T	Pentachlo...	8.422	8.098	5507584	2481619	<MDL	<MDL #
11) T	2,4,5-TP ...	8.974	8.462	8206754	3666315	<MDL	<MDL #
12) T	2,4,5-T	9.268	8.850	45484318	9172721	4.522	2.330 #
13) T	2,4-DB	9.828	0.000	8826322	0	5.079	N.D. #
14) T	DINOSEB	10.941	9.661	16379017	3570800	2.108	1.228 #
15) T	Picloram	10.799	10.656	257.8E6	142.0E6	20.291	24.558
16) T	DCPA	11.209	10.584	12555303	9266954	1.044	1.866 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022322\
Data File : PS018402.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Feb 2022 22:50
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 24 01:07:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
Quant Title : 8080.M
QLast Update : Tue Feb 22 00:27:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

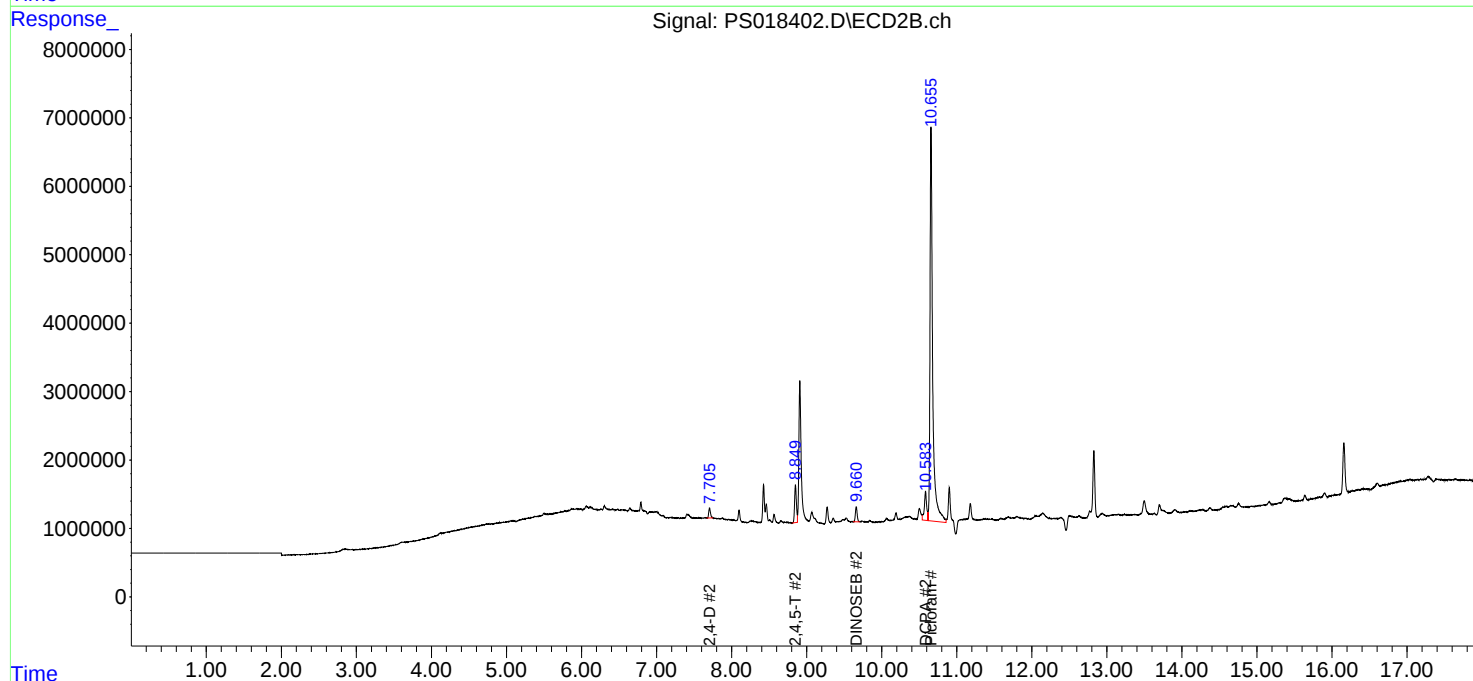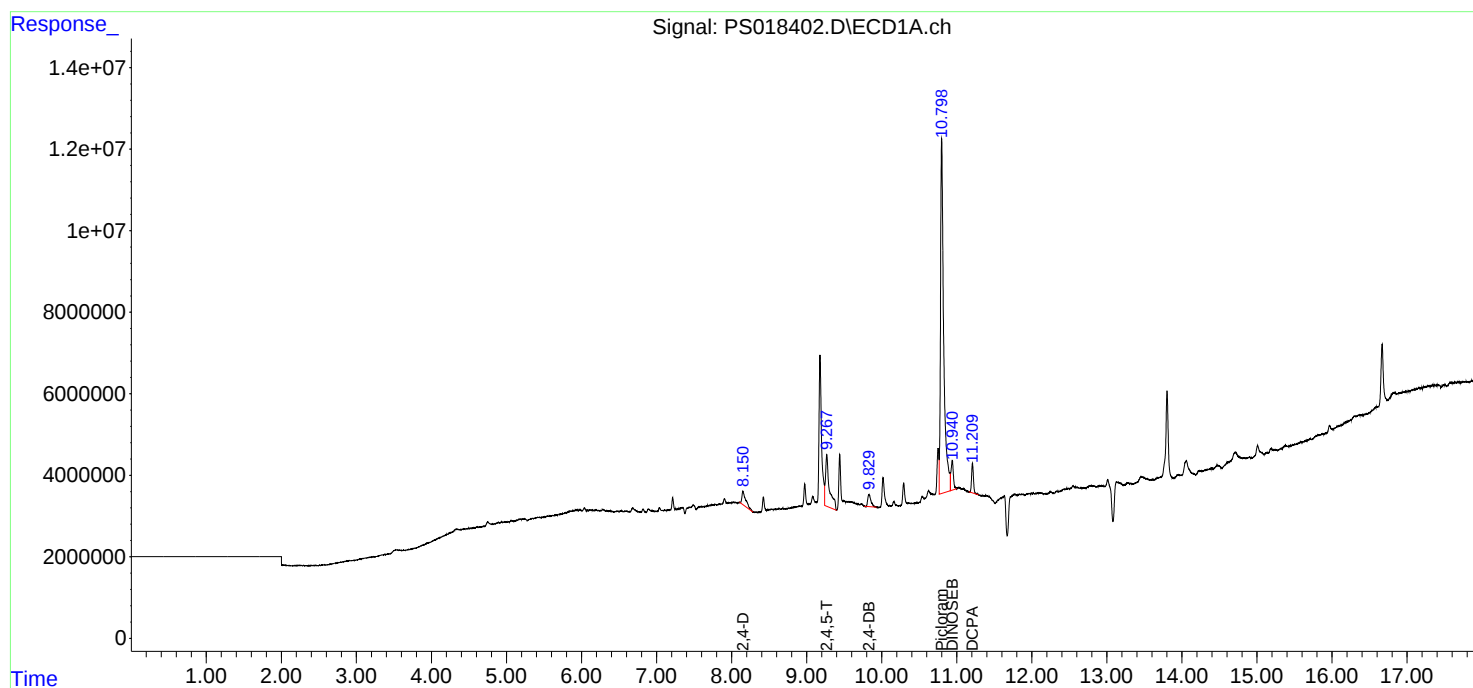


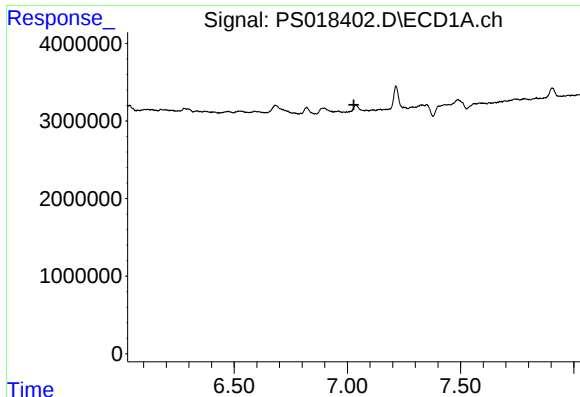

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.029 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

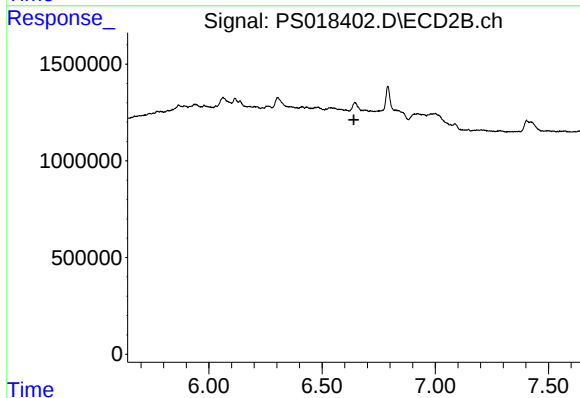


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.640 min
Response: 0
Conc: N.D.

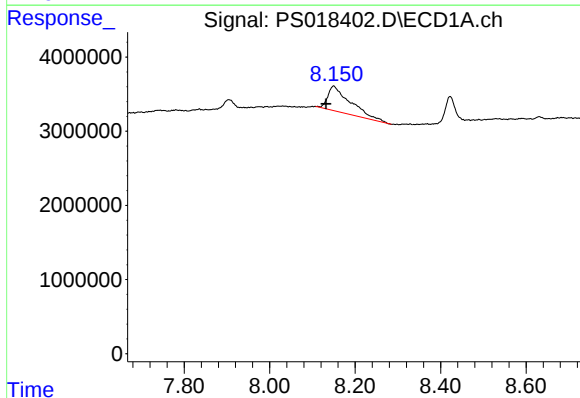


#9 2,4-D

R.T.: 8.150 min
Delta R.T.: 0.018 min
Response: 12464474
Conc: 6.11 ng/ml

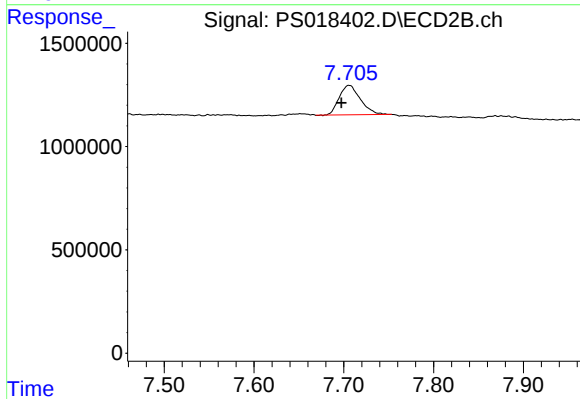

#9 2,4-D


R.T.: 7.706 min
Delta R.T.: 0.008 min
Response: 2336859
Conc: 2.50 ng/ml

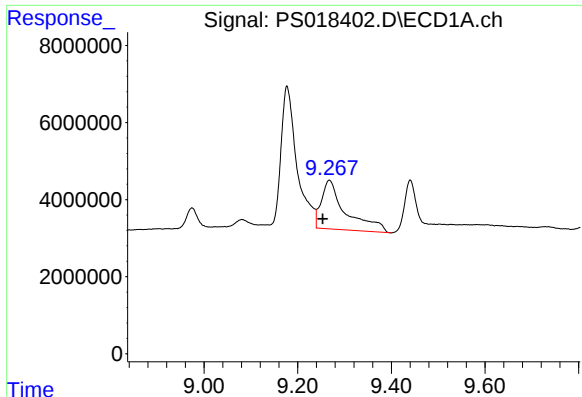

#12 2,4,5-T


R.T.: 9.268 min
Delta R.T.: 0.014 min
Response: 45484318
Conc: 4.52 ng/ml

Instrument :
ECD_S
ClientSampleId :

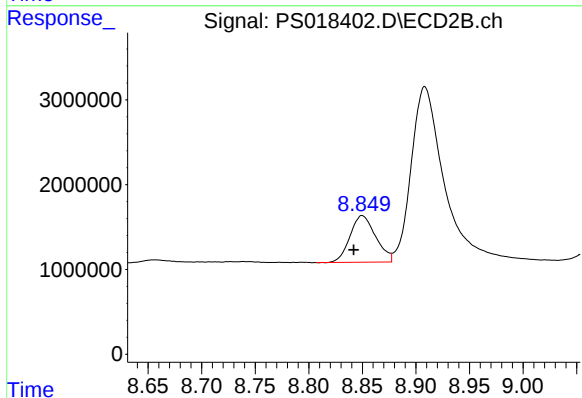


#12 2,4,5-T

R.T.: 8.850 min
Delta R.T.: 0.008 min
Response: 9172721
Conc: 2.33 ng/ml

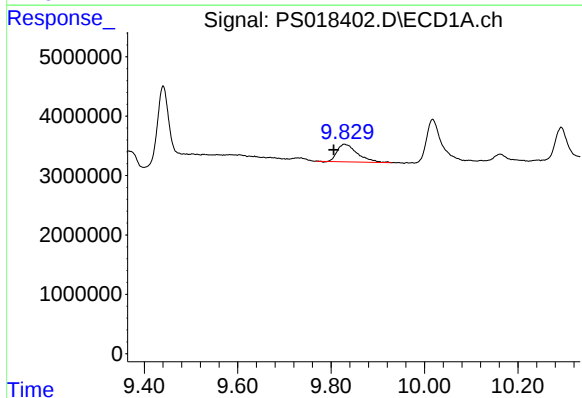


#13 2,4-DB

R.T.: 9.828 min
Delta R.T.: 0.022 min
Response: 8826322
Conc: 5.08 ng/ml

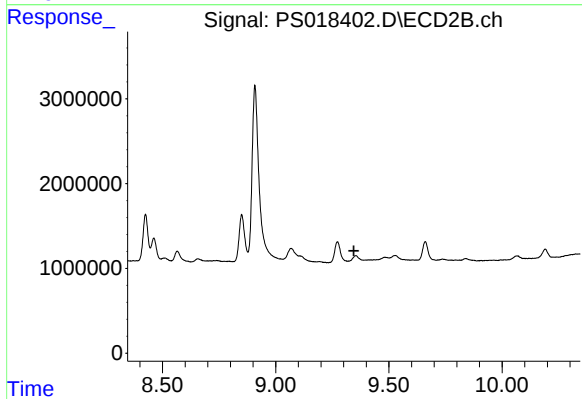

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.345 min
Response: 0
Conc: N.D.

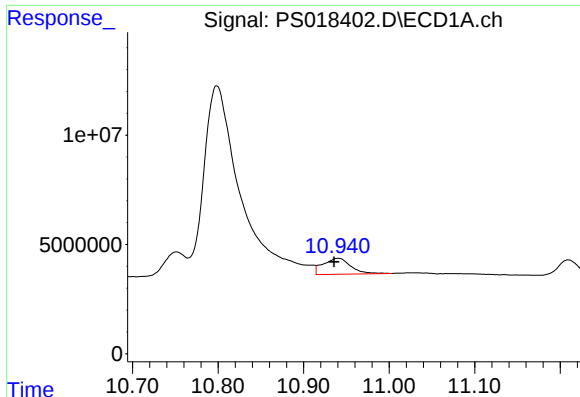

#14 DINOSEB


R.T.: 10.941 min
Delta R.T.: 0.005 min
Response: 16379017
Conc: 2.11 ng/ml

Instrument :
ECD_S
ClientSampleId :

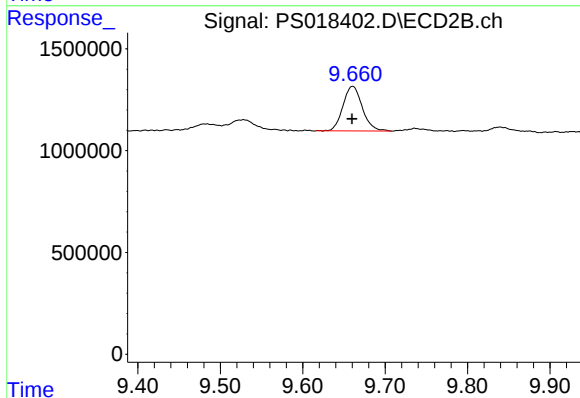


#14 DINOSEB

R.T.: 9.661 min
Delta R.T.: 0.000 min
Response: 3570800
Conc: 1.23 ng/ml

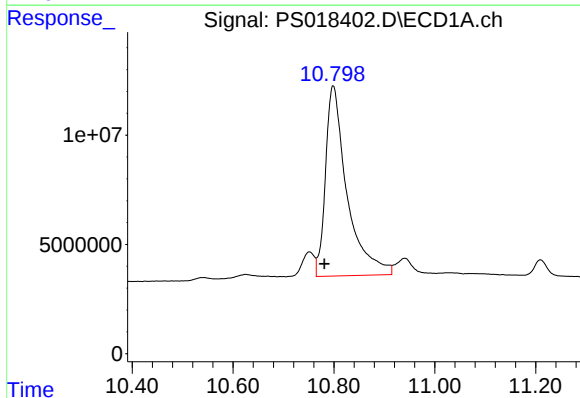


#15 Picloram

R.T.: 10.799 min
Delta R.T.: 0.017 min
Response: 257813618
Conc: 20.29 ng/ml

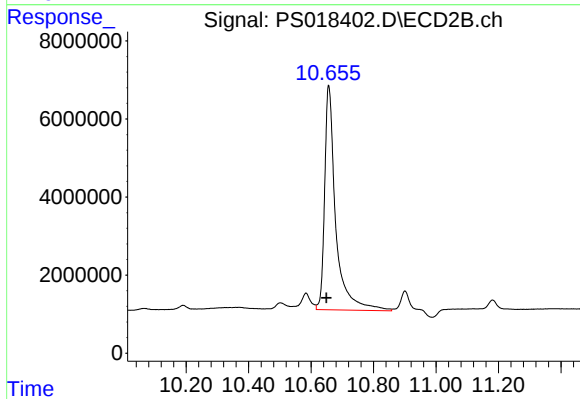

#15 Picloram


R.T.: 10.656 min
Delta R.T.: 0.007 min
Response: 142018689
Conc: 24.56 ng/ml

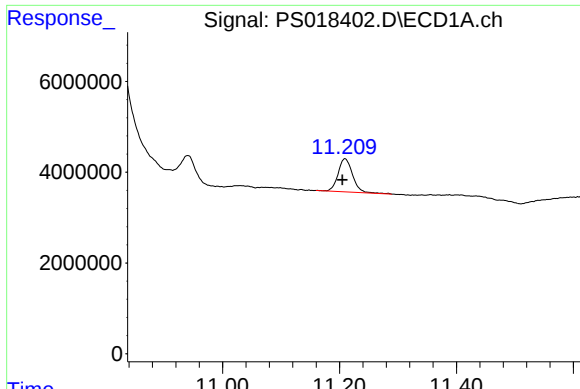

#16 DCPA

R.T.: 11.209 min
Delta R.T.: 0.004 min
Response: 12555303
Conc: 1.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

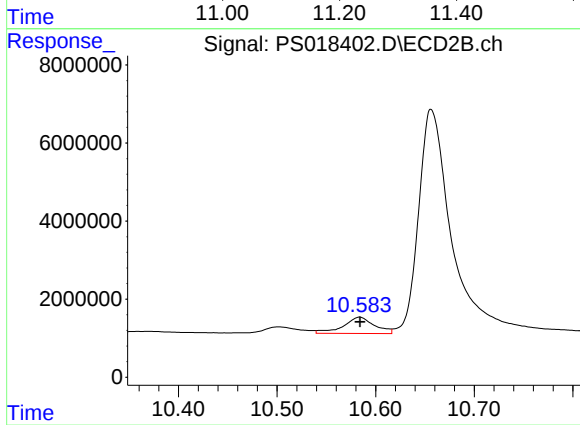

#16 DCPA

R.T.: 10.584 min
Delta R.T.: 0.000 min
Response: 9266954
Conc: 1.87 ng/ml