

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022322\
 Data File : PS018403.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Feb 2022 23:14
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 24 01:07:38 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 22 00:27:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.032	6.644	537.6E6	357.8E6	323.045	536.923 #
Target Compounds							
9) T	2,4-D	8.191f	0.000	2011242	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	8.453	0	8360989	N.D.	2.025
12) T	2,4,5-T	9.256	0.000	52116117	0	5.181	N.D. #
13) T	2,4-DB	0.000	9.297f	0	4907375	N.D.	9.083
14) T	DINOSEB	10.876f	0.000	137.3E6	0	17.672	N.D. #
15) T	Picloram	0.000	10.593f	0	2138379	N.D.	<MDL
16) T	DCPA	0.000	10.593	0	2138379	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022322\
Data File : PS018403.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Feb 2022 23:14
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 24 01:07:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
Quant Title : 8080.M
QLast Update : Tue Feb 22 00:27:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

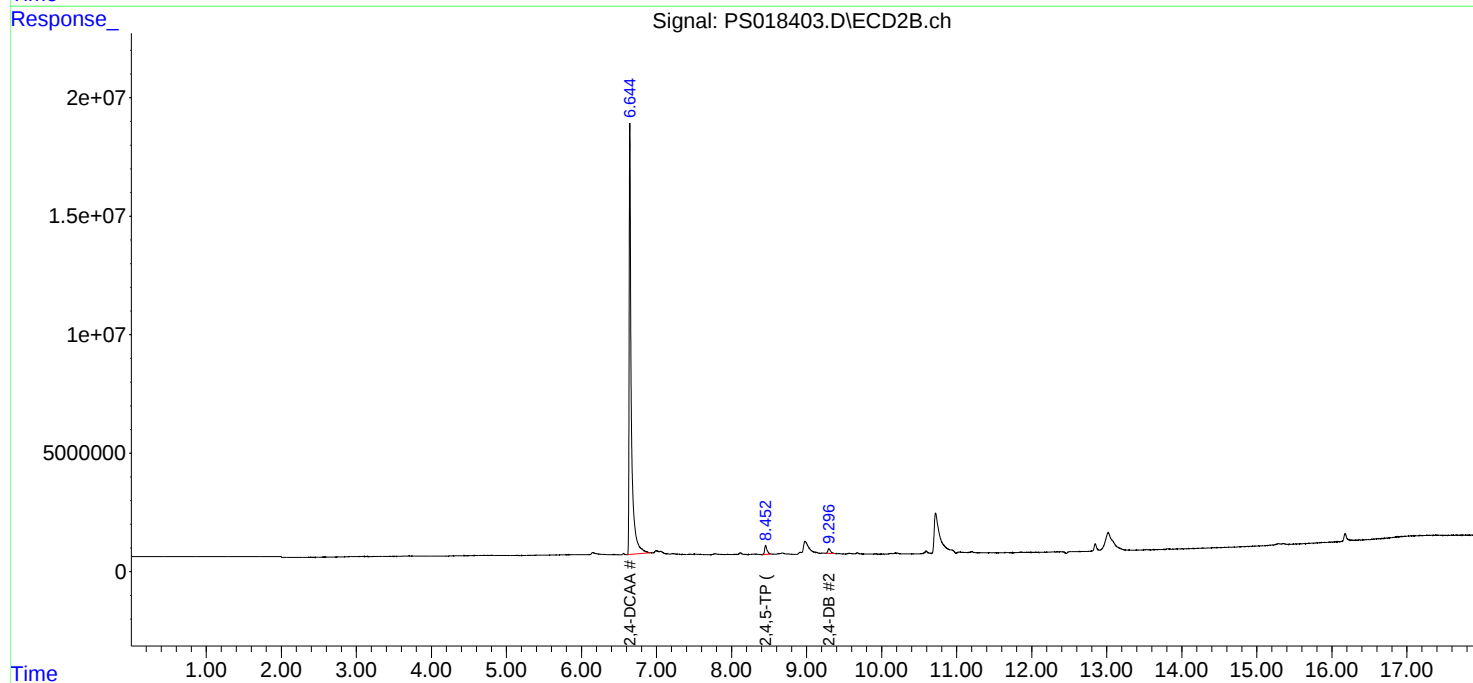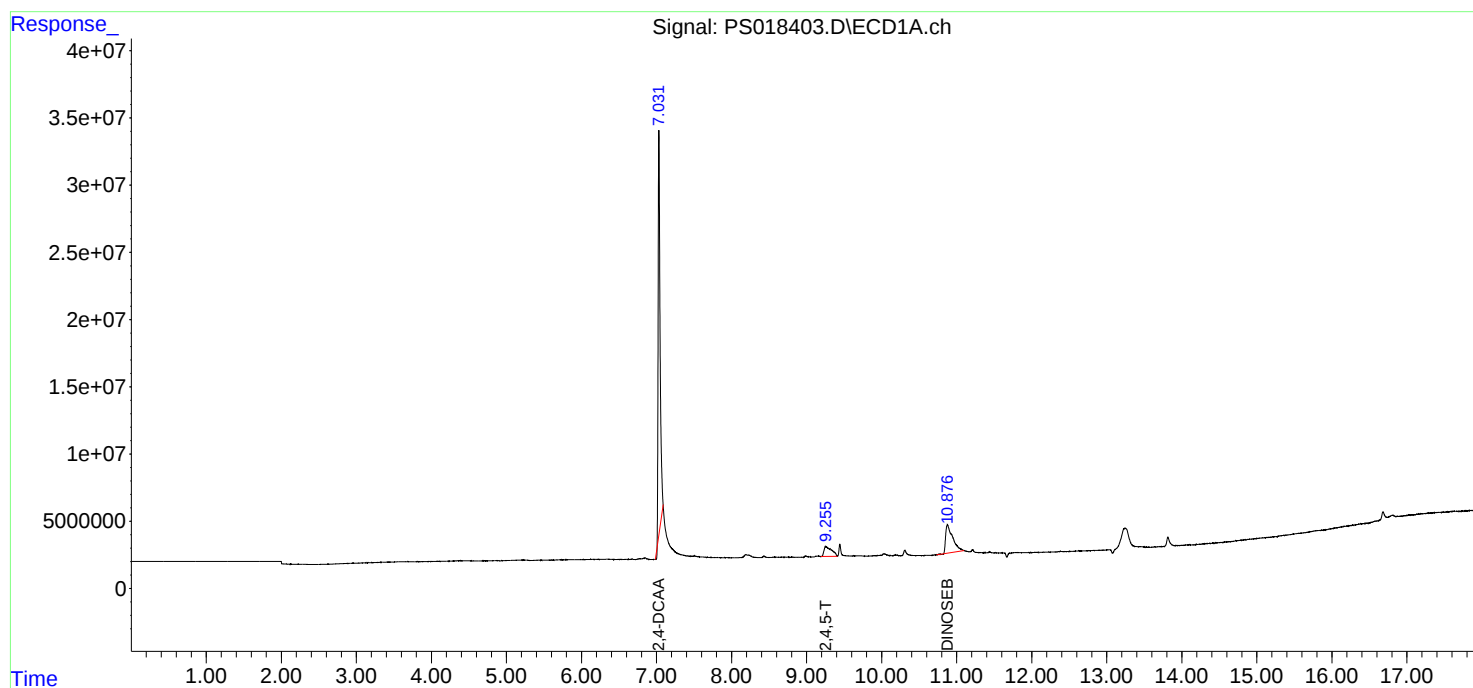


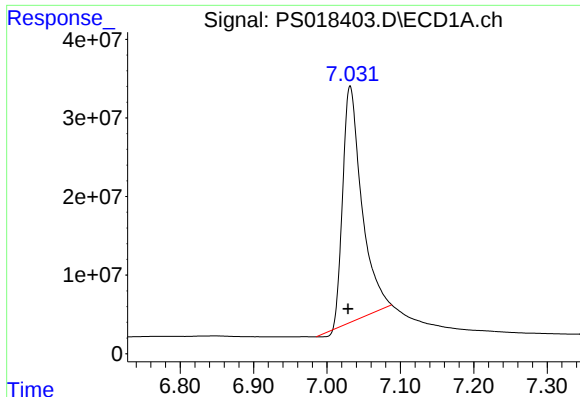

#4 2,4-DCAA


R.T.: 7.032 min
Delta R.T.: 0.003 min
Response: 537562421
Conc: 323.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

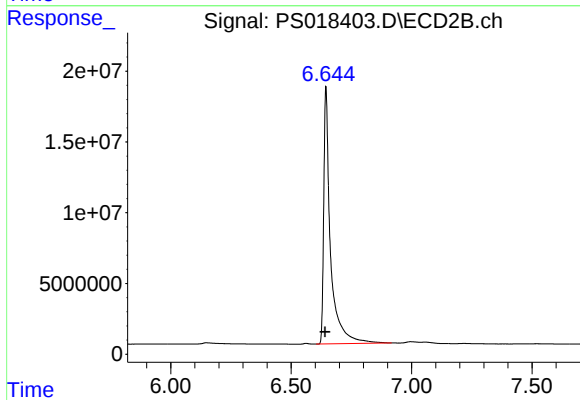


#4 2,4-DCAA

R.T.: 6.644 min
Delta R.T.: 0.004 min
Response: 357774607
Conc: 536.92 ng/ml

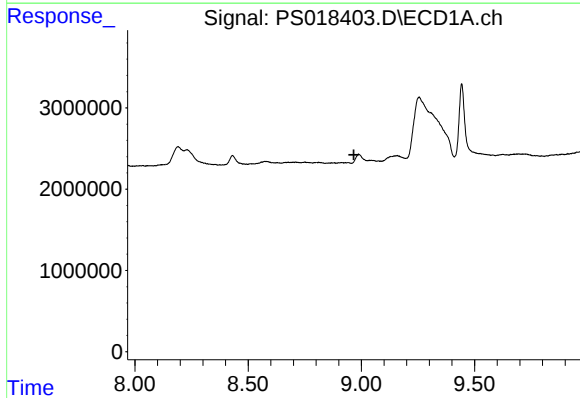


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 8.967 min
Response: 0
Conc: N.D.

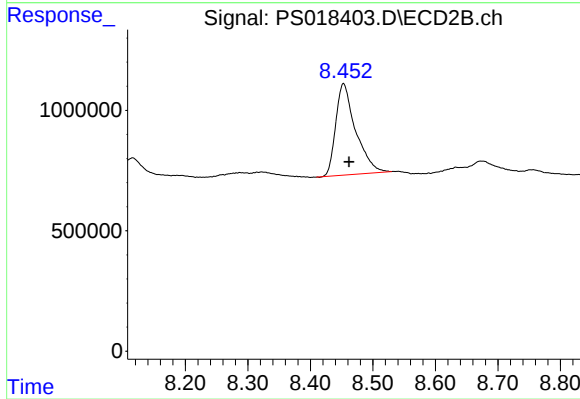

#11 2,4,5-TP (SILVEX)


R.T.: 8.453 min
Delta R.T.: -0.009 min
Response: 8360989
Conc: 2.03 ng/ml

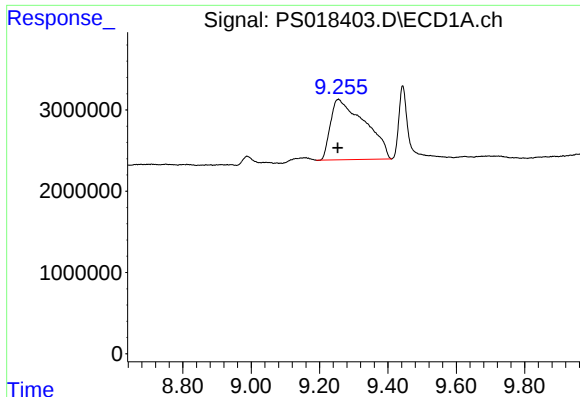

#12 2,4,5-T


R.T.: 9.256 min
Delta R.T.: 0.002 min
Response: 52116117
Conc: 5.18 ng/ml

Instrument :
ECD_S
ClientSampleId :

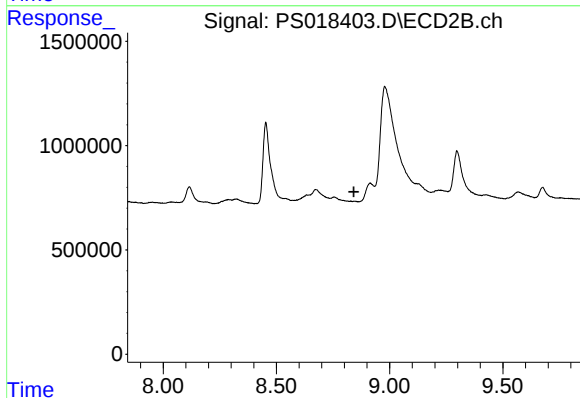


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 8.842 min
Response: 0
Conc: N.D.

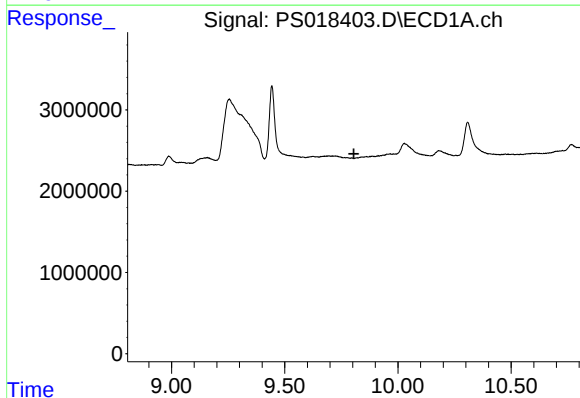


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.806 min
Response: 0
Conc: N.D.

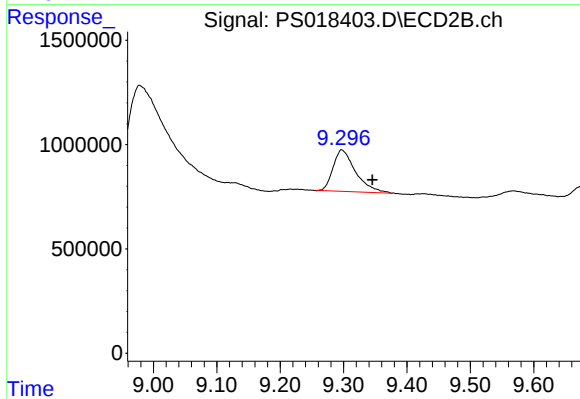

#13 2,4-DB


R.T.: 9.297 min
Delta R.T.: -0.048 min
Response: 4907375
Conc: 9.08 ng/ml

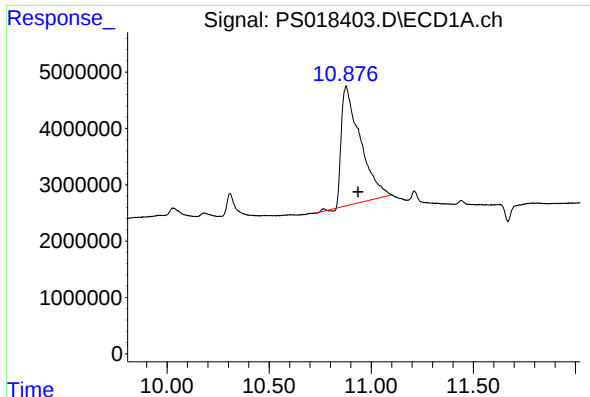

#14 DINOSEB

R.T.: 10.876 min
Delta R.T.: -0.059 min
Response: 137295026
Conc: 17.67 ng/ml

Instrument :
ECD_S
ClientSampleId :

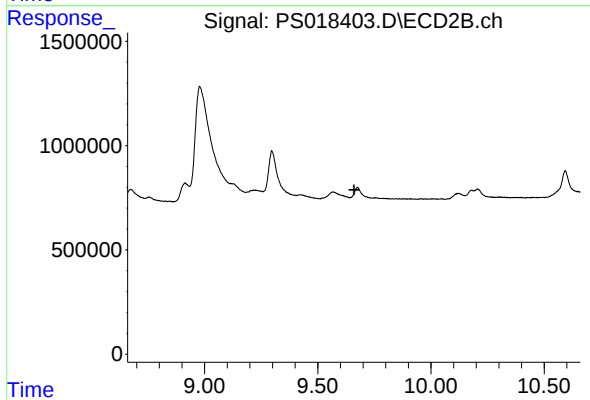

#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.660 min
Response: 0
Conc: N.D.