

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022323\
 Data File : PS022250.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Feb 2023 09:38
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 23 18:57:30 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022023.M
 Quant Title : 8080.M
 QLast Update : Mon Feb 20 13:26:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.270	0.000	1261852	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	2.453f	2.518	2039064	847738	<MDL	<MDL #
2) T	3,5-DICHL...	5.675	0.000	23180463	0	6.236	N.D. #
3) T	4-Nitroph...	6.162	0.000	1859166	0	1.461	N.D. #
5) T	DICAMBA	0.000	6.942f	0	18091109	N.D.	1.872
6) T	MCP	0.000	6.942	0	18091109	N.D.	2.370
9) T	2,4-D	7.235	0.000	118.6E6	0	36.162	N.D. #
11) T	2,4,5-TP ...	7.986	0.000	308698	0	<MDL	N.D. #
12) T	2,4,5-T	8.175f	0.000	106241	0	<MDL	N.D. #
14) T	DINOSEB	9.814	0.000	26936070	0	1.960	N.D. #
15) T	Picloram	9.674f	10.703f	5708190	485135	<MDL	<MDL #
16) T	DCPA	0.000	10.703	0	485135	N.D.	<MDL


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022323\
Data File : PS022250.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Feb 2023 09:38
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 23 18:57:30 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022023.M
Quant Title : 8080.M
QLast Update : Mon Feb 20 13:26:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

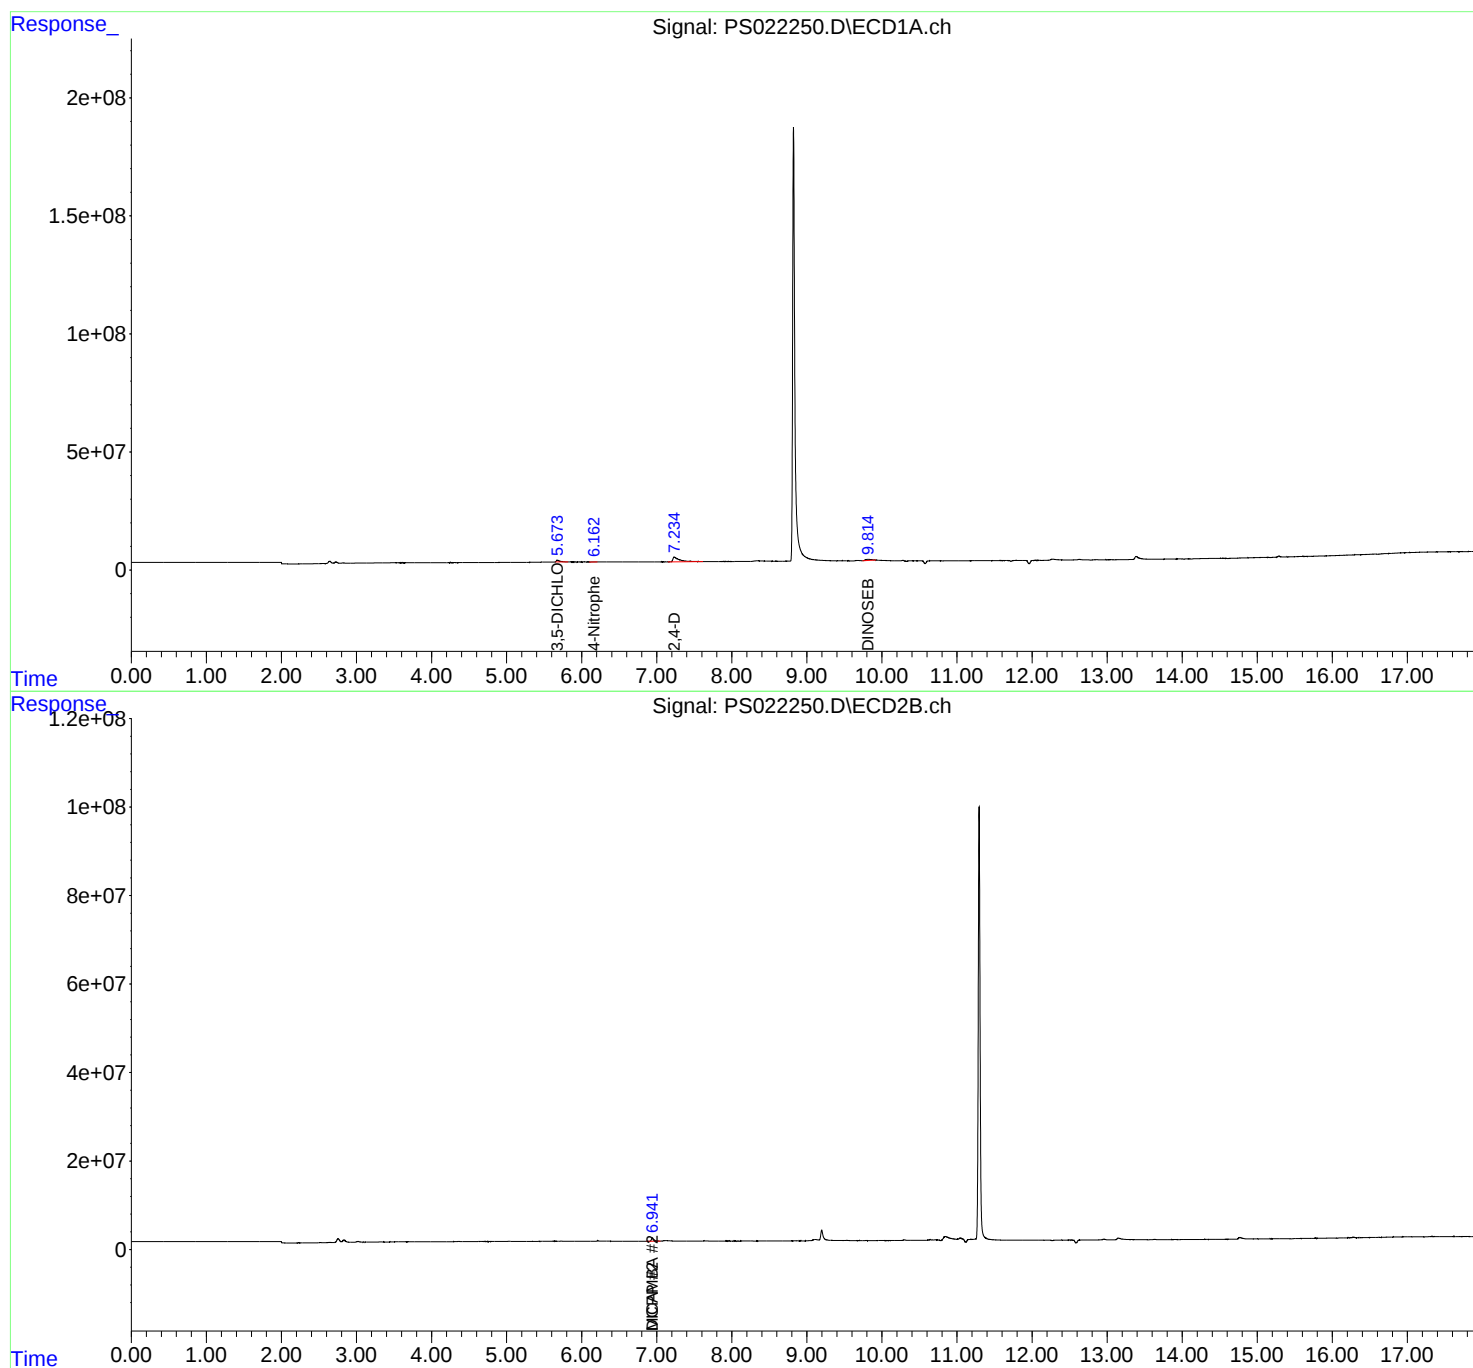


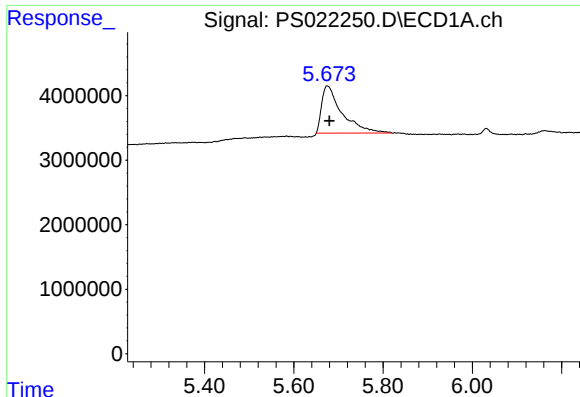

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.675 min
Delta R.T.: -0.004 min
Response: 23180463
Conc: 6.24 ng/ml

Instrument :
ECD_S
ClientSampleId :

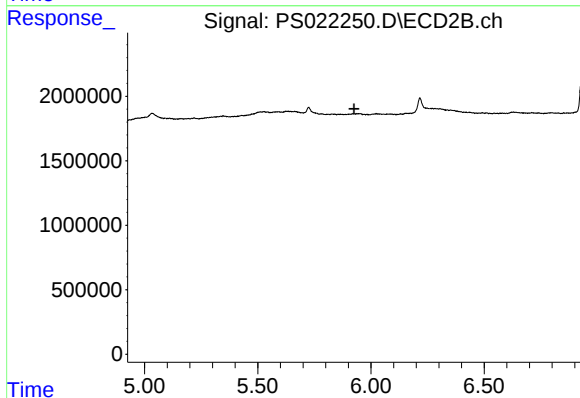


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.925 min
Response: 0
Conc: N.D.

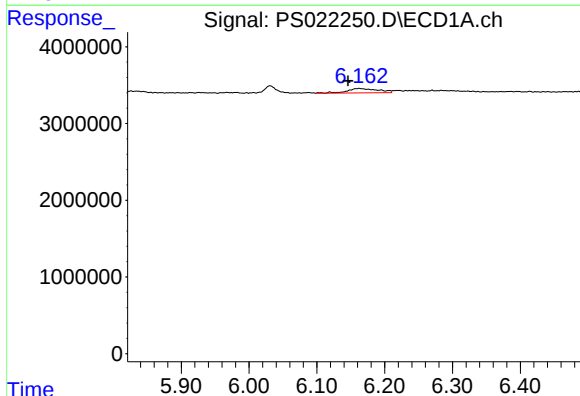


#3 4-Nitrophenol

R.T.: 6.162 min
Delta R.T.: 0.016 min
Response: 1859166
Conc: 1.46 ng/ml

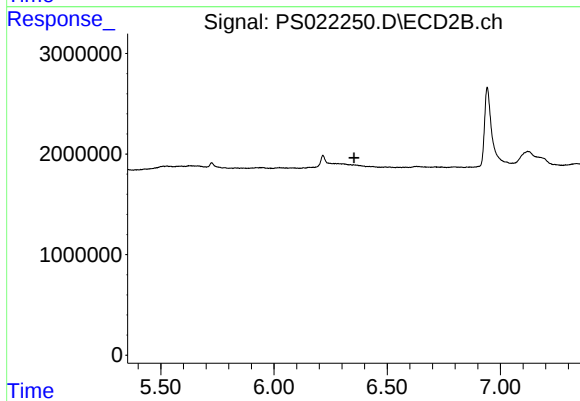

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.353 min
Response: 0
Conc: N.D.

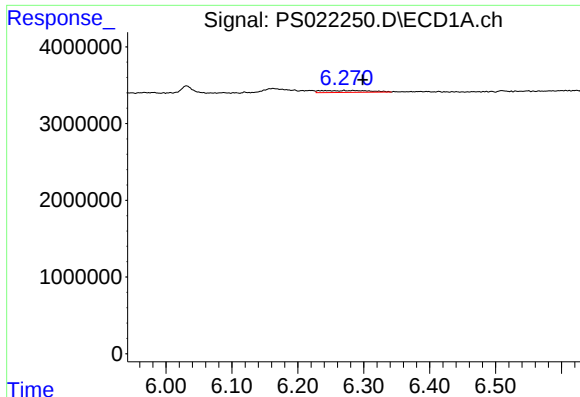

#4 2,4-DCAA


R.T.: 6.270 min
Delta R.T.: -0.028 min
Response: 1261852
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

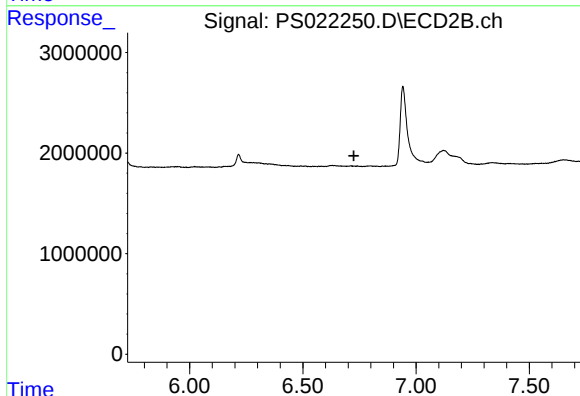


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.726 min
Response: 0
Conc: N.D.

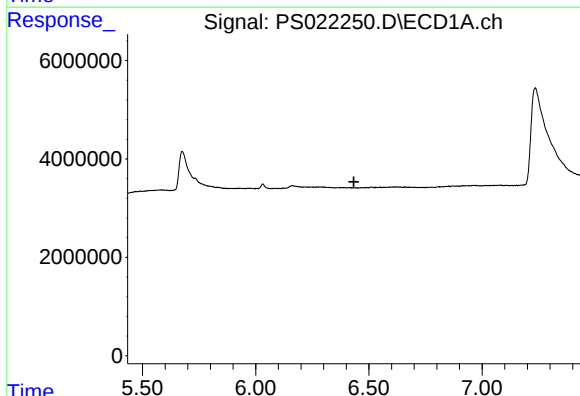


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 6.434 min
Response: 0
Conc: N.D.

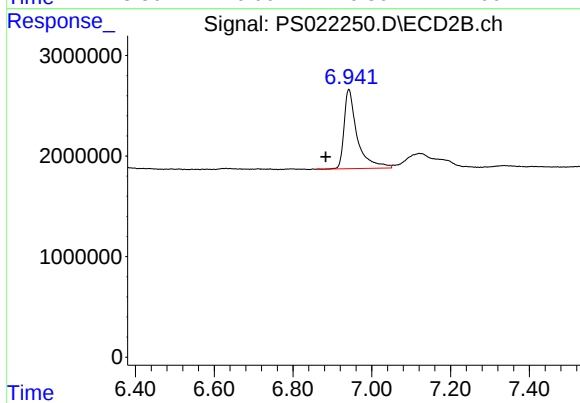

#5 DICAMBA


R.T.: 6.942 min
Delta R.T.: 0.059 min
Response: 18091109
Conc: 1.87 ng/ml

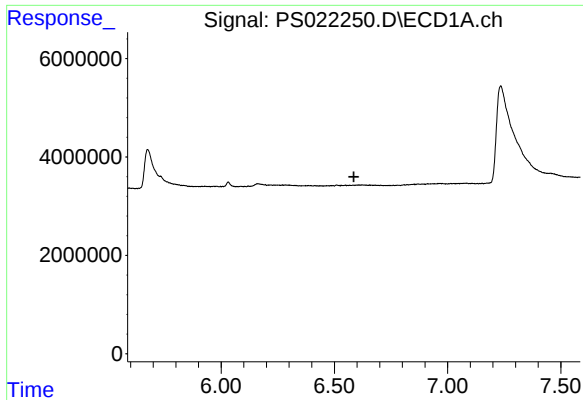

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 6.586 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

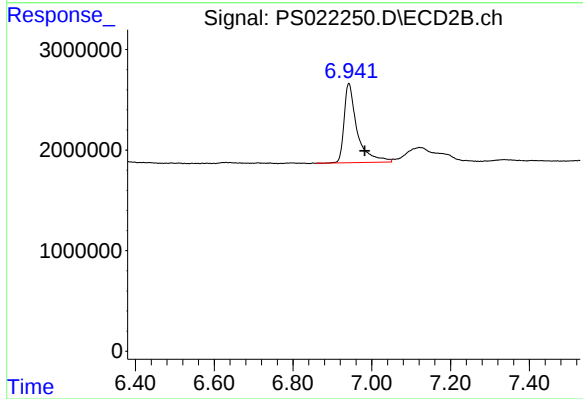


#6 MCPP

R.T.: 6.942 min
Delta R.T.: -0.040 min
Response: 18091109
Conc: 2.37 ug/ml

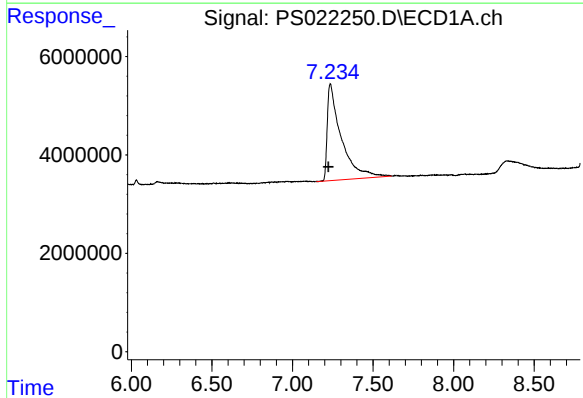


#9 2,4-D

R.T.: 7.235 min
Delta R.T.: 0.012 min
Response: 118565120
Conc: 36.16 ng/ml

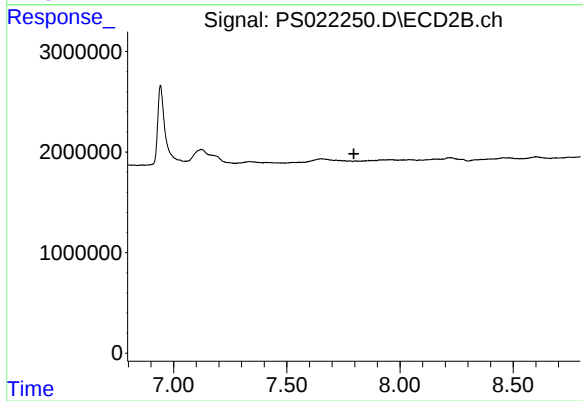

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.796 min
Response: 0
Conc: N.D.

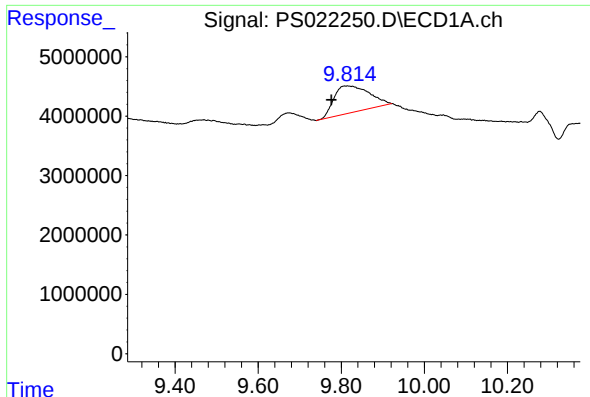

#14 DINOSEB

R.T.: 9.814 min
Delta R.T.: 0.038 min
Response: 26936070
Conc: 1.96 ng/ml

Instrument :
ECD_S
ClientSampleId :

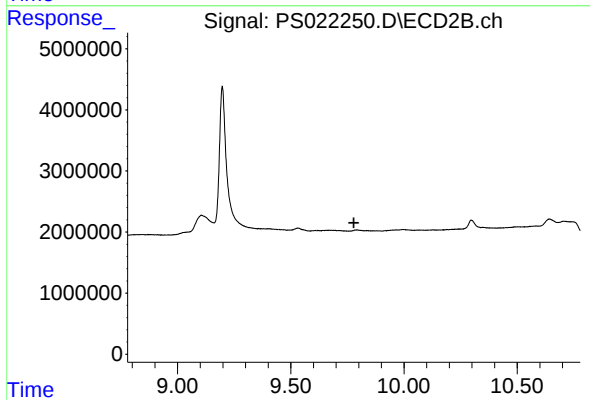

#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.779 min
Response: 0
Conc: N.D.