

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022420\
 Data File : PS008961.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Feb 2020 12:50
 Operator : DD\AJ
 Sample : L1626-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 FK-GF-02-051-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 24 14:22:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.248	6.941	557.3E6	221.9E6	254.872	230.267
Target Compounds							
2) T	3,5-DICHL...	0.000	6.115	0	114.1E6	N.D.	78.182
5) T	DICAMBA	7.375	0.000	166.8E6	0	20.534	N.D. #
7) T	MCPA	7.742	7.409	75211401	-4158805	9.350	N.D. #
11) T	2,4,5-TP ...	0.000	8.796	0	56620948	N.D.	10.453
12) T	2,4,5-T	9.457	0.000	103.4E6	0	9.672	N.D. #
13) T	2,4-DB	10.111	0.000	73712411	0	51.081	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022420\
Data File : PS008961.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Feb 2020 12:50
Operator : DD\AJ
Sample : L1626-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
FK-GF-02-051-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 24 14:22:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

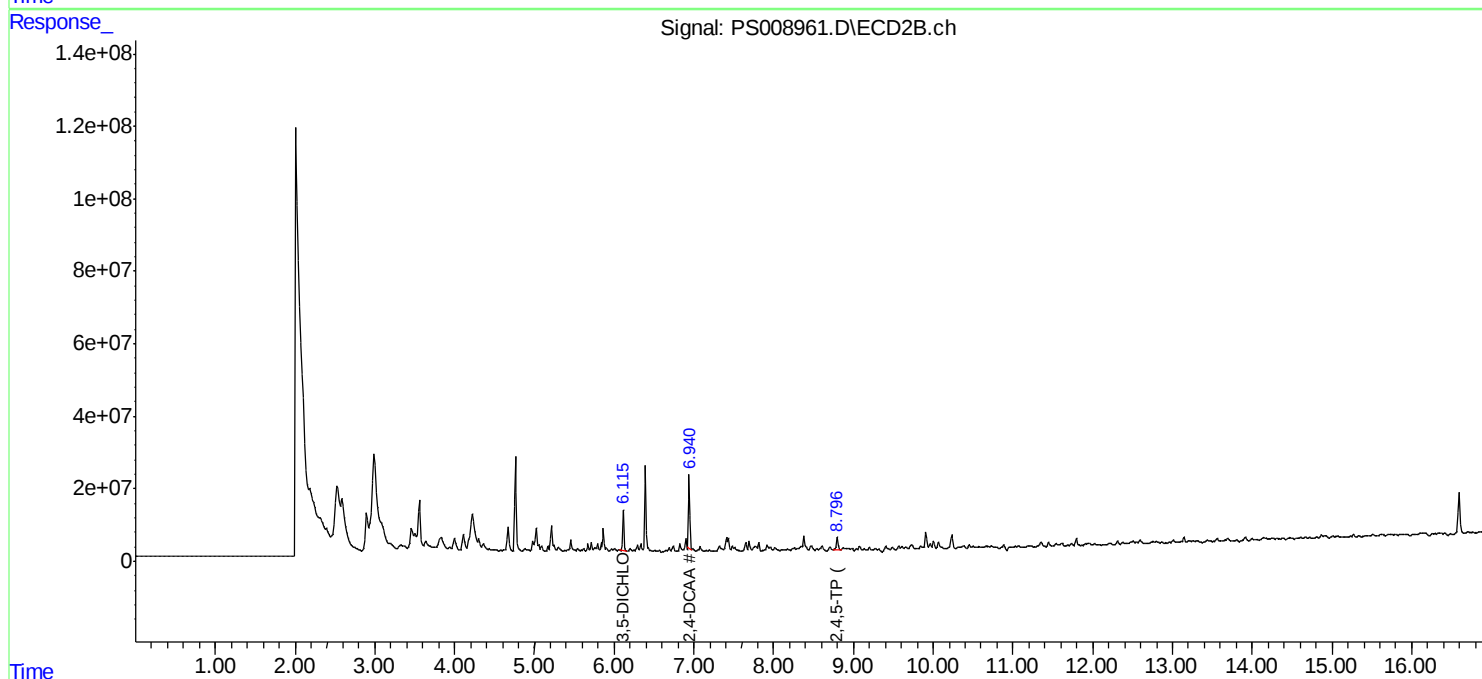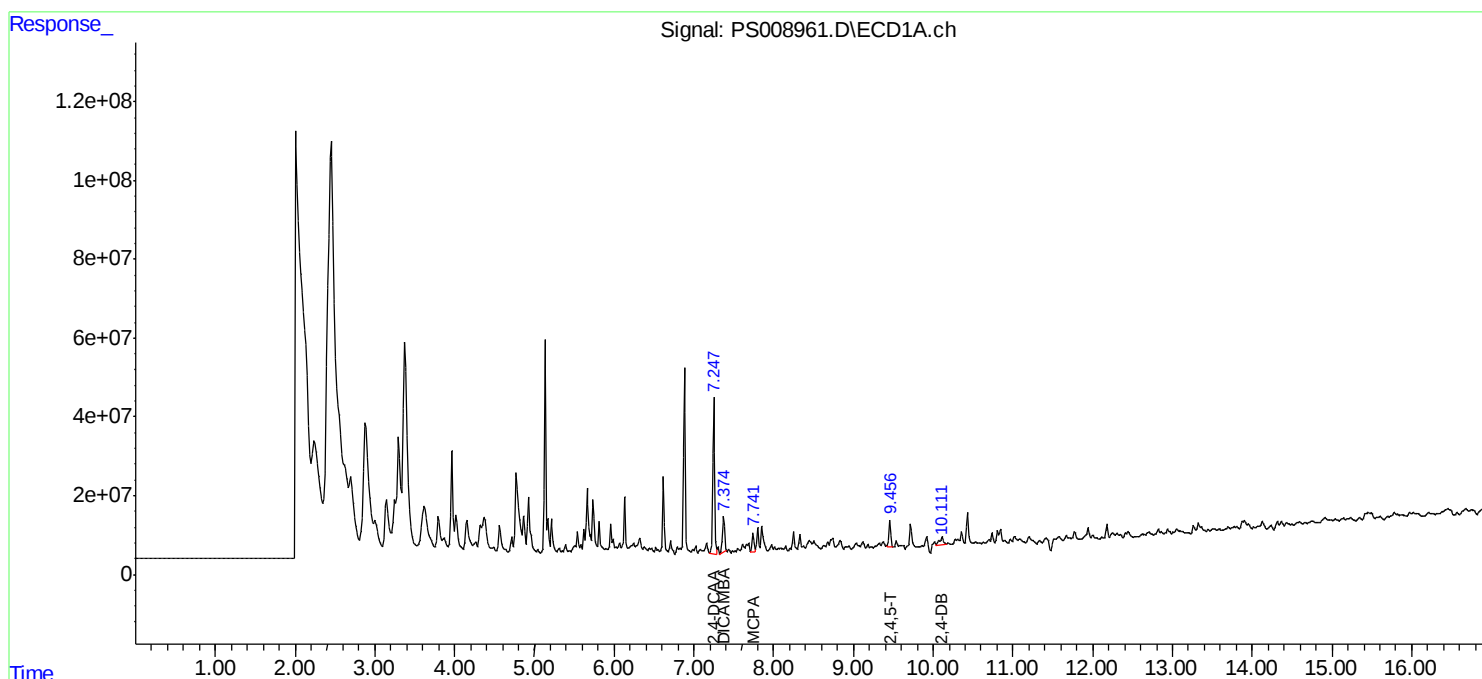


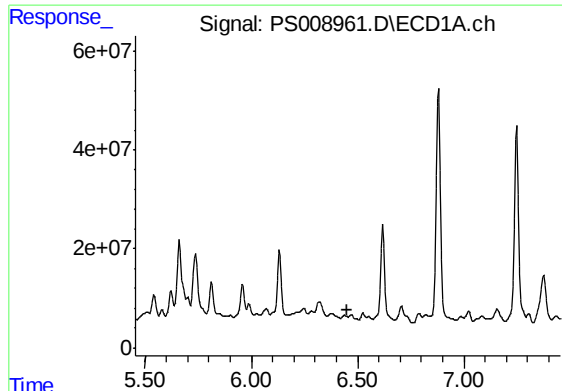

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
FK-GF-02-051-A

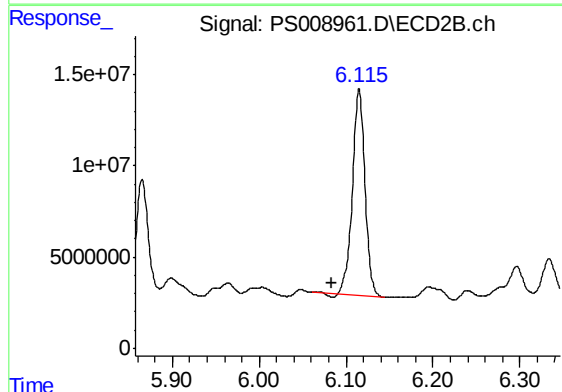


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.115 min
Delta R.T.: 0.032 min
Response: 114088251
Conc: 78.18 ng/ml

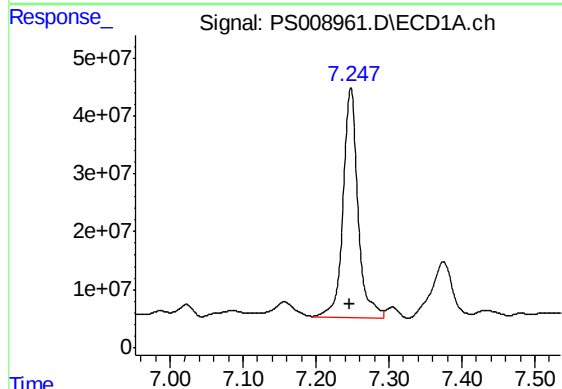


#4 2,4-DCAA

R.T.: 7.248 min
Delta R.T.: 0.000 min
Response: 557300903
Conc: 254.87 ng/ml

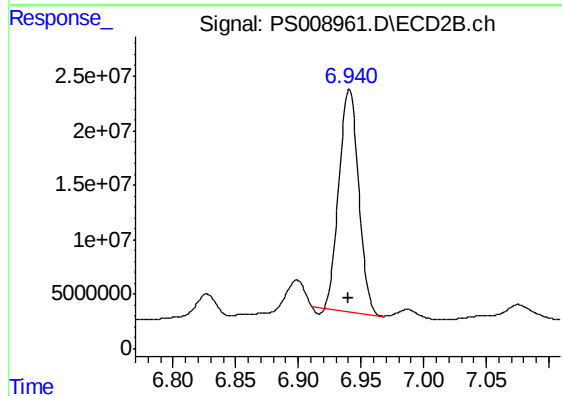

#4 2,4-DCAA


R.T.: 6.941 min
Delta R.T.: 0.000 min
Response: 221874629
Conc: 230.27 ng/ml

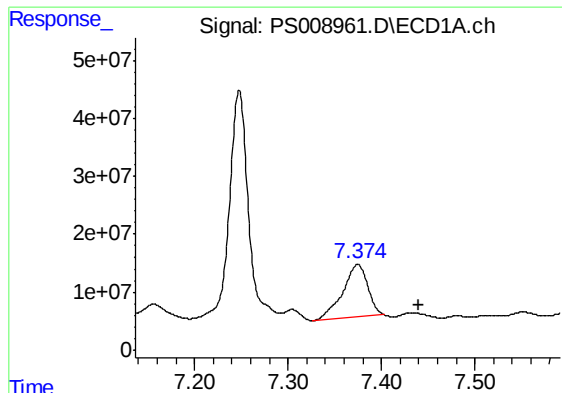

#5 DICAMBA


R.T.: 7.375 min
Delta R.T.: -0.066 min
Response: 166817714
Conc: 20.53 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-GF-02-051-A

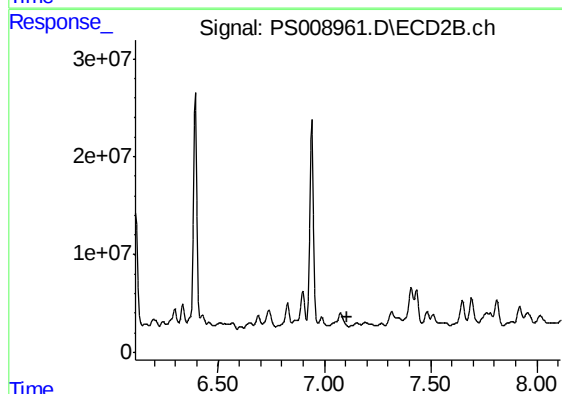


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.111 min
Response: 0
Conc: N.D.

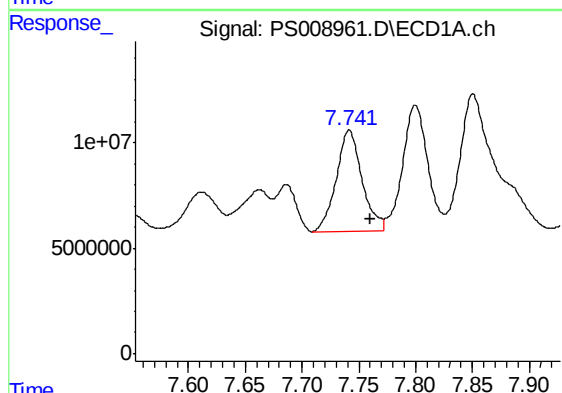


#7 MCPA

R.T.: 7.742 min
Delta R.T.: -0.019 min
Response: 75211401
Conc: 9.35 ug/ml

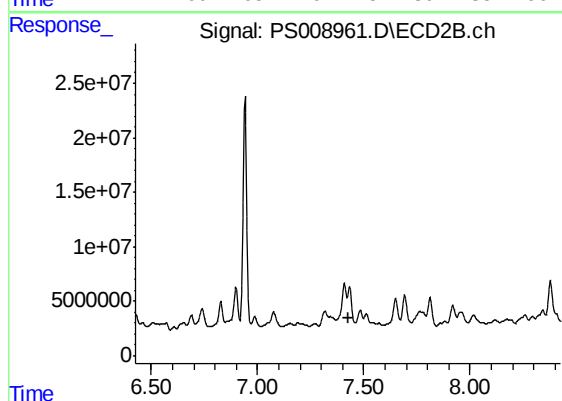

#7 MCPA


R.T.: 7.409 min
Delta R.T.: -0.017 min
Response: -4158805
Conc: N.D.

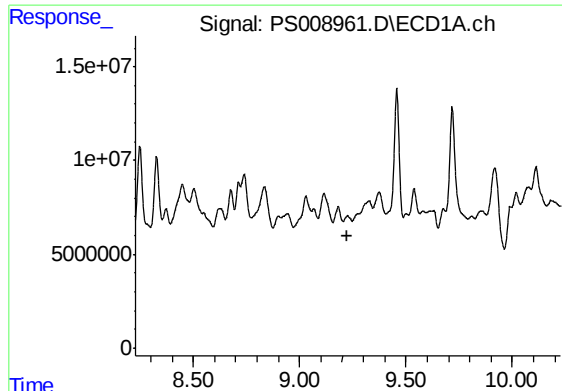

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 9.227 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
FK-GF-02-051-A

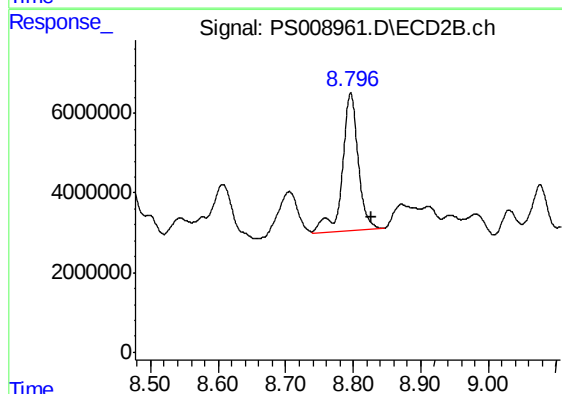


#11 2,4,5-TP (SILVEX)

R.T.: 8.796 min
Delta R.T.: -0.032 min
Response: 56620948
Conc: 10.45 ng/ml

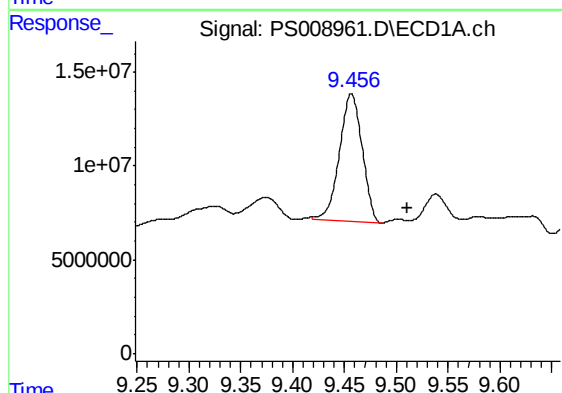


#12 2,4,5-T

R.T.: 9.457 min
Delta R.T.: -0.054 min
Response: 103412718
Conc: 9.67 ng/ml

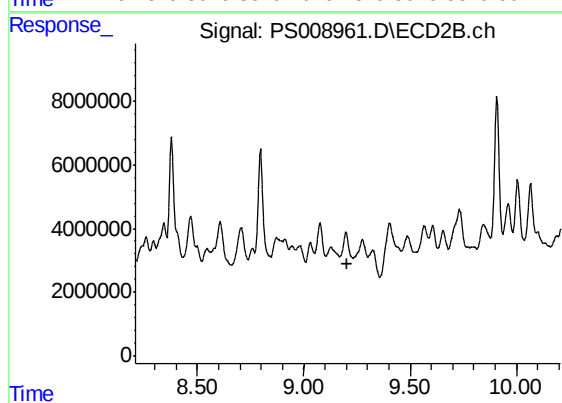

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 9.208 min
Response: 0
Conc: N.D.

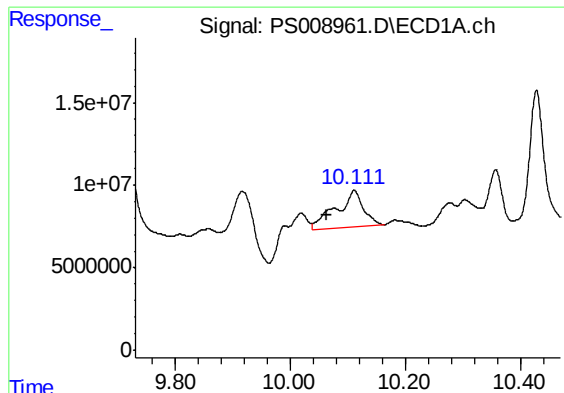

#13 2,4-DB

R.T.: 10.111 min
Delta R.T.: 0.047 min
Response: 73712411
Conc: 51.08 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-GF-02-051-A

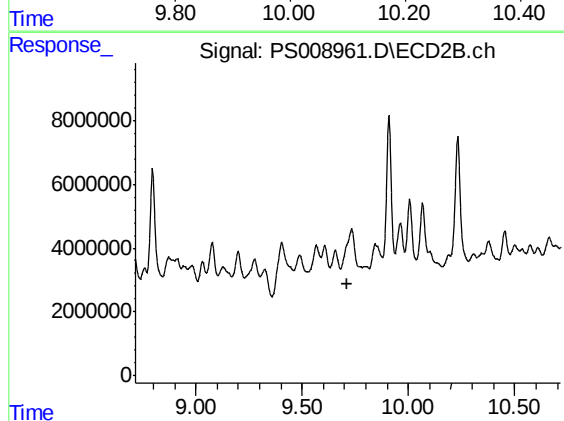

#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.715 min
Response: 0
Conc: N.D.